

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112219\
 Data File : VX013563.D
 Acq On : 23 Nov 2019 03:36
 Operator : JC/SP
 Sample : K5962-15 50X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-01-20191120

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	1553657	1943383	26.83%	7.329%
2	1.600	106	117	120	rBV	36016	85246	1.18%	0.321%
3	4.581	597	606	619	rBV	294397	796128	10.99%	3.002%
4	5.490	744	755	768	rBV	368288	1048650	14.48%	3.955%
5	5.648	771	781	794	rVV	613390	1693604	23.38%	6.387%
6	6.051	836	847	862	rBV	406126	1062560	14.67%	4.007%
7	6.849	966	978	991	rBV	999142	2298951	31.74%	8.669%
8	7.203	1026	1036	1050	rBV	3446993	7242532	100.00%	27.312%
9	8.709	1275	1283	1297	rBV	2111345	3219416	44.45%	12.141%
10	10.111	1507	1513	1519	rBV	1936800	2668400	36.84%	10.063%
11	11.135	1675	1681	1692	rVB	1598204	2028876	28.01%	7.651%
12	12.074	1829	1835	1845	rBV	1987088	2429953	33.55%	9.164%


Sum of corrected areas: 26517699

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112219\
Data File : VX013563.D
Acq On : 23 Nov 2019 03:36
Operator : JC/SP
Sample : K5962-15 50X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20191120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

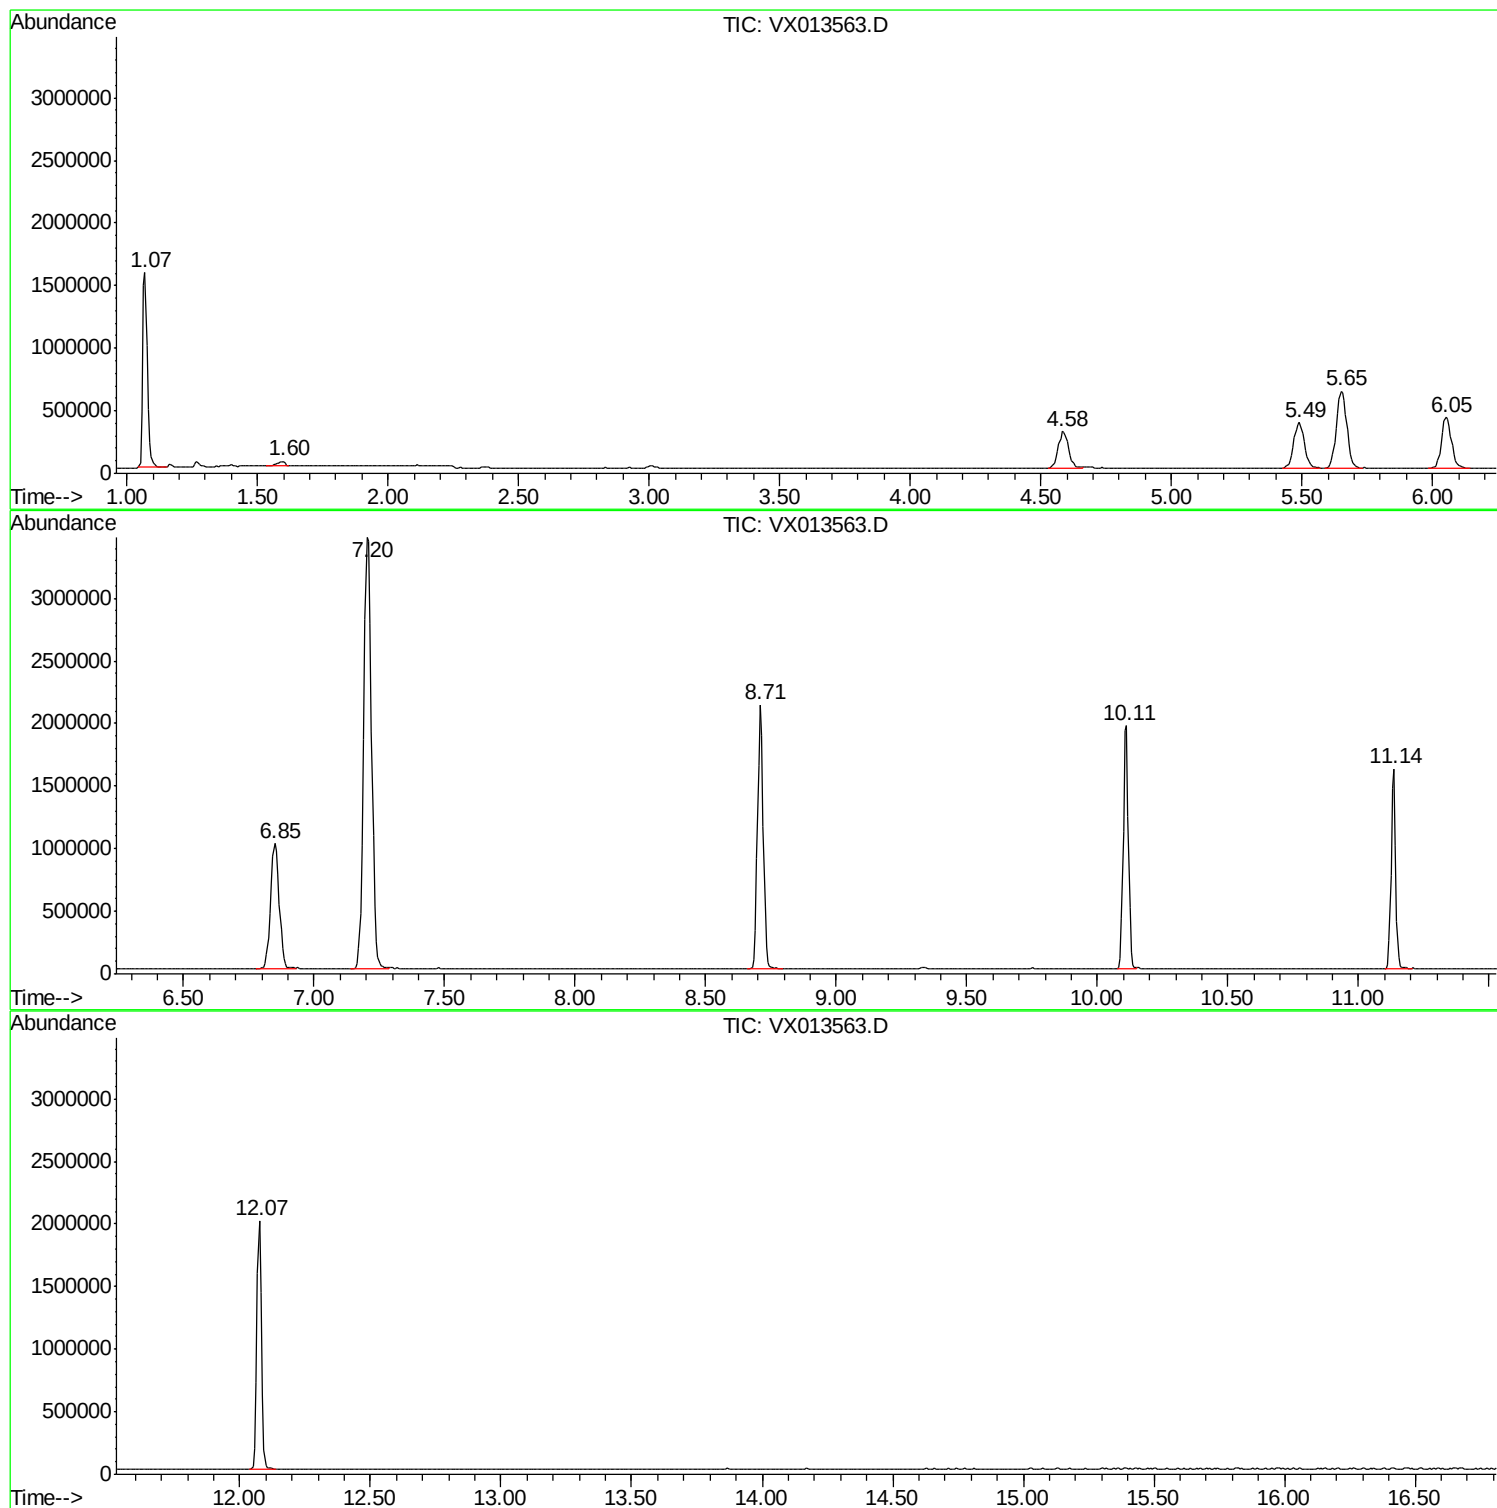

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112219\
Data File : VX013563.D
Acq On : 23 Nov 2019 03:36
Operator : JC/SP
Sample : K5962-15 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20191120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112219\
Data File : VX013563.D
Acq On : 23 Nov 2019 03:36
Operator : JC/SP
Sample : K5962-15 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20191120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc