

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112219\
 Data File : VX013571.D
 Acq On : 23 Nov 2019 06:43
 Operator : JC/SP
 Sample : K5968-11 50X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-140N-20191121

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	1552755	1968907	61.32%	10.574%
2	1.265	58	62	69	rBV	46740	64877	2.02%	0.348%
3	1.600	107	117	120	rBV10	39784	90944	2.83%	0.488%
4	3.003	342	347	354	rVB2	13657	32201	1.00%	0.173%
5	5.490	744	755	766	rBV	358716	1034294	32.21%	5.555%
6	5.649	771	781	794	rVB	603846	1670205	52.02%	8.970%
7	6.051	838	847	861	rBV	408178	1044964	32.55%	5.612%
8	6.850	967	978	990	rBV	995197	2308616	71.90%	12.399%
9	8.709	1277	1283	1296	rBV	2130113	3210670	100.00%	17.243%
10	10.111	1507	1513	1520	rBV	1937598	2695911	83.97%	14.479%
11	11.135	1676	1681	1689	rBV	1602842	2033940	63.35%	10.924%
12	12.074	1830	1835	1844	rBV	2031531	2464211	76.75%	13.234%


Sum of corrected areas: 18619740

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112219\
Data File : VX013571.D
Acq On : 23 Nov 2019 06:43
Operator : JC/SP
Sample : K5968-11 50X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-140N-20191121

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

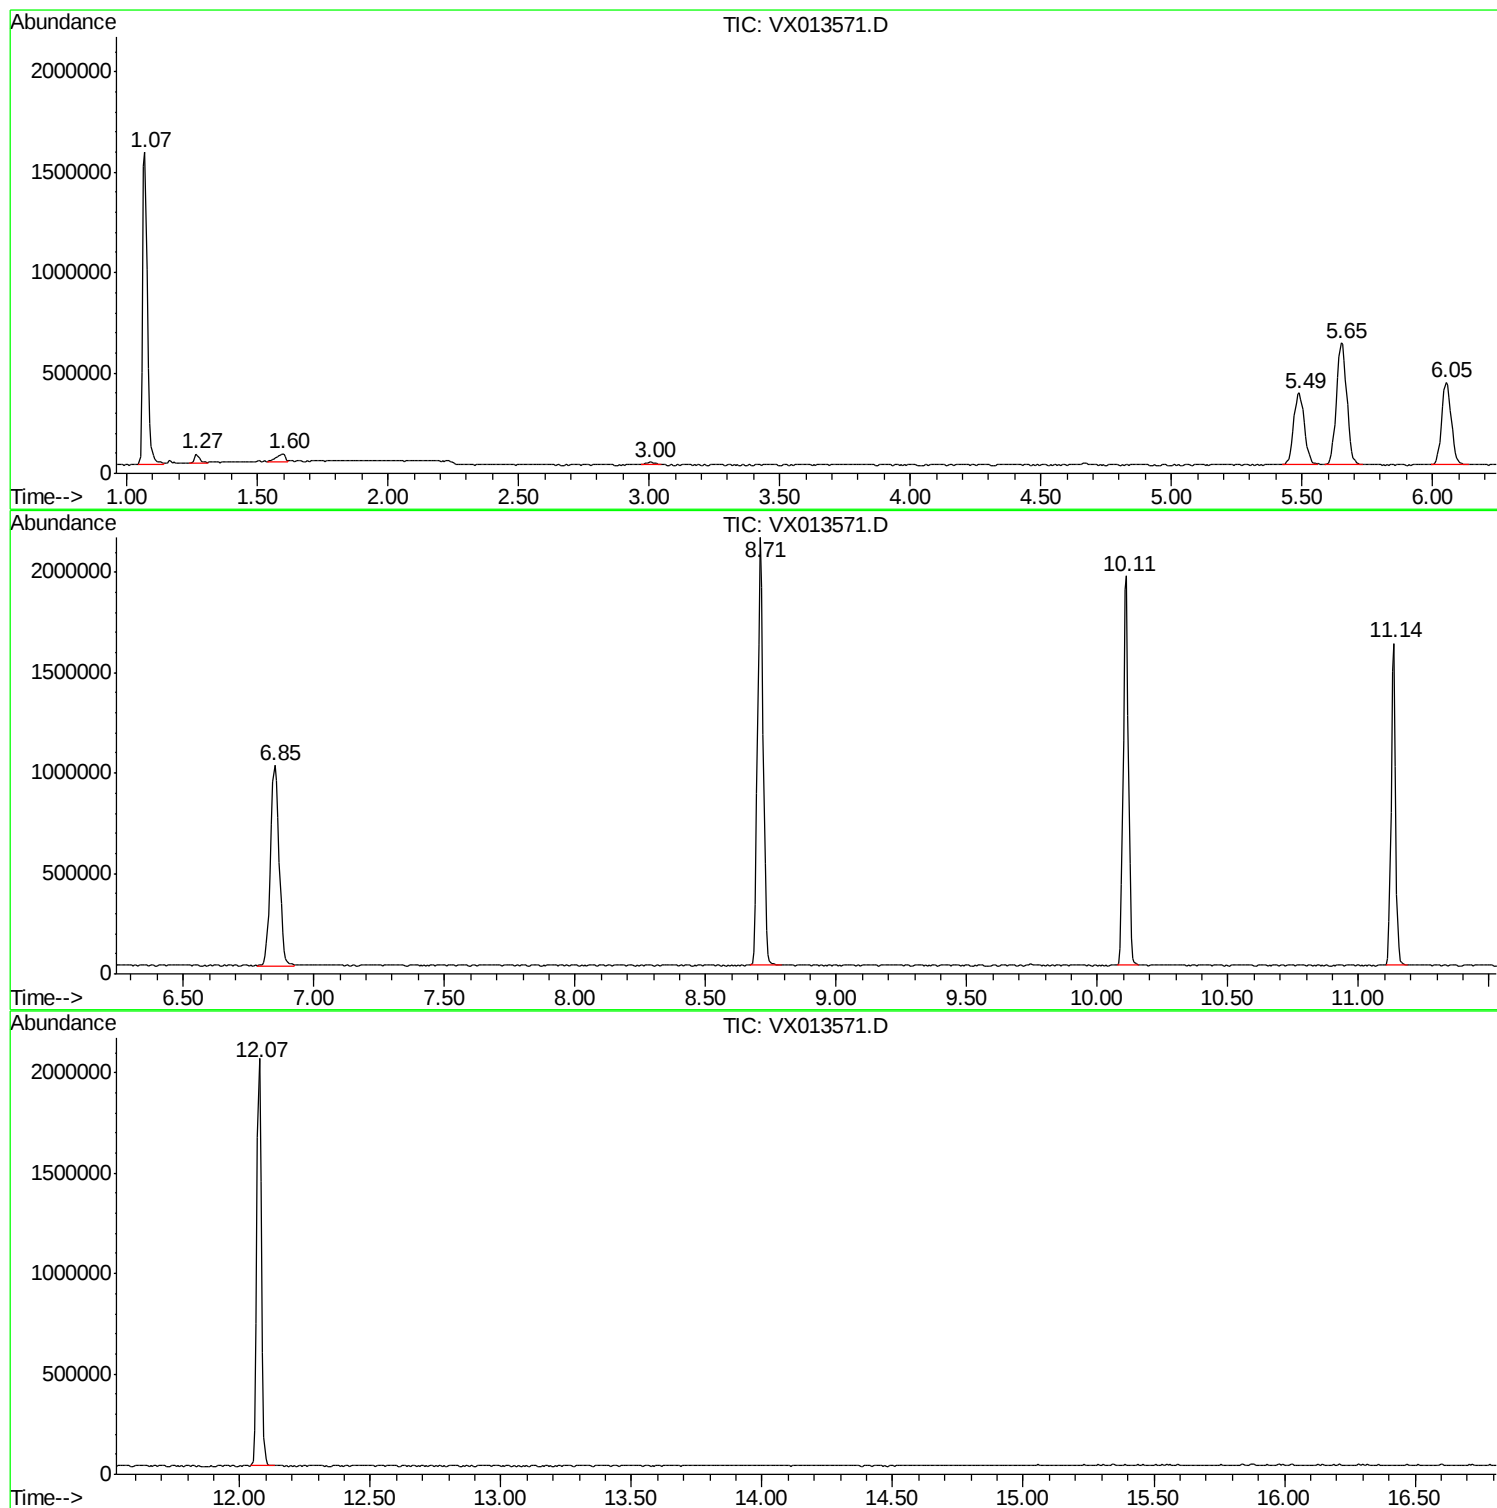

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112219\
Data File : VX013571.D
Acq On : 23 Nov 2019 06:43
Operator : JC/SP
Sample : K5968-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-140N-20191121

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112219\
Data File : VX013571.D
Acq On : 23 Nov 2019 06:43
Operator : JC/SP
Sample : K5968-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-140N-20191121

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc