


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112219\
 Data File : VX013548.D
 Acq On : 22 Nov 2019 21:24
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\624X111119W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Nov 12 01:16:13 2019

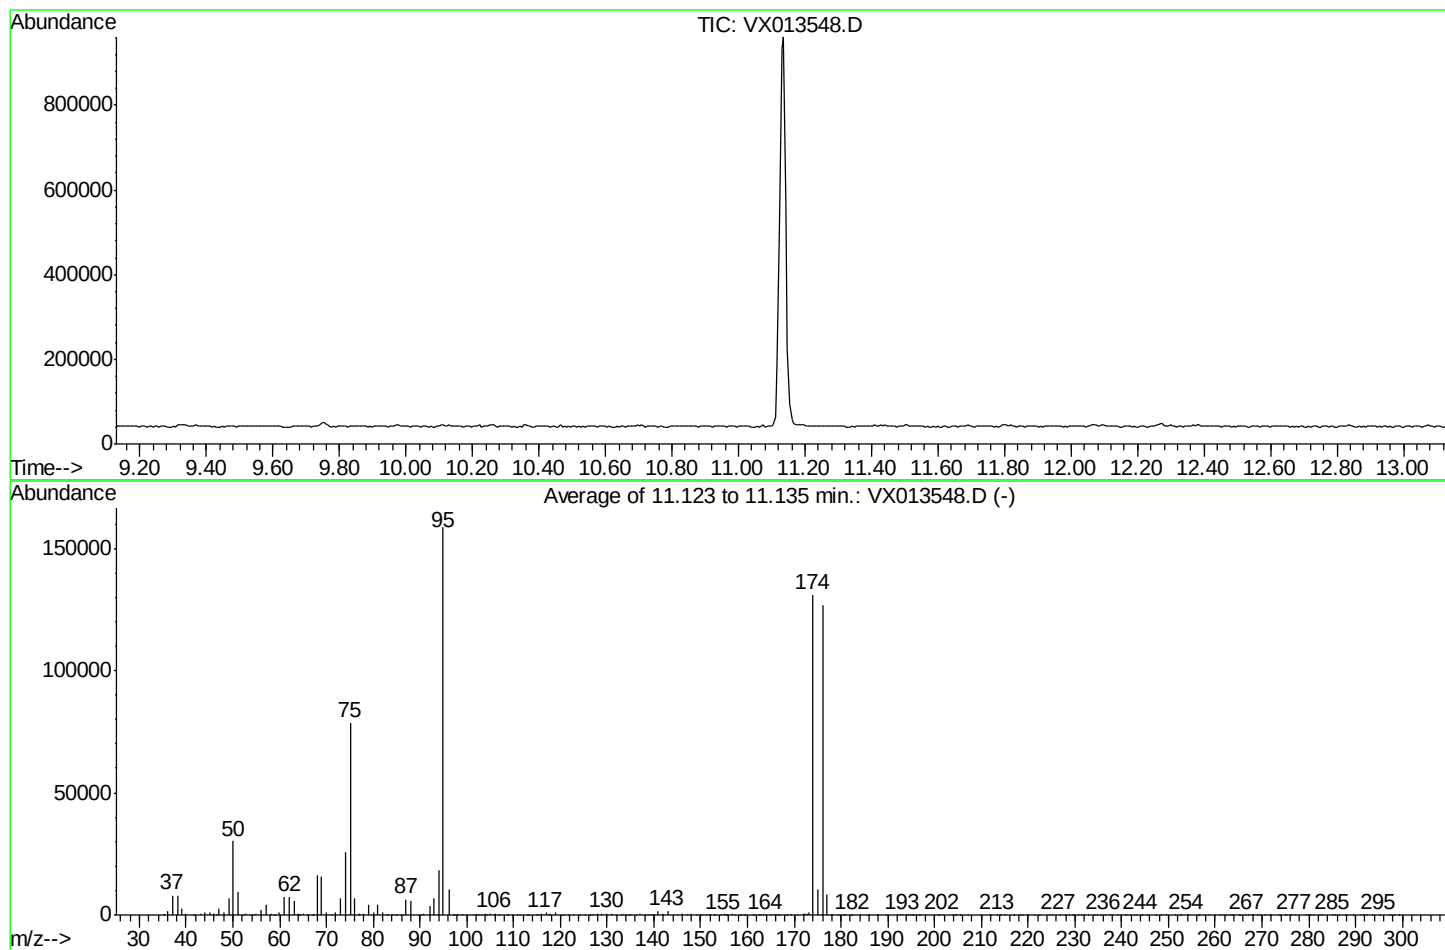

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	30176	PASS
75	95	30	60	49.6	78624	PASS
95	95	100	100	100.0	158643	PASS
96	95	5	9	6.8	10753	PASS
173	174	0.00	2	0.9	1149	PASS
174	95	50	100	82.7	131154	PASS
175	174	5	9	7.9	10377	PASS
176	174	95	101	96.8	127006	PASS
177	176	5	9	6.7	8453	PASS