

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025255.D
 Acq On : 22 Nov 2021 15:36
 Operator : JC/MD
 Sample : VX1122WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV2	3168	5363	0.92%	0.115%
2	1.368	42	46	53	rBV	91833	88423	15.22%	1.899%
3	1.666	90	95	104	rVB	65555	89622	15.43%	1.924%
4	2.306	194	200	211	rBV	123454	201384	34.67%	4.324%
5	2.434	219	221	222	rBV2	199	177	0.03%	0.004%
6	2.514	229	234	240	rBV	1536	2353	0.41%	0.051%
7	2.654	255	257	259	rBV	197	142	0.02%	0.003%
8	2.703	261	265	267	rBV2	232	245	0.04%	0.005%
9	2.788	275	279	284	rVB4	629	1306	0.22%	0.028%
10	2.947	299	305	306	rBV3	410	593	0.10%	0.013%
11	3.087	325	328	335	rVB4	610	1092	0.19%	0.023%
12	3.294	361	362	366	rBV2	159	184	0.03%	0.004%
13	3.532	398	401	403	rVB2	182	214	0.04%	0.005%
14	3.721	428	432	434	rBV	107	184	0.03%	0.004%
15	3.934	465	467	469	rBV2	126	139	0.02%	0.003%
16	4.013	478	480	482	rVB2	165	148	0.03%	0.003%
17	4.032	482	483	487	rBV2	149	163	0.03%	0.004%
18	4.123	496	498	500	rVB2	217	163	0.03%	0.004%
19	4.148	500	502	503	rBV2	159	129	0.02%	0.003%
20	4.458	542	553	574	rBV	51403	144303	24.84%	3.099%
21	4.635	580	582	584	rBV2	196	225	0.04%	0.005%
22	4.721	592	596	597	rBV2	188	233	0.04%	0.005%
23	5.062	639	652	667	rBV	73383	230908	39.75%	4.958%
24	5.452	714	716	718	rBV2	359	382	0.07%	0.008%
25	5.556	728	733	740	rBV2	526	984	0.17%	0.021%
26	5.672	751	752	757	rVB2	136	189	0.03%	0.004%
27	5.970	789	801	817	rBV2	197391	580840	100.00%	12.472%
28	6.245	844	846	849	rBV2	158	183	0.03%	0.004%
29	6.641	908	911	912	rVB2	148	130	0.02%	0.003%
30	6.763	921	931	943	rVV	160294	377093	64.92%	8.097%
31	6.873	947	949	950	rVV	212	149	0.03%	0.003%
32	7.110	982	988	995	rVV5	3433	7741	1.33%	0.166%
33	7.226	1006	1007	1010	rBV2	114	144	0.02%	0.003%
34	7.312	1013	1021	1032	rBV	123106	262749	45.24%	5.642%
35	7.476	1045	1048	1052	rVB3	308	471	0.08%	0.010%
36	7.775	1094	1097	1098	rBV2	130	131	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025255.D
 Acq On : 22 Nov 2021 15:36
 Operator : JC/MD
 Sample : VX1122WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.885	1110	1115	1116	rBV	127	150	0.03%	0.003%
38	7.927	1118	1122	1128	rVV2	934	1589	0.27%	0.034%
39	7.976	1128	1130	1134	rVB2	129	132	0.02%	0.003%
40	8.116	1148	1153	1156	rVB2	103	159	0.03%	0.003%
41	8.190	1162	1165	1167	rBV	157	145	0.02%	0.003%
42	8.220	1167	1170	1171	rBV2	119	152	0.03%	0.003%
43	8.324	1181	1187	1198	rVV	87461	145628	25.07%	3.127%
44	8.476	1207	1212	1218	rVB4	576	1118	0.19%	0.024%
45	8.653	1234	1241	1248	rBV	298747	482019	82.99%	10.350%
46	8.720	1249	1252	1261	rVB	4556	7286	1.25%	0.156%
47	8.952	1284	1290	1301	rBV	67137	95346	16.42%	2.047%
48	9.122	1316	1318	1320	rBV2	113	131	0.02%	0.003%
49	9.275	1339	1343	1346	rBV3	1392	1619	0.28%	0.035%
50	9.384	1355	1361	1375	rBV	228430	318971	54.92%	6.849%
51	9.610	1396	1398	1400	rBV	205	235	0.04%	0.005%
52	10.055	1465	1471	1486	rBV	331693	446661	76.90%	9.591%
53	10.195	1491	1494	1499	rVB2	709	1021	0.18%	0.022%
54	10.305	1508	1512	1516	rVB2	1567	1940	0.33%	0.042%
55	10.470	1536	1539	1541	rBV2	129	146	0.03%	0.003%
56	10.659	1564	1570	1574	rBV3	1183	1948	0.34%	0.042%
57	10.963	1617	1620	1624	rVV	699	857	0.15%	0.018%
58	11.031	1628	1631	1637	rVB2	144	213	0.04%	0.005%
59	11.122	1641	1646	1651	rVB4	1435	1858	0.32%	0.040%
60	11.195	1652	1658	1669	rVV	228220	291534	50.19%	6.260%
61	11.274	1669	1671	1675	rVV2	309	492	0.08%	0.011%
62	11.329	1678	1680	1683	rBV2	219	183	0.03%	0.004%
63	11.457	1697	1701	1704	rVV2	1200	1344	0.23%	0.029%
64	11.506	1707	1709	1711	rVB2	252	158	0.03%	0.003%
65	11.549	1711	1716	1718	rBV2	200	279	0.05%	0.006%
66	11.750	1744	1749	1756	rVB2	2511	3438	0.59%	0.074%
67	11.841	1760	1764	1768	rBV2	212	361	0.06%	0.008%
68	11.890	1770	1772	1775	rBV	161	144	0.02%	0.003%
69	11.939	1775	1780	1782	rBV3	660	875	0.15%	0.019%
70	11.969	1782	1785	1789	rBV	1472	1754	0.30%	0.038%
71	12.024	1789	1794	1807	rVB	332197	417717	71.92%	8.970%
72	12.128	1807	1811	1812	rBV2	554	719	0.12%	0.015%
73	12.152	1812	1815	1819	rVB2	1109	1285	0.22%	0.028%
74	12.213	1823	1825	1827	rBV	150	136	0.02%	0.003%
75	12.323	1837	1843	1850	rBV	323944	416737	71.75%	8.949%
76	12.420	1858	1859	1864	rVB3	393	444	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025255.D
 Acq On : 22 Nov 2021 15:36
 Operator : JC/MD
 Sample : VX1122WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.670	1897	1900	1908	rVV3	227	394	0.07%	0.008%
78	12.756	1912	1914	1919	rBV3	308	438	0.08%	0.009%
79	12.945	1943	1945	1948	rBV2	164	240	0.04%	0.005%
80	13.000	1953	1954	1959	rVV2	173	194	0.03%	0.004%
81	13.055	1961	1963	1966	rBV2	350	277	0.05%	0.006%
82	13.115	1969	1973	1979	rVB2	1659	1894	0.33%	0.041%
83	13.280	1997	2000	2001	rBV	166	137	0.02%	0.003%
84	13.378	2012	2016	2018	rBV	132	183	0.03%	0.004%
85	13.548	2042	2044	2048	rVV	110	131	0.02%	0.003%
86	13.591	2048	2051	2056	rVB	1594	1727	0.30%	0.037%
87	13.731	2072	2074	2078	rBV2	155	287	0.05%	0.006%
88	13.780	2079	2082	2087	rVB	1084	1437	0.25%	0.031%
89	13.908	2098	2103	2107	rBV2	125	221	0.04%	0.005%
90	13.963	2109	2112	2116	rBV3	1033	1273	0.22%	0.027%
91	14.085	2129	2132	2133	rBV2	206	171	0.03%	0.004%
92	14.134	2137	2140	2143	rVB3	522	652	0.11%	0.014%
93	14.268	2159	2162	2163	rBV	166	166	0.03%	0.004%
94	14.432	2185	2189	2191	rBV2	155	203	0.03%	0.004%
95	14.530	2202	2205	2206	rBV	316	231	0.04%	0.005%
96	14.573	2211	2212	2216	rVV	205	193	0.03%	0.004%
97	15.103	2298	2299	2301	rVV2	244	159	0.03%	0.003%
98	15.146	2304	2306	2309	rBV2	215	187	0.03%	0.004%
99	16.170	2470	2474	2475	rBV	253	211	0.04%	0.005%
100	16.298	2493	2495	2497	rVB2	303	240	0.04%	0.005%




Sum of corrected areas: 4657049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025255.D
Acq On : 22 Nov 2021 15:36
Operator : JC/MD
Sample : VX1122WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

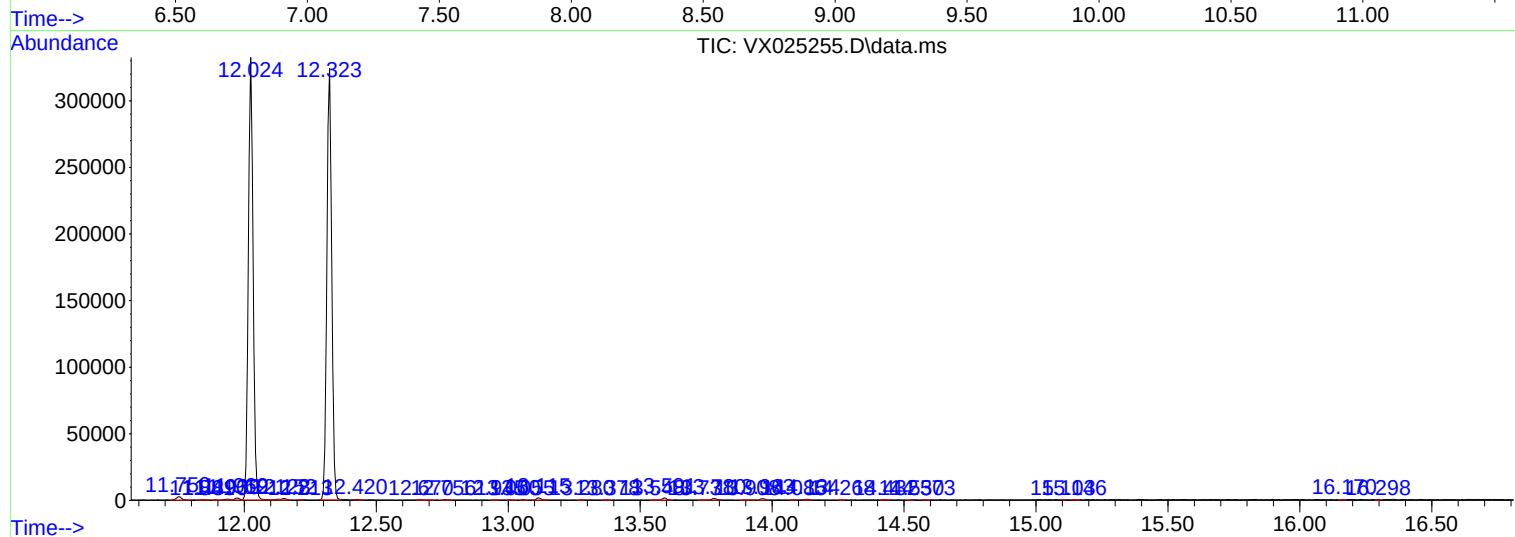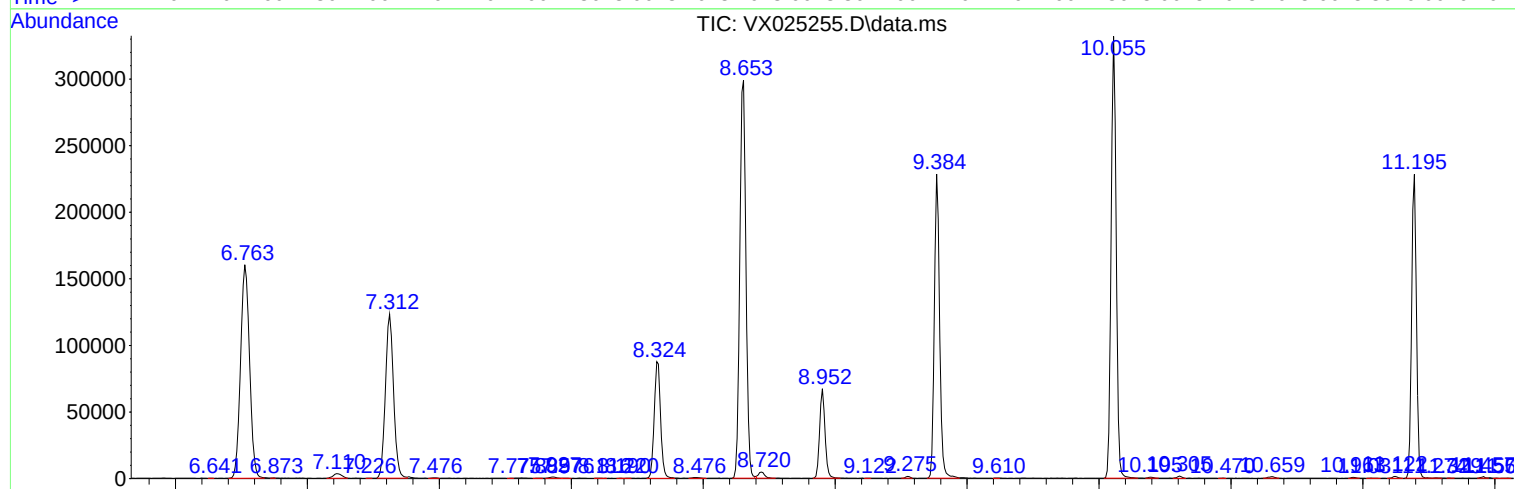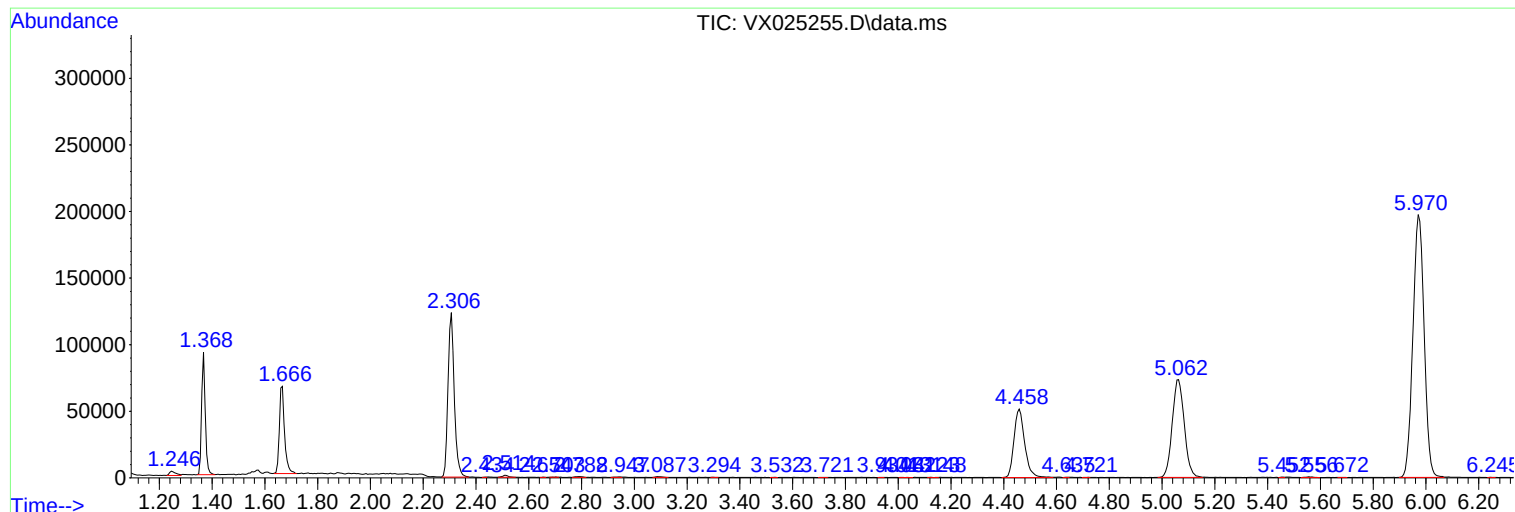

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025255.D
Acq On : 22 Nov 2021 15:36
Operator : JC/MD
Sample : VX1122WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025255.D
Acq On : 22 Nov 2021 15:36
Operator : JC/MD
Sample : VX1122WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc