

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025258.D
 Acq On : 22 Nov 2021 17:51
 Operator : JC/MD
 Sample : M4779-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	41	rBV	18554	36709	6.53%	0.795%
2	1.368	42	46	53	rVB	84144	81858	14.55%	1.774%
3	1.666	91	95	104	rVB	62850	84871	15.09%	1.839%
4	2.306	193	200	212	rBV	114182	187681	33.37%	4.067%
5	2.441	218	222	226	rBV3	242	353	0.06%	0.008%
6	2.508	229	233	237	rBV3	474	843	0.15%	0.018%
7	2.788	276	279	286	rVB4	612	980	0.17%	0.021%
8	2.947	302	305	310	rVV2	321	547	0.10%	0.012%
9	2.995	311	313	315	rVB	191	143	0.03%	0.003%
10	3.507	395	397	399	rVB2	203	145	0.03%	0.003%
11	4.459	543	553	571	rVV	50866	142802	25.39%	3.095%
12	4.654	584	585	587	rBV	283	186	0.03%	0.004%
13	4.708	593	594	598	rBV2	171	176	0.03%	0.004%
14	4.806	607	610	612	rBV	90	146	0.03%	0.003%
15	5.062	639	652	668	rBV	72036	225032	40.01%	4.876%
16	5.233	678	680	682	rVB2	277	185	0.03%	0.004%
17	5.562	728	734	735	rBV3	259	479	0.09%	0.010%
18	5.714	757	759	761	rBV2	155	159	0.03%	0.003%
19	5.775	768	769	772	rBV	188	141	0.03%	0.003%
20	5.861	781	783	786	rBV	149	141	0.03%	0.003%
21	5.970	789	801	820	rVV2	191558	562481	100.00%	12.189%
22	6.098	820	822	824	rBV	280	272	0.05%	0.006%
23	6.214	837	841	842	rBV	150	193	0.03%	0.004%
24	6.458	874	881	882	rBV	222	220	0.04%	0.005%
25	6.550	894	896	898	rBV2	191	177	0.03%	0.004%
26	6.763	921	931	943	rBV	156236	370257	65.83%	8.024%
27	7.056	975	979	982	rVV2	140	230	0.04%	0.005%
28	7.110	982	988	995	rVB3	2309	5087	0.90%	0.110%
29	7.312	1012	1021	1032	rBV	117076	255089	45.35%	5.528%
30	7.482	1044	1049	1053	rBV4	266	542	0.10%	0.012%
31	7.799	1098	1101	1105	rBV3	303	484	0.09%	0.010%
32	7.897	1113	1117	1118	rBV	124	140	0.02%	0.003%
33	7.927	1118	1122	1127	rVV2	1004	1589	0.28%	0.034%
34	8.043	1137	1141	1145	rBV2	109	161	0.03%	0.003%
35	8.086	1147	1148	1152	rBV2	112	144	0.03%	0.003%
36	8.123	1152	1154	1158	rVB	214	198	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025258.D
 Acq On : 22 Nov 2021 17:51
 Operator : JC/MD
 Sample : M4779-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.324	1180	1187	1197	rBV	83064	138462	24.62%	3.000%
38	8.470	1206	1211	1215	rBV3	627	1084	0.19%	0.023%
39	8.653	1234	1241	1249	rBV	287026	460657	81.90%	9.983%
40	8.720	1249	1252	1262	rVB2	4793	7326	1.30%	0.159%
41	8.952	1284	1290	1299	rBV	63360	89725	15.95%	1.944%
42	9.195	1328	1330	1333	rBV2	124	200	0.04%	0.004%
43	9.275	1340	1343	1345	rBV	437	328	0.06%	0.007%
44	9.384	1356	1361	1379	rVV	230459	312896	55.63%	6.781%
45	9.549	1386	1388	1390	rBV	148	142	0.03%	0.003%
46	9.634	1400	1402	1406	rBV2	110	157	0.03%	0.003%
47	9.708	1413	1414	1419	rBV2	94	164	0.03%	0.004%
48	9.799	1426	1429	1431	rBV2	126	153	0.03%	0.003%
49	10.055	1465	1471	1489	rVB	324474	438698	77.99%	9.507%
50	10.195	1491	1494	1498	rVV	743	873	0.16%	0.019%
51	10.305	1508	1512	1516	rVB	1186	1632	0.29%	0.035%
52	10.518	1545	1547	1550	rVB	155	150	0.03%	0.003%
53	10.653	1563	1569	1573	rVV2	814	1273	0.23%	0.028%
54	10.957	1617	1619	1620	rBV2	183	142	0.03%	0.003%
55	11.122	1641	1646	1650	rBV2	1440	1700	0.30%	0.037%
56	11.195	1652	1658	1665	rVV	229498	293100	52.11%	6.352%
57	11.274	1668	1671	1673	rBV	441	404	0.07%	0.009%
58	11.360	1682	1685	1687	rBV2	143	161	0.03%	0.003%
59	11.384	1687	1689	1692	rBV2	189	292	0.05%	0.006%
60	11.451	1698	1700	1703	rVB2	494	402	0.07%	0.009%
61	11.482	1703	1705	1708	rVB3	206	264	0.05%	0.006%
62	11.604	1722	1725	1730	rBV2	159	231	0.04%	0.005%
63	11.750	1745	1749	1754	rVB5	1684	2221	0.39%	0.048%
64	11.841	1762	1764	1769	rVB3	293	313	0.06%	0.007%
65	11.939	1775	1780	1783	rBV4	587	799	0.14%	0.017%
66	11.969	1783	1785	1789	rBV2	335	322	0.06%	0.007%
67	12.024	1789	1794	1801	rBV	330583	419158	74.52%	9.083%
68	12.128	1808	1811	1813	rBV3	405	598	0.11%	0.013%
69	12.250	1827	1831	1833	rVB3	642	875	0.16%	0.019%
70	12.323	1837	1843	1849	rBV	331434	411348	73.13%	8.914%
71	12.414	1855	1858	1865	rVB2	1235	1924	0.34%	0.042%
72	12.475	1865	1868	1871	rVB3	272	261	0.05%	0.006%
73	12.664	1896	1899	1902	rBV3	264	281	0.05%	0.006%
74	12.768	1913	1916	1919	rBV2	404	324	0.06%	0.007%
75	12.823	1922	1925	1926	rBV2	242	269	0.05%	0.006%
76	13.055	1961	1963	1967	rVB2	401	371	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025258.D
 Acq On : 22 Nov 2021 17:51
 Operator : JC/MD
 Sample : M4779-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	13.097	1967	1970	1971	rBV2	123	169	0.03%	0.004%
78	13.116	1971	1973	1977	rVB2	319	374	0.07%	0.008%
79	13.280	1996	2000	2003	rVV2	129	218	0.04%	0.005%
80	13.311	2003	2005	2008	rVV2	224	198	0.04%	0.004%
81	13.481	2031	2033	2036	rVB	176	141	0.03%	0.003%
82	13.548	2041	2044	2046	rBV2	127	176	0.03%	0.004%
83	13.622	2055	2056	2059	rBV2	205	229	0.04%	0.005%
84	13.652	2059	2061	2065	rVB3	131	167	0.03%	0.004%
85	13.780	2075	2082	2092	rVB	38202	53935	9.59%	1.169%
86	13.871	2094	2097	2103	rVB	1122	1451	0.26%	0.031%
87	14.134	2137	2140	2143	rVV2	424	552	0.10%	0.012%
88	14.463	2190	2194	2195	rBV3	209	265	0.05%	0.006%
89	14.548	2206	2208	2211	rVB2	237	250	0.04%	0.005%
90	14.573	2211	2212	2215	rVB2	207	197	0.04%	0.004%
91	14.597	2215	2216	2218	rBV2	217	199	0.04%	0.004%
92	14.640	2219	2223	2229	rVB2	1463	2149	0.38%	0.047%
93	14.786	2241	2247	2251	rBV3	1164	1759	0.31%	0.038%
94	14.859	2257	2259	2261	rBV2	173	193	0.03%	0.004%
95	14.975	2276	2278	2280	rBV2	243	237	0.04%	0.005%
96	15.127	2302	2303	2309	rBB2	179	219	0.04%	0.005%
97	15.207	2314	2316	2321	rVB3	362	551	0.10%	0.012%
98	15.548	2369	2372	2373	rBV	175	180	0.03%	0.004%
99	16.145	2468	2470	2472	rBV2	166	155	0.03%	0.003%
100	16.237	2484	2485	2488	rVB	218	156	0.03%	0.003%

Sum of corrected areas: 4614641




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025258.D
Acq On : 22 Nov 2021 17:51
Operator : JC/MD
Sample : M4779-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

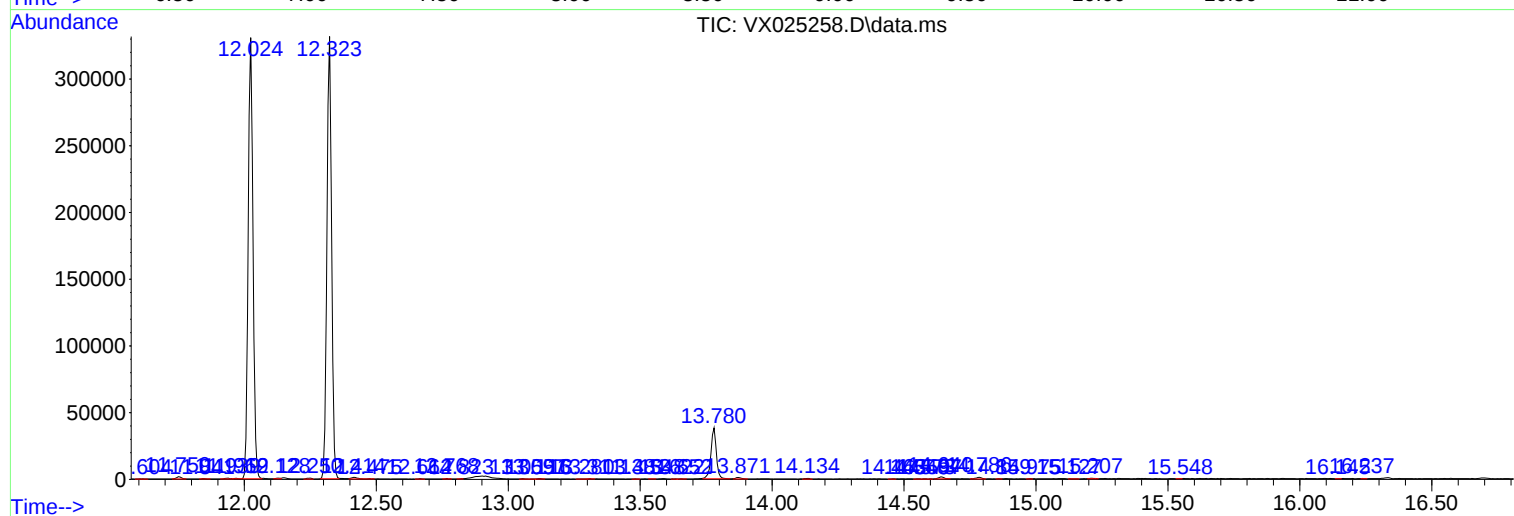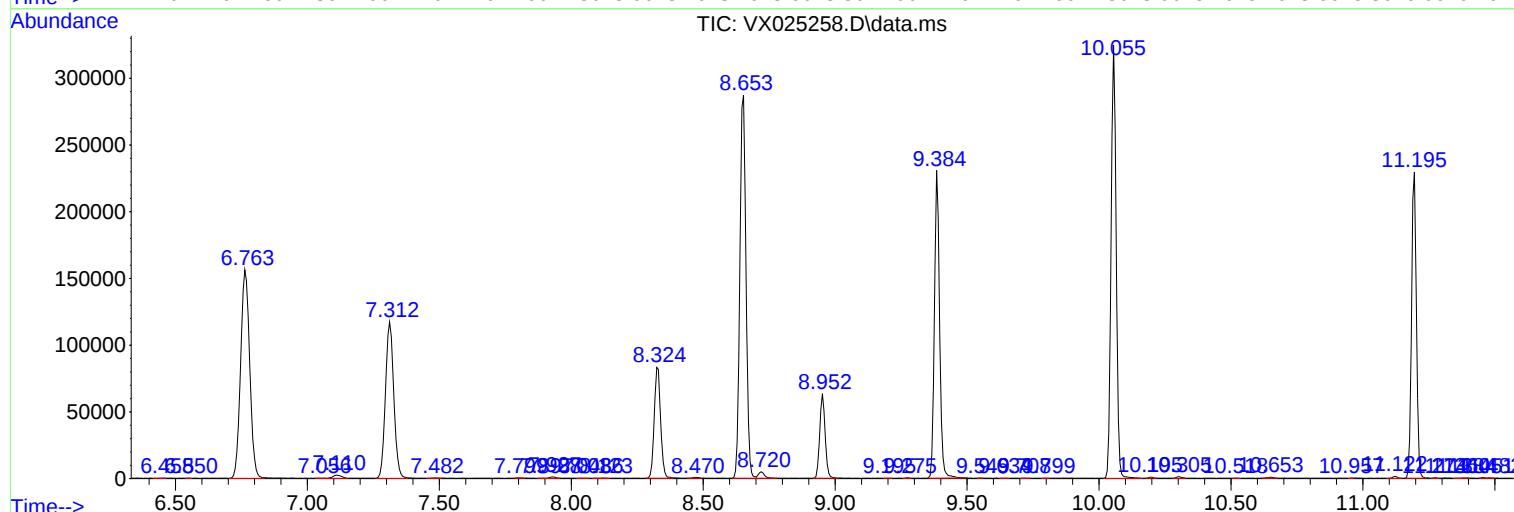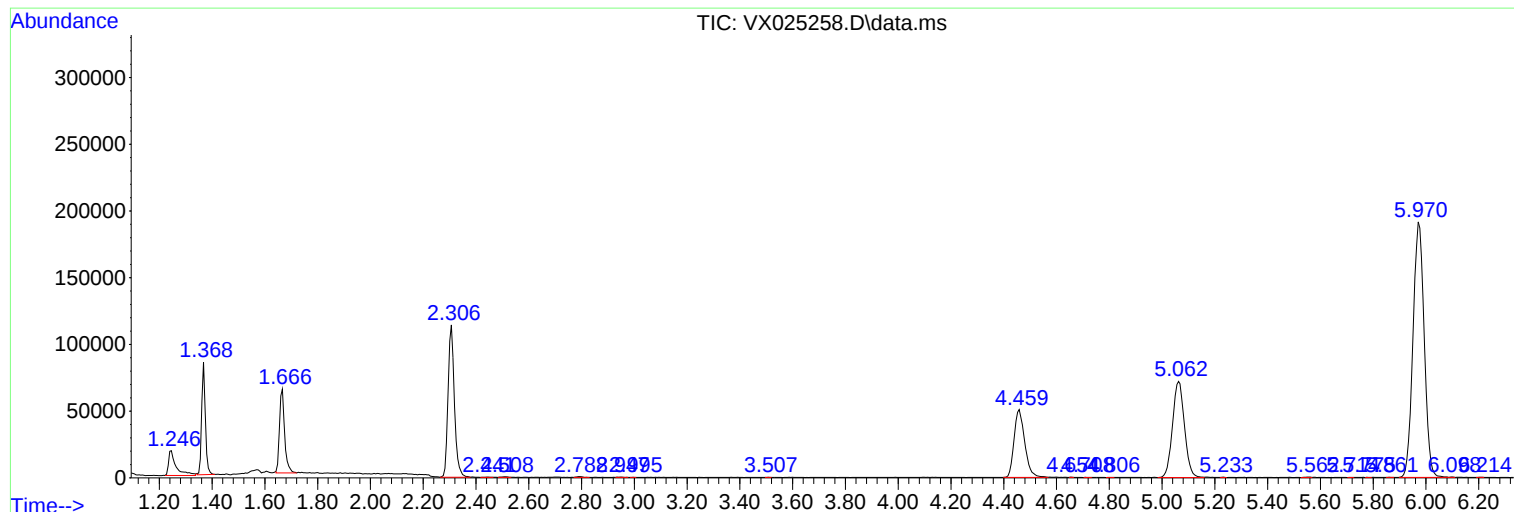

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025258.D
Acq On : 22 Nov 2021 17:51
Operator : JC/MD
Sample : M4779-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025258.D
Acq On : 22 Nov 2021 17:51
Operator : JC/MD
Sample : M4779-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc