

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025259.D
 Acq On : 22 Nov 2021 18:15
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	13350	22347	3.98%	0.497%
2	1.368	42	46	55	rVB	87108	83688	14.92%	1.861%
3	1.660	90	94	104	rVB	58979	82553	14.72%	1.836%
4	2.307	193	200	210	rBV	117146	192931	34.40%	4.291%
5	2.489	227	230	231	rBV2	181	185	0.03%	0.004%
6	2.788	277	279	284	rVB3	696	867	0.15%	0.019%
7	3.136	334	336	338	rBV	153	133	0.02%	0.003%
8	3.367	372	374	377	rBV	120	116	0.02%	0.003%
9	3.422	381	383	385	rBV	121	124	0.02%	0.003%
10	3.514	396	398	399	rBV	170	113	0.02%	0.003%
11	3.593	410	411	415	rBV2	92	114	0.02%	0.003%
12	3.684	422	426	428	rBV2	94	142	0.03%	0.003%
13	4.007	478	479	482	rVV	139	142	0.03%	0.003%
14	4.459	544	553	568	rBV	49087	138291	24.66%	3.076%
15	4.910	626	627	629	rVB	163	117	0.02%	0.003%
16	4.965	635	636	640	rVB	163	125	0.02%	0.003%
17	5.068	640	653	668	rBV	72581	225666	40.23%	5.020%
18	5.306	686	692	693	rBV2	150	217	0.04%	0.005%
19	5.550	728	732	734	rBV2	209	257	0.05%	0.006%
20	5.970	789	801	817	rBV2	190322	560900	100.00%	12.476%
21	6.531	889	893	895	rBV2	157	219	0.04%	0.005%
22	6.763	921	931	946	rBV	149816	356173	63.50%	7.922%
23	7.111	982	988	995	rVB2	2800	6028	1.07%	0.134%
24	7.312	1012	1021	1035	rVB	116967	254927	45.45%	5.670%
25	7.476	1045	1048	1053	rVV3	339	626	0.11%	0.014%
26	7.531	1055	1057	1060	rVV2	116	124	0.02%	0.003%
27	7.574	1062	1064	1066	rVB2	130	122	0.02%	0.003%
28	7.635	1072	1074	1077	rBV	154	153	0.03%	0.003%
29	7.671	1077	1080	1082	rVV2	138	160	0.03%	0.004%
30	7.799	1096	1101	1102	rBV2	246	341	0.06%	0.008%
31	7.927	1118	1122	1128	rVB3	876	1564	0.28%	0.035%
32	8.324	1181	1187	1198	rVV	83453	138822	24.75%	3.088%
33	8.421	1202	1203	1205	rBV2	223	176	0.03%	0.004%
34	8.470	1208	1211	1216	rVB2	665	969	0.17%	0.022%
35	8.653	1234	1241	1248	rBV	300489	464746	82.86%	10.337%
36	8.720	1249	1252	1260	rVB2	4118	6764	1.21%	0.150%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025259.D
 Acq On : 22 Nov 2021 18:15
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.909	1281	1283	1284	rBV	165	114	0.02%	0.003%
38	8.952	1284	1290	1300	rVV	64268	89615	15.98%	1.993%
39	9.074	1309	1310	1312	rBV2	173	126	0.02%	0.003%
40	9.385	1355	1361	1375	rBV	216142	306575	54.66%	6.819%
41	9.519	1381	1383	1387	rVB	179	163	0.03%	0.004%
42	9.567	1387	1391	1392	rBV2	129	133	0.02%	0.003%
43	9.677	1408	1409	1413	rBV2	121	113	0.02%	0.003%
44	10.055	1465	1471	1484	rBV	318474	424022	75.60%	9.432%
45	10.189	1491	1493	1498	rVB	373	511	0.09%	0.011%
46	10.305	1508	1512	1516	rVB2	843	1150	0.21%	0.026%
47	10.342	1516	1518	1521	rBV2	97	114	0.02%	0.003%
48	10.616	1562	1563	1566	rBV	127	118	0.02%	0.003%
49	10.653	1566	1569	1572	rVV2	429	641	0.11%	0.014%
50	10.744	1581	1584	1588	rBV2	128	153	0.03%	0.003%
51	10.781	1588	1590	1591	rBV2	154	135	0.02%	0.003%
52	10.963	1617	1620	1621	rBV	133	114	0.02%	0.003%
53	11.043	1629	1633	1636	rVB	131	162	0.03%	0.004%
54	11.122	1642	1646	1651	rVB	1491	1820	0.32%	0.040%
55	11.195	1652	1658	1667	rVV	228581	290777	51.84%	6.468%
56	11.268	1669	1670	1672	rVV2	409	284	0.05%	0.006%
57	11.323	1676	1679	1681	rBV2	166	174	0.03%	0.004%
58	11.457	1698	1701	1702	rBV2	293	299	0.05%	0.007%
59	11.482	1702	1705	1707	rVV	305	445	0.08%	0.010%
60	11.543	1713	1715	1717	rVV	244	185	0.03%	0.004%
61	11.622	1724	1728	1729	rBV2	207	195	0.03%	0.004%
62	11.750	1743	1749	1753	rBV4	1524	2035	0.36%	0.045%
63	11.854	1764	1766	1767	rBV	215	138	0.02%	0.003%
64	11.939	1777	1780	1782	rVV2	584	644	0.11%	0.014%
65	11.969	1784	1785	1789	rBV2	246	164	0.03%	0.004%
66	12.024	1789	1794	1803	rVV	324539	402470	71.75%	8.952%
67	12.122	1808	1810	1813	rBV2	513	588	0.10%	0.013%
68	12.323	1837	1843	1855	rVV	326090	413239	73.67%	9.192%
69	12.421	1855	1859	1863	rVB4	601	951	0.17%	0.021%
70	12.488	1868	1870	1872	rVB	222	142	0.03%	0.003%
71	12.658	1896	1898	1902	rVB2	227	243	0.04%	0.005%
72	12.768	1910	1916	1920	rVB4	272	462	0.08%	0.010%
73	13.116	1970	1973	1978	rBV3	260	398	0.07%	0.009%
74	13.225	1987	1991	1993	rBV2	164	156	0.03%	0.003%
75	13.317	2003	2006	2010	rBV	145	267	0.05%	0.006%
76	13.658	2059	2062	2063	rBV2	107	116	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025259.D
 Acq On : 22 Nov 2021 18:15
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	13.780	2077	2082	2091	rVB	7187	9738	1.74%	0.217%
78	13.963	2111	2112	2115	rVB	203	177	0.03%	0.004%
79	13.993	2115	2117	2118	rBV	176	123	0.02%	0.003%
80	14.012	2118	2120	2122	rBV	110	113	0.02%	0.003%
81	14.067	2126	2129	2130	rVB2	157	123	0.02%	0.003%
82	14.085	2130	2132	2133	rBV	143	122	0.02%	0.003%
83	14.140	2137	2141	2145	rVB2	619	812	0.14%	0.018%
84	14.378	2177	2180	2183	rVV2	158	225	0.04%	0.005%
85	14.426	2186	2188	2192	rVB2	99	127	0.02%	0.003%
86	14.493	2197	2199	2201	rBV3	103	129	0.02%	0.003%
87	14.640	2221	2223	2226	rVB2	530	498	0.09%	0.011%
88	14.695	2231	2232	2234	rBV2	233	174	0.03%	0.004%
89	14.719	2234	2236	2239	rBV3	127	153	0.03%	0.003%
90	14.786	2245	2247	2251	rVB2	403	415	0.07%	0.009%
91	14.884	2262	2263	2265	rBV2	163	130	0.02%	0.003%
92	15.024	2284	2286	2289	rVB2	265	191	0.03%	0.004%
93	15.207	2313	2316	2319	rBV3	212	264	0.05%	0.006%
94	15.237	2319	2321	2322	rBV	172	149	0.03%	0.003%
95	15.371	2341	2343	2344	rBV	210	140	0.02%	0.003%
96	15.774	2407	2409	2410	rBV	248	178	0.03%	0.004%
97	15.865	2422	2424	2426	rBV2	223	163	0.03%	0.004%
98	15.981	2441	2443	2444	rBV	253	183	0.03%	0.004%
99	16.341	2500	2502	2505	rVB4	262	198	0.04%	0.004%
100	16.682	2557	2558	2559	rBV4	244	166	0.03%	0.004%


Sum of corrected areas: 4495784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025259.D
Acq On : 22 Nov 2021 18:15
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

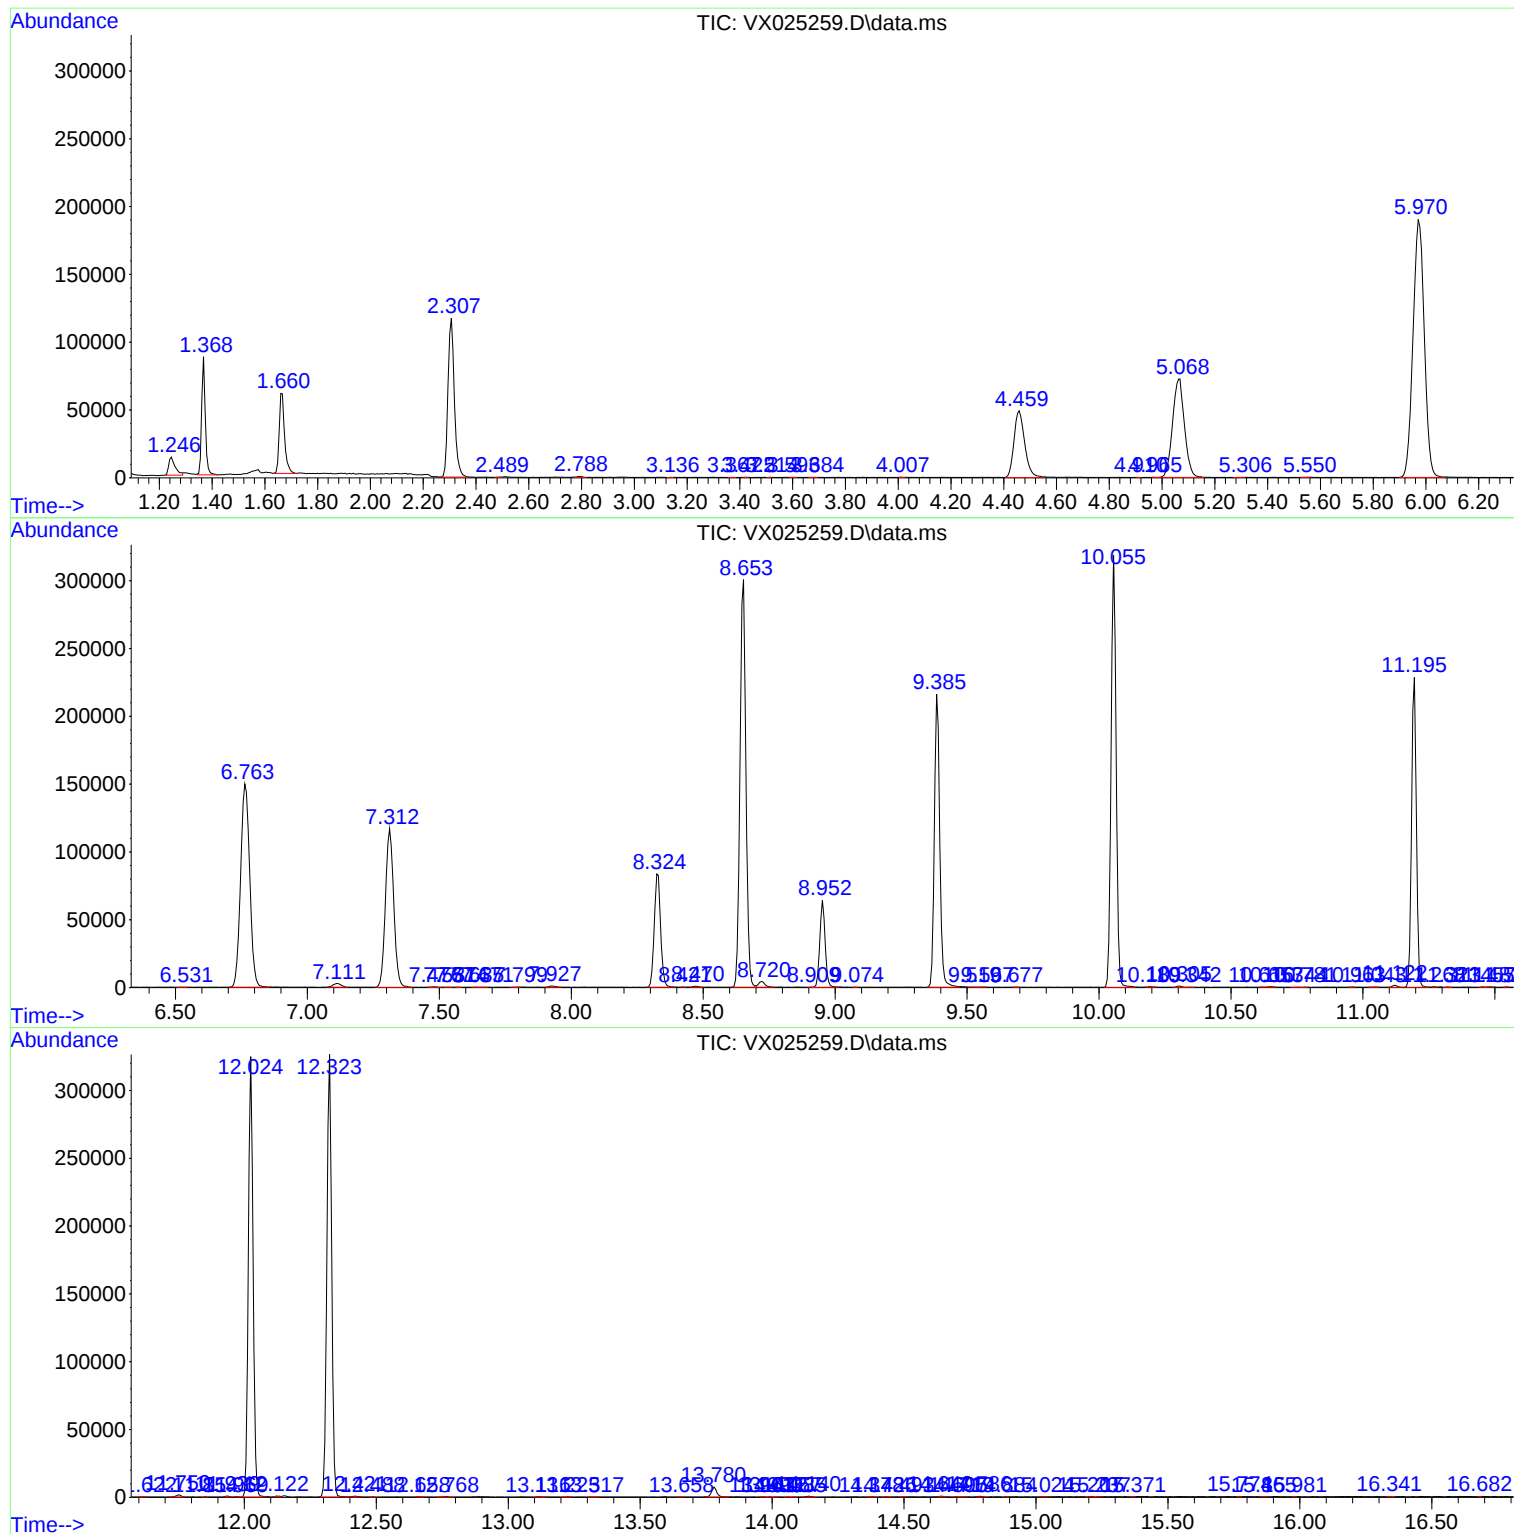

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025259.D
Acq On : 22 Nov 2021 18:15
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
Data File : VX025259.D
Acq On : 22 Nov 2021 18:15
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc