


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112221\
 Data File : VX025246.D
 Acq On : 22 Nov 2021 09:32
 Operator : JC/MD
 Sample : BFB617
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB617

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 26 23:56:11 2021

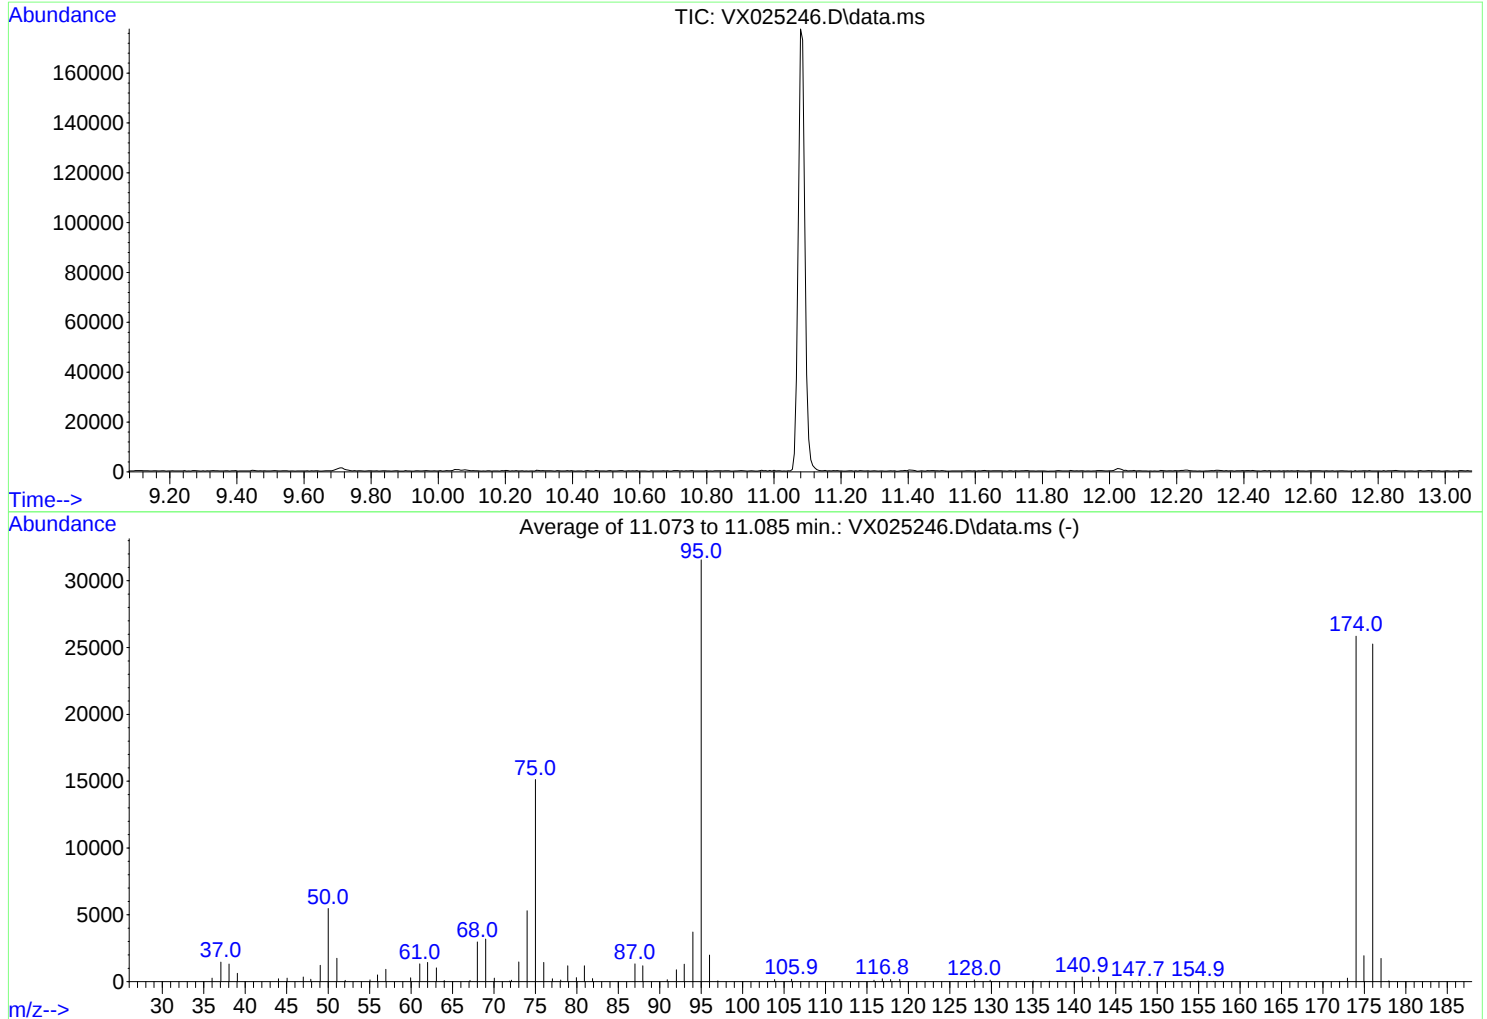

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5474	PASS
75	95	30	80	47.9	15118	PASS
95	95	100	100	100.0	31565	PASS
96	95	5	9	6.3	1983	PASS
173	174	0.00	2	1.0	269	PASS
174	95	50	120	81.9	25856	PASS
175	174	5	9	7.5	1936	PASS
176	174	95	101	97.7	25260	PASS
177	176	5	9	6.9	1739	PASS

m/z	Abundance
36.00	292.0
37.00	1446.0
38.00	1176.0
39.00	647.0
39.90	242.0
44.00	304.0
45.00	269.0
47.00	328.0
47.90	136.0
49.00	1242.0
50.00	5512.0
51.00	1760.0
52.00	98.0
55.10	162.0
55.90	493.0
56.90	917.0
59.90	279.0
61.10	1376.0
62.00	1513.0
63.10	1059.0
64.00	113.0
67.10	108.0
68.00	3076.0
69.00	3246.0
70.00	247.0
72.10	173.0
73.00	1563.0
74.00	5437.0
75.00	15842.0
76.00	1491.0
77.10	214.0
78.10	124.0
78.90	1269.0
80.00	262.0
80.90	1258.0
81.80	238.0
87.00	1377.0
88.00	1315.0
90.90	170.0
92.10	856.0
93.00	1496.0
94.00	4211.0
95.00	35472.0
96.00	1993.0
97.00	81.0
103.90	154.0
105.90	198.0
115.80	107.0
116.80	219.0
117.90	205.0
118.90	157.0
128.00	188.0
129.80	109.0
135.10	81.0
141.00	421.0
143.00	449.0
147.70	87.0
154.90	77.0
156.80	79.0
161.00	51.0
172.00	72.0
172.90	278.0
174.00	32808.0
175.00	2430.0
176.00	31968.0
177.00	2150.0
177.90	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB617

m/z	Abundance
40.00	255.0
43.20	52.0
44.00	144.0

Instrument :
MSVOA_X
ClientSampleId :
BFB617

m/z	Abundance
36.00	222.0
37.00	1218.0
38.10	1141.0
39.10	522.0
40.00	176.0
44.00	336.0
45.10	216.0
47.00	310.0
47.90	162.0
49.00	912.0
50.00	4427.0
51.00	1263.0
52.10	72.0
55.10	108.0
56.00	367.0
57.00	735.0
60.00	241.0
61.00	1049.0
62.00	979.0
63.00	719.0
63.90	104.0
67.10	84.0
68.00	2268.0
69.00	2427.0
70.10	210.0
71.90	137.0
73.00	1059.0
74.00	4264.0
75.00	11471.0
76.00	1097.0
77.00	214.0
78.00	107.0
78.90	915.0
79.90	230.0
80.90	915.0
82.00	175.0
87.00	1098.0
88.00	892.0
90.90	122.0
92.00	690.0
92.90	855.0
94.00	2696.0
95.00	21960.0
96.00	1642.0
103.80	99.0
105.90	153.0
115.90	61.0
116.90	165.0
117.80	87.0
118.90	125.0
127.90	65.0
129.90	89.0
137.00	64.0
140.90	274.0
142.90	247.0
172.90	218.0
174.00	15791.0
174.90	1158.0
176.00	14708.0
177.00	1094.0

Instrument :
MSVOA_X
ClientSampleId :
BFB617

m/z	Abundance
36.00	272.0
37.10	1734.0
38.10	1643.0
39.10	707.0
40.00	282.0
44.00	429.0
45.10	319.0
47.00	387.0
47.90	242.0
49.10	1521.0
50.00	6483.0
51.10	2216.0
52.10	110.0
54.90	67.0
55.20	69.0
56.00	658.0
57.00	1117.0
59.90	332.0
61.00	1565.0
62.00	1812.0
63.00	1299.0
64.10	125.0
67.10	99.0
68.00	3549.0
69.00	3869.0
70.10	344.0
72.10	154.0
73.00	1783.0
74.00	6215.0
75.00	18040.0
76.00	1742.0
77.00	203.0
78.00	144.0
78.90	1355.0
79.90	399.0
80.90	1374.0
81.90	257.0
87.00	1506.0
87.90	1348.0
90.90	139.0
91.90	1124.0
93.00	1583.0
94.00	4241.0
95.00	37264.0
96.00	2314.0
97.00	103.0
103.90	211.0
105.90	189.0
115.90	176.0
116.90	261.0
117.80	166.0
119.00	217.0
128.00	159.0
129.90	139.0
135.00	82.0
137.10	52.0
140.90	363.0
143.00	352.0
147.70	58.0
155.00	72.0
173.00	311.0
174.00	28968.0
175.00	2220.0
176.00	29104.0
177.00	1974.0
178.00	82.0

Instrument :
MSVOA_X
ClientSampleId :
BFB617