

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
 Data File : VX032998.D
 Acq On : 22 Nov 2022 22:59
 Operator : JC/MD
 Sample : N5730-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT158S1-20221118

Quant Time: Nov 23 05:51:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 22 13:58:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	119587	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	192335	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	168737	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	76777	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	56101	47.876	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.760%
35) Dibromofluoromethane	5.385	113	46609	42.985	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	85.960%
50) Toluene-d8	8.647	98	140446	42.735	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	85.480%#
62) 4-Bromofluorobenzene	11.079	95	63692	44.716	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.440%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032998.D
Acq On : 22 Nov 2022 22:59
Operator : JC/MD
Sample : N5730-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT158S1-20221118

Quant Time: Nov 23 05:51:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration




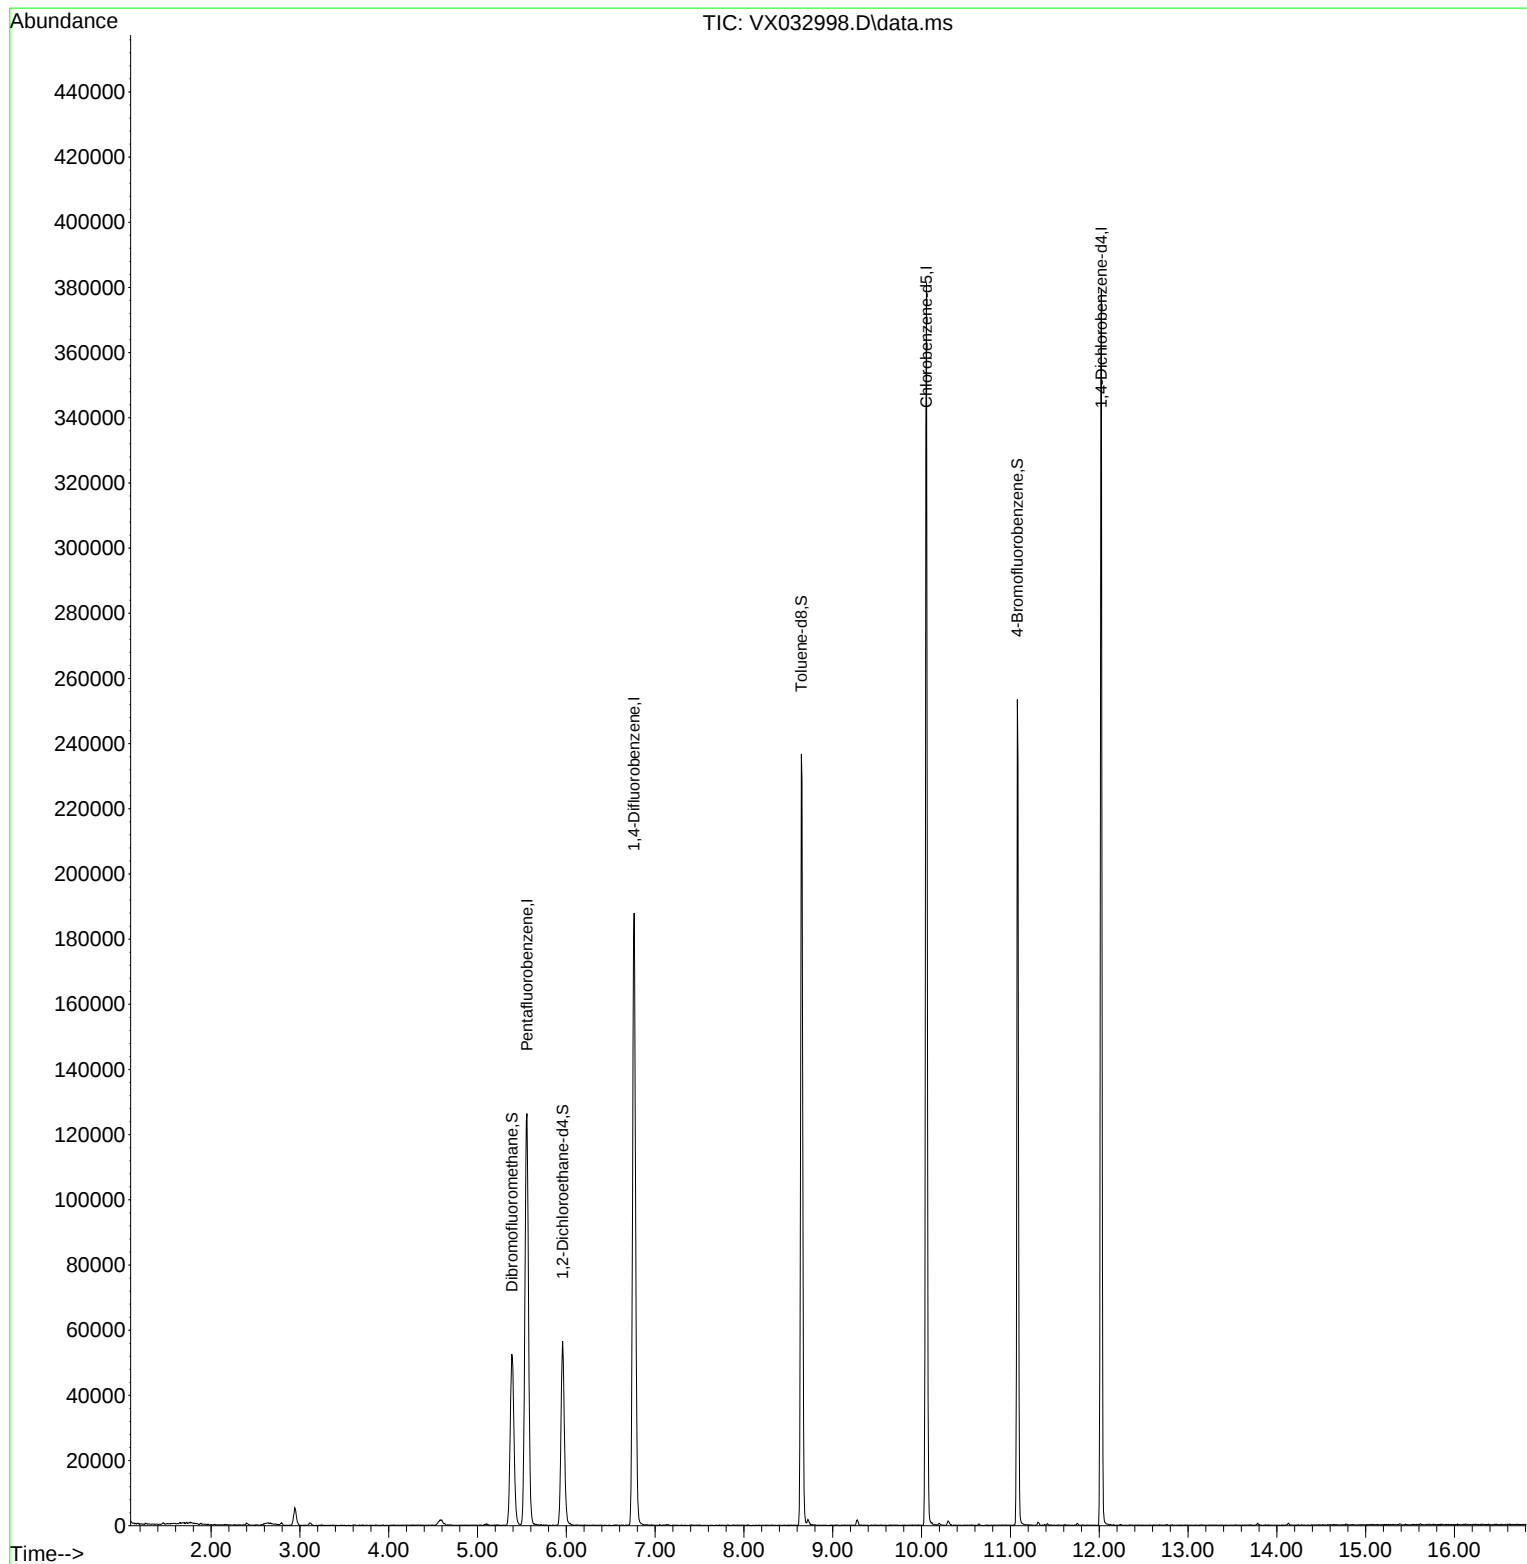




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59




Instrument :
MSVOA_X
ClientSampleId :
TT158S1-20221118

Tgt Ion:168 Resp: 119587
Ion Ratio Lower Upper
168 100
99 61.1 46.1 69.1

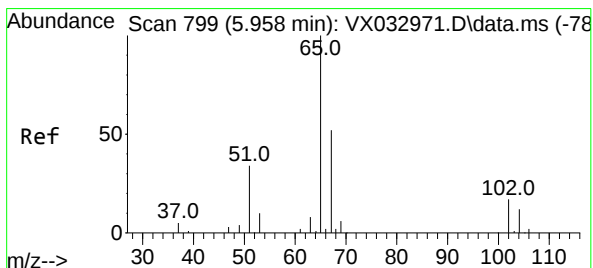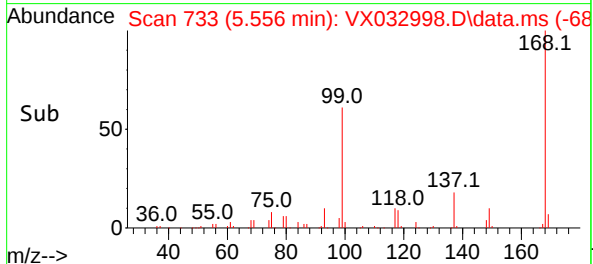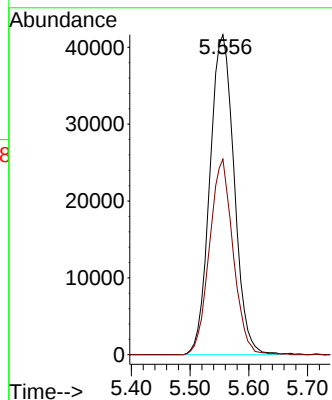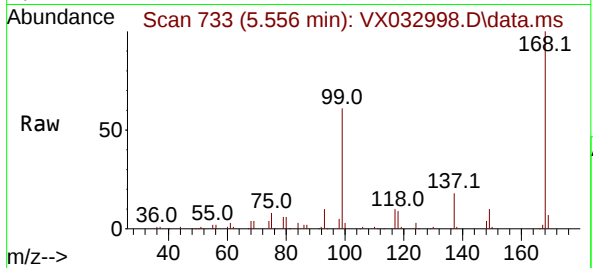

#33
1,2-Dichloroethane-d4
Concen: 47.876 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59

Tgt Ion: 65 Resp: 56101
Ion Ratio Lower Upper
65 100
67 51.7 0.0 101.8

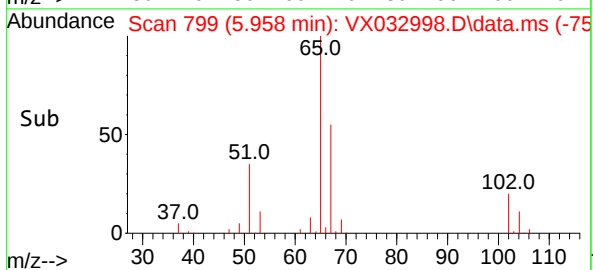
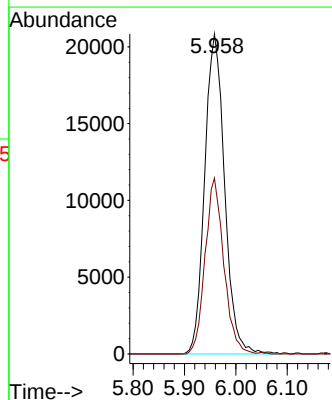
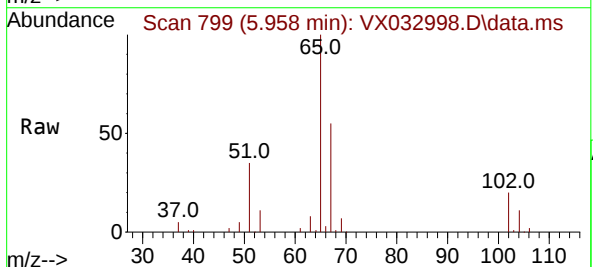




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59




Instrument :
MSVOA_X
ClientSampleId :
TT158S1-20221118


Tgt Ion:114 Resp: 192335
Ion Ratio Lower Upper
114 100
63 19.7 0.0 41.6
88 16.4 0.0 33.4

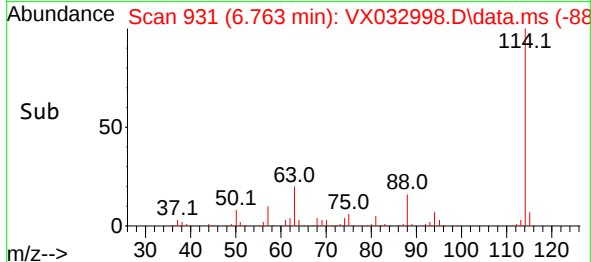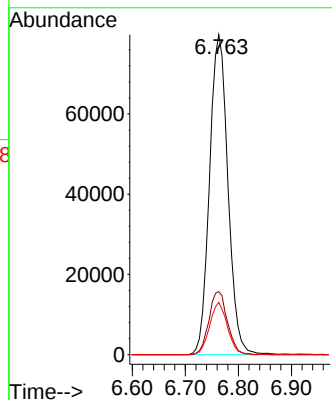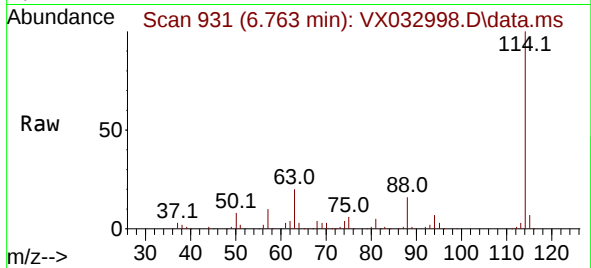

#35
Dibromofluoromethane
Concen: 42.985 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59

Tgt Ion:113 Resp: 46609
Ion Ratio Lower Upper
113 100
111 100.5 82.4 123.6
192 19.2 15.4 23.2


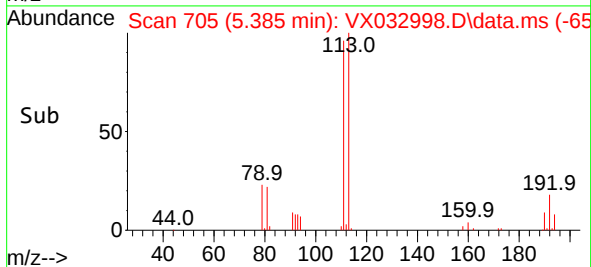
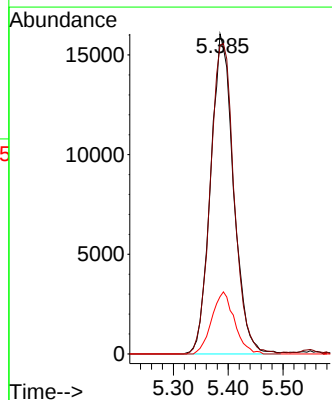
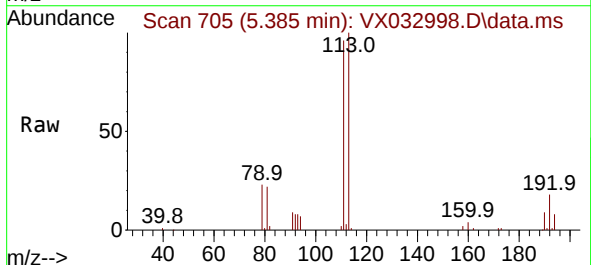


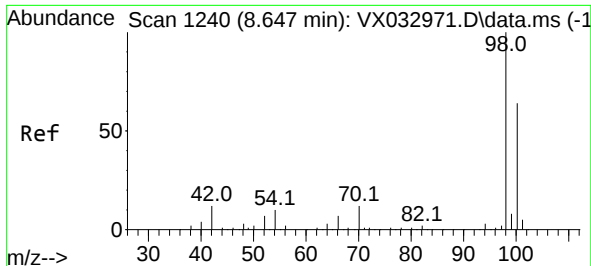

#50
Toluene-d8
Concen: 42.735 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59




Instrument :
MSVOA_X
ClientSampleId :
TT158S1-20221118


Tgt Ion: 98 Resp: 140446
Ion Ratio Lower Upper
98 100
100 65.7 50.9 76.3

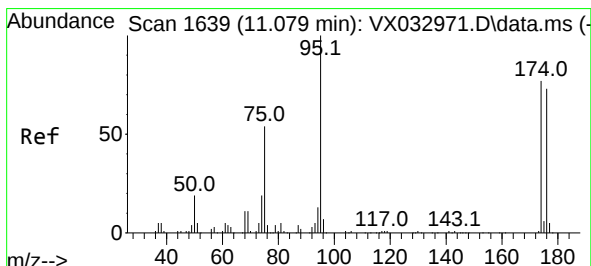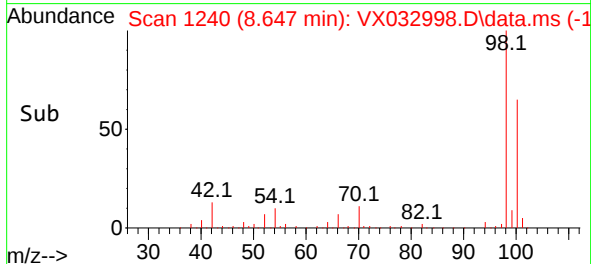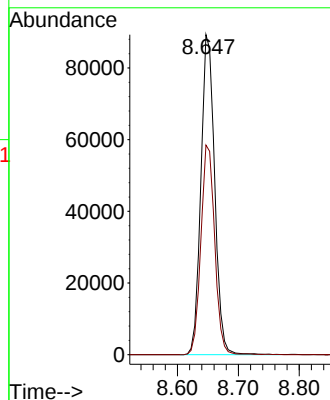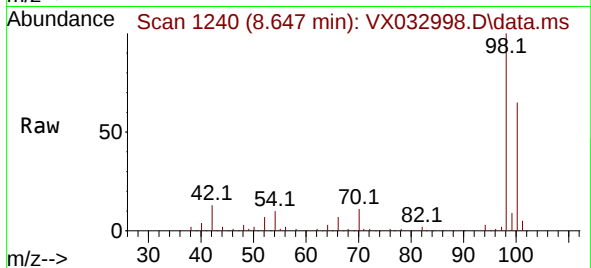

#62
4-Bromofluorobenzene
Concen: 44.716 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59

Tgt Ion: 95 Resp: 63692
Ion Ratio Lower Upper
95 100
174 81.8 0.0 164.0
176 78.8 0.0 154.4


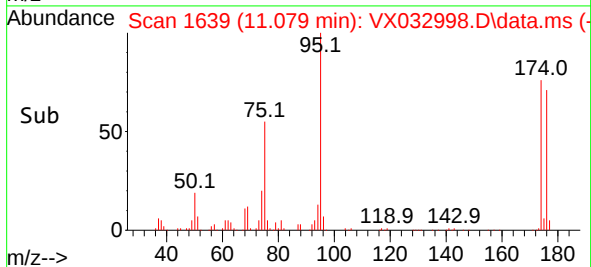
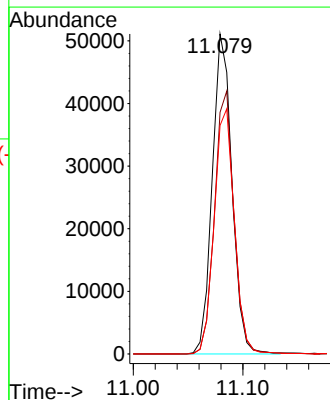
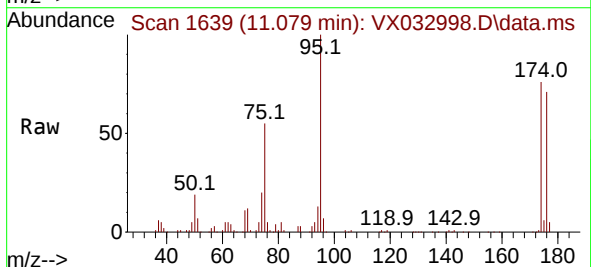


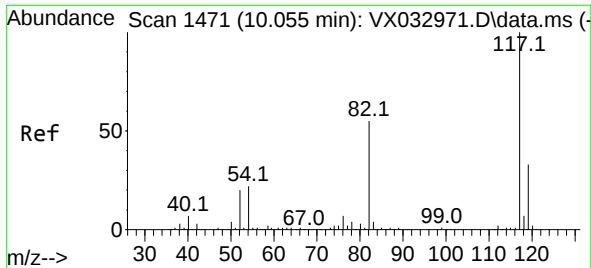

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59

Instrument :
MSVOA_X
ClientSampleId :
TT158S1-20221118

Tgt Ion:117 Resp: 168737
Ion Ratio Lower Upper
117 100
82 56.2 44.3 66.5
119 32.3 25.7 38.5

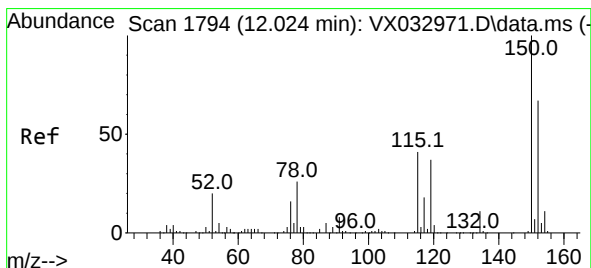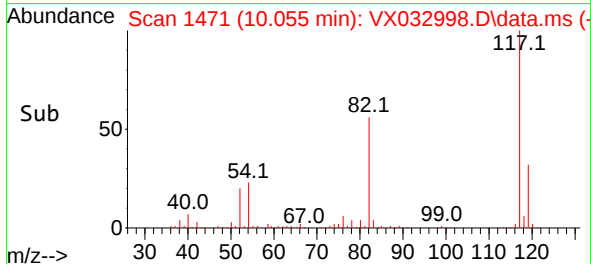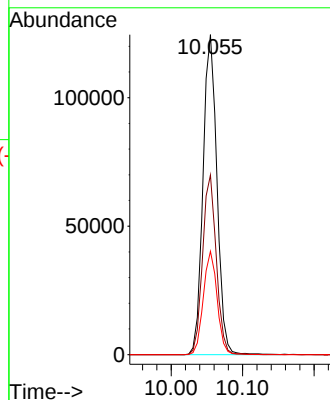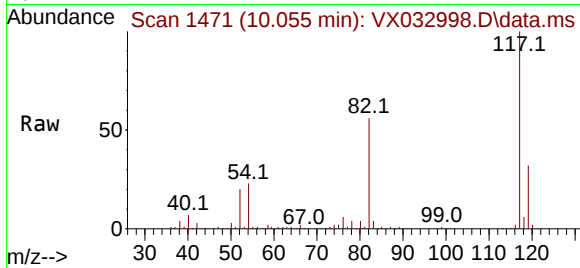

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032998.D
Acq: 22 Nov 2022 22:59

Tgt Ion:152 Resp: 76777
Ion Ratio Lower Upper
152 100
115 60.8 44.0 132.0
150 159.0 0.0 351.8

