

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
 Data File : VX032991.D
 Acq On : 22 Nov 2022 20:18
 Operator : JC/MD
 Sample : N5729-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20221117

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX032991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	212	rBV3	18132	33750	6.80%	1.120%
2	5.385	695	705	721	rBV2	46697	136171	27.43%	4.517%
3	5.556	721	733	746	rVV	120681	339330	68.35%	11.257%
4	5.964	789	800	813	rBV2	35732	96628	19.46%	3.205%
5	6.763	920	931	944	rBV	180535	427463	86.10%	14.180%
6	7.129	982	991	1006	rBV	227872	496485	100.00%	16.470%
7	8.647	1234	1240	1248	rBV	137226	218008	43.91%	7.232%
8	8.720	1248	1252	1259	rVB	4894	8186	1.65%	0.272%
9	10.055	1465	1471	1484	rBV	367451	495579	99.82%	16.440%
10	11.079	1634	1639	1650	rBV	244792	311170	62.67%	10.322%
11	12.024	1788	1794	1803	rBV	349002	451718	90.98%	14.985%




Sum of corrected areas: 3014488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032991.D
Acq On : 22 Nov 2022 20:18
Operator : JC/MD
Sample : N5729-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20221117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

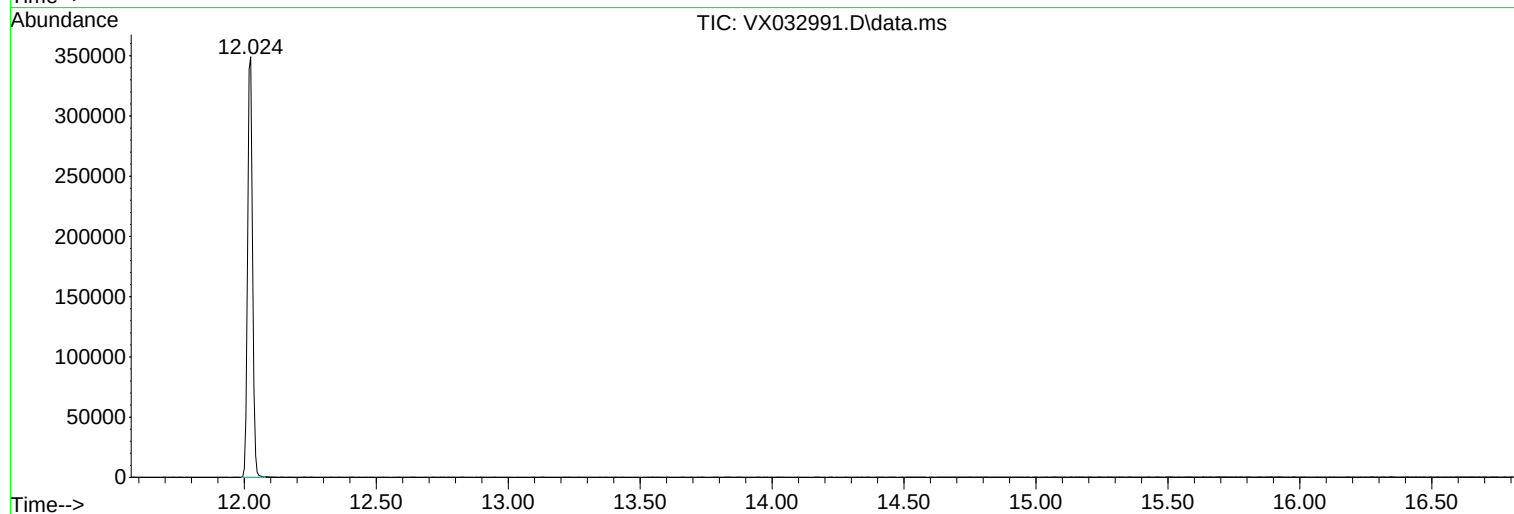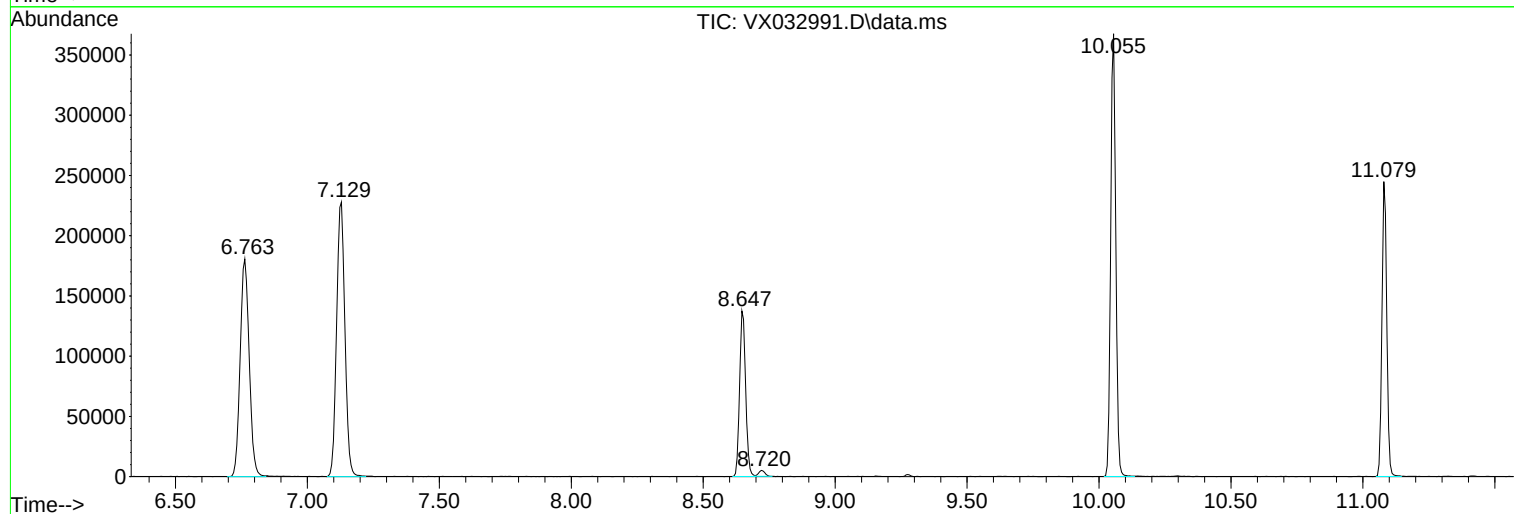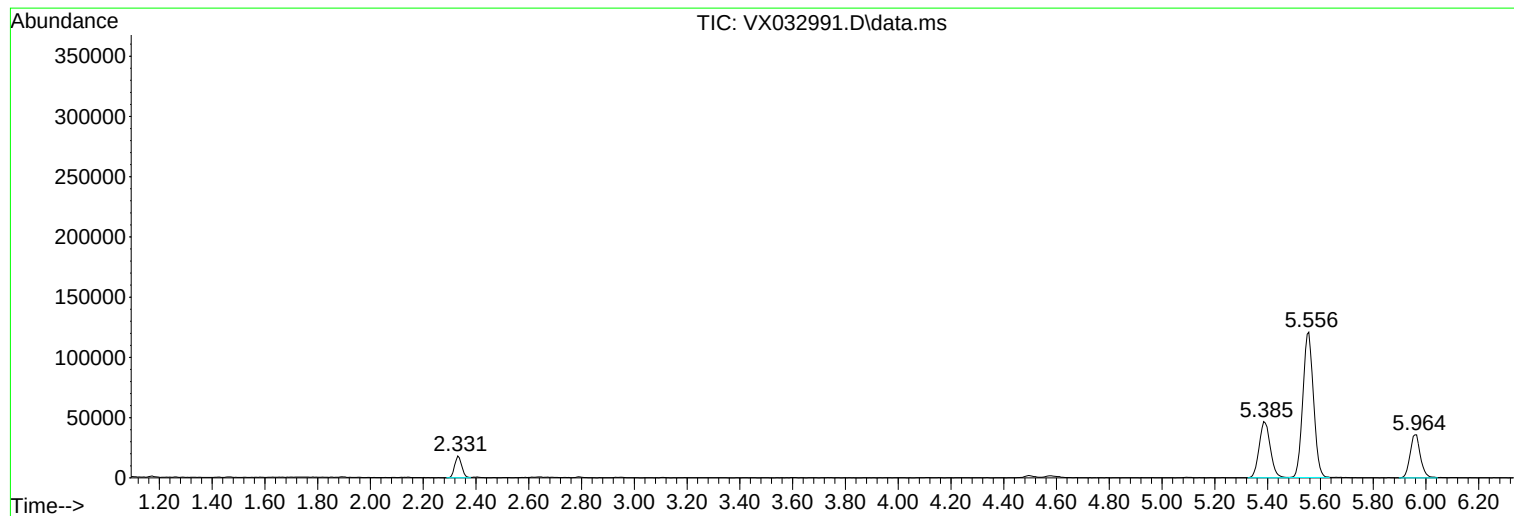

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032991.D
Acq On : 22 Nov 2022 20:18
Operator : JC/MD
Sample : N5729-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20221117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032991.D
Acq On : 22 Nov 2022 20:18
Operator : JC/MD
Sample : N5729-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20221117

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc