

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
 Data File : VX032999.D
 Acq On : 22 Nov 2022 23:22
 Operator : JC/MD
 Sample : N5730-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D5-20221118

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX032999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	211	rBV2	32895	62766	6.76%	1.650%
2	2.946	296	305	314	rVB	5179	11865	1.28%	0.312%
3	5.391	692	706	721	rBV	54825	161663	17.40%	4.250%
4	5.556	721	733	746	rVV	124269	352564	37.95%	9.268%
5	5.958	789	799	812	rBV2	56895	149240	16.07%	3.923%
6	6.763	921	931	946	rBV	188796	445595	47.97%	11.714%
7	7.128	980	991	1005	rBV	428669	928902	100.00%	24.419%
8	8.646	1234	1240	1249	rBV	246379	385806	41.53%	10.142%
9	10.055	1465	1471	1483	rBV	388436	511090	55.02%	13.435%
10	11.079	1634	1639	1649	rBV	257669	326789	35.18%	8.591%
11	12.024	1788	1794	1806	rBV	373774	467768	50.36%	12.297%




Sum of corrected areas: 3804048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032999.D
Acq On : 22 Nov 2022 23:22
Operator : JC/MD
Sample : N5730-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

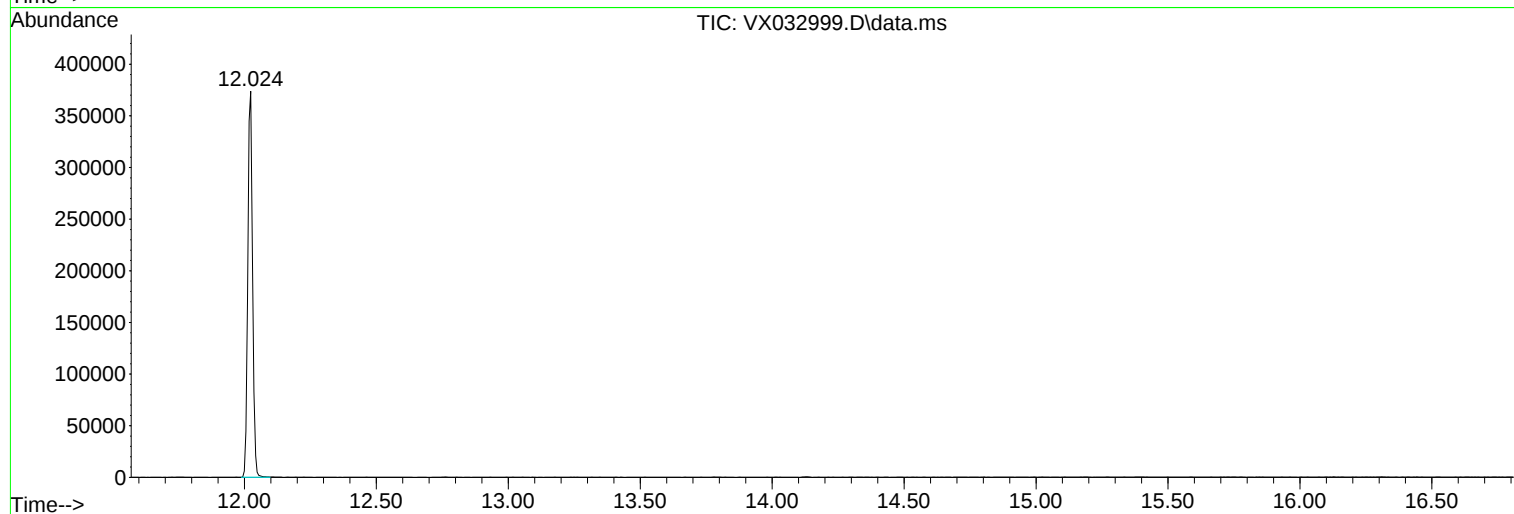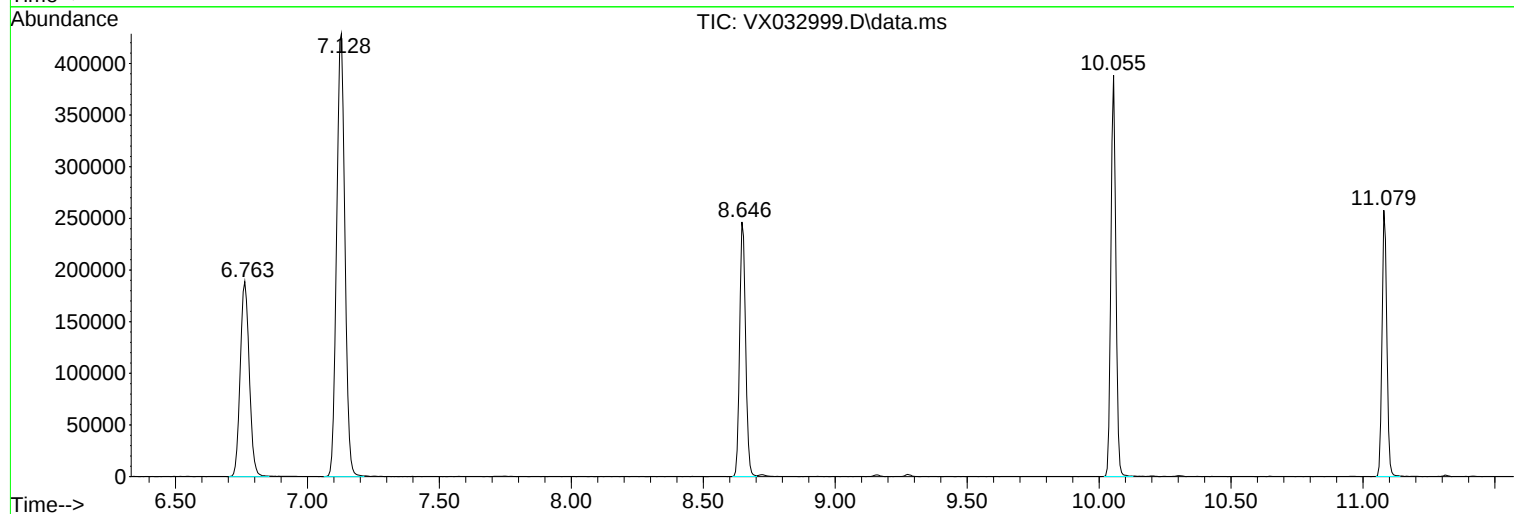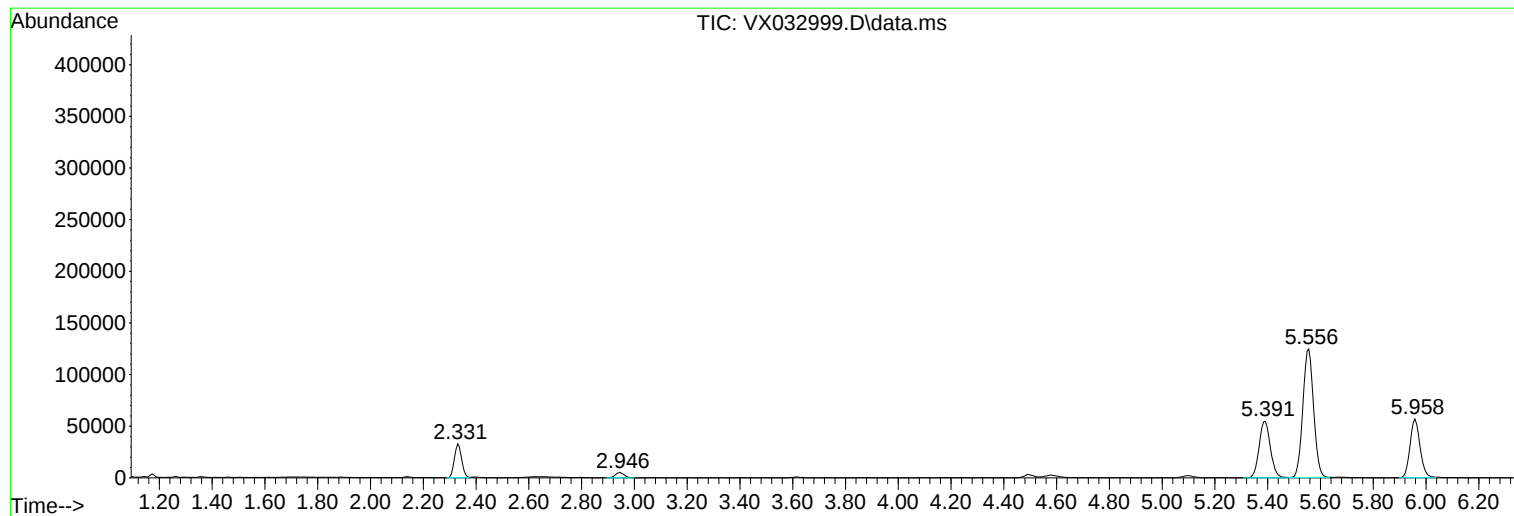

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032999.D
Acq On : 22 Nov 2022 23:22
Operator : JC/MD
Sample : N5730-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032999.D
Acq On : 22 Nov 2022 23:22
Operator : JC/MD
Sample : N5730-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------