

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112222\  
Data File : VX033002.D  
Acq On : 23 Nov 2022 00:31  
Operator : JC/MD  
Sample : N5741-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-14

Integration Parameters: RTEINT.P  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Title : SW846 8260

Signal : TIC: VX033002.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.111       | 324           | 332         | 344          | rBV2     | 21846          | 52555         | 10.32%          | 1.992%        |
| 2         | 5.385       | 695           | 705         | 718          | rBV2     | 45303          | 131869        | 25.89%          | 4.999%        |
| 3         | 5.556       | 722           | 733         | 746          | rVV      | 122311         | 348732        | 68.46%          | 13.220%       |
| 4         | 5.952       | 788           | 798         | 816          | rBV      | 36057          | 97698         | 19.18%          | 3.704%        |
| 5         | 6.763       | 922           | 931         | 950          | rBV      | 183995         | 438794        | 86.14%          | 16.635%       |
| 6         | 7.129       | 984           | 991         | 1001         | rVB2     | 9777           | 21066         | 4.14%           | 0.799%        |
| 7         | 8.647       | 1233          | 1240        | 1249         | rBV      | 137289         | 219262        | 43.05%          | 8.312%        |
| 8         | 10.055      | 1465          | 1471        | 1481         | rBV      | 384822         | 509370        | 100.00%         | 19.310%       |
| 9         | 11.079      | 1634          | 1639        | 1651         | rBV      | 273743         | 349623        | 68.64%          | 13.254%       |
| 10        | 12.024      | 1788          | 1794        | 1807         | rVB      | 371967         | 468869        | 92.05%          | 17.775%       |




Sum of corrected areas: 2637838

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112222\  
Data File : VX033002.D  
Acq On : 23 Nov 2022 00:31  
Operator : JC/MD  
Sample : N5741-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

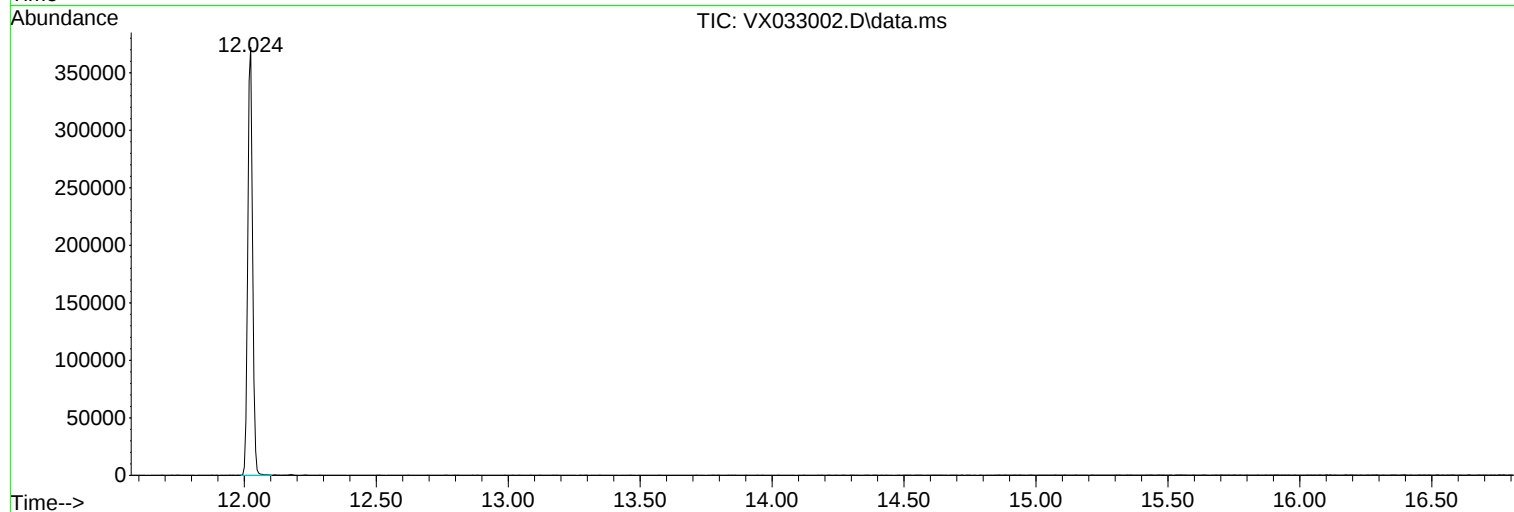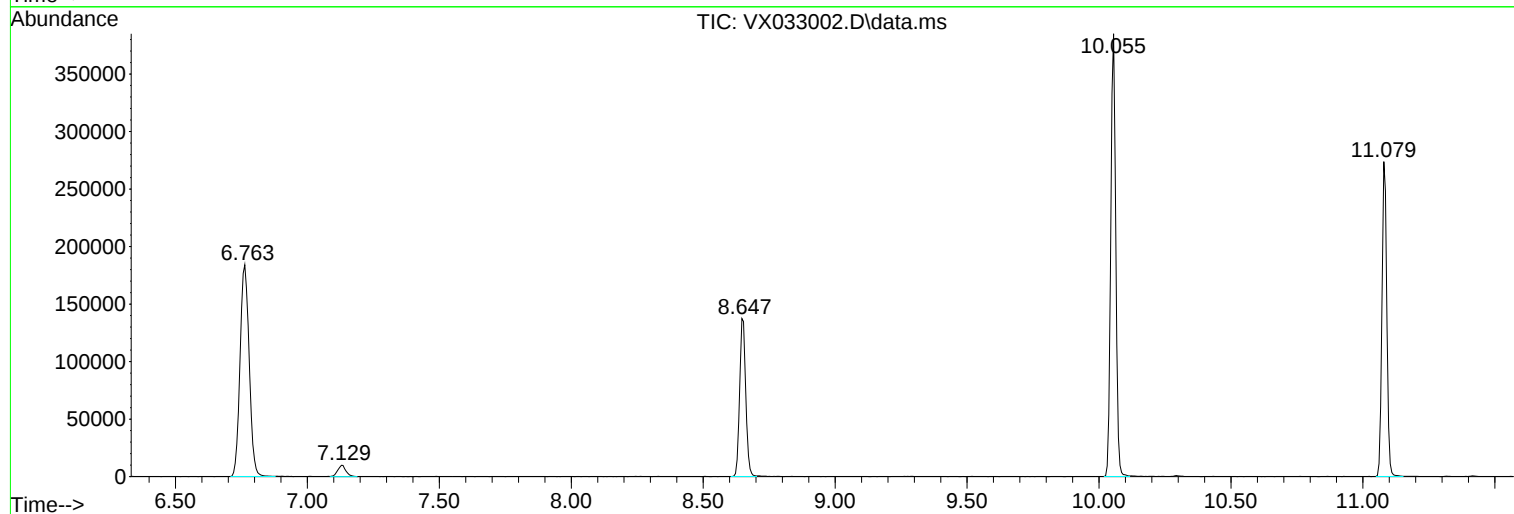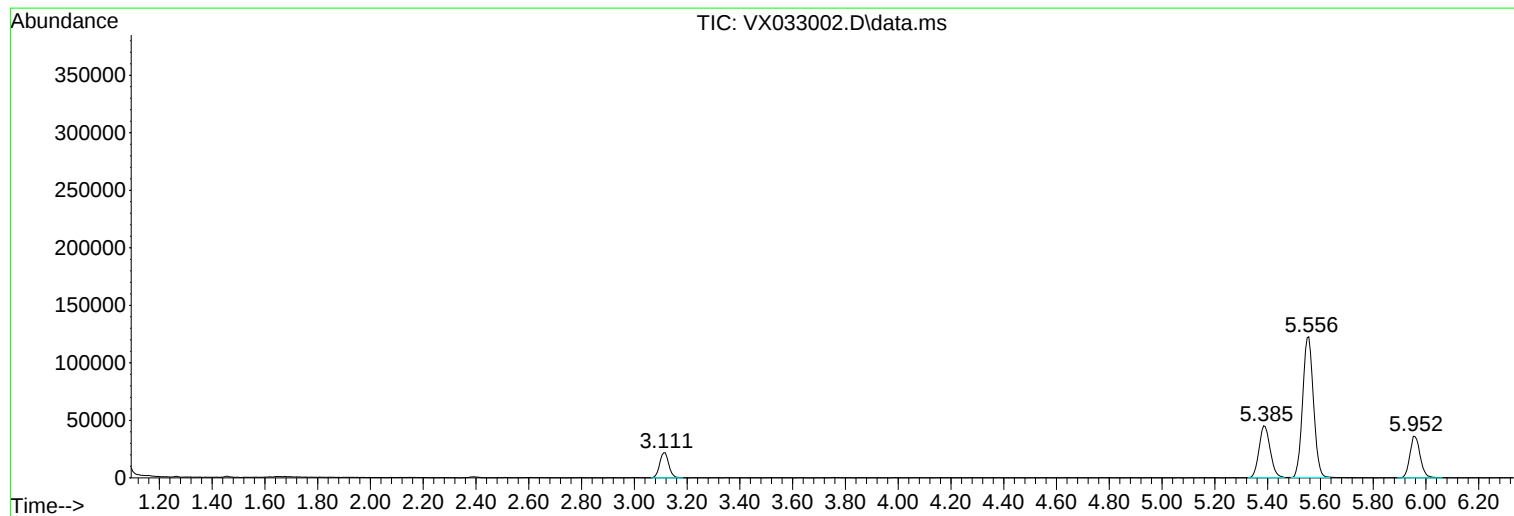

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112222\  
Data File : VX033002.D  
Acq On : 23 Nov 2022 00:31  
Operator : JC/MD  
Sample : N5741-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112222\  
Data File : VX033002.D  
Acq On : 23 Nov 2022 00:31  
Operator : JC/MD  
Sample : N5741-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|