


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112222\
Data File : VX032979.D
Acq On : 22 Nov 2022 15:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260
Last Update : Tue Nov 22 13:58:46 2022

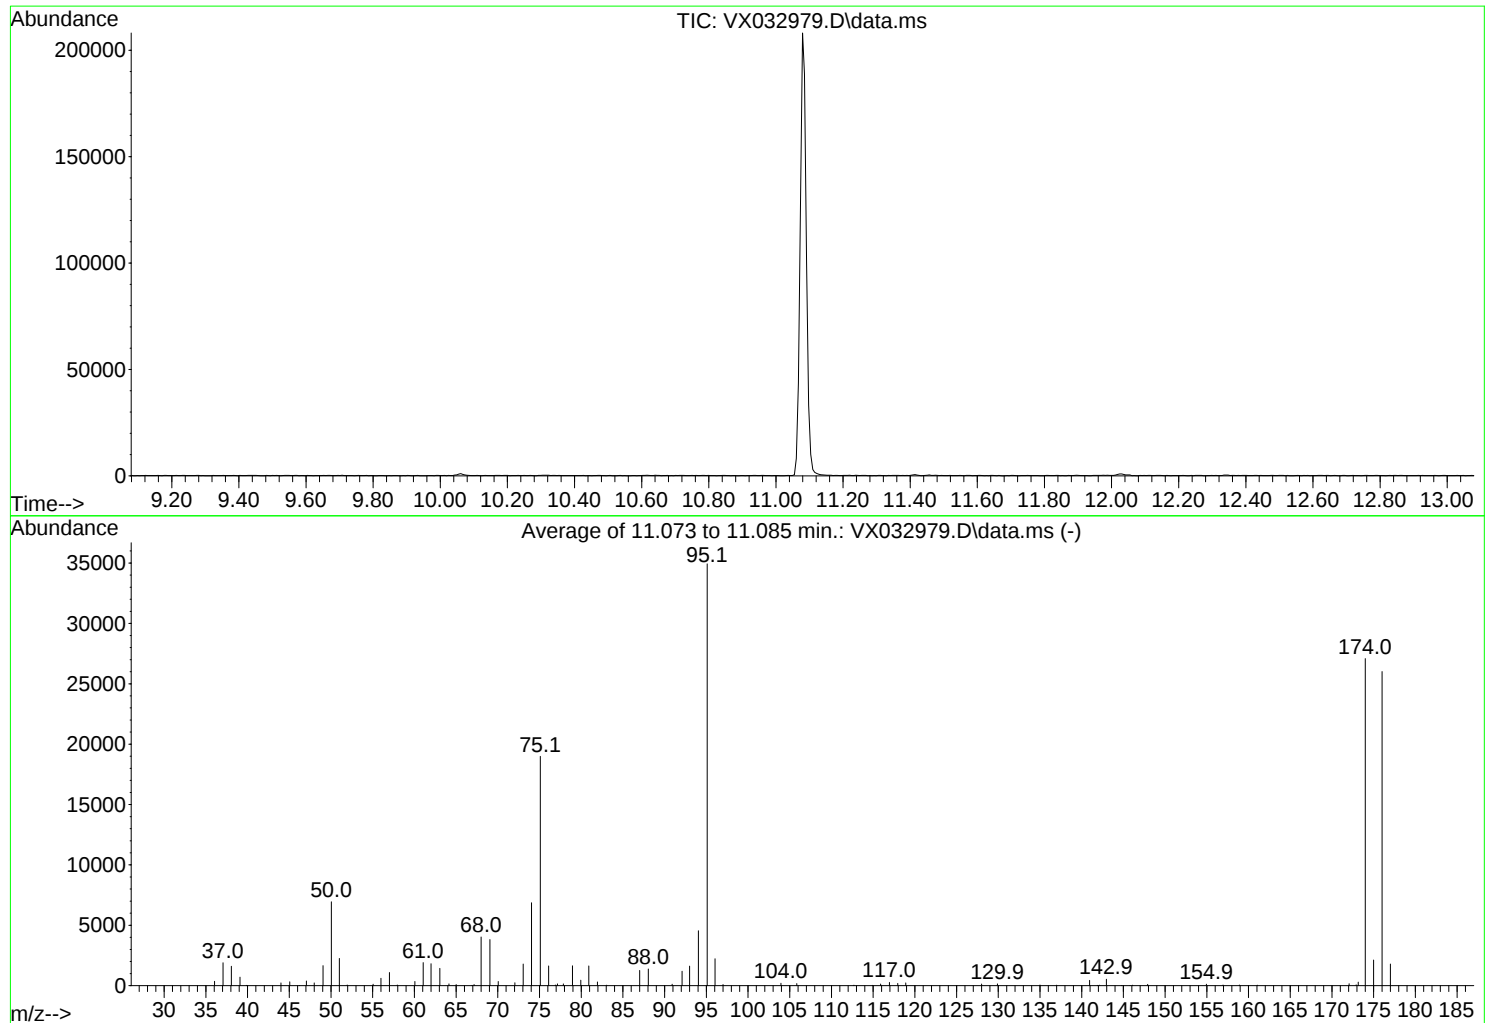

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	6950	PASS
75	95	30	60	54.4	18988	PASS
95	95	100	100	100.0	34936	PASS
96	95	5	9	6.4	2222	PASS
173	174	0.00	2	1.1	288	PASS
174	95	50	100	77.6	27093	PASS
175	174	5	9	7.8	2119	PASS
176	174	95	101	96.0	26012	PASS
177	176	5	9	6.9	1794	PASS