
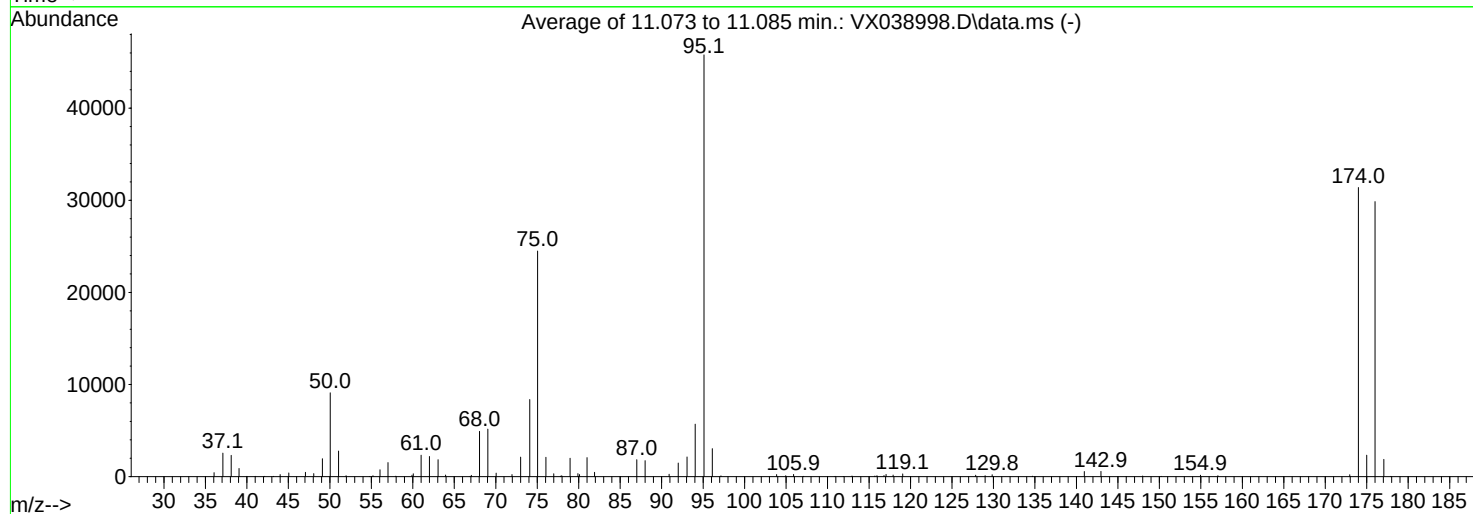


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112223\
Data File : VX038998.D
Acq On : 22 Nov 2023 12:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Title : SW846 8260
Last Update : Thu Nov 16 22:59:22 2023

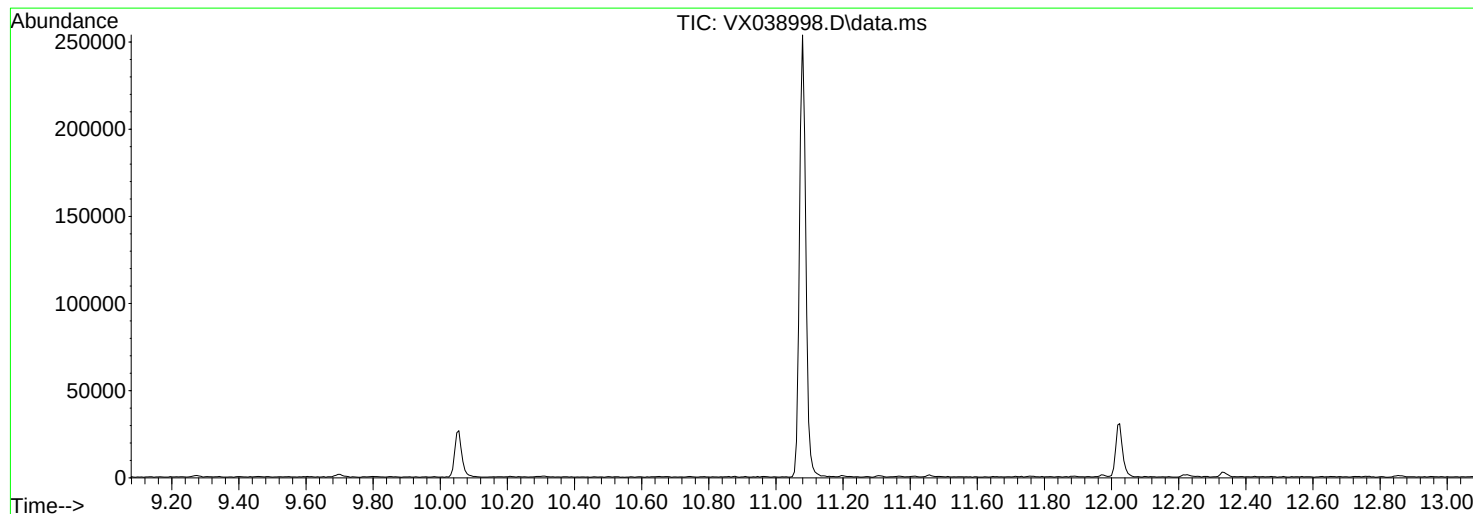

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	9110	PASS
75	95	30	60	53.5	24491	PASS
95	95	100	100	100.0	45789	PASS
96	95	5	9	6.6	3038	PASS
173	174	0.00	2	0.7	205	PASS
174	95	50	100	68.6	31389	PASS
175	174	5	9	7.4	2328	PASS
176	174	95	101	95.2	29867	PASS
177	176	5	9	6.3	1869	PASS