

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043959.D
Acq On : 22 Nov 2024 14:57
Operator : JC/MD
Sample : P4846-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-03S-20241113

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Title : SW846 8260

Signal : TIC: VX043959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	21	25	31	rBV	13712	17627	2.41%	0.385%
2	1.617	67	87	90	rBV5	17401	86167	11.80%	1.884%
3	5.379	693	704	720	rBV	82411	248266	34.01%	5.429%
4	5.543	720	731	750	rVV	126939	370196	50.72%	8.096%
5	5.952	789	798	814	rBV	102353	270838	37.10%	5.923%
6	6.757	920	930	943	rBV2	214949	532094	72.90%	11.636%
7	7.116	982	989	1004	rBV	319339	717721	98.33%	15.695%
8	8.647	1233	1240	1255	rBV	436688	729945	100.00%	15.963%
9	10.049	1465	1470	1489	rBV	423749	635841	87.11%	13.905%
10	11.079	1634	1639	1652	rBV	340579	443809	60.80%	9.705%
11	12.018	1788	1793	1807	rBV	395891	520348	71.29%	11.379%




Sum of corrected areas: 4572852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043959.D
Acq On : 22 Nov 2024 14:57
Operator : JC/MD
Sample : P4846-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-03S-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

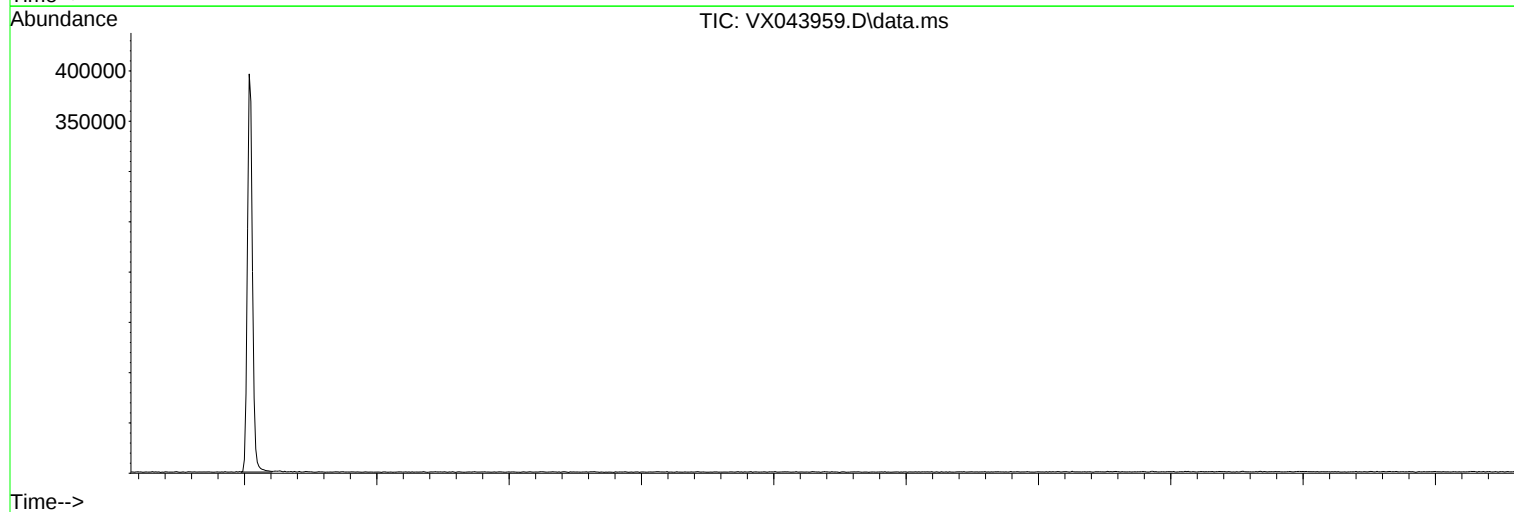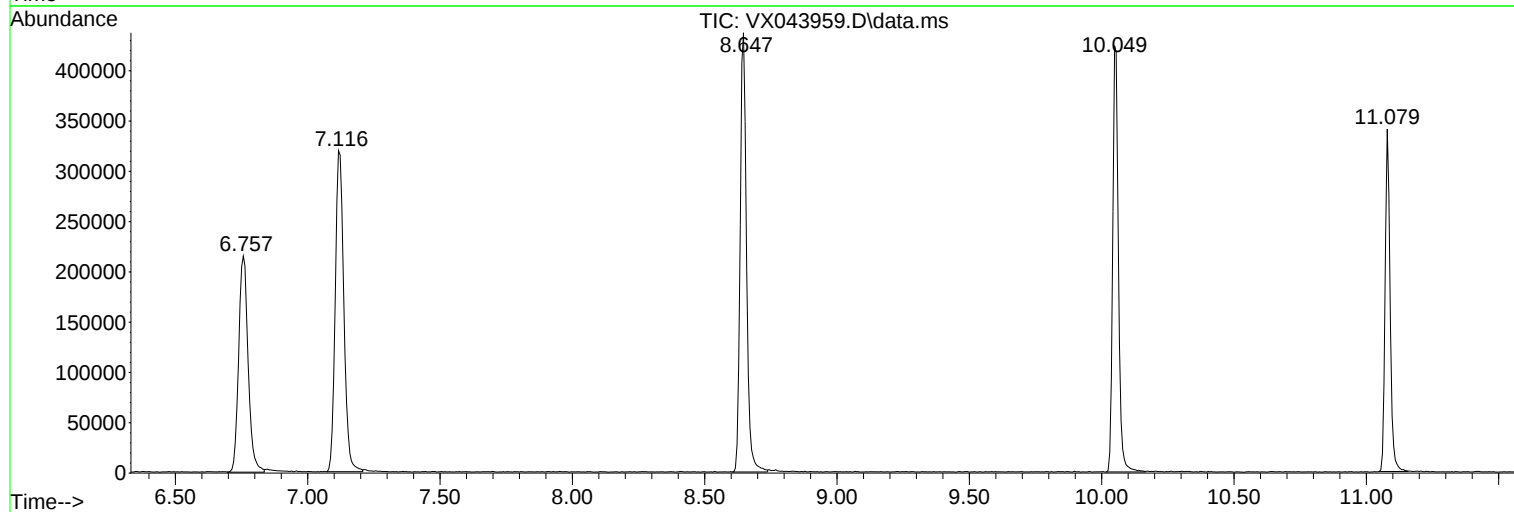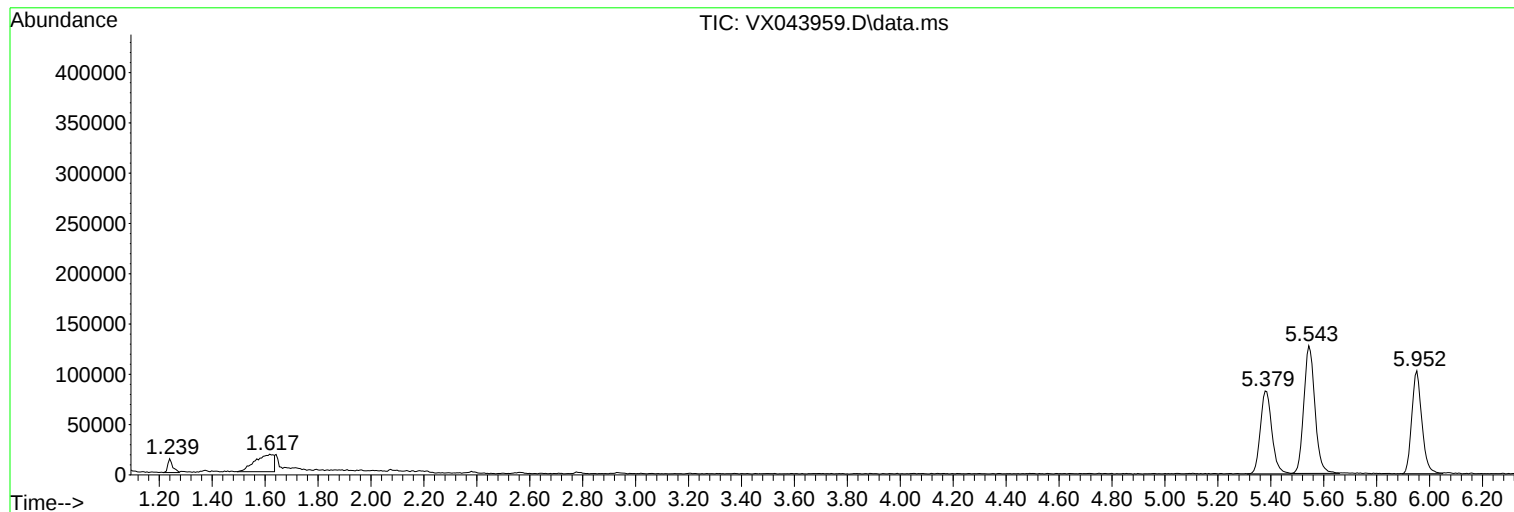

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043959.D
Acq On : 22 Nov 2024 14:57
Operator : JC/MD
Sample : P4846-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-03S-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043959.D
Acq On : 22 Nov 2024 14:57
Operator : JC/MD
Sample : P4846-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-03S-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------