

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
 Data File : VX043970.D
 Acq On : 22 Nov 2024 19:10
 Operator : JC/MD
 Sample : P4846-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-FD-3-20241113

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Title : SW846 8260

Signal : TIC: VX043970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	32	rBV3	7190	10643	1.48%	0.242%
2	1.557	68	77	78	rBV3	10360	21689	3.02%	0.494%
3	5.379	694	704	717	rBV	78102	237234	33.05%	5.399%
4	5.550	720	732	751	rVV	123249	361284	50.34%	8.222%
5	5.952	787	798	815	rBV	100685	267668	37.29%	6.092%
6	6.757	922	930	949	rBV	213698	517573	72.12%	11.779%
7	7.123	979	990	1004	rBV	326139	717705	100.00%	16.334%
8	8.647	1233	1240	1254	rBV	441829	707601	98.59%	16.104%
9	10.049	1465	1470	1487	rBV	419674	618044	86.11%	14.066%
10	11.079	1634	1639	1651	rBV	325138	430593	60.00%	9.800%
11	12.018	1788	1793	1804	rBV	387471	503981	70.22%	11.470%




Sum of corrected areas: 4394015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043970.D
Acq On : 22 Nov 2024 19:10
Operator : JC/MD
Sample : P4846-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-3-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

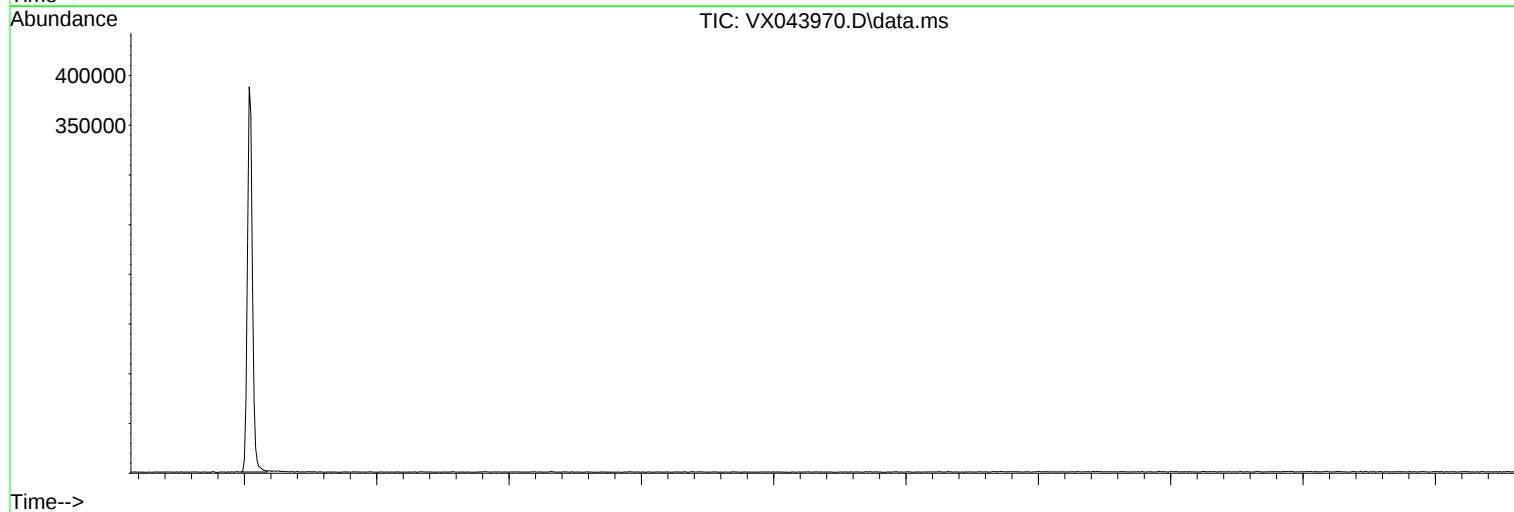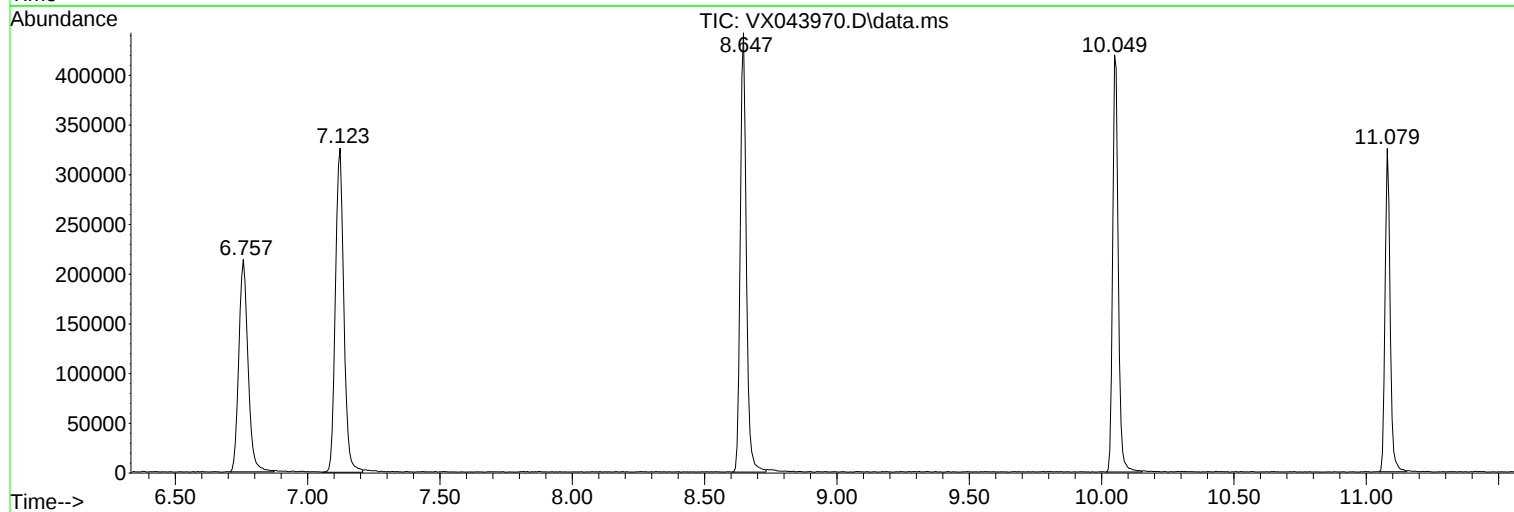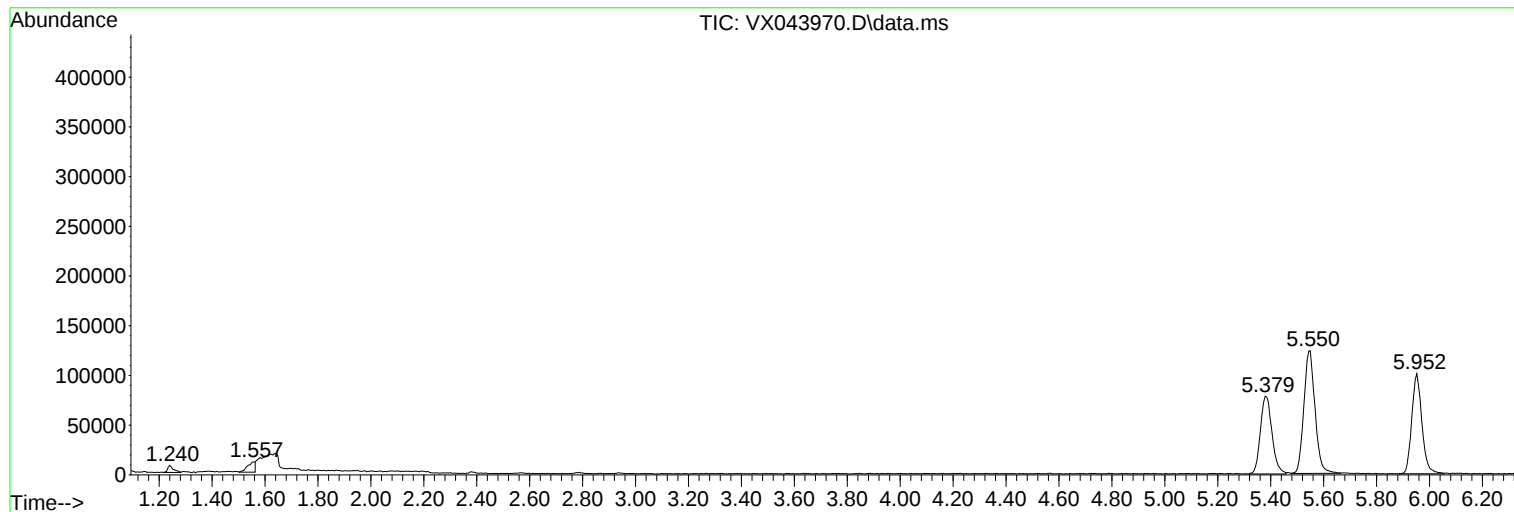

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043970.D
Acq On : 22 Nov 2024 19:10
Operator : JC/MD
Sample : P4846-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-3-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112224\
Data File : VX043970.D
Acq On : 22 Nov 2024 19:10
Operator : JC/MD
Sample : P4846-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-3-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------