

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112320\
 Data File : VX019582.D
 Acq On : 24 Nov 2020 04:18
 Operator : JC/MD
 Sample : L4848-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-1-TOP

Quant Time: Nov 24 05:18:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.62	168	304889	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	503080	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	458835	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	186007	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	190269	48.13	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.26%
35) Dibromofluoromethane	5.46	113	150585	47.69	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.38%
50) Toluene-d8	8.70	98	611030	49.79	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.58%
62) 4-Bromofluorobenzene	11.12	95	209708	47.50	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	95.00%

Target Compounds


					Qvalue	
6) Chloroethane	1.70	64	616	Below Cal	#	53
11) Tert butyl alcohol	2.99	59	5199	6.949	ug/l #	73
13) Acrolein	2.28	56	191	0.380	ug/l #	36
16) Acetone	2.42	43	26274	17.187	ug/l	99
17) Carbon Disulfide	2.54	76	1834	0.226	ug/l #	86
18) Methyl Acetate	2.75	43	2906	1.400	ug/l	99
20) Methylene Chloride	2.83	84	52355	13.702	ug/l	96
25) 2-Butanone	4.64	43	4641	2.021	ug/l	96
29) Tetrahydrofuran	5.09	42	1588	1.084	ug/l #	87
31) Cyclohexane	5.62	56	5904	1.148	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	23506	4.984	ug/l #	49
38) Carbon Tetrachloride	5.63	117	30099	6.593	ug/l #	16
43) Isopropyl Acetate	6.42	43	23686	3.182	ug/l	99
44) Trichloroethene	7.19	130	2256	0.594	ug/l	95
48) Methyl methacrylate	7.65	41	6087	1.746	ug/l #	9
49) 1,4-Dioxane	7.85	88	86	1.087	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	83440	19.225	ug/l #	47
54) cis-1,3-Dichloropropene	8.59	75	43788	7.711	ug/l #	60
57) 1,3-Dichloropropane	9.52	76	18969	3.138	ug/l #	43
59) 2-Hexanone	9.52	43	226035	68.668	ug/l #	48
70) Styrene	10.70	104	117	1.656	ug/l #	30
74) N-amyl acetate	10.80	43	1010	0.209	ug/l #	47
76) 1,2,3-Trichloropropane	11.12	75	102695	25.299	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	102695	66.778	ug/l #	12
95) Naphthalene	13.82	128	282	2.198	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112320\
Data File : VX019582.D
Acq On : 24 Nov 2020 04:18
Operator : JC/MD
Sample : L4848-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR5-1-TOP

Quant Time: Nov 24 05:18:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

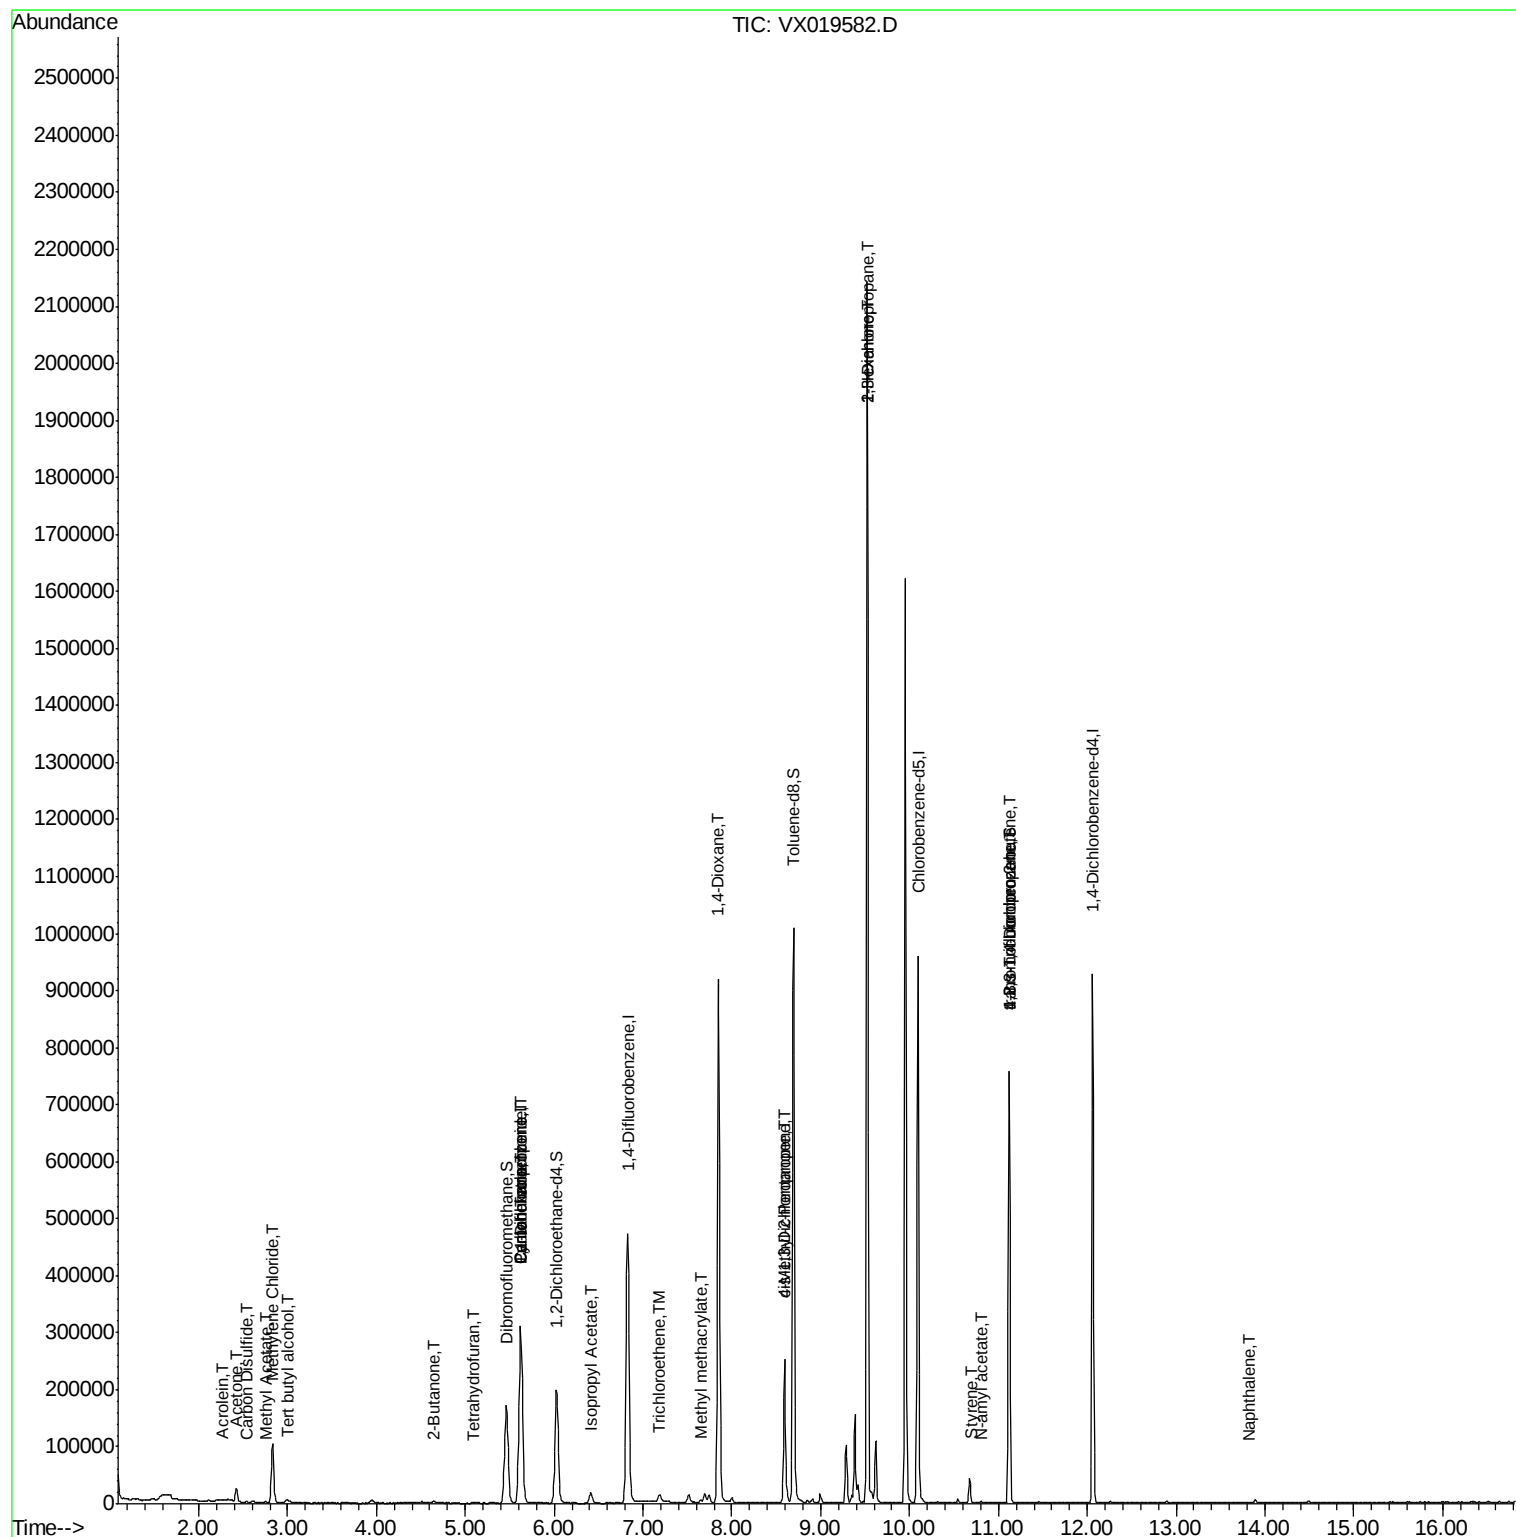



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.01 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampled :


TR5-1-TOP

Tot Ion:168 Resp: 304889

Ion Ratio Lower Upper

168 100

99 58.3 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.62

120000

100000

80000



60000

40000

20000

0

Time-->

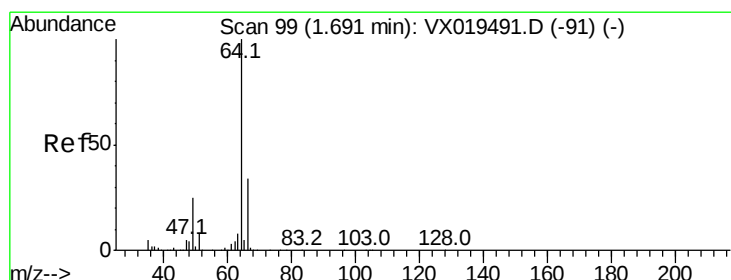

#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 100

Delta R.T. 0.01 min

Lab File: VX019582.D


Acq: 24 Nov 2020 04:18

Tgt Ion: 64 Resp: 616

Ion Ratio Lower Upper

64 100

66 7.1 27.1 40.7#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

1.70

600

500

400


300


200

100

0

Time-->









#11

Tert butyl alcohol
 Concen: 6.949 ug/l
 RT: 2.99 min Scan# 312
 Delta R.T. -0.06 min
 Lab File: VX019582.D
 Acq: 24 Nov 2020 04:18

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-1-TOP




Tot Ion: 59 Resp: 5199
 Ion Ratio Lower Upper
 59 100
 57 0.0 7.9 11.9#

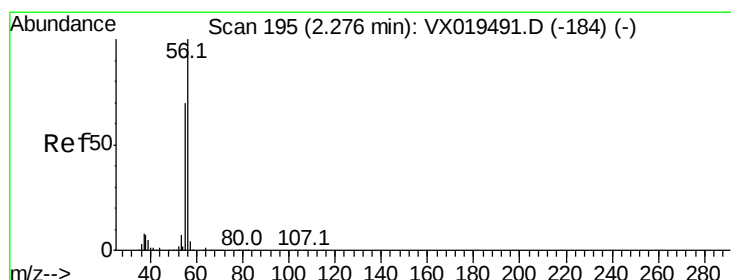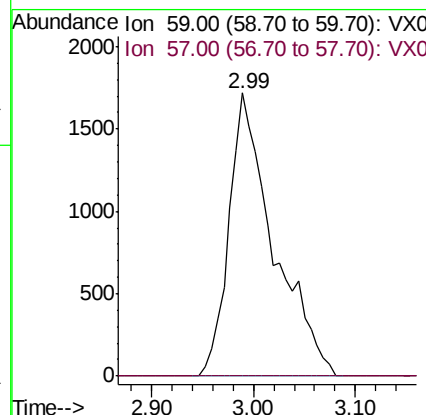


#13

Acrolein
 Concen: 0.380 ug/l
 RT: 2.28 min Scan# 195
 Delta R.T. -0.00 min
 Lab File: VX019582.D
 Acq: 24 Nov 2020 04:18

Tgt Ion: 56 Resp: 191
 Ion Ratio Lower Upper
 56 100
 55 16.8 55.5 83.3#

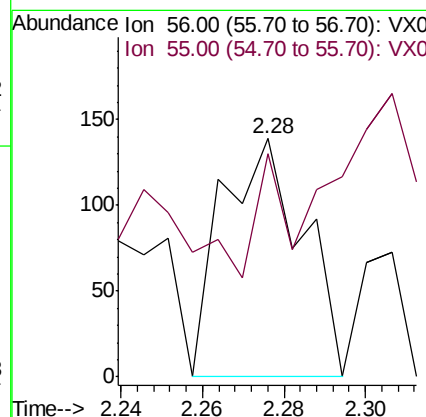



#16

Acetone

Concen: 17.187 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.01 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :





TR5-1-TOP

Tot Ion: 43 Resp: 26274

Ion Ratio Lower Upper

43 100

58 33.8 27.4 41.2

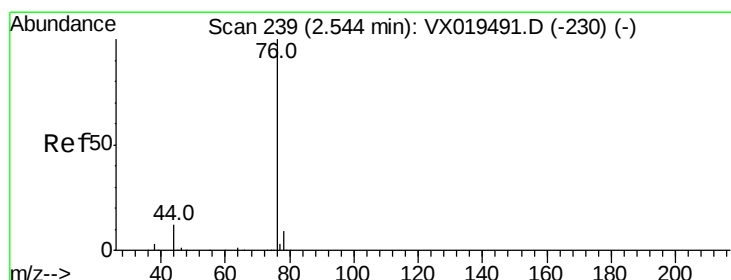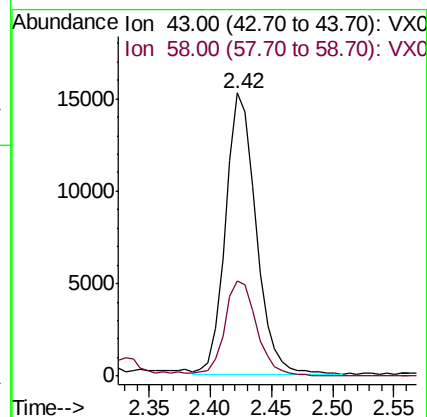

#17

Carbon Disulfide

Concen: 0.226 ug/l

RT: 2.54 min Scan# 239

Delta R.T. -0.00 min

Lab File: VX019582.D




Acq: 24 Nov 2020 04:18


Tgt Ion: 76 Resp: 1834

Ion Ratio Lower Upper

76 100

78 13.9 7.2 10.8#

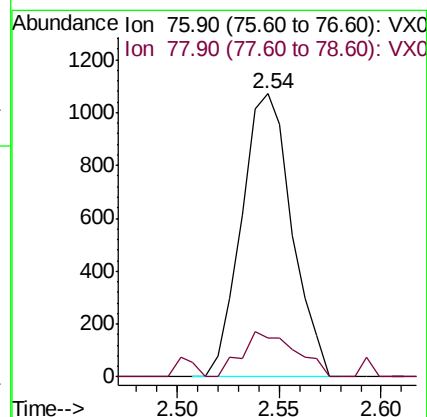



#18

Methvl Acetate

Concen: 1.400 ug/l

RT: 2.75 min Scan# 273

Delta R.T. 0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :


TR5-1-TOP

Tot Ion: 43 Resp: 2906

Ion Ratio Lower Upper




43 100

74 27.1 22.2 33.4

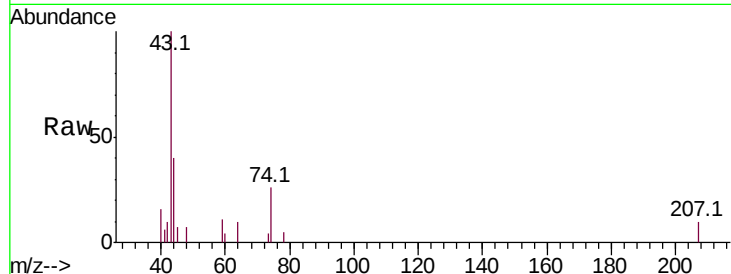

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

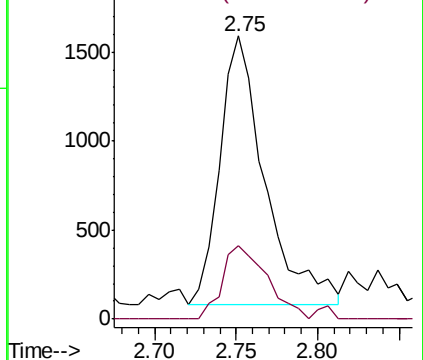

#20

Methylene Chloride

Concen: 13.702 ug/l

RT: 2.83 min Scan# 286

Delta R.T. -0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Tgt Ion: 84 Resp: 52355


Ion Ratio Lower Upper

84 100

49 105.9 88.5 132.7

51 34.4 28.0 42.0

86 62.0 53.0 79.4






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0




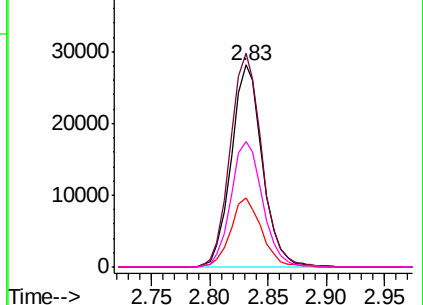




#25
2-Butanone
Concen: 2.021 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.00 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18




Instrument :
MSVOA_X
ClientSampleId :
TR5-1-TOP


Tot Ion: 43 Resp: 4641
Ion Ratio Lower Upper
43 100
72 28.0 24.0 36.0

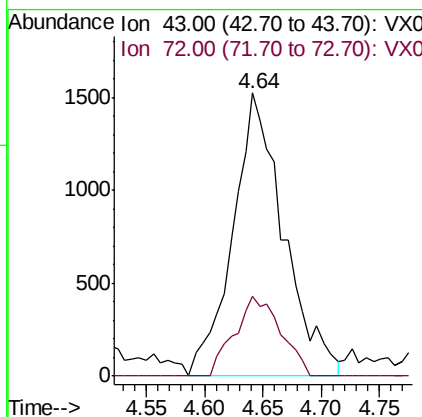

#29
Tetrahydrofuran
Concen: 1.084 ug/l
RT: 5.09 min Scan# 657
Delta R.T. -0.00 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Tgt Ion: 42 Resp: 1588
Ion Ratio Lower Upper
42 100
72 39.7 42.6 63.8#
71 44.7 39.0 58.6

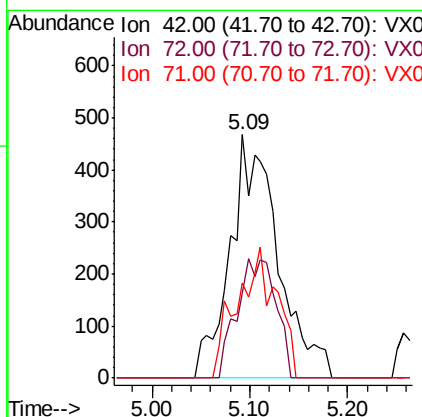







#31
Cvclohexane
Concen: 1.148 ug/l
RT: 5.62 min Scan# 744
Delta R.T. 0.09 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Instrument :
MSVOA_X
ClientSampleId :
TR5-1-TOP

Tot Ion: 56 Resp: 5904
Ion Ratio Lower Upper
56 100
69 190.4 25.5 38.3#
84 153.8 71.1 106.7#




Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

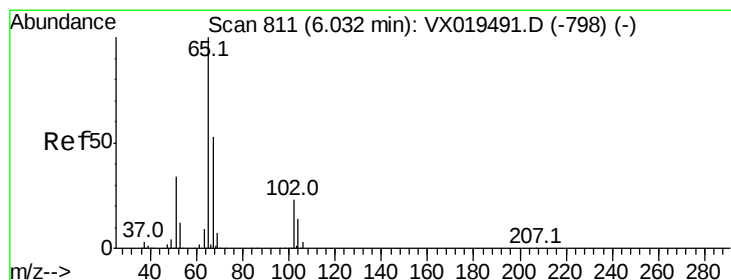
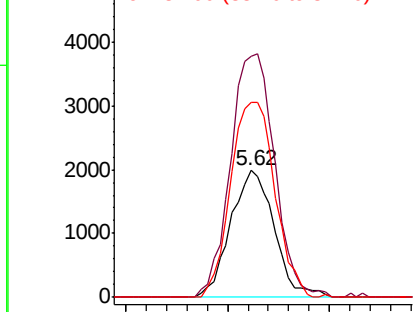



#33
1,2-Dichloroethane-d4
Concen: 48.131 ug/l
RT: 6.03 min Scan# 810
Delta R.T. -0.01 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Tgt Ion: 65 Resp: 190269
Ion Ratio Lower Upper
65 100
67 52.1 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

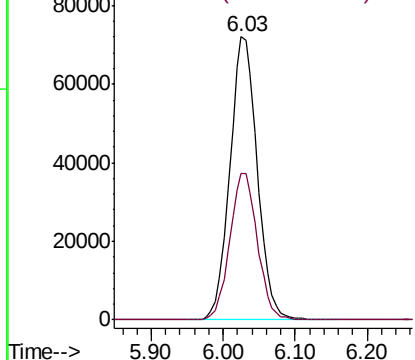



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP


Tot Ion:114 Resp: 503080

Ion Ratio Lower Upper

114 100

63 19.6 0.0 38.8




88 15.9 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

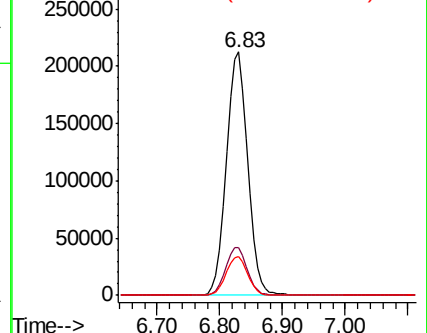

#35

Dibromofluoromethane

Concen: 47.686 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18


Tgt Ion:113 Resp: 150585

Ion Ratio Lower Upper

113 100

111 101.8 81.5 122.3



192 20.3 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

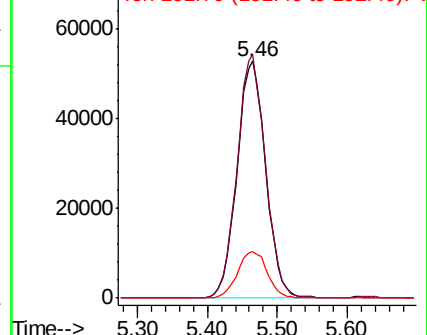



#36

1,1-Dichloropropene

Concen: 4.984 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP


Tot Ion: 75 Resp: 23506

Ion Ratio Lower Upper

75 100

110 8.8 18.1 54.3#




77 0.0 24.2 36.4#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

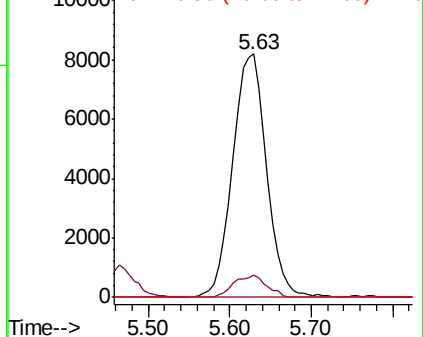

#38

Carbon Tetrachloride

Concen: 6.593 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18


Tgt Ion: 117 Resp: 30099

Ion Ratio Lower Upper

117 100

119 4.8 75.9 113.9#



121 0.0 24.0 36.0#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

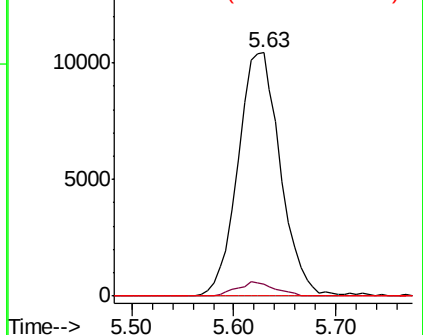



#43

Isopropyl Acetate

Concen: 3.182 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP


Tot Ion: 43 Resp: 23686

Ion Ratio Lower Upper

43 100

61 22.0 18.2 27.2




87 15.5 12.6 18.8



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

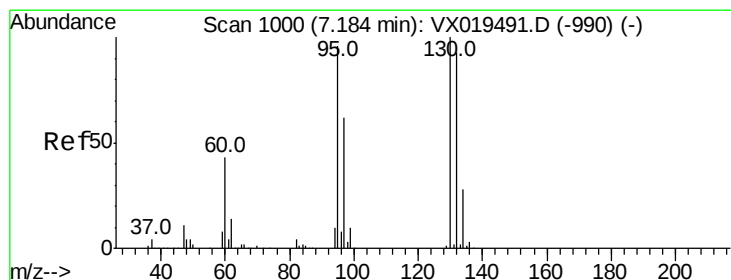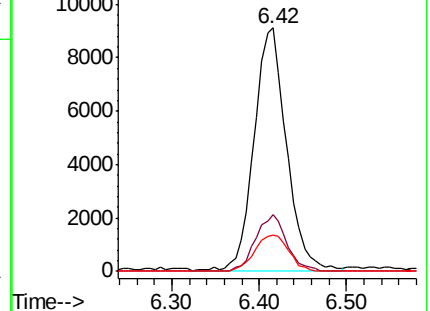

#44

Trichloroethene

Concen: 0.594 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. 0.01 min

Lab File: VX019582.D


Acq: 24 Nov 2020 04:18

Tgt Ion: 130 Resp: 2256

Ion Ratio Lower Upper



130 100


95 100.5 0.0 191.2



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

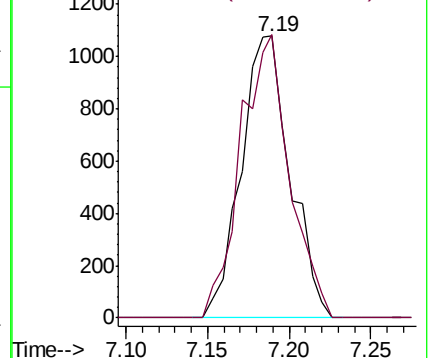

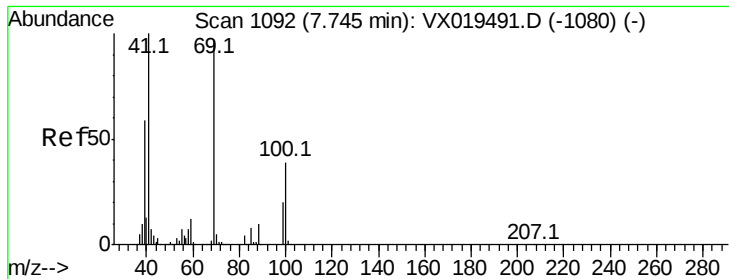

#48

Methvl methacrylate

Concen: 1.746 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP


Tot Ion: 41 Resp: 6087

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#




39 0.0 45.6 68.4#



Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

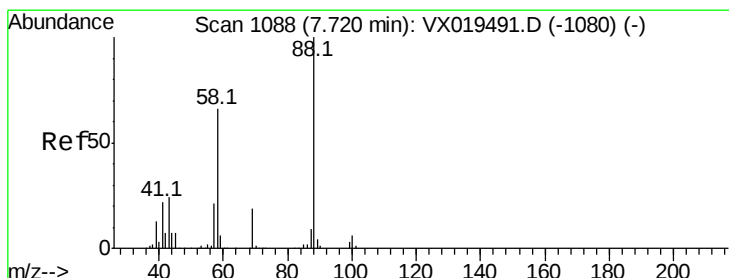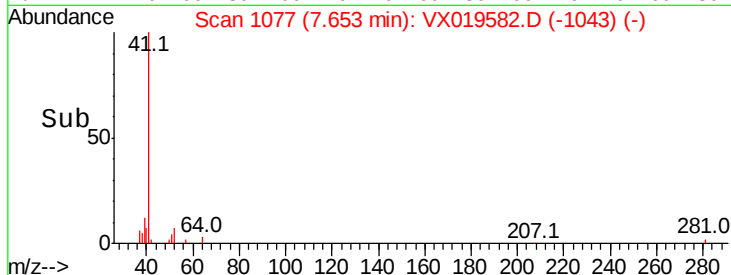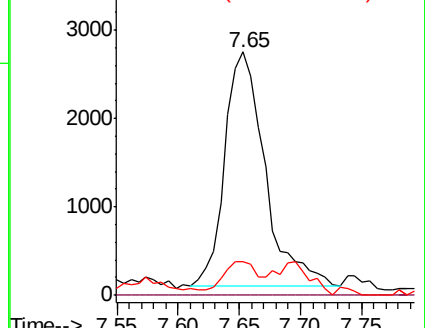

#49

1,4-Dioxane

Concen: 1.087 ug/l

RT: 7.85 min Scan# 1110

Delta R.T. 0.13 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18


Tgt Ion: 88 Resp: 86

Ion Ratio Lower Upper

88 100

43 935968.6 23.8 35.6#



58 4523.3 54.2 81.2#

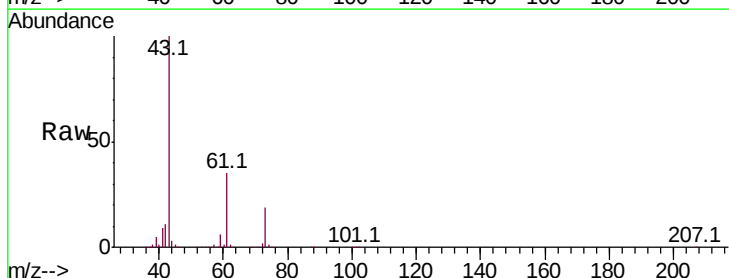


Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



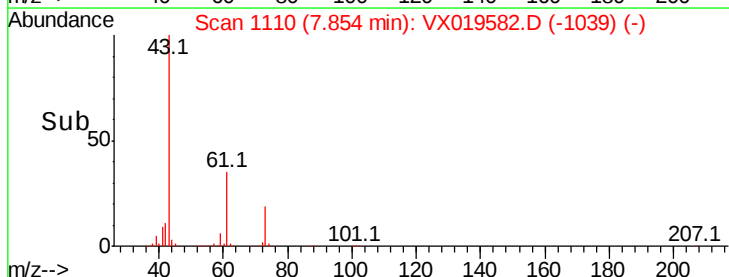
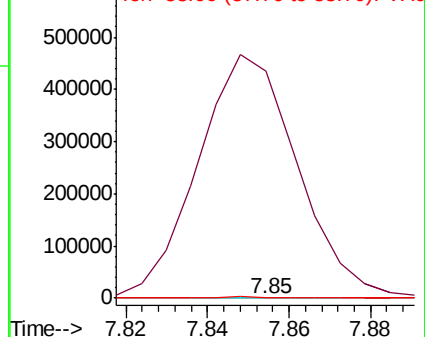




#50
Toluene-d8
Concen: 49.795 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18




Instrument :
MSVOA_X
ClientSampleId :
TR5-1-TOP


Tot Ion: 98 Resp: 611030
Ion Ratio Lower Upper
98 100
100 66.1 52.4 78.6

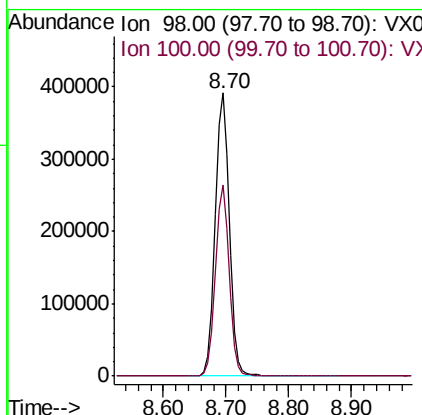

#51
4-Methyl-2-Pentanone
Concen: 19.225 ug/l
RT: 8.59 min Scan# 1231
Delta R.T. -0.03 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Tgt Ion: 43 Resp: 83440
Ion Ratio Lower Upper
43 100
58 9.9 35.1 52.7#

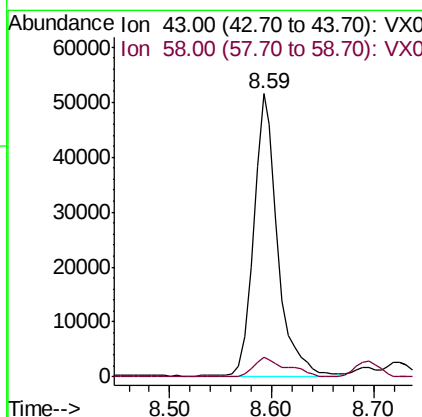







#54

cis-1,3-Dichloropropene
 Concen: 7.711 ug/l
 RT: 8.59 min Scan# 1231
 Delta R.T. 0.18 min
 Lab File: VX019582.D
 Acq: 24 Nov 2020 04:18

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-1-TOP




Tot Ion: 75 Resp: 43788
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.8 38.6#
 39 25.4 34.6 51.8#

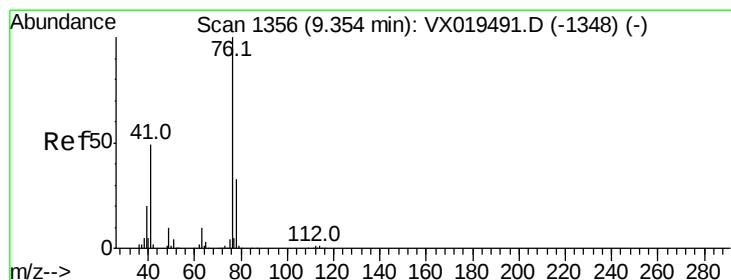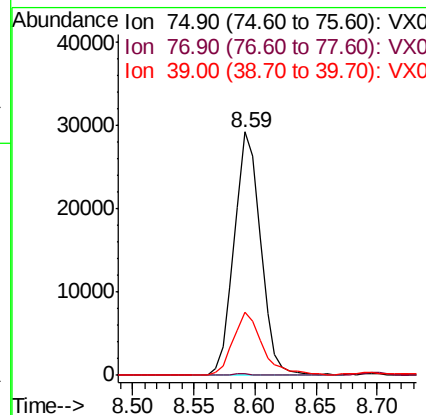


#57

1,3-Dichloropropane
 Concen: 3.138 ug/l
 RT: 9.52 min Scan# 1384
 Delta R.T. 0.17 min
 Lab File: VX019582.D
 Acq: 24 Nov 2020 04:18

Tgt Ion: 76 Resp: 18969
 Ion Ratio Lower Upper
 76 100
 78 0.4 25.7 38.5#



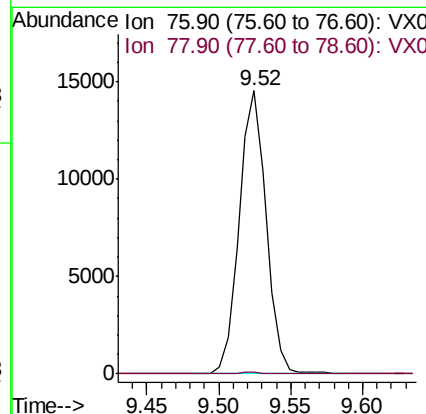





#59
2-Hexanone
Concen: 68.668 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18




Instrument :
MSVOA_X
ClientSampleId :
TR5-1-TOP


Tot Ion: 43 Resp: 226035
Ion Ratio Lower Upper
43 100
58 21.1 30.6 91.6#

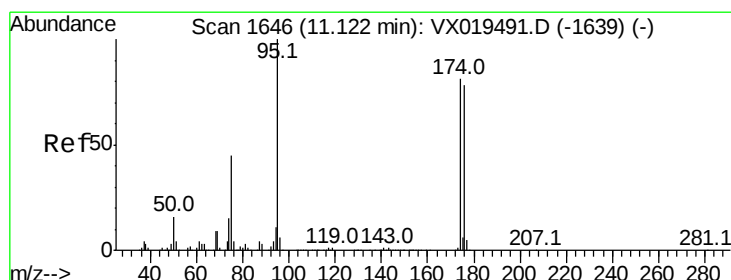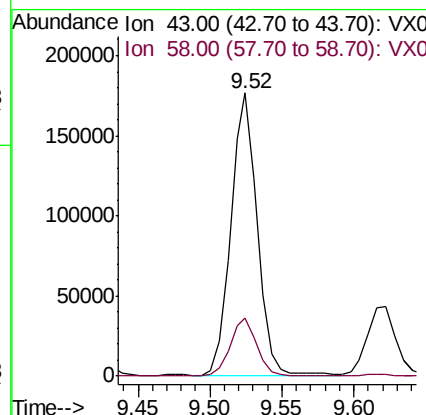

#62
4-Bromofluorobenzene
Concen: 47.500 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Tgt Ion: 95 Resp: 209708
Ion Ratio Lower Upper
95 100
174 76.1 0.0 156.2
176 74.5 0.0 151.4


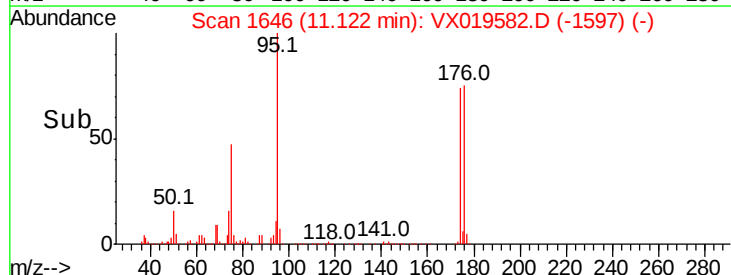
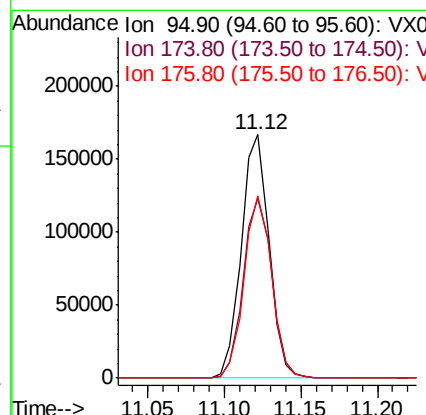





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18




Instrument :
MSVOA_X
ClientSampled :
TR5-1-TOP


Tot Ion:117 Resp: 458835
Ion Ratio Lower Upper
117 100
82 54.4 43.0 64.4
119 32.2 25.6 38.4

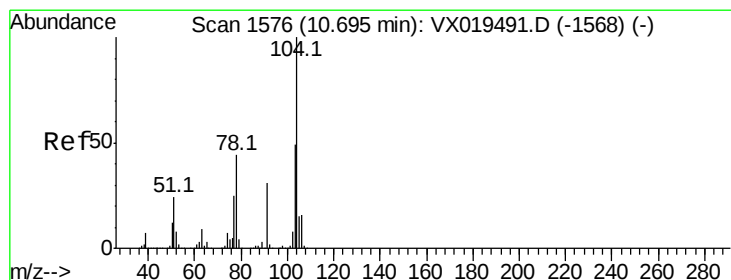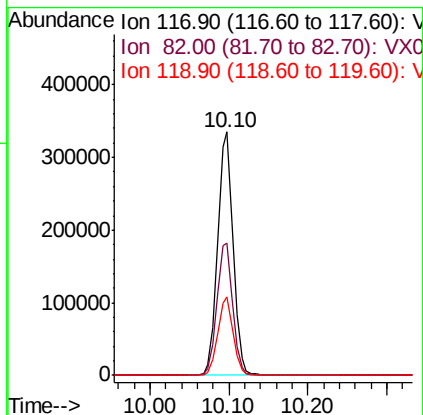

#70
Styrene
Concen: 1.656 ug/l
RT: 10.70 min Scan# 1577
Delta R.T. 0.01 min
Lab File: VX019582.D
Acq: 24 Nov 2020 04:18

Tgt Ion:104 Resp: 117
Ion Ratio Lower Upper
104 100
78 0.0 39.5 59.3#
103 103.4 43.6 65.4#

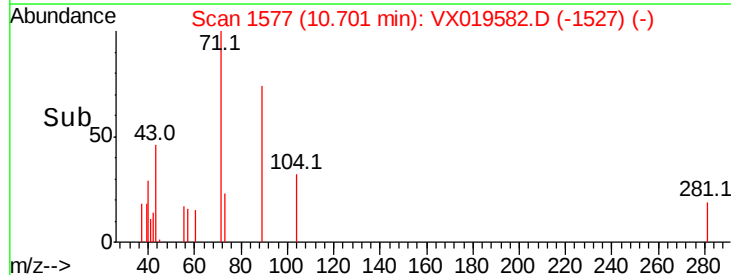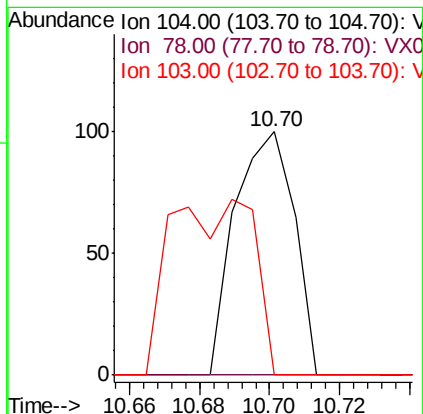



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP


Tot Ion:152 Resp: 186007

Ion Ratio Lower Upper

152 100

115 61.9 41.8 125.4




150 159.4 0.0 348.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

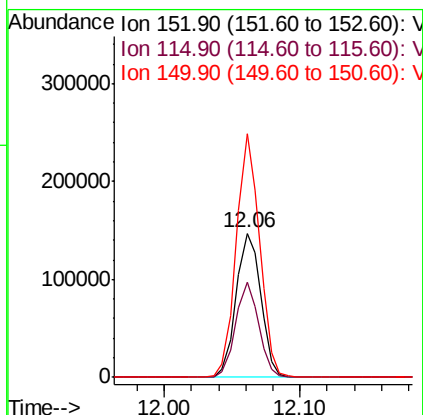

#74

N-ethyl acetate

Concen: 0.209 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Tgt Ion: 43 Resp: 1010


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 18.5 21.8 32.6#

61 0.0 22.2 33.4#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

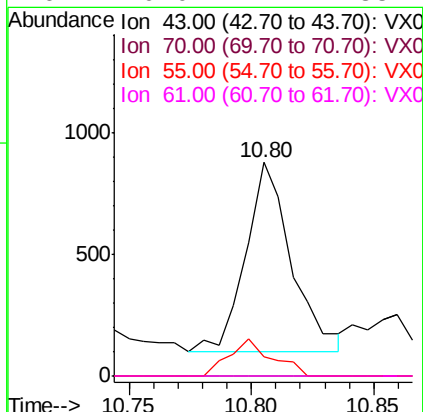

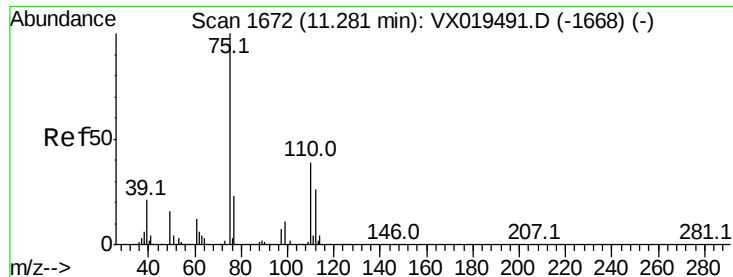

#76

1,2,3-Trichloropropane

Concen: 25.299 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :





TR5-1-TOP

Tot Ion: 75 Resp: 102695

Ion Ratio Lower Upper

75 100

77 1.3 20.0 60.0#

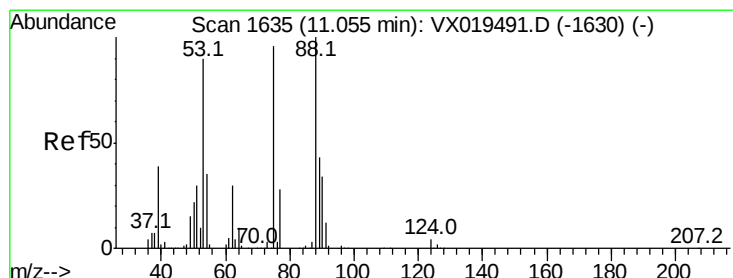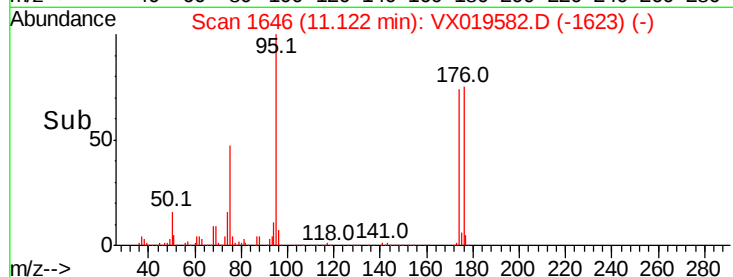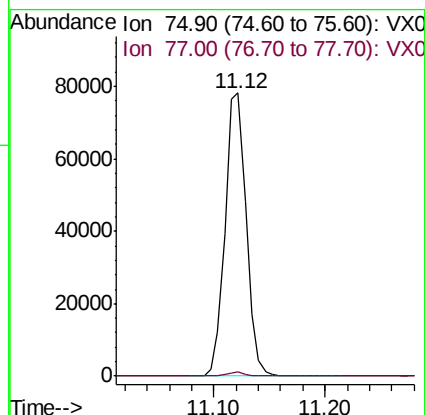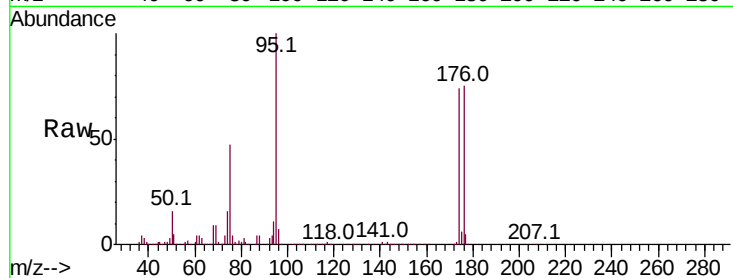

#81

trans-1,4-Dichloro-2-butene

Concen: 66.778 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18




Tgt Ion: 75 Resp: 102695


Ion Ratio Lower Upper

75 100

53 0.0 73.9 110.9#

89 0.0 37.3 55.9#

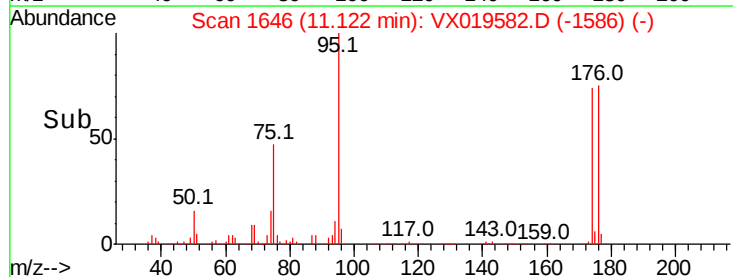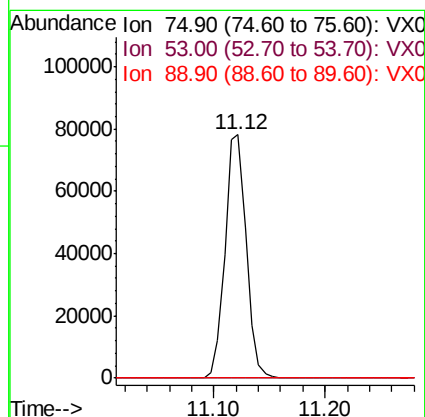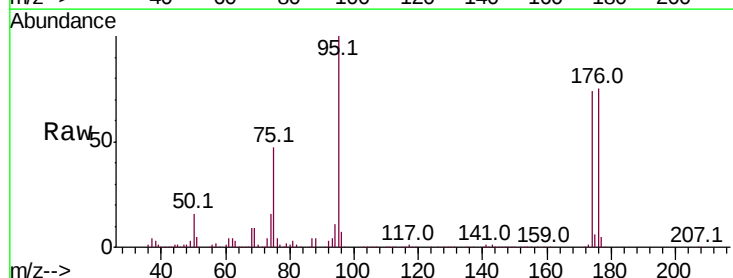

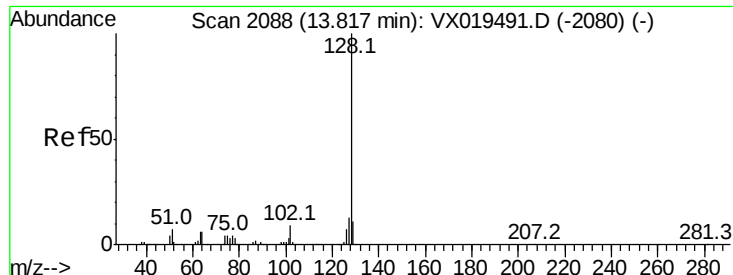

#95

Naphthalene

Concen: 2.198 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019582.D

Acq: 24 Nov 2020 04:18

Instrument :

MSVOA_X

ClientSampleId :

TR5-1-TOP

Tot Ion:128 Resp: 282

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.7 13.1#

