

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112320\
 Data File : VX019589.D
 Acq On : 24 Nov 2020 07:01
 Operator : JC/MD
 Sample : L4848-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-4-BOTTOM

Quant Time: Nov 24 08:09:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	322479	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.82	114	525500	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	454575	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	200348	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	199841	47.79	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.58%	
35) Dibromofluoromethane		5.46	113	157409	47.72	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.44%	
50) Toluene-d8		8.70	98	621405	48.48	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.96%	
62) 4-Bromofluorobenzene		11.12	95	210230	45.59	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.18%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Chloroethane	1.68	64	225	Below Cal	#	65
11) Tert butyl alcohol	3.04	59	977	1.235	ug/l #	92
13) Acrolein	2.28	56	172	0.323	ug/l #	47
16) Acetone	2.43	43	28796	17.809	ug/l	99
17) Carbon Disulfide	2.54	76	2592	0.301	ug/l #	95
18) Methyl Acetate	2.76	43	3022	1.387	ug/l	98
20) Methylene Chloride	2.83	84	42900	10.615	ug/l	95
25) 2-Butanone	4.65	43	5060	2.083	ug/l	94
29) Tetrahydrofuran	5.10	42	1732	1.118	ug/l #	82
31) Cyclohexane	5.62	56	6307	1.160	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	24293	4.931	ug/l #	49
38) Carbon Tetrachloride	5.62	117	31671	6.642	ug/l #	16
43) Isopropyl Acetate	6.42	43	22267	2.864	ug/l	100
44) Trichloroethene	7.18	130	2408	0.607	ug/l	95
48) Methyl methacrylate	7.66	41	5837	1.603	ug/l #	9
49) 1,4-Dioxane	7.84	88	64	0.774	ug/l #	1
51) 4-Methyl-2-Pentanone	8.60	43	78257	17.261	ug/l #	48
54) cis-1,3-Dichloropropene	8.59	75	41941	7.071	ug/l #	60
57) 1,3-Dichloropropane	9.52	76	18126	2.871	ug/l #	44
59) 2-Hexanone	9.42	43	14164	4.119	ug/l #	20
70) Styrene	10.70	104	126	1.657	ug/l #	81
74) N-amyl acetate	10.81	43	1187	0.229	ug/l #	44
76) 1,2,3-Trichloropropane	11.12	75	103288	23.623	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	103288	62.636	ug/l #	12
95) Naphthalene	13.82	128	338	2.200	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112320\
Data File : VX019589.D
Acq On : 24 Nov 2020 07:01
Operator : JC/MD
Sample : L4848-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR5-4-BOTTOM

Quant Time: Nov 24 08:09:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

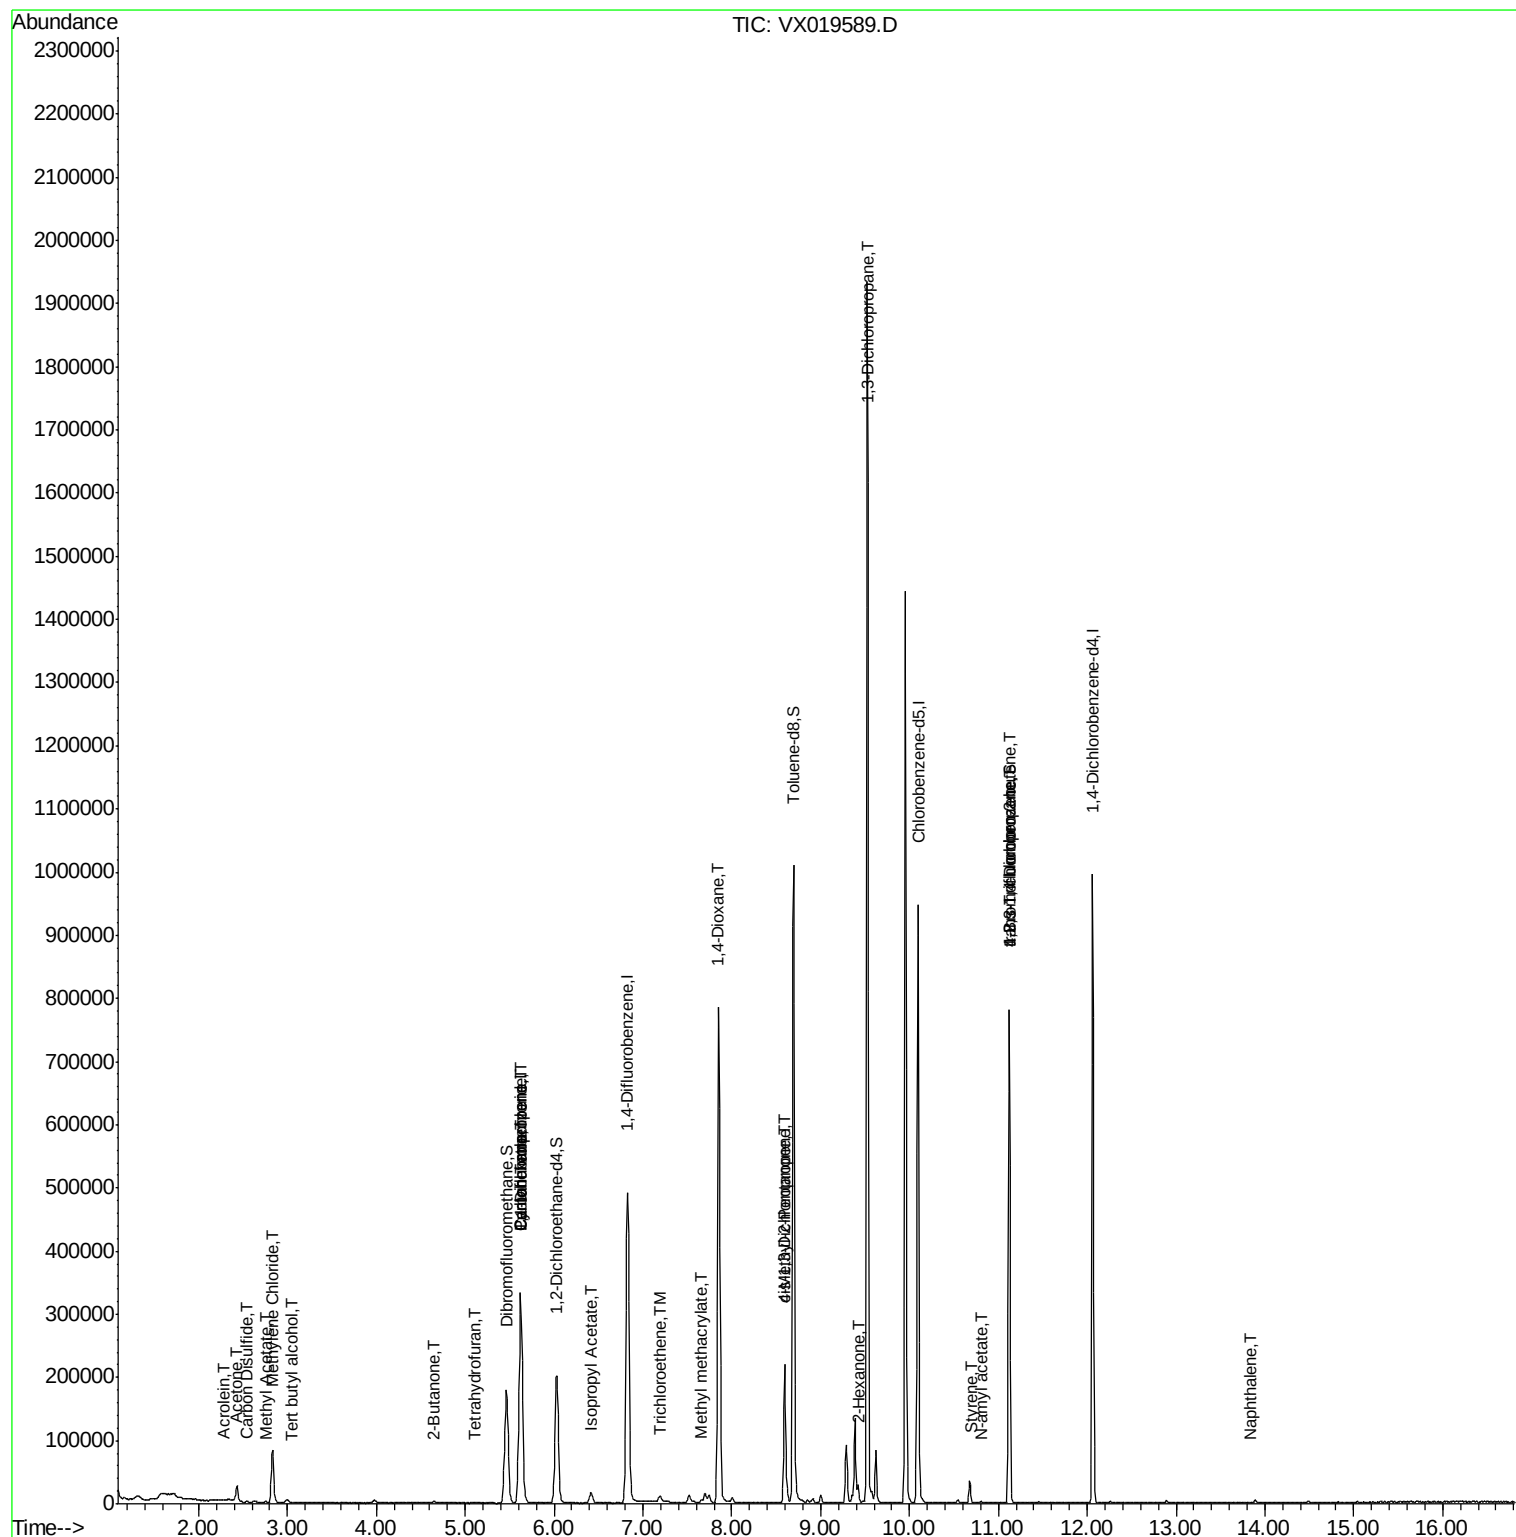



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :


TR5-4-BOTTOM

Tot Ion:168 Resp: 322479

Ion Ratio Lower Upper




168 100

99 54.1 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

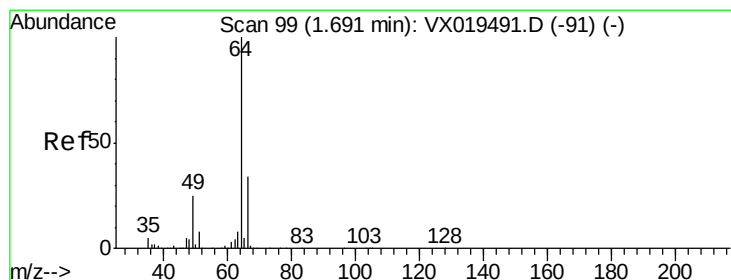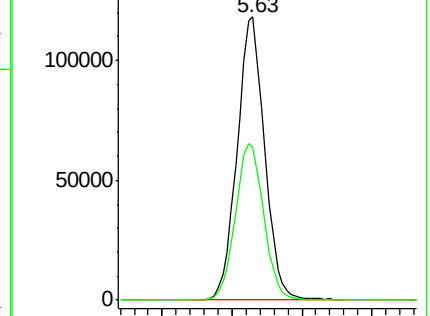

#6

Chloroethane

Concen: Below Cal

RT: 1.68 min Scan# 98

Delta R.T. -0.01 min

Lab File: VX019589.D


Acq: 24 Nov 2020 07:01

Tgt Ion: 64 Resp: 225

Ion Ratio Lower Upper



64 100


66 13.8 27.1 40.7#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

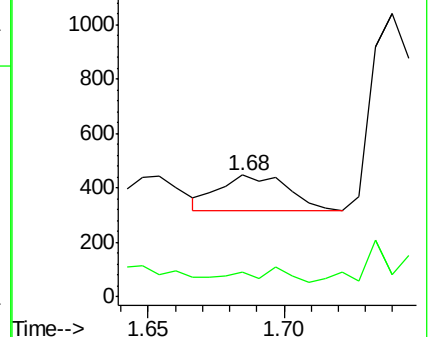



#11

Tert butyl alcohol

Concen: 1.235 ug/l

RT: 3.04 min Scan# 321

Delta R.T. -0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :





TR5-4-BOTTOM

Tot Ion: 59 Resp: 977

Ion Ratio Lower Upper

59 100

57 7.1 7.9 11.9#

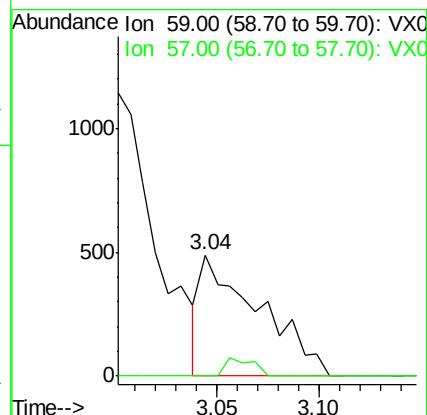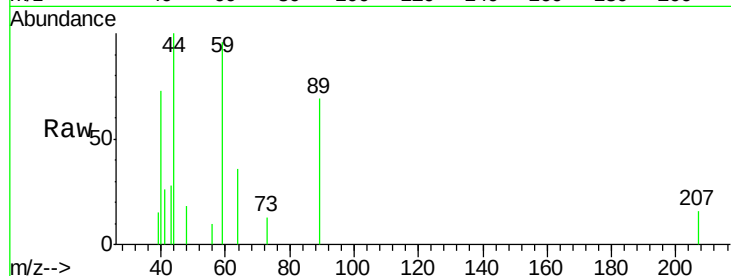

#13

Acrolein

Concen: 0.323 ug/l

RT: 2.28 min Scan# 195

Delta R.T. -0.00 min

Lab File: VX019589.D




Acq: 24 Nov 2020 07:01


Tgt Ion: 56 Resp: 172

Ion Ratio Lower Upper

56 100

55 26.2 55.5 83.3#

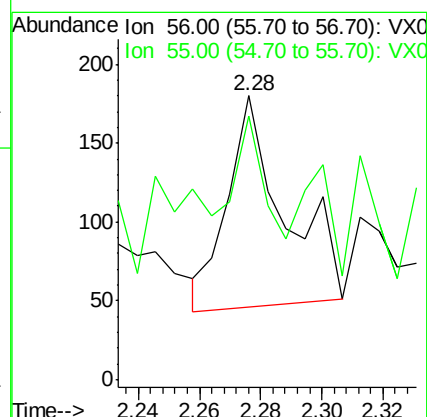



#16

Acetone

Concen: 17.809 ug/l

RT: 2.43 min Scan# 220

Delta R.T. 0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :





TR5-4-BOTTOM

Tot Ion: 43 Resp: 28796

Ion Ratio Lower Upper

43 100

58 34.8 27.4 41.2

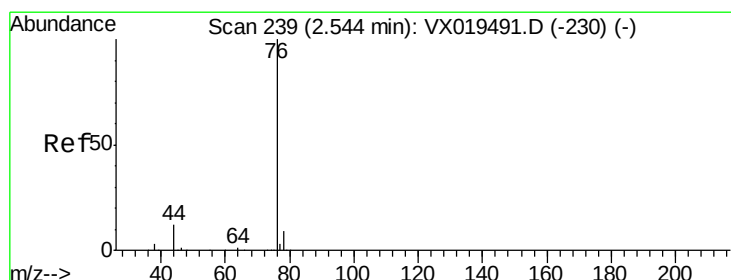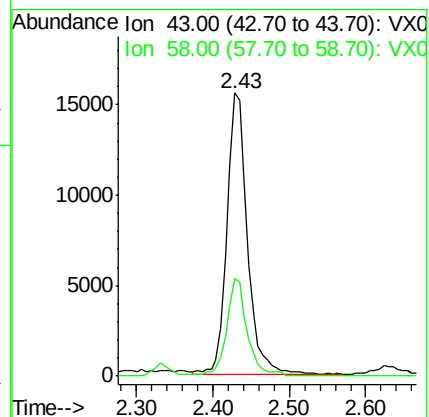

#17

Carbon Disulfide

Concen: 0.301 ug/l

RT: 2.54 min Scan# 238

Delta R.T. -0.01 min

Lab File: VX019589.D




Acq: 24 Nov 2020 07:01


Tgt Ion: 76 Resp: 2592

Ion Ratio Lower Upper

76 100

78 7.0 7.2 10.8#



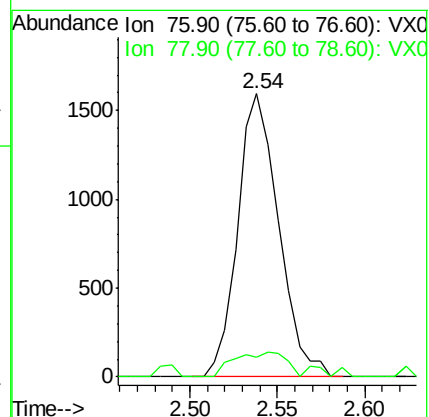





#18
Methyl Acetate
Concen: 1.387 ug/l
RT: 2.76 min Scan# 274
Delta R.T. 0.01 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01




Instrument :
MSVOA_X
ClientSampleId :
TR5-4-BOTTOM


Tot Ion: 43 Resp: 3022
Ion Ratio Lower Upper
43 100
74 26.6 22.2 33.4

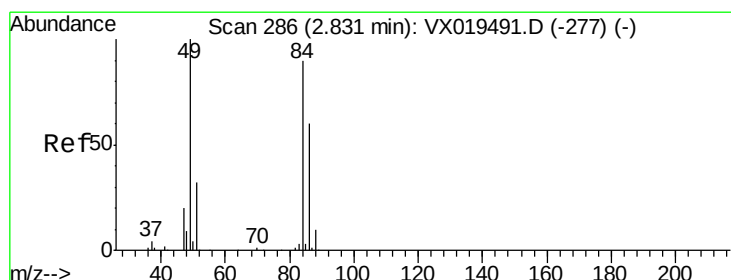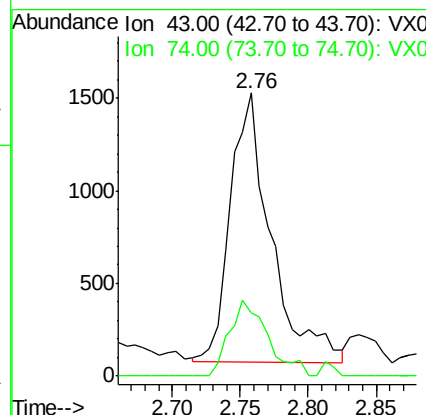

#20
Methylene Chloride
Concen: 10.615 ug/l
RT: 2.83 min Scan# 286
Delta R.T. 0.00 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01

Tgt Ion: 84 Resp: 42900
Ion Ratio Lower Upper
84 100
49 105.2 88.5 132.7
51 32.7 28.0 42.0
86 62.3 53.0 79.4

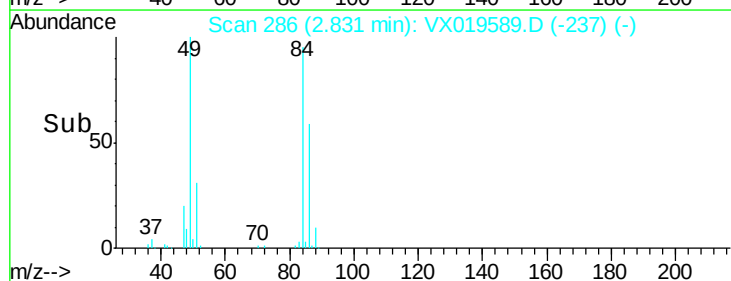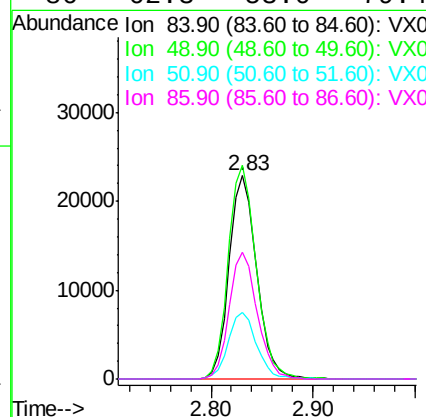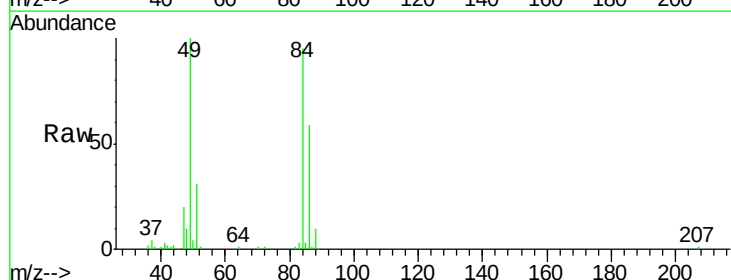



#25

2-Butanone

Concen: 2.083 ug/l

RT: 4.65 min Scan# 585

Delta R.T. 0.01 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :


TR5-4-BOTTOM

Tot Ion: 43 Resp: 5060

Ion Ratio Lower Upper




43 100

72 27.0 24.0 36.0

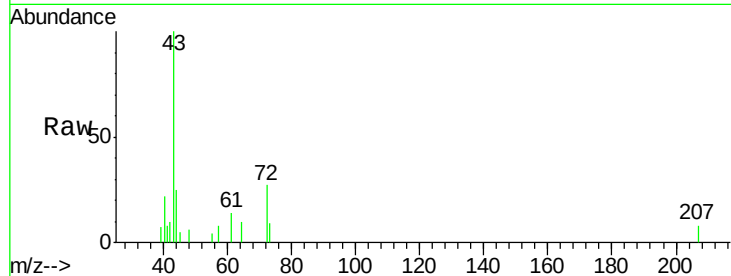

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

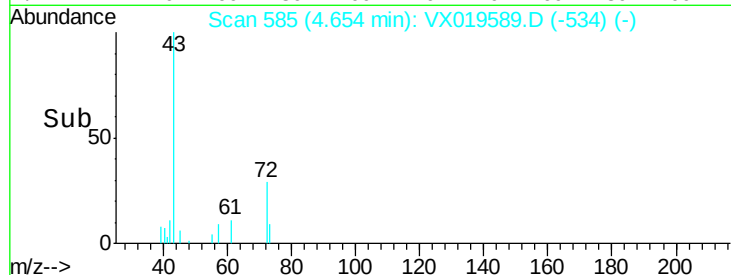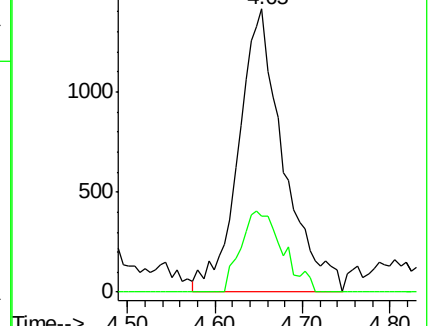

#29

Tetrahydrofuran

Concen: 1.118 ug/l

RT: 5.10 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01


Tgt Ion: 42 Resp: 1732

Ion Ratio Lower Upper

42 100

72 40.0 42.6 63.8#



71 37.2 39.0 58.6#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

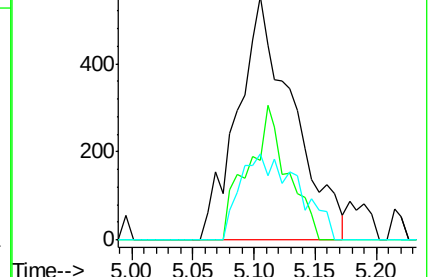

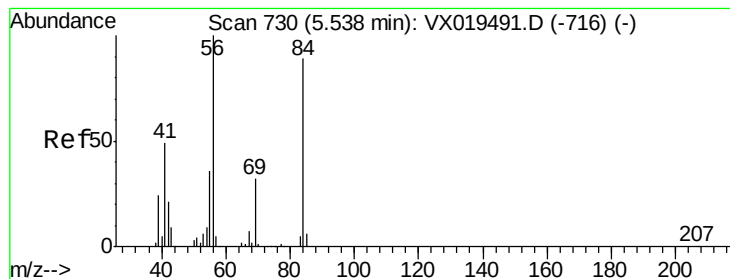

#31

Cyclohexane

Concen: 1.160 ug/l

RT: 5.62 min Scan# 743

Delta R.T. 0.08 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampled :

TR5-4-BOTTOM


Tot Ion: 56 Resp: 6307

Ion Ratio Lower Upper

56 100

69 162.2 25.5 38.3#




84 138.1 71.1 106.7#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

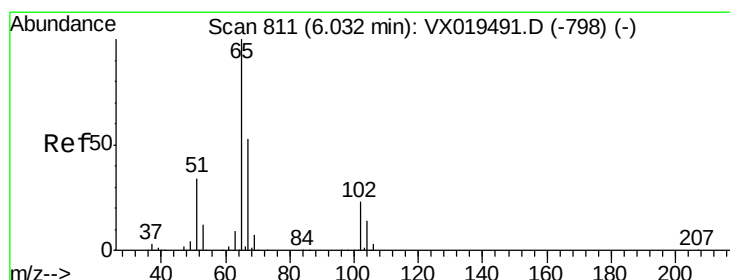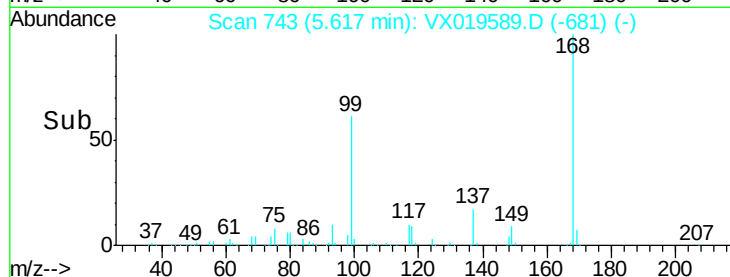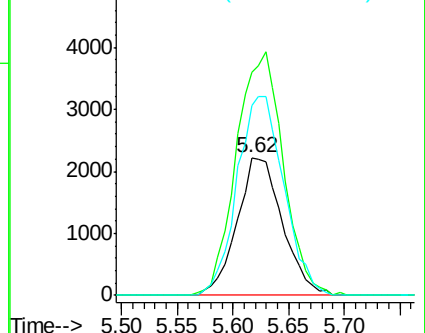

#33

1,2-Dichloroethane-d4

Concen: 47.795 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX019589.D


Acq: 24 Nov 2020 07:01

Tgt Ion: 65 Resp: 199841

Ion Ratio Lower Upper



65 100


67 51.7 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

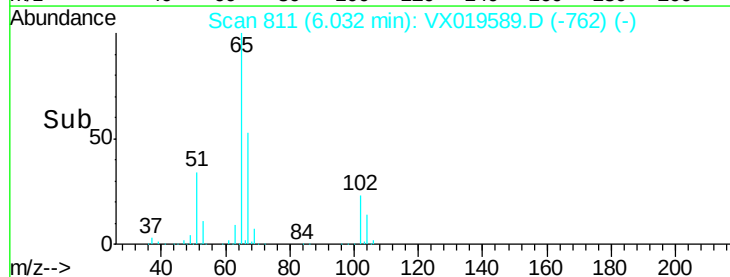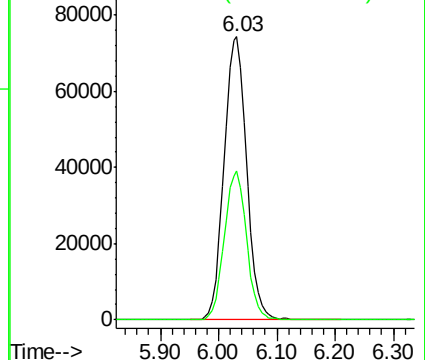



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.82 min Scan# 941

Delta R.T. -0.01 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :

TR5-4-BOTTOM


Tot Ion:114 Resp: 525500

Ion Ratio Lower Upper

114 100

63 20.4 0.0 38.8




88 15.5 0.0 31.6

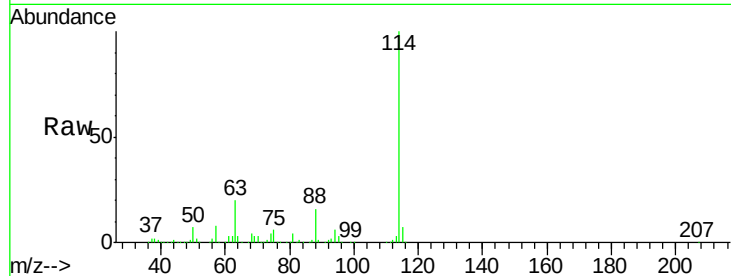

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

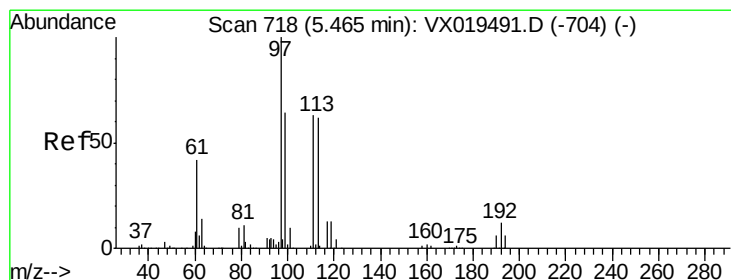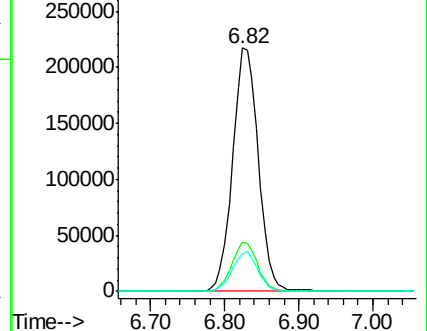

#35

Dibromofluoromethane

Concen: 47.720 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01


Tgt Ion:113 Resp: 157409

Ion Ratio Lower Upper

113 100

111 102.4 81.5 122.3



192 20.3 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

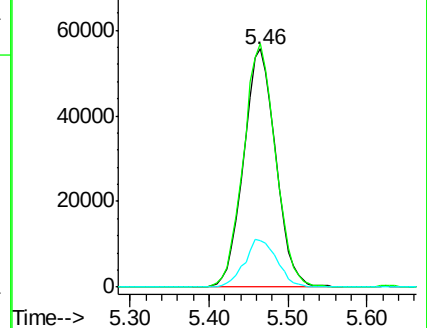







#36
 1,1-Dichloropropene
 Concen: 4.931 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX019589.D
 Acq: 24 Nov 2020 07:01

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-4-BOTTOM

Tot Ion: 75 Resp: 24293
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.1 54.3#
 77 0.0 24.2 36.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VX0


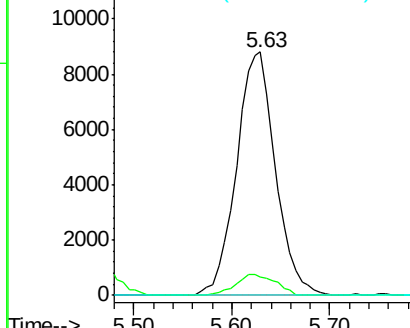



#38
 Carbon Tetrachloride
 Concen: 6.642 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.13 min
 Lab File: VX019589.D
 Acq: 24 Nov 2020 07:01

Tgt Ion: 117 Resp: 31671
 Ion Ratio Lower Upper
 117 100
 119 4.6 75.9 113.9#
 121 0.0 24.0 36.0#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

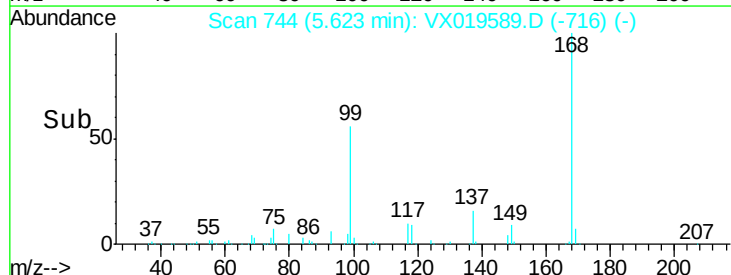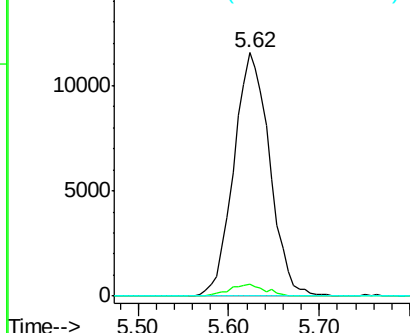

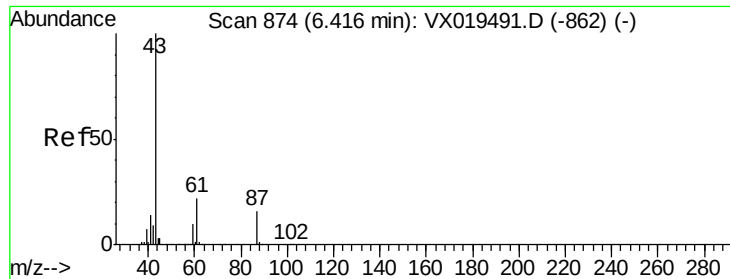

#43

Isopropyl Acetate

Concen: 2.864 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :

TR5-4-BOTTOM


Tot Ion: 43 Resp: 22267

Ion Ratio Lower Upper

43 100

61 22.7 18.2 27.2




87 15.8 12.6 18.8

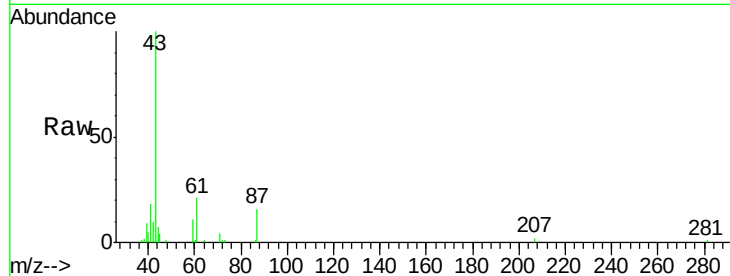

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

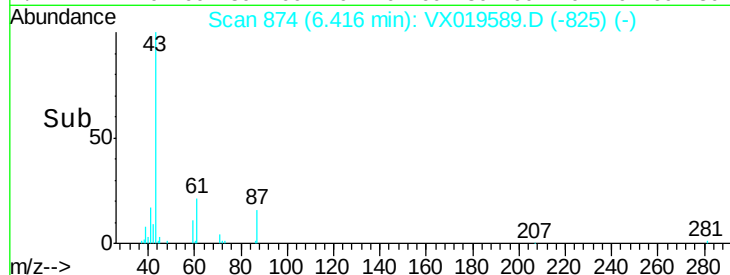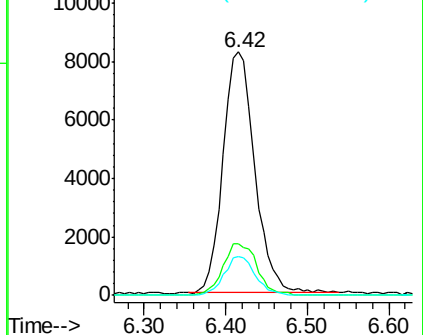

#44

Trichloroethene

Concen: 0.607 ug/l

RT: 7.18 min Scan# 1000

Delta R.T. -0.00 min

Lab File: VX019589.D


Acq: 24 Nov 2020 07:01

Tgt Ion: 130 Resp: 2408

Ion Ratio Lower Upper



130 100


95 100.9 0.0 191.2



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

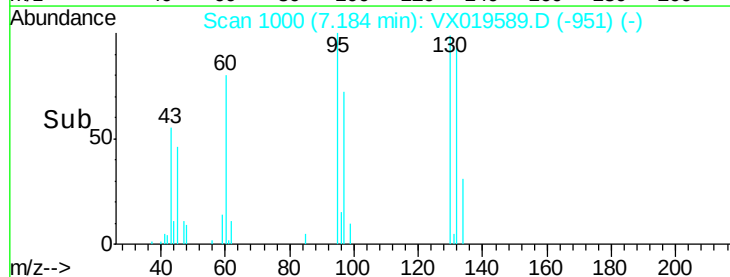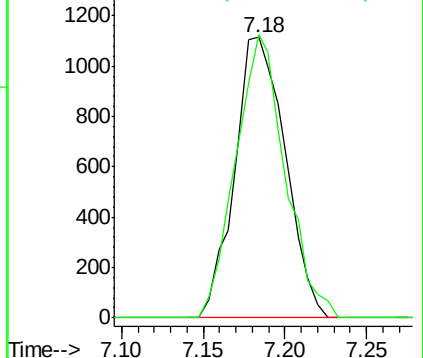

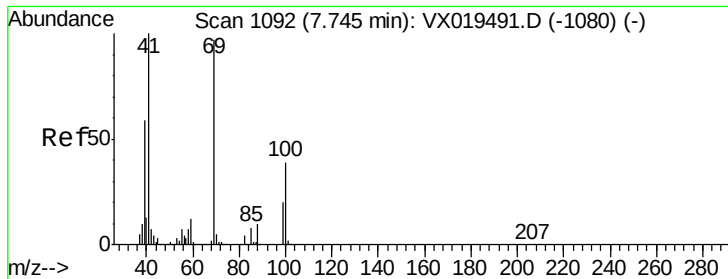

#48

Methvl methacrylate

Concen: 1.603 ug/l

RT: 7.66 min Scan# 1078

Delta R.T. -0.09 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :

TR5-4-BOTTOM


Tot Ion: 41 Resp: 5837

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#




39 0.0 45.6 68.4#

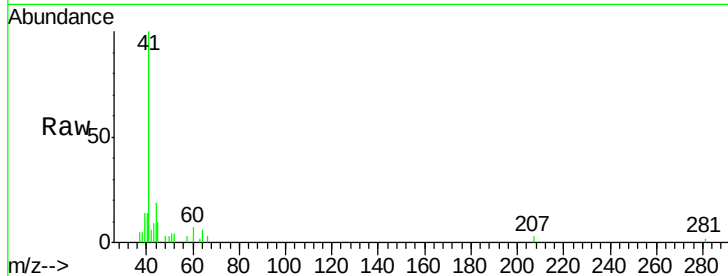

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

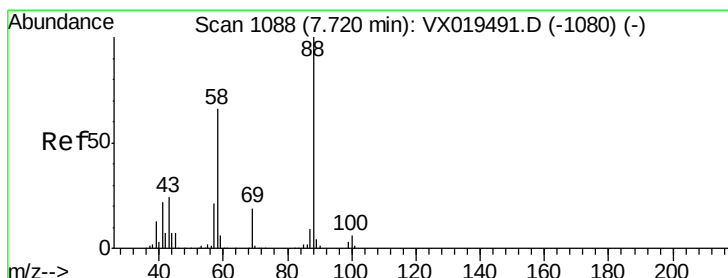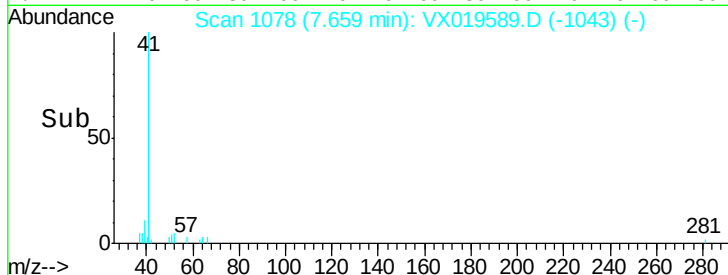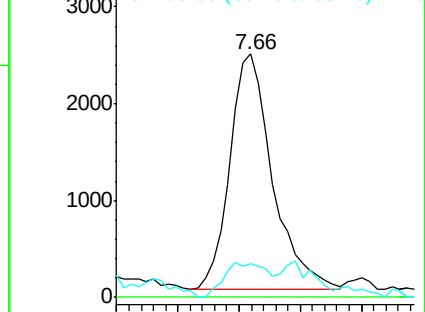

#49

1,4-Dioxane

Concen: 0.774 ug/l

RT: 7.84 min Scan# 1108

Delta R.T. 0.12 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01


Tgt Ion: 88 Resp: 64

Ion Ratio Lower Upper

88 100

43 1167834.4 23.8 35.6#



58 5690.6 54.2 81.2#

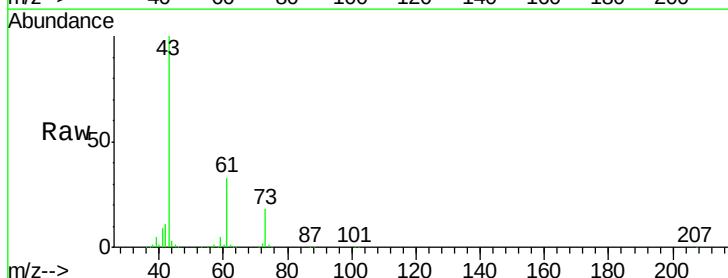


Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



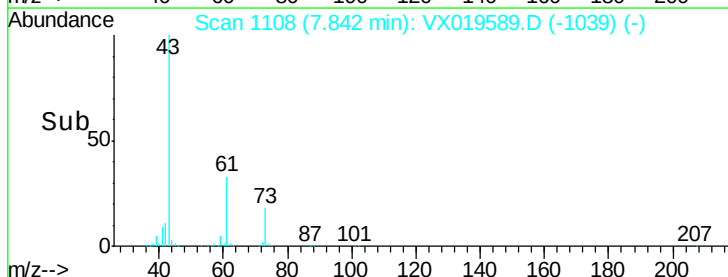
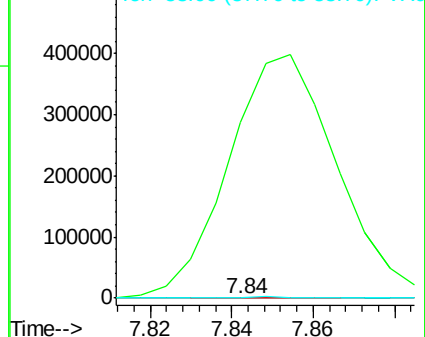


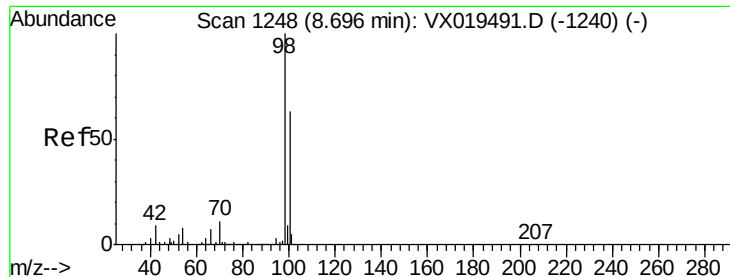

#50
Toluene-d8
Concen: 48.480 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. 0.00 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01




Instrument :
MSVOA_X
ClientSampleId :
TR5-4-BOTTOM


Tot Ion: 98 Resp: 621405
Ion Ratio Lower Upper
98 100
100 65.2 52.4 78.6

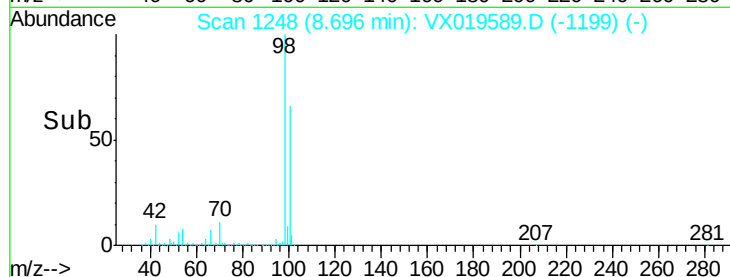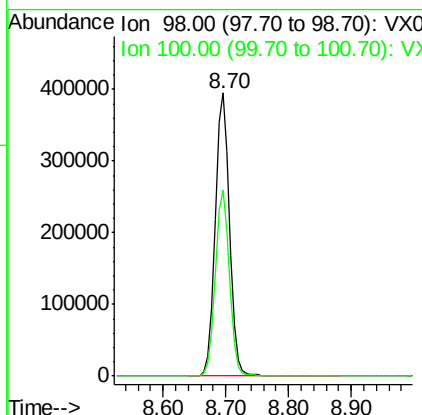

#51
4-Methyl-2-Pentanone
Concen: 17.261 ug/l
RT: 8.60 min Scan# 1232
Delta R.T. -0.02 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01

Tgt Ion: 43 Resp: 78257
Ion Ratio Lower Upper
43 100
58 10.0 35.1 52.7#

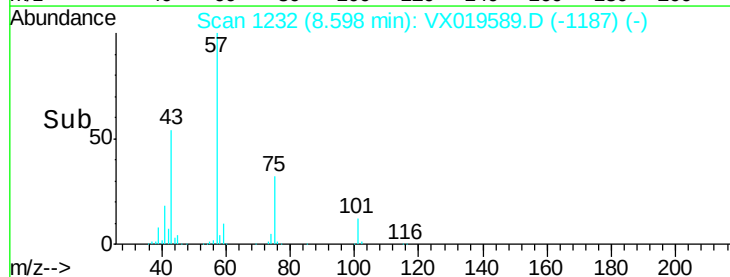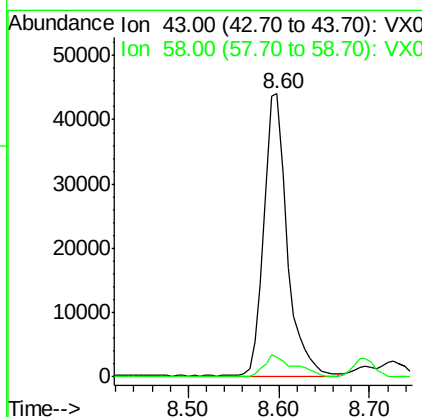







#54

cis-1,3-Dichloropropene
 Concen: 7.071 ug/l
 RT: 8.59 min Scan# 1231
 Delta R.T. 0.18 min
 Lab File: VX019589.D
 Acq: 24 Nov 2020 07:01

Instrument :
 MSVOA_X
 ClientSampleId :
 TR5-4-BOTTOM




Tot Ion	Ratio	Lower	Upper
75	100		
77	0.8	25.8	38.6#
39	24.8	34.6	51.8#

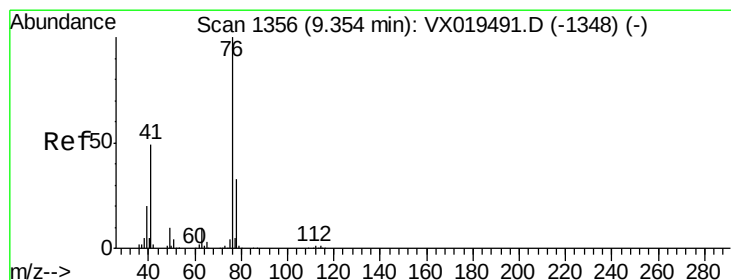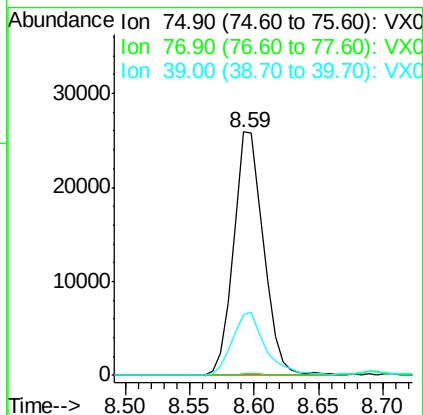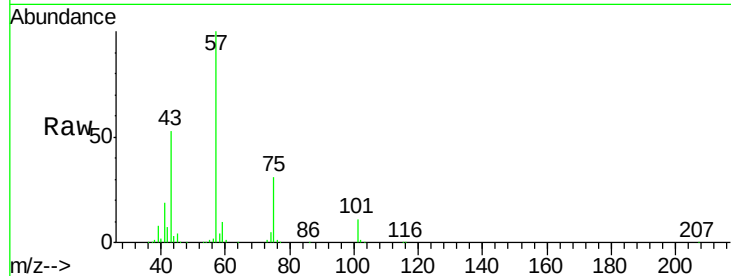


#57

1,3-Dichloropropane
 Concen: 2.871 ug/l
 RT: 9.52 min Scan# 1384
 Delta R.T. 0.17 min
 Lab File: VX019589.D
 Acq: 24 Nov 2020 07:01

Tgt Ion	Ratio	Lower	Upper
76	100		
78	1.0	25.7	38.5#


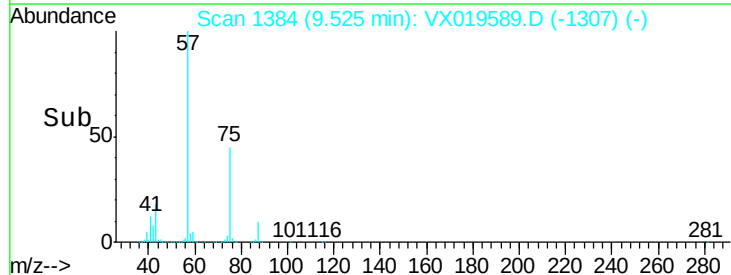
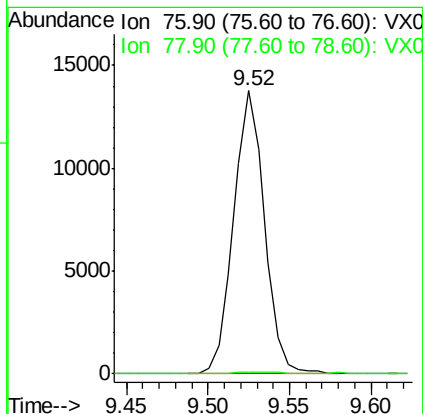





#59
2-Hexanone
Concen: 4.119 ug/l
RT: 9.42 min Scan# 1367
Delta R.T. -0.05 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01




Instrument :
MSVOA_X
ClientSampleId :
TR5-4-BOTTOM


Tot Ion: 43 Resp: 14164
Ion Ratio Lower Upper
43 100
58 0.0 30.6 91.6#

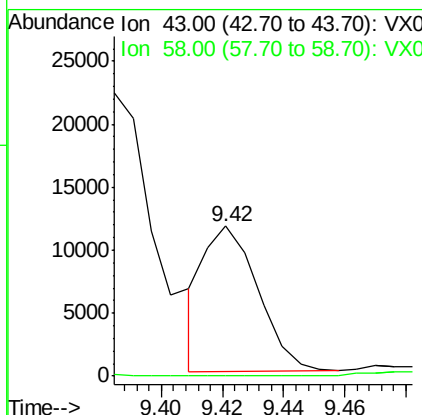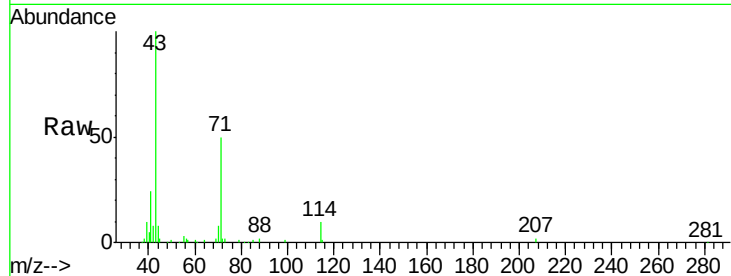

#62
4-Bromofluorobenzene
Concen: 45.586 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01

Tgt Ion: 95 Resp: 210230
Ion Ratio Lower Upper
95 100
174 77.7 0.0 156.2
176 74.3 0.0 151.4



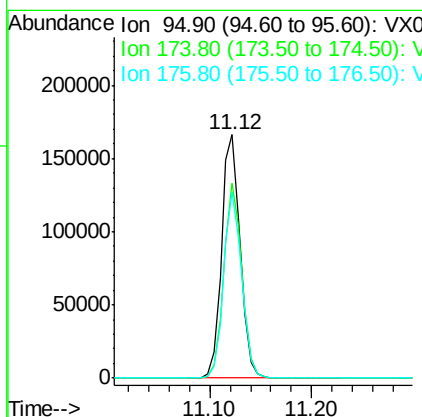





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01




Instrument :
MSVOA_X
ClientSampleId :
TR5-4-BOTTOM


Tot Ion:117 Resp: 454575
Ion Ratio Lower Upper
117 100
82 54.9 43.0 64.4
119 32.6 25.6 38.4

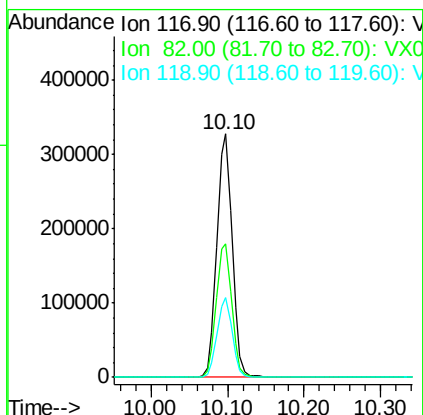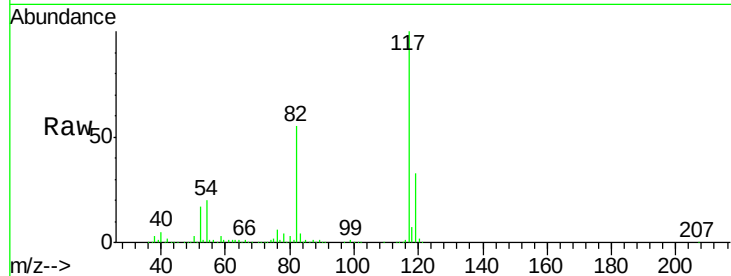

#70
Styrene
Concen: 1.657 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. 0.00 min
Lab File: VX019589.D
Acq: 24 Nov 2020 07:01

Tgt Ion:104 Resp: 126
Ion Ratio Lower Upper
104 100
78 34.1 39.5 59.3#
103 43.7 43.6 65.4

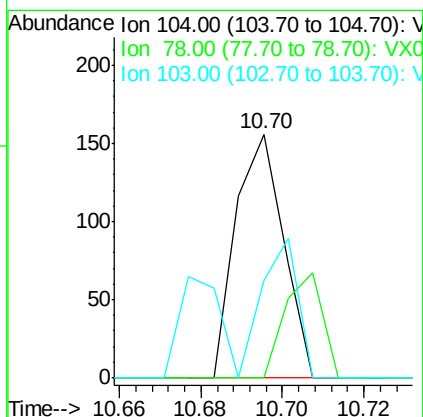

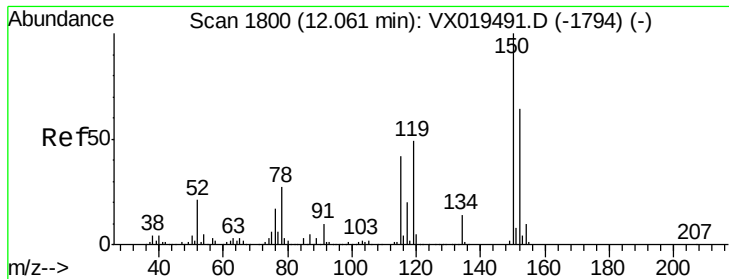

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. 0.00 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :

TR5-4-BOTTOM


Tot Ion:152 Resp: 200348

Ion Ratio Lower Upper

152 100

115 59.8 41.8 125.4




150 155.5 0.0 348.2

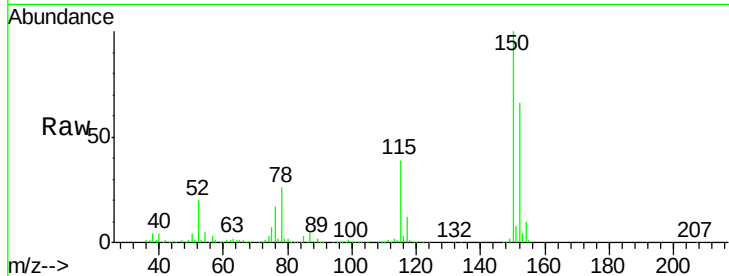

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

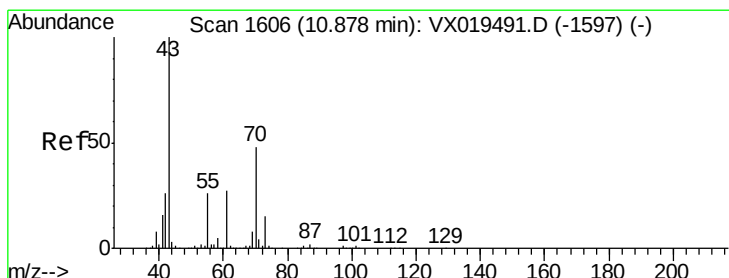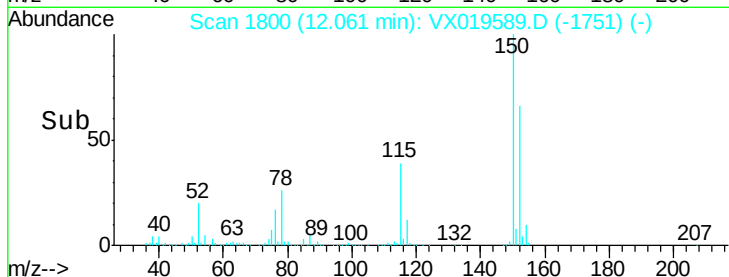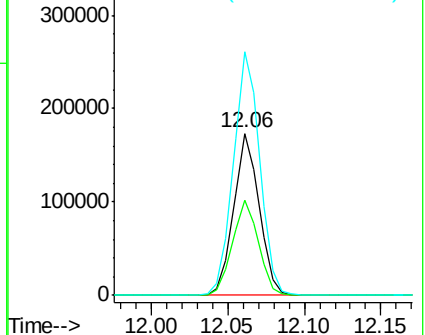

#74

N-ethyl acetate

Concen: 0.229 ug/l

RT: 10.81 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Tgt Ion: 43 Resp: 1187


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 12.6 21.8 32.6#

61 0.0 22.2 33.4#


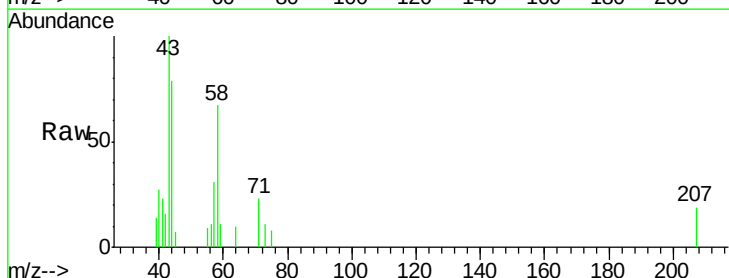



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

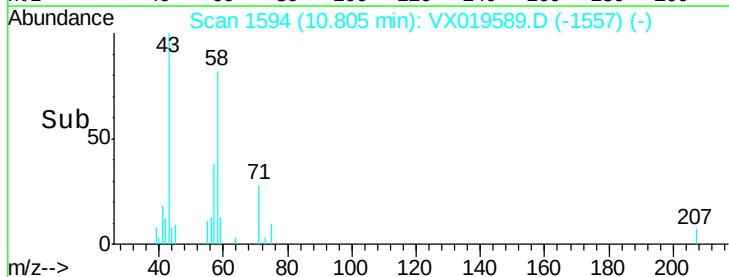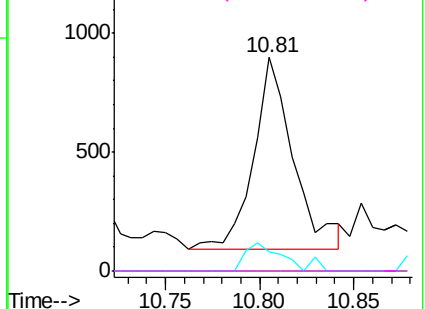

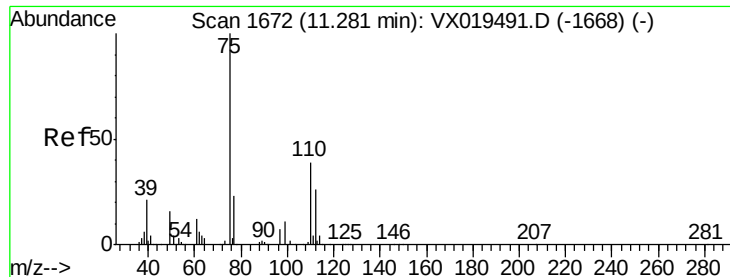

#76

1,2,3-Trichloropropane

Concen: 23.623 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :





TR5-4-BOTTOM

Tot Ion: 75 Resp: 103288

Ion Ratio Lower Upper

75 100

77 1.2 20.0 60.0#

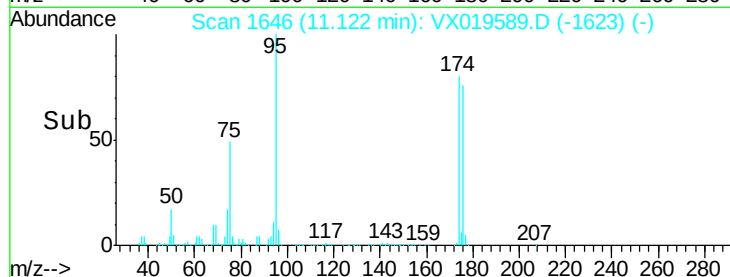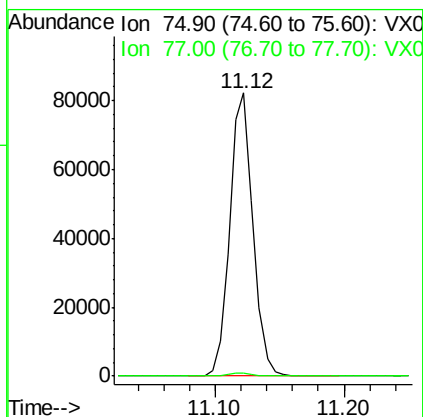

#81

trans-1,4-Dichloro-2-butene

Concen: 62.636 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01




Tgt Ion: 75 Resp: 103288




Ion Ratio Lower Upper

75 100

53 0.1 73.9 110.9#

89 0.0 37.3 55.9#

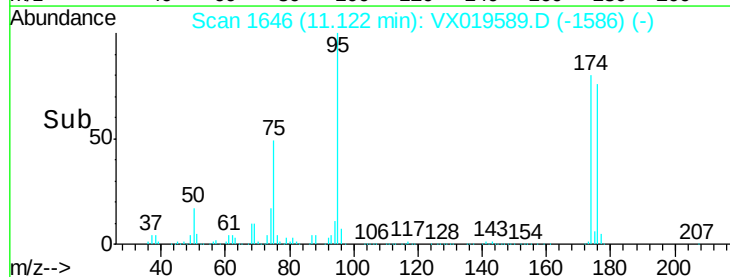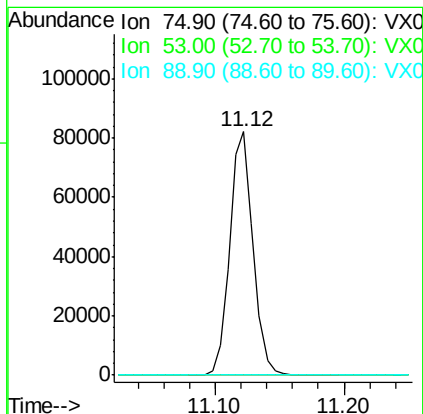

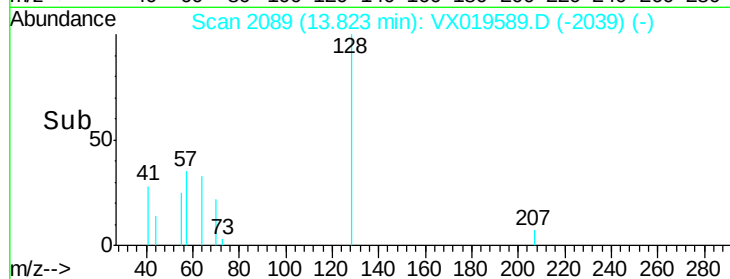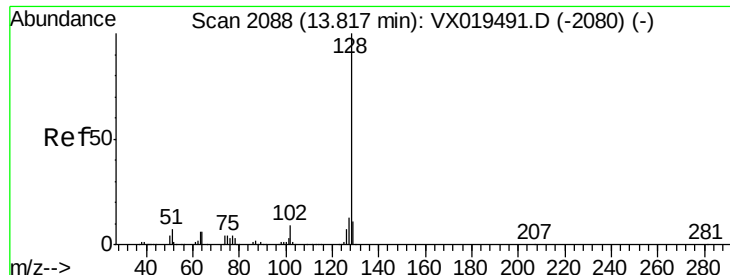

#95

Naphthalene

Concen: 2.200 ug/l

RT: 13.82 min Scan# 2089

Delta R.T. 0.01 min

Lab File: VX019589.D

Acq: 24 Nov 2020 07:01

Instrument :

MSVOA_X

ClientSampleId :

TR5-4-BOTTOM

Tot Ion:128 Resp: 338

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.7 13.1#

