

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
 Data File : VX025269.D
 Acq On : 23 Nov 2021 13:10
 Operator : JC/MD
 Sample : M4788-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-111921

Quant Time: Nov 23 15:21:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.555	168	98162	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	175465	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	169993	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	75177	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	58687	56.719	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 113.440%	
35) Dibromofluoromethane	5.391	113	57263	53.189	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.380%	
50) Toluene-d8	8.652	98	208132	51.418	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 102.840%	
62) 4-Bromofluorobenzene	11.085	95	78222	51.081	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.160%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
Data File : VX025269.D
Acq On : 23 Nov 2021 13:10
Operator : JC/MD
Sample : M4788-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-111921

Quant Time: Nov 23 15:21:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration




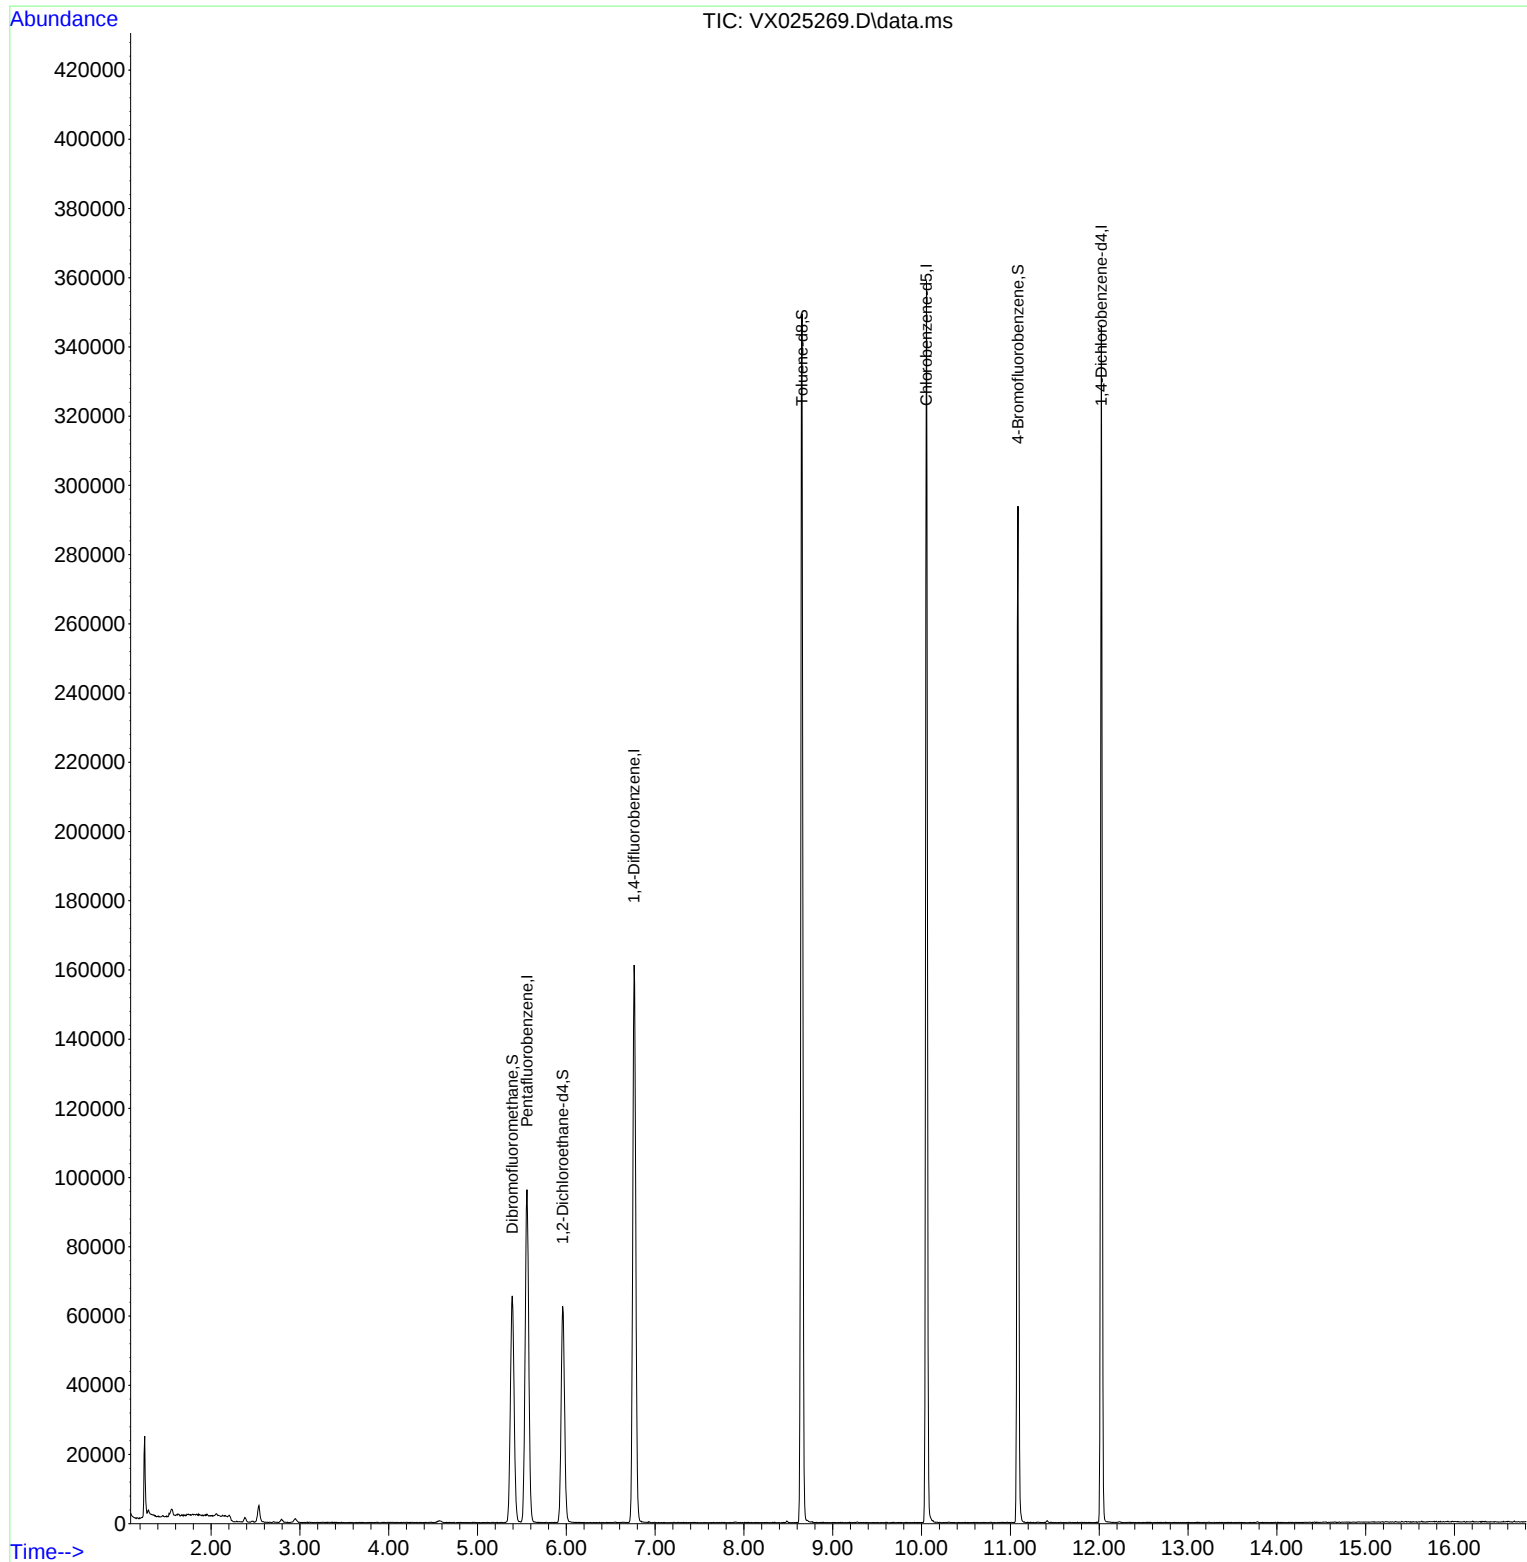


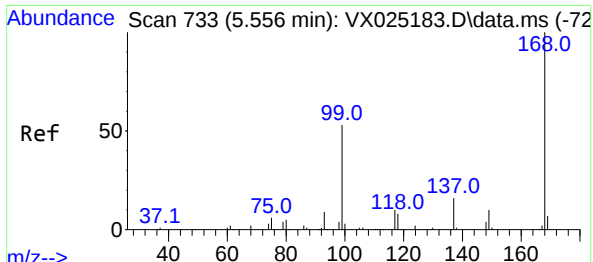

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.555 min Scan# 711
Delta R.T. -0.001 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10




Instrument :
MSVOA_X
ClientSampleId :
TB-01-111921


Tgt Ion:168 Resp: 98162
Ion Ratio Lower Upper
168 100
99 50.8 46.4 69.6

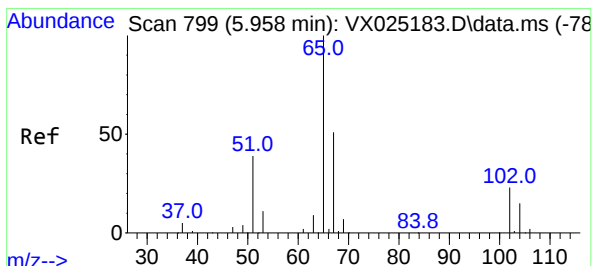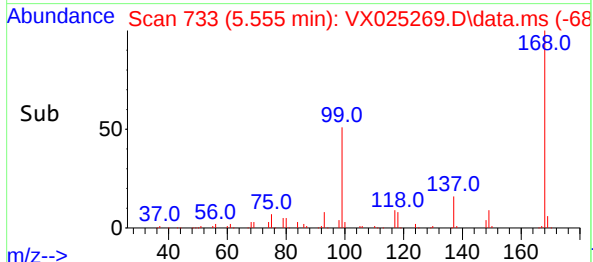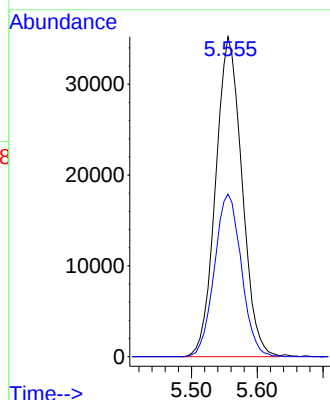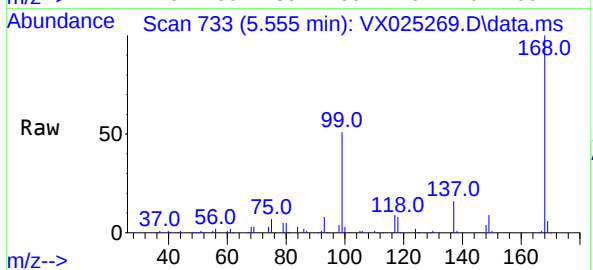

#33
1,2-Dichloroethane-d4
Concen: 56.719 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10

Tgt Ion: 65 Resp: 58687
Ion Ratio Lower Upper
65 100
67 52.3 0.0 101.0


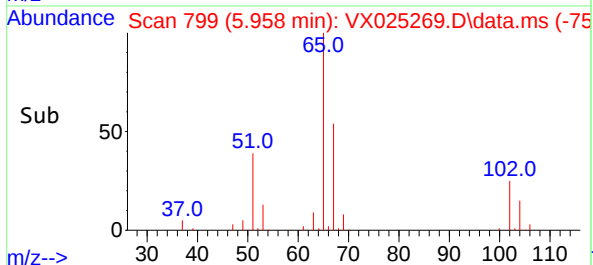
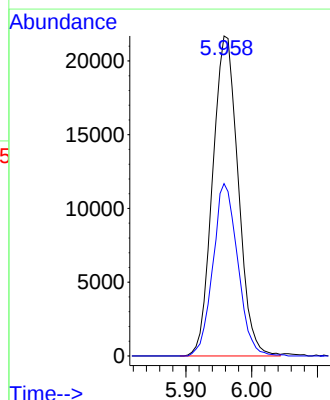
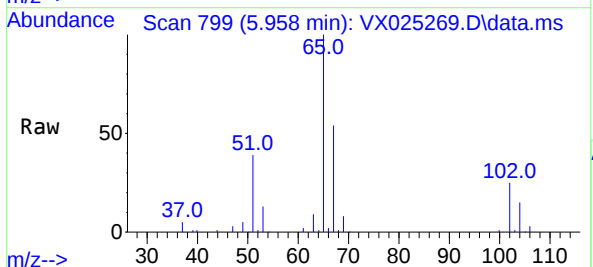


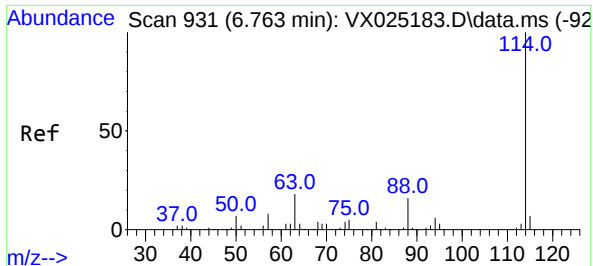

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10




Instrument :
MSVOA_X
ClientSampleId :
TB-01-111921


Tgt Ion:114 Resp: 175465
Ion Ratio Lower Upper
114 100
63 18.2 0.0 41.0
88 15.5 0.0 34.8

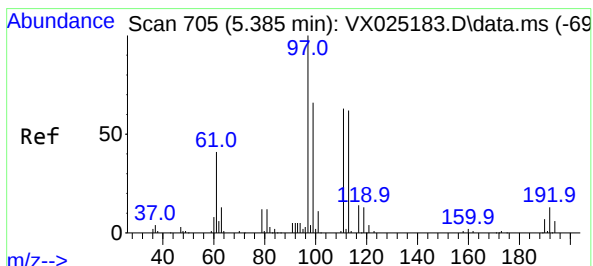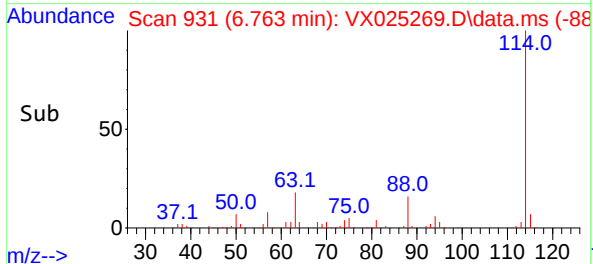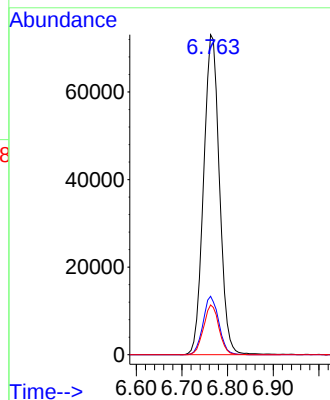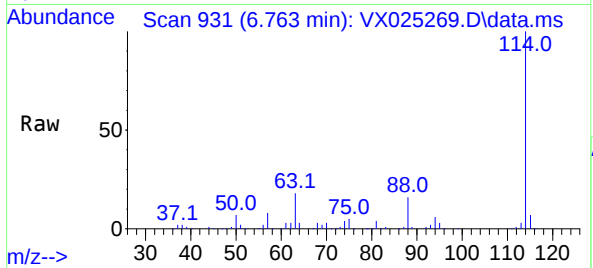

#35
Dibromofluoromethane
Concen: 53.189 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10

Tgt Ion:113 Resp: 57263
Ion Ratio Lower Upper
113 100
111 102.6 82.1 123.1
192 21.6 15.6 23.4


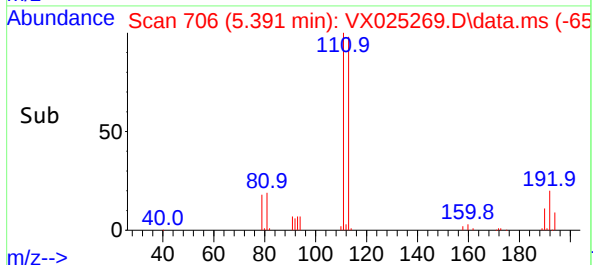
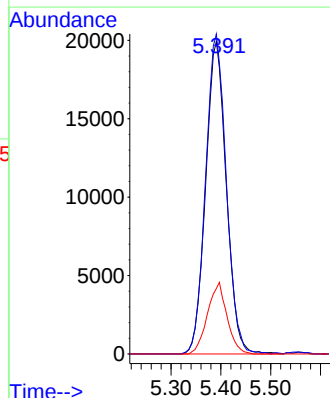
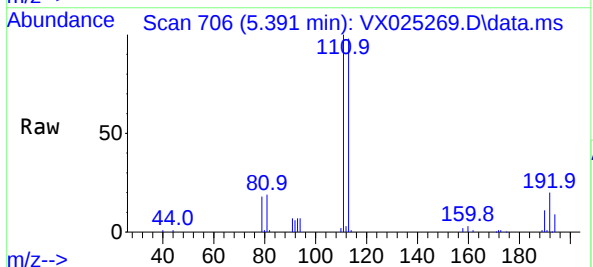


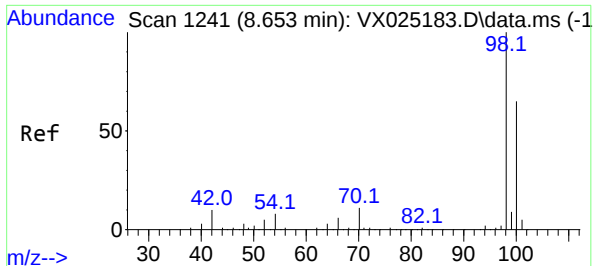

#50
Toluene-d8
Concen: 51.418 ug/l
RT: 8.652 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10




Instrument :
MSVOA_X
ClientSampleId :
TB-01-111921


Tgt Ion: 98 Resp: 208132
Ion Ratio Lower Upper
98 100
100 66.6 51.4 77.0

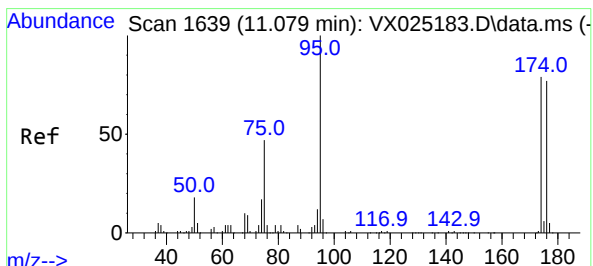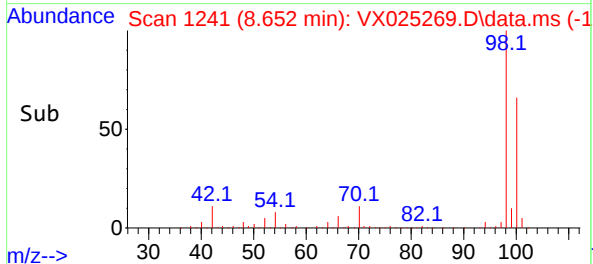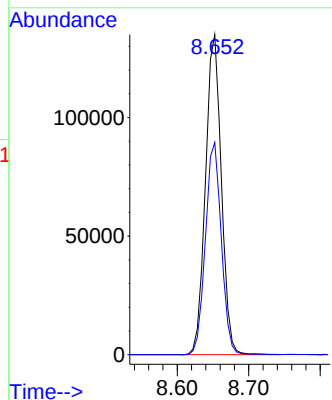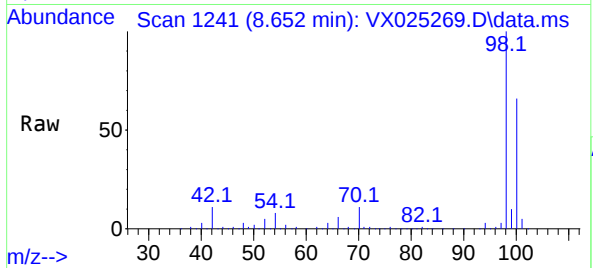

#62
4-Bromofluorobenzene
Concen: 51.081 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10

Tgt Ion: 95 Resp: 78222
Ion Ratio Lower Upper
95 100
174 86.1 0.0 158.0
176 83.2 0.0 153.6


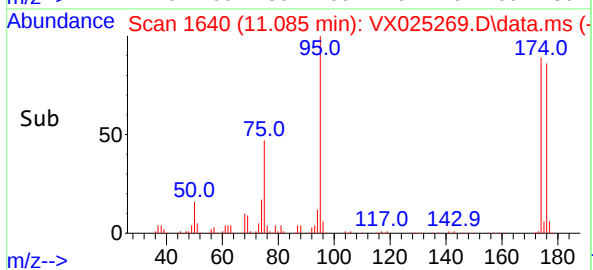
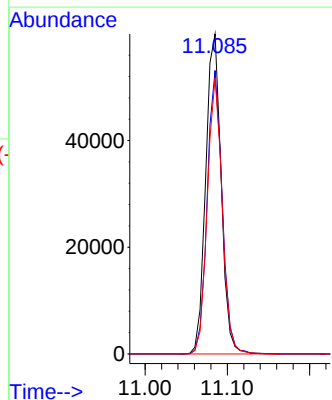
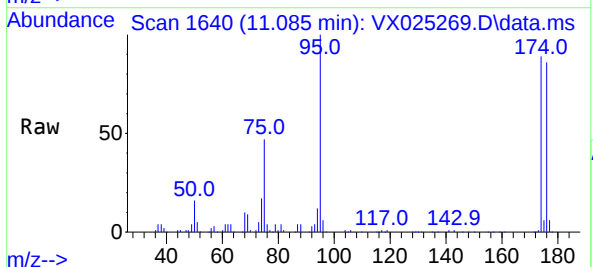


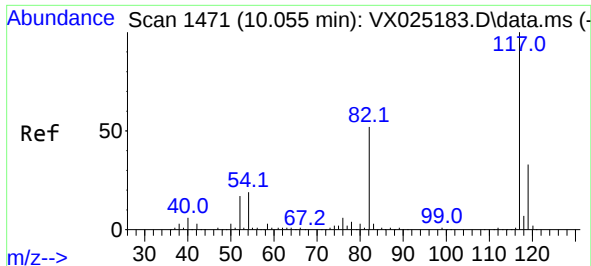

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10

Instrument :
MSVOA_X
ClientSampleId :
TB-01-111921

Tgt Ion:117 Resp: 169993
Ion Ratio Lower Upper
117 100
82 51.1 44.6 67.0
119 32.2 24.8 37.2

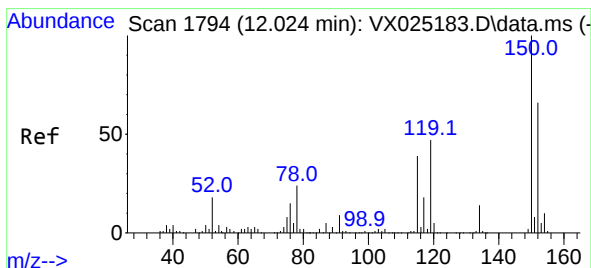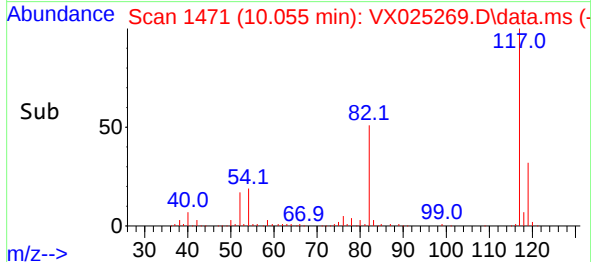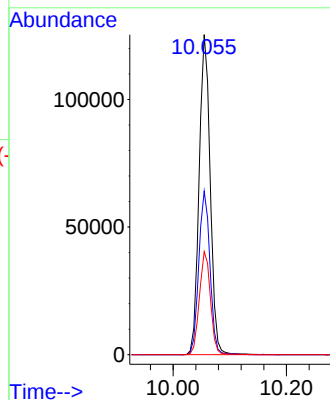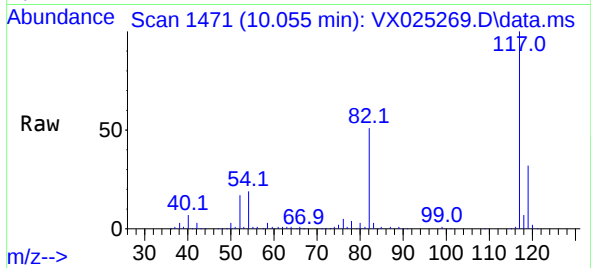

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX025269.D
Acq: 23 Nov 2021 13:10

Tgt Ion:152 Resp: 75177
Ion Ratio Lower Upper
152 100
115 56.0 43.3 129.8
150 156.0 0.0 351.2

