

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
 Data File : VX025284.D
 Acq On : 23 Nov 2021 19:01
 Operator : JC/MD
 Sample : M4809-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1994

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	35	rBV	30885	52359	9.95%	1.795%
2	2.532	230	237	245	rBV	6153	10868	2.06%	0.373%
3	5.391	693	706	720	rBV	63208	183109	34.79%	6.276%
4	5.556	722	733	749	rVB2	92399	258147	49.05%	8.848%
5	5.958	789	799	815	rBV	61783	163110	30.99%	5.591%
6	6.763	922	931	947	rBV	160402	373188	70.90%	12.792%
7	8.653	1234	1241	1250	rBV	329077	526329	100.00%	18.041%
8	9.574	1387	1392	1409	rBV	10506	33074	6.28%	1.134%
9	10.055	1465	1471	1487	rBV	351157	475148	90.28%	16.287%
10	11.085	1634	1640	1650	rBV	275614	372102	70.70%	12.754%
11	12.024	1789	1794	1802	rBV	352668	438156	83.25%	15.019%
12	12.226	1822	1827	1835	rBV	3068	5432	1.03%	0.186%
13	14.432	2185	2189	2200	rBV	20428	26402	5.02%	0.905%




Sum of corrected areas: 2917424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
Data File : VX025284.D
Acq On : 23 Nov 2021 19:01
Operator : JC/MD
Sample : M4809-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1994

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

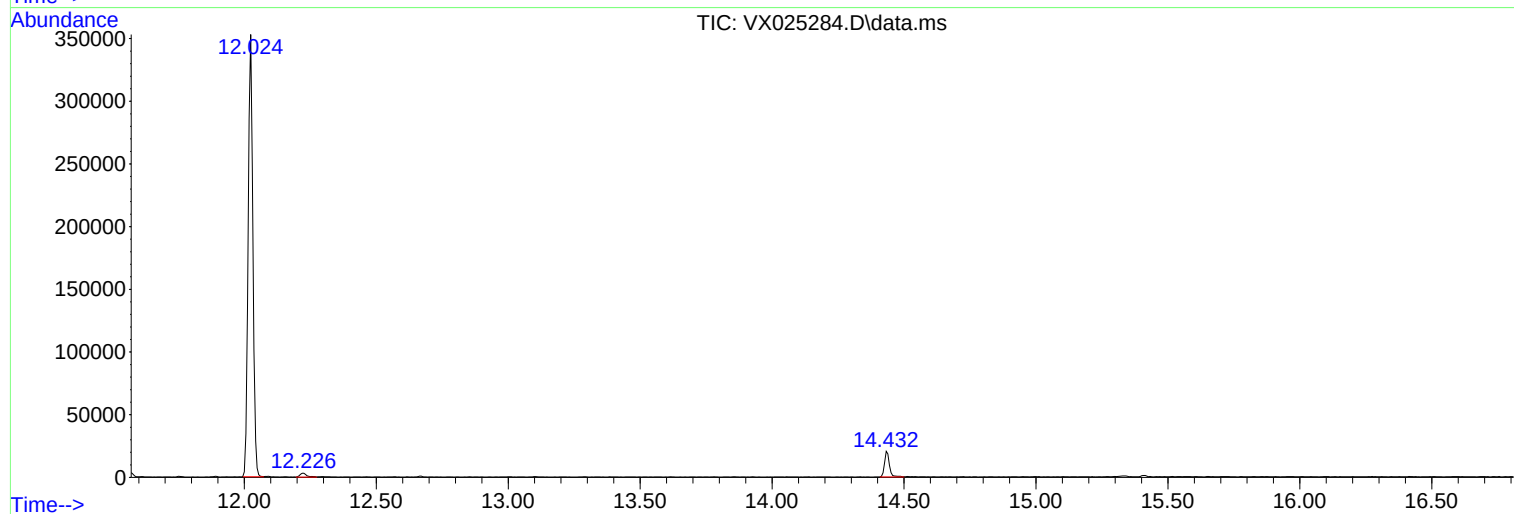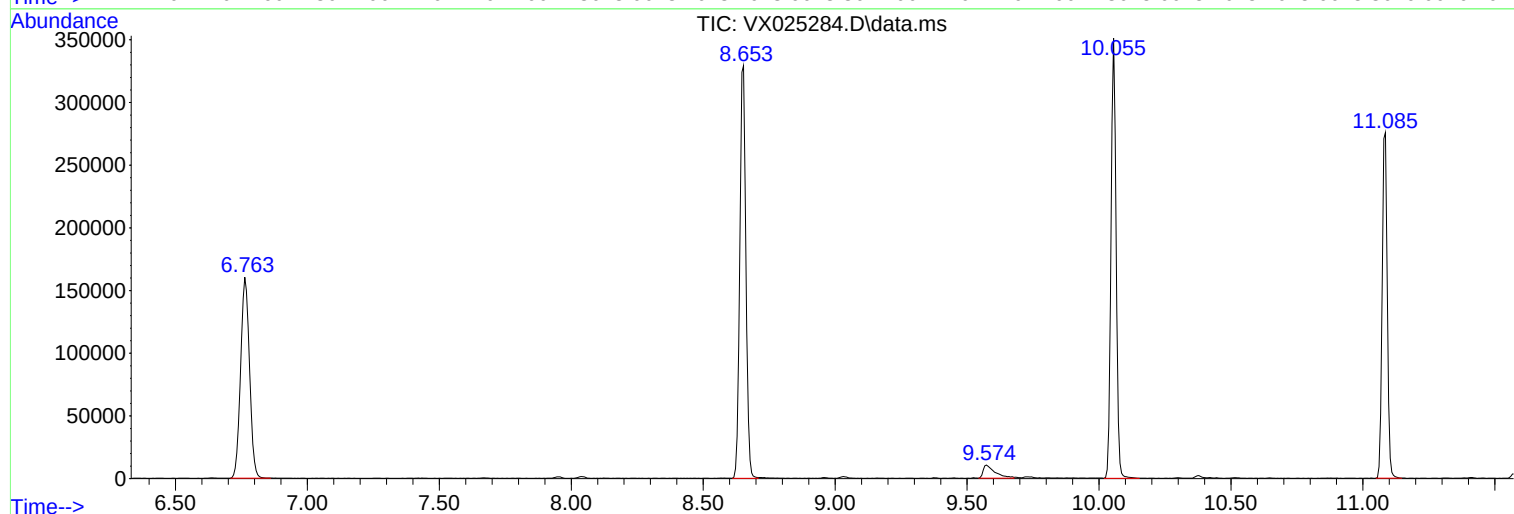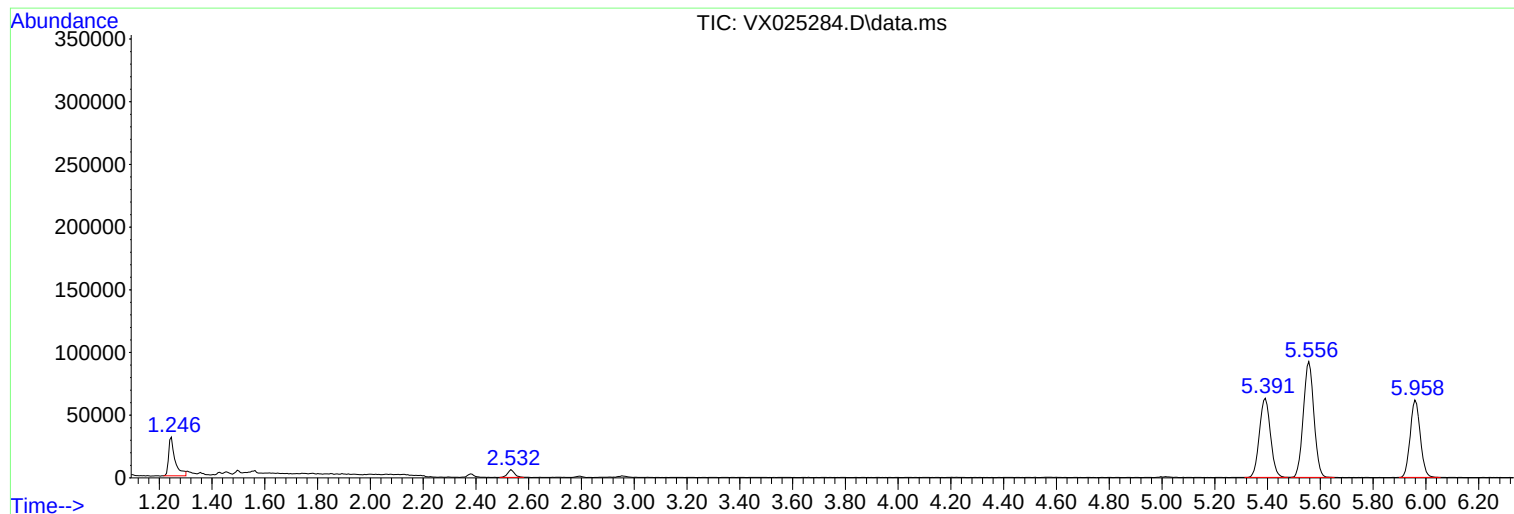

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
Data File : VX025284.D
Acq On : 23 Nov 2021 19:01
Operator : JC/MD
Sample : M4809-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1994










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	10.14 ug/l	52359	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

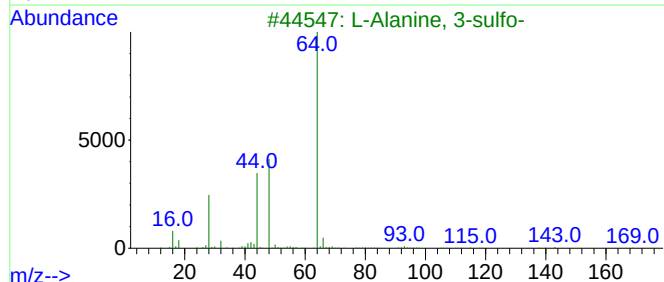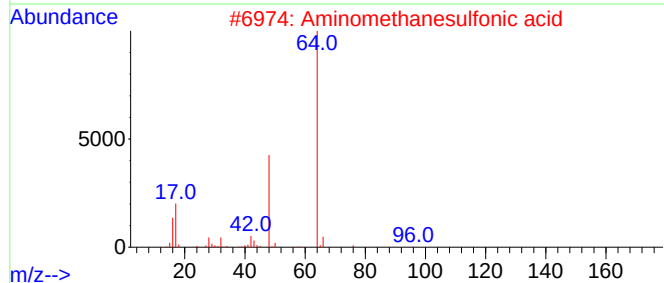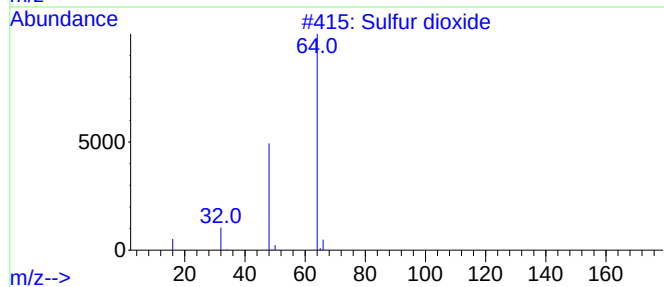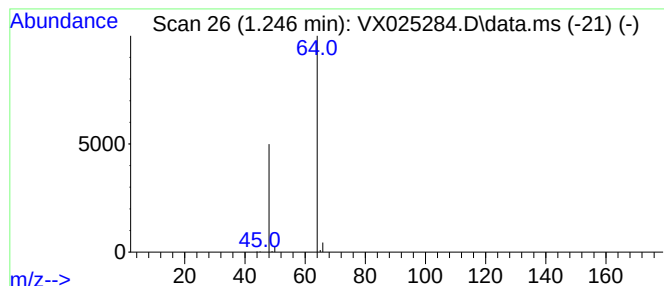

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112321\
Data File : VX025284.D
Acq On : 23 Nov 2021 19:01
Operator : JC/MD
Sample : M4809-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1994

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	10.1	ug/l	52359	1	5.556	258147	50.0