

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033046.D
 Acq On : 24 Nov 2022 07:59
 Operator : JC/MD
 Sample : N5741-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40

Quant Time: Nov 25 06:38:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 22 13:58:46 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	129620	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	212701	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	189738	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	89077	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	70553	56.085	ug/l	0.00
Spiked Amount 50.000	Range	78 - 117	Recovery	=	112.160%	
35) Dibromofluoromethane	5.385	113	56861	47.419	ug/l	0.00
Spiked Amount 50.000	Range	75 - 124	Recovery	=	94.840%	
50) Toluene-d8	8.647	98	193169	53.699	ug/l	0.00
Spiked Amount 50.000	Range	92 - 112	Recovery	=	107.400%	
62) 4-Bromofluorobenzene	11.079	95	70314	44.639	ug/l	0.00
Spiked Amount 50.000	Range	83 - 123	Recovery	=	89.280%	
Target Compounds						Qvalue
3) Chloromethane	1.246	50	7221	6.755	ug/l #	43
6) Chloroethane	1.886	64	941	0.971	ug/l #	53
11) Tert butyl alcohol	2.995	59	97062	485.067	ug/l	100
13) Acrolein	2.215	56	141	0.613	ug/l #	1
14) Allyl chloride	2.751	41	545	0.298	ug/l #	1
15) Acrylonitrile	3.105	53	691	1.221	ug/l #	25
16) Acetone	2.392	43	789	1.338	ug/l #	83
17) Carbon Disulfide	2.514	76	978	0.313	ug/l #	74
18) Methyl Acetate	2.776	43	444	0.272	ug/l #	51
19) Methyl tert-butyl Ether	3.111	73	53483	13.633	ug/l #	90
20) Methylene Chloride	2.776	84	116	Below Cal	#	5
22) Diisopropyl ether	3.757	45	27596	6.940	ug/l #	86
23) Vinyl Acetate	3.757	43	15208	4.886	ug/l #	72
29) Tetrahydrofuran	5.019	42	113	0.219	ug/l #	31
31) Cyclohexane	5.464	56	2173	1.062	ug/l	95
36) 1,1-Dichloropropene	5.550	75	9849	5.137	ug/l #	50
38) Carbon Tetrachloride	5.556	117	13549	6.370	ug/l #	16
39) Methylcyclohexane	7.385	83	1506	0.688	ug/l	97
40) Benzene	6.037	78	672903	125.172	ug/l	100
42) 1,2-Dichloroethane	6.043	62	6210	2.869	ug/l #	77
43) Isopropyl Acetate	6.251	43	1929	0.697	ug/l #	61
52) Toluene	8.720	92	2547	0.720	ug/l	93
59) 2-Hexanone	9.451	43	2844	2.255	ug/l	97
67) Ethyl Benzene	10.195	91	5998	0.894	ug/l	94
68) m/p-Xylenes	10.305	106	1809	0.688	ug/l	99
69) o-Xylene	10.640	106	2669	1.050	ug/l	95
73) Isopropylbenzene	10.963	105	6092	0.957	ug/l	98
74) N-amyl acetate	10.854	43	459	0.212	ug/l #	56
76) 1,2,3-Trichloropropane	11.079	75	38116	22.594	ug/l #	37
78) n-propylbenzene	11.305	91	1458	0.200	ug/l	97
80) 1,3,5-Trimethylbenzene	11.451	105	3362	0.629	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	38116	73.442	ug/l #	6
84) 1,2,4-Trimethylbenzene	11.750	105	6060	1.137	ug/l	98
85) sec-Butylbenzene	11.896	105	1661	0.261	ug/l	88
86) p-Isopropyltoluene	12.177	119	1216	0.225	ug/l	96
90) Hexachloroethane	12.615	117	255	0.288	ug/l #	12

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033046.D
Acq On : 24 Nov 2022 07:59
Operator : JC/MD
Sample : N5741-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Quant Time: Nov 25 06:38:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
92) 1,2-Dibromo-3-Chloropr...	12.695	75	121	0.316	ug/l #	1
95) Naphthalene	13.780	128	1366	0.240	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033046.D
Acq On : 24 Nov 2022 07:59
Operator : JC/MD
Sample : N5741-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Quant Time: Nov 25 06:38:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration




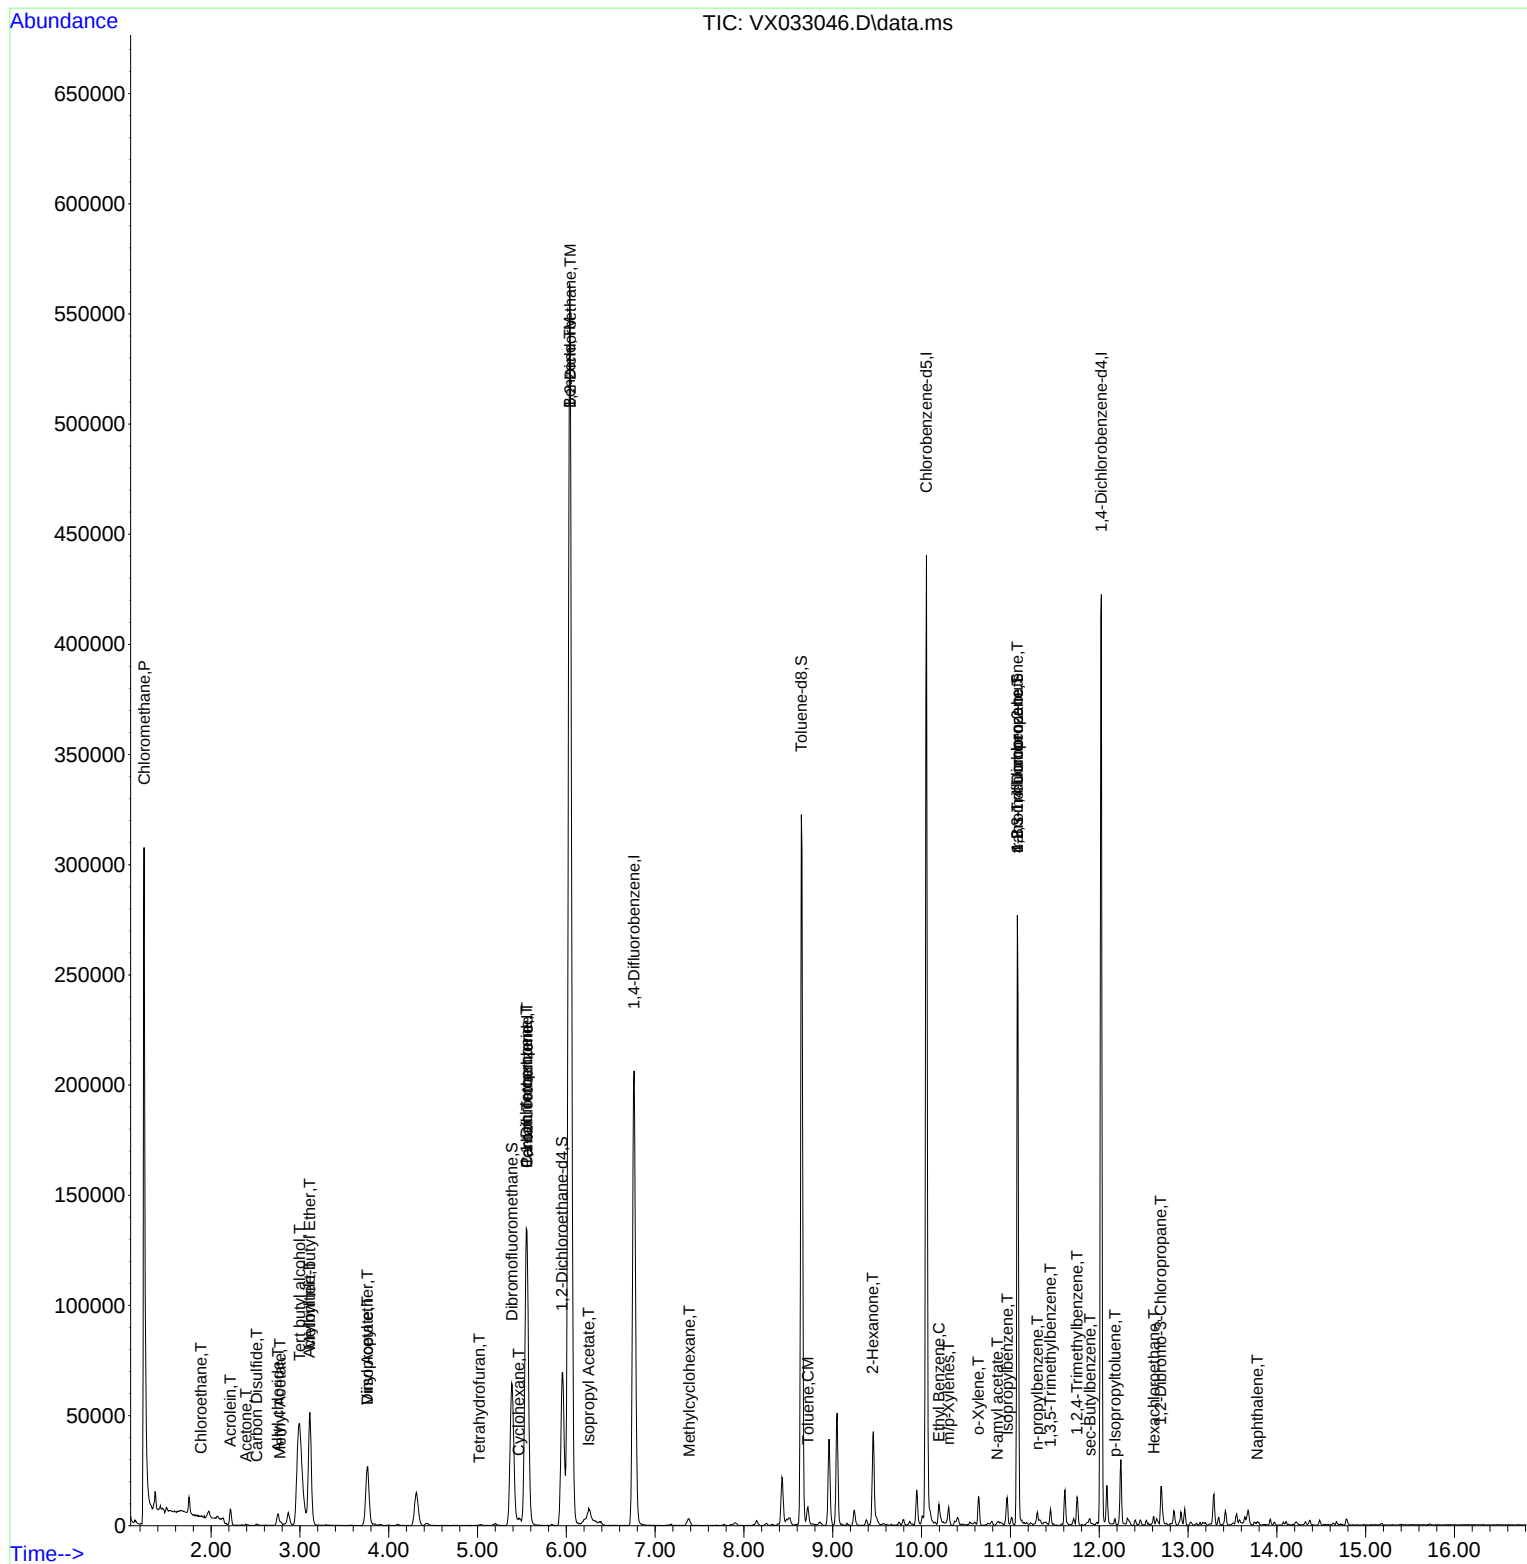


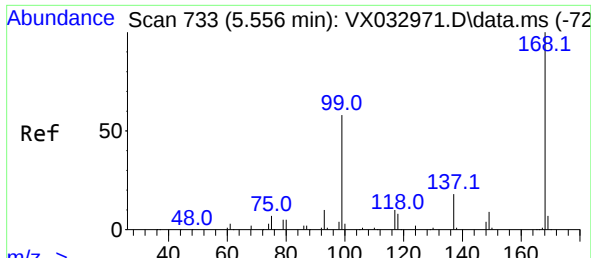

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40

Tgt Ion:168 Resp: 129620
Ion Ratio Lower Upper
168 100
99 56.8 46.1 69.1

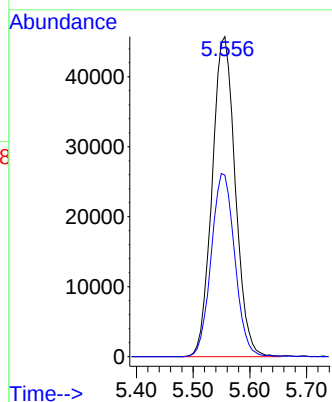


#3
Chloromethane
Concen: 6.755 ug/l
RT: 1.246 min Scan# 26
Delta R.T. -0.048 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 50 Resp: 7221
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#

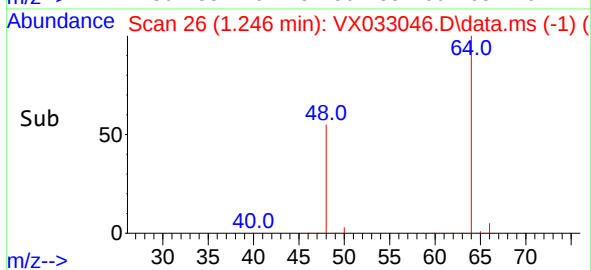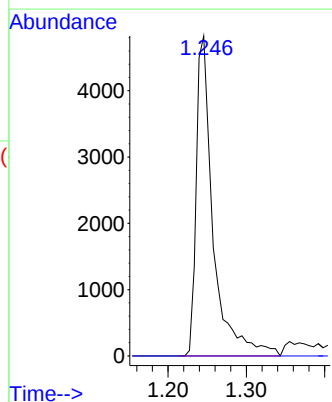

Abundance Scan 99 (1.691 min): VX032971.D\data.ms (-93)

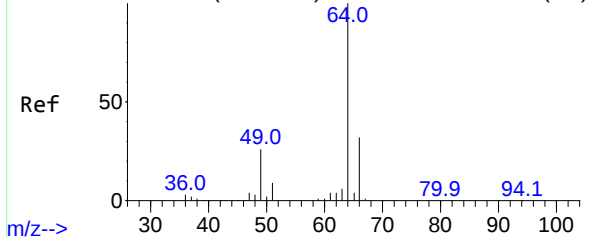

#6

Chloroethane

Concen: 0.971 ug/l

RT: 1.886 min Scan# 11

Delta R.T. 0.201 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Instrument :

MSVOA_X

ClientSampleId :

MW-40



Tgt Ion: 64 Resp: 941

Ion Ratio Lower Upper


64 100

66 5.9 26.0 39.0#


Abundance Scan 131 (1.886 min): VX033046.D\data.ms

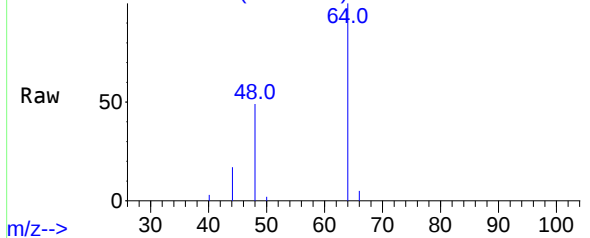

Abundance Scan 131 (1.886 min): VX033046.D\data.ms (-49)

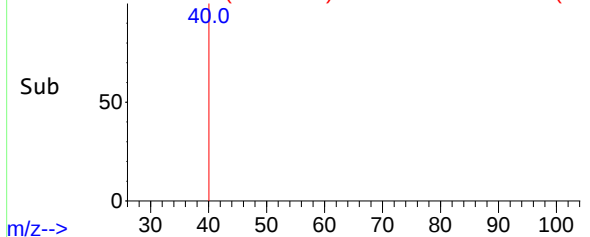

Abundance Scan 316 (3.014 min): VX032971.D\data.ms (-29)

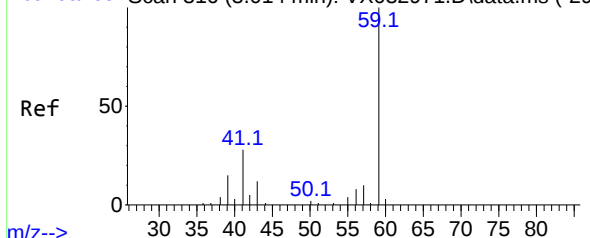

#11

Tert butyl alcohol

Concen: 485.067 ug/l

RT: 2.995 min Scan# 313

Delta R.T. 0.030 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59



Tgt Ion: 59 Resp: 97062

Ion Ratio Lower Upper


59 100


57 10.3 8.2 12.4

Abundance Scan 313 (2.995 min): VX033046.D\data.ms

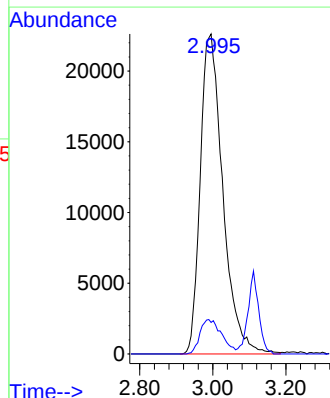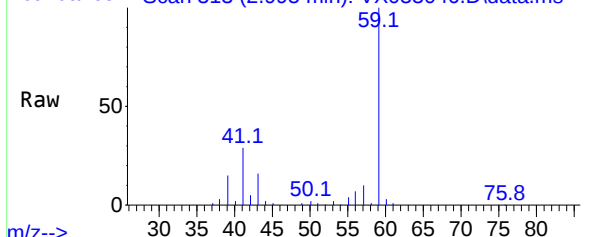

Abundance Scan 313 (2.995 min): VX033046.D\data.ms (-25)




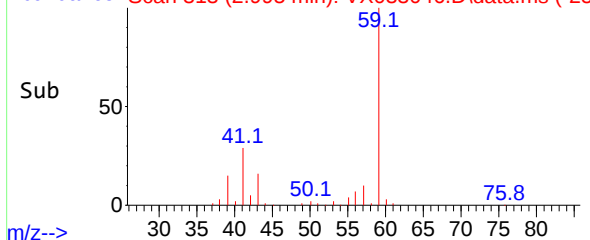




#13
Acrolein
Concen: 0.613 ug/l
RT: 2.215 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 56 Resp: 141
Ion Ratio Lower Upper
56 100
55 2748.2 56.9 85.3#



#14
Allyl chloride
Concen: 0.298 ug/l
RT: 2.751 min Scan# 273
Delta R.T. 0.085 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 41 Resp: 545
Ion Ratio Lower Upper
41 100
39 234.3 61.4 92.2#
76 19.6 29.2 43.8#


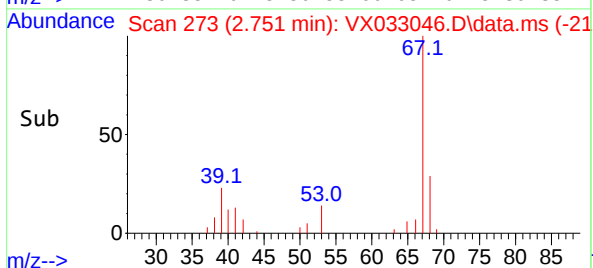
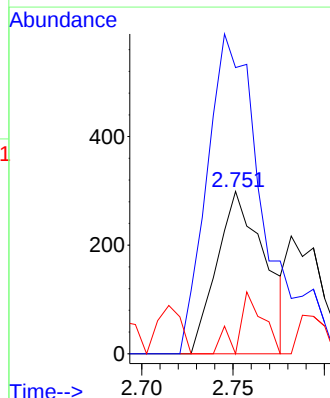





#15
Acrylonitrile
Concen: 1.221 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.043 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 53 Resp: 691
Ion Ratio Lower Upper
53 100
52 14.8 67.4 101.0#
51 81.2 30.3 45.5#

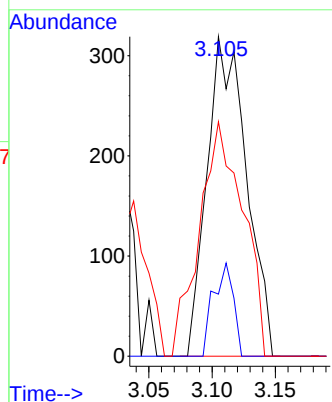

#16
Acetone
Concen: 1.338 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.012 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 43 Resp: 789
Ion Ratio Lower Upper
43 100
58 20.6 23.8 35.8#


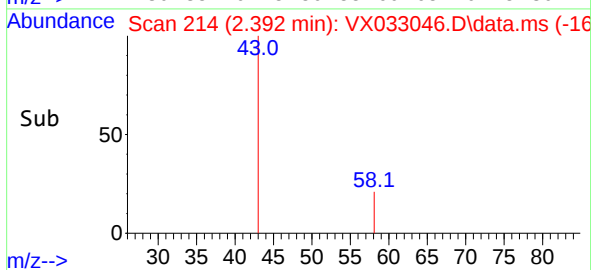




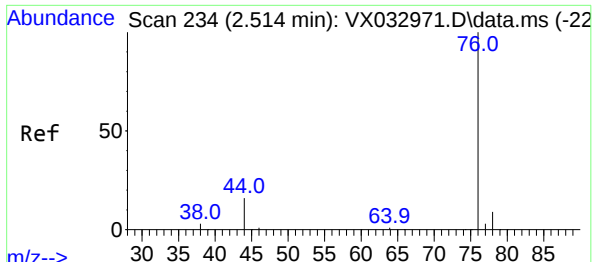

#17
Carbon Disulfide
Concen: 0.313 ug/l
RT: 2.514 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 76 Resp: 978
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

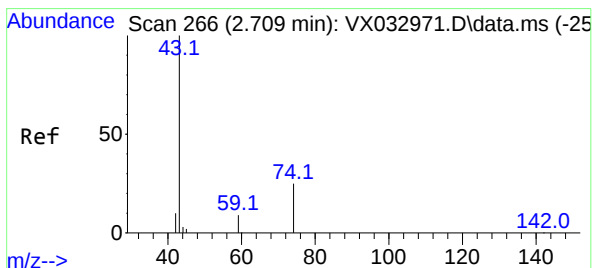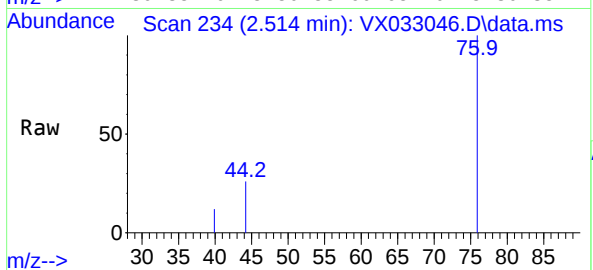

#18
Methyl Acetate
Concen: 0.272 ug/l
RT: 2.776 min Scan# 277
Delta R.T. 0.073 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 43 Resp: 444
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#

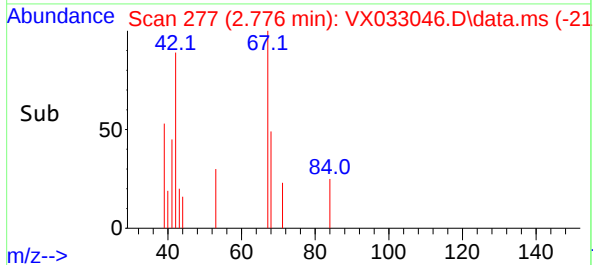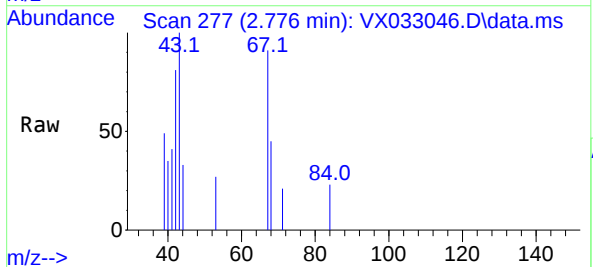



#19

Methyl tert-butyl Ether

Concen: 13.633 ug/l

RT: 3.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 73 Resp: 53483

Ion Ratio Lower Upper

73 100

57 25.4 16.6 25.0#



#20

Methylene Chloride

Concen: Below Cal

RT: 2.776 min Scan# 277

Delta R.T. -0.012 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Tgt Ion: 84 Resp: 116




Ion Ratio Lower Upper


84 100

49 0.0 101.0 151.6#

51 0.0 31.1 46.7#

86 0.0 52.3 78.5#


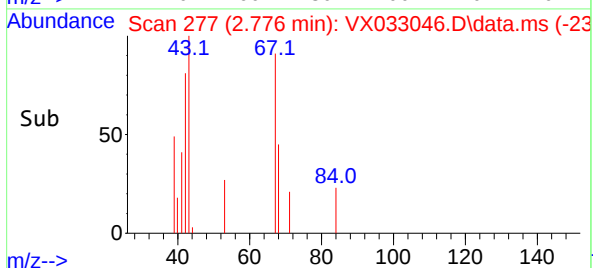
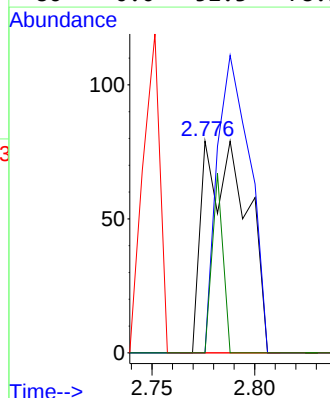





#22
Diisopropyl ether
Concen: 6.940 ug/l
RT: 3.757 min Scan# 41
Delta R.T. -0.006 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:	45	Resp:	27596
Ion	Ratio	Lower	Upper
45	100		
43	54.9	56.4	84.6#
87	25.8	24.4	36.6
59	11.9	9.5	14.3

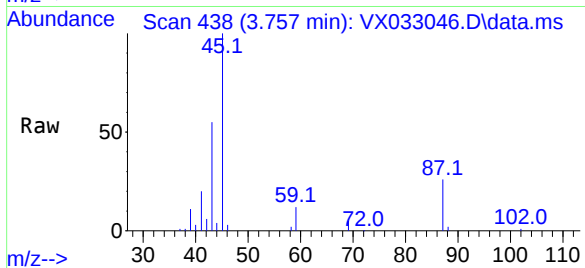

#23
Vinyl Acetate
Concen: 4.886 ug/l
RT: 3.757 min Scan# 438
Delta R.T. 0.036 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion:	43	Resp:	15208
Ion	Ratio	Lower	Upper
43	100		
86	0.0	8.6	12.8#

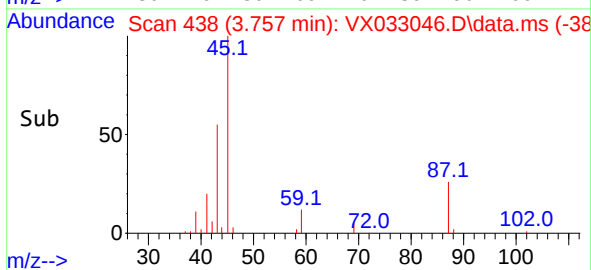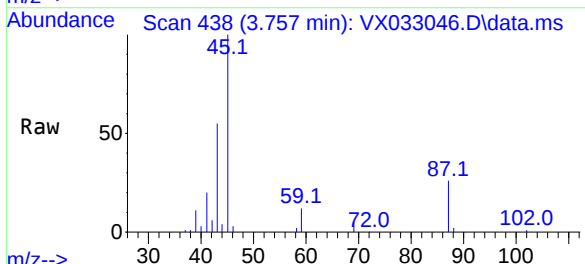



#29

Tetrahydrofuran

Concen: 0.219 ug/l

RT: 5.019 min Scan# 644

Delta R.T. 0.018 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion: 42 Resp: 113

Ion Ratio Lower Upper

42 100

72 0.0 37.6 56.4#

71 0.0 34.7 52.1#

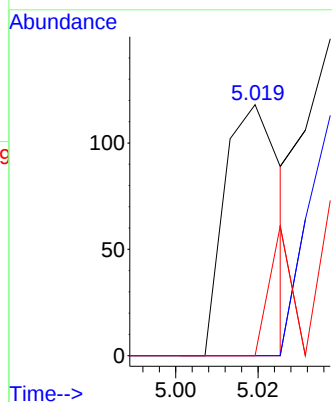

#31

Cyclohexane

Concen: 1.062 ug/l

RT: 5.464 min Scan# 718

Delta R.T. -0.006 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59




Tgt Ion: 56 Resp: 2173


Ion Ratio Lower Upper

56 100

69 24.5 24.1 36.1

84 86.6 66.9 100.3


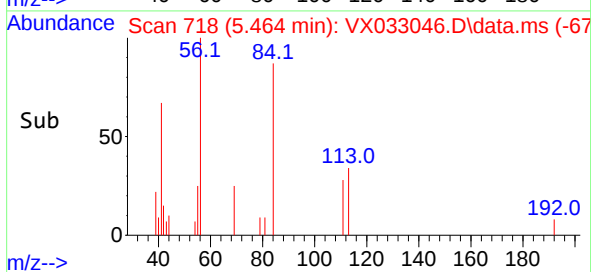
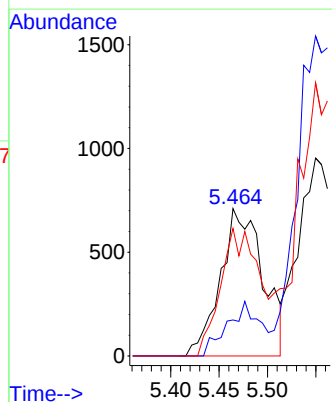





#33
1,2-Dichloroethane-d4
Concen: 56.085 ug/l
RT: 5.952 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 65 Resp: 70553
Ion Ratio Lower Upper
65 100
67 49.7 0.0 101.8



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 114 Resp: 212701
Ion Ratio Lower Upper
114 100
63 19.8 0.0 41.6
88 15.1 0.0 33.4

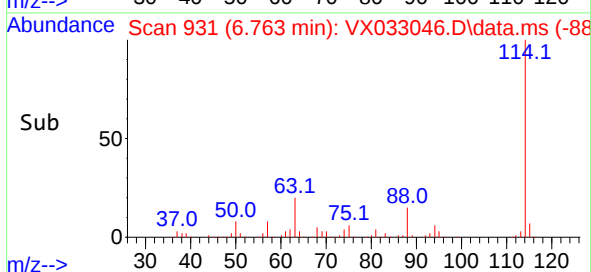



#35

Dibromofluoromethane

Concen: 47.419 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion:113 Resp: 56861

Ion Ratio Lower Upper

113 100

111 101.4 82.4 123.6

192 18.8 15.4 23.2

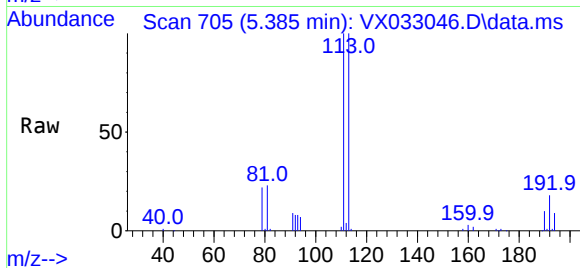

#36

1,1-Dichloropropene

Concen: 5.137 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59




Tgt Ion: 75 Resp: 9849


Ion Ratio Lower Upper

75 100

110 9.5 18.4 55.2#


77 0.0 24.5 36.7#

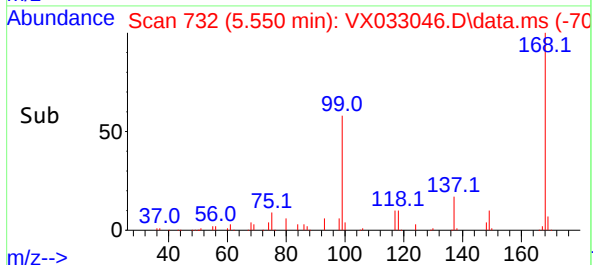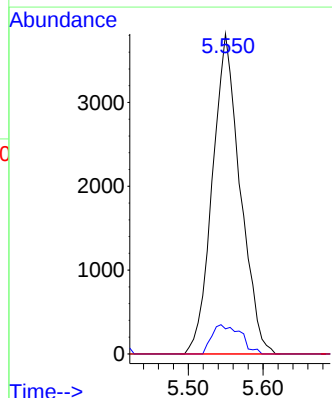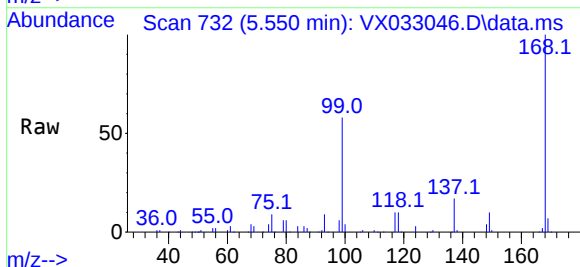



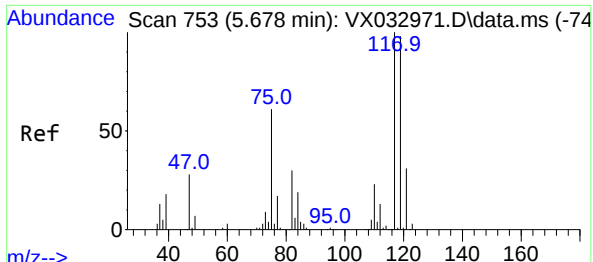


#38
Carbon Tetrachloride
Concen: 6.370 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59


Instrument :
MSVOA_X
ClientSampleId :
MW-40

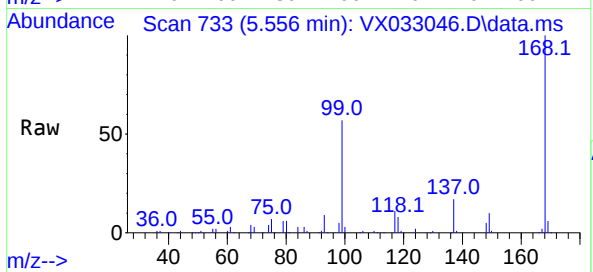



Tgt Ion:117 Resp: 13549
Ion Ratio Lower Upper
117 100
119 5.3 77.2 115.8#
121 0.0 25.8 38.6#

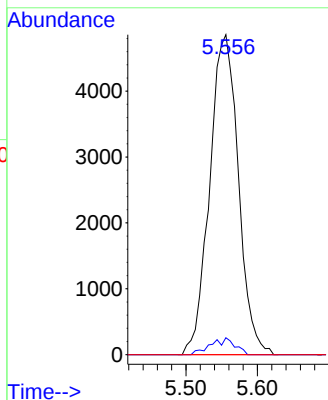


#39
Methylcyclohexane
Concen: 0.688 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

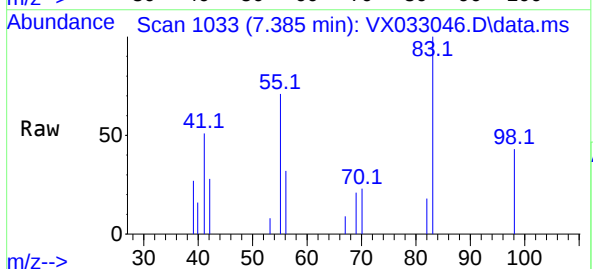

Tgt Ion: 83 Resp: 1506
Ion Ratio Lower Upper
83 100
55 71.5 58.4 87.6
98 42.6 37.2 55.8



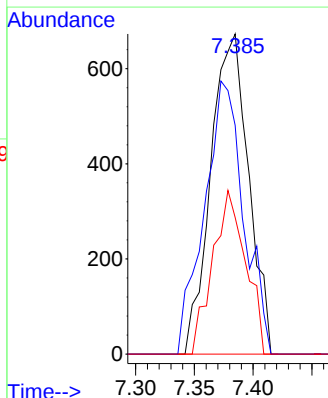
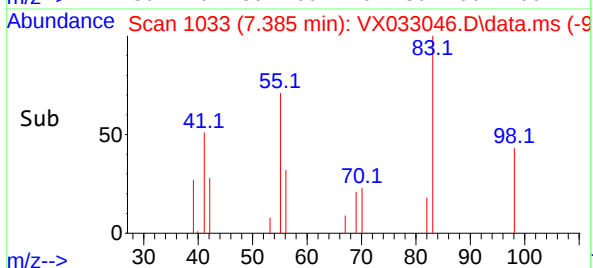




#40
Benzene
Concen: 125.172 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 78 Resp: 672903
Ion Ratio Lower Upper
78 100
77 23.7 19.0 28.4

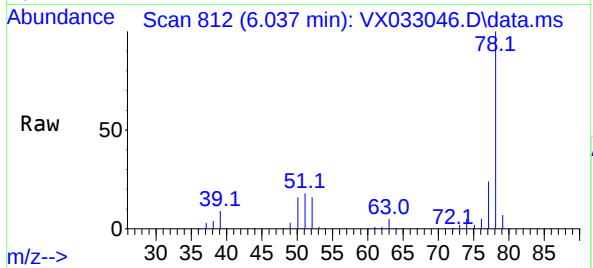

#42
1,2-Dichloroethane
Concen: 2.869 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.043 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 62 Resp: 6210
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0


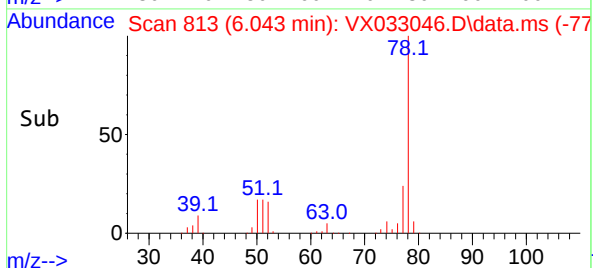
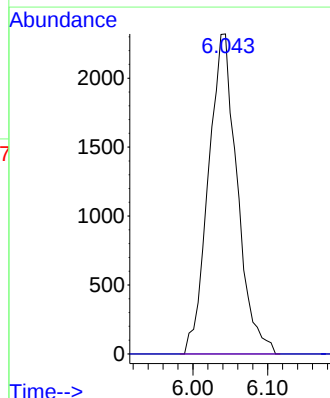





#43
Isopropyl Acetate
Concen: 0.697 ug/l
RT: 6.251 min Scan# 847
Delta R.T. -0.091 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 1929
Ion Ratio Lower Upper
43 100
61 0.0 15.4 23.0#
87 0.0 10.8 16.2#

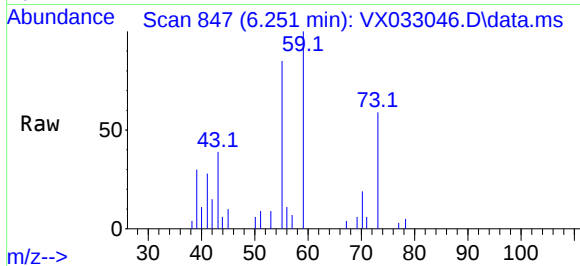

#50
Toluene-d8
Concen: 53.699 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 98 Resp: 193169
Ion Ratio Lower Upper
98 100
100 63.5 50.9 76.3

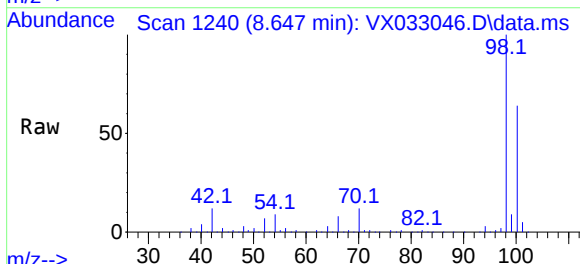



#52

Toluene

Concen: 0.720 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX033046.D

Acq: 24 Nov 2022 07:59

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 92 Resp: 2547

Ion Ratio Lower Upper

92 100

91 163.8 138.3 207.5

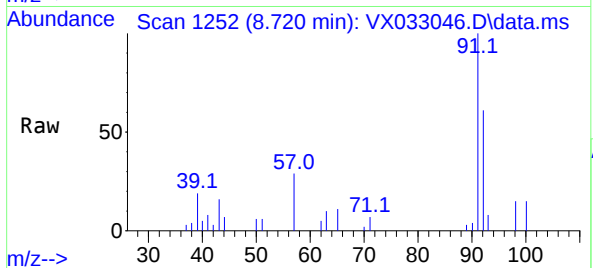

#59

2-Hexanone

Concen: 2.255 ug/l

RT: 9.451 min Scan# 1372

Delta R.T. 0.018 min

Lab File: VX033046.D




Acq: 24 Nov 2022 07:59


Tgt Ion: 43 Resp: 2844

Ion Ratio Lower Upper

43 100

58 50.9 26.5 79.5


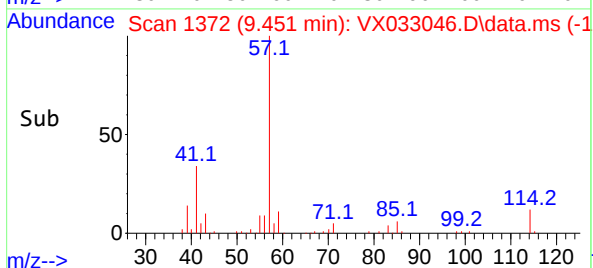
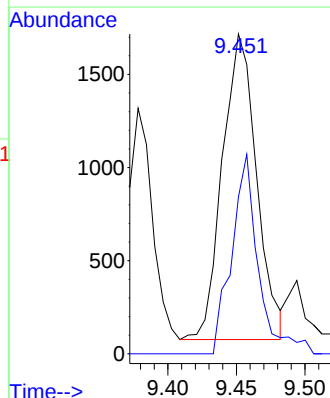





#62
4-Bromofluorobenzene
Concen: 44.639 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 95 Resp: 70314
Ion Ratio Lower Upper
95 100
174 79.6 0.0 164.0
176 76.5 0.0 154.4

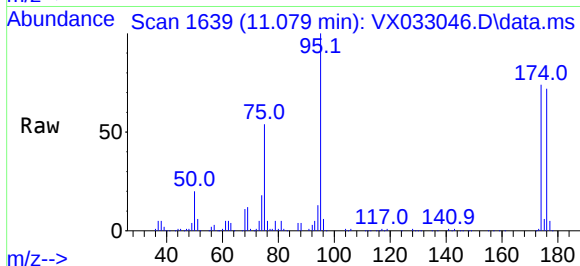

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 117 Resp: 189738
Ion Ratio Lower Upper
117 100
82 53.7 44.3 66.5
119 31.3 25.7 38.5



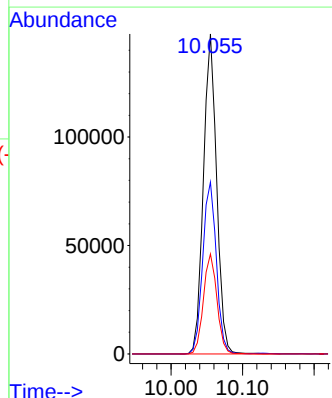
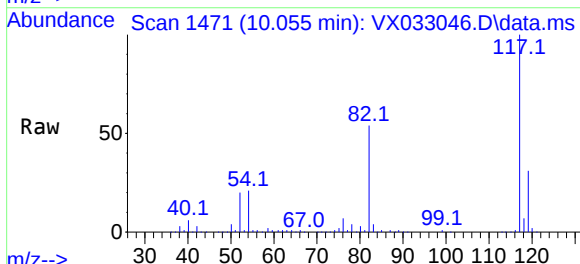




#67
Ethyl Benzene
Concen: 0.894 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 91 Resp: 5998
Ion Ratio Lower Upper
91 100
106 27.7 25.0 37.6

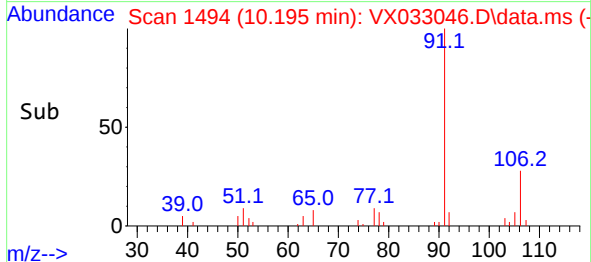

#68
m/p-Xylenes
Concen: 0.688 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 106 Resp: 1809
Ion Ratio Lower Upper
106 100
91 207.1 164.5 246.7


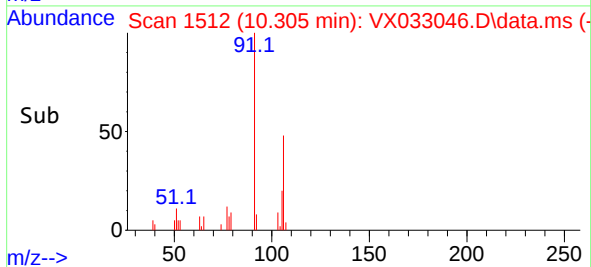

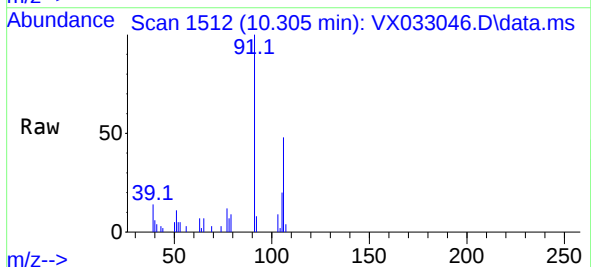




#69
o-Xylene
Concen: 1.050 ug/l
RT: 10.640 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:106 Resp: 2669
Ion Ratio Lower Upper
106 100
91 225.9 109.2 327.6

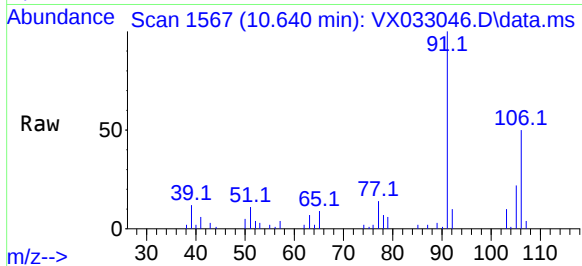

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion:152 Resp: 89077
Ion Ratio Lower Upper
152 100
115 60.0 44.0 132.0
150 156.5 0.0 351.8


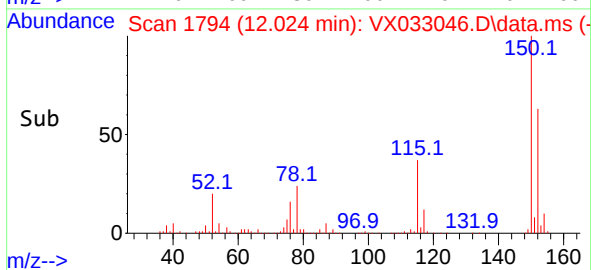

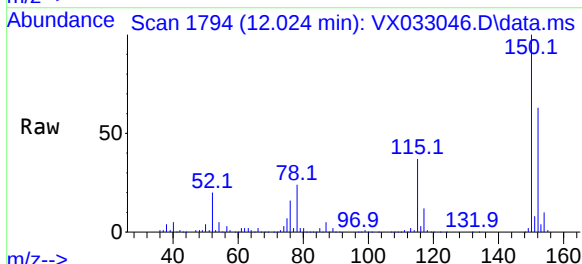




#73
Isopropylbenzene
Concen: 0.957 ug/l
RT: 10.963 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:105 Resp: 6092
Ion Ratio Lower Upper
105 100
120 27.1 13.1 39.3

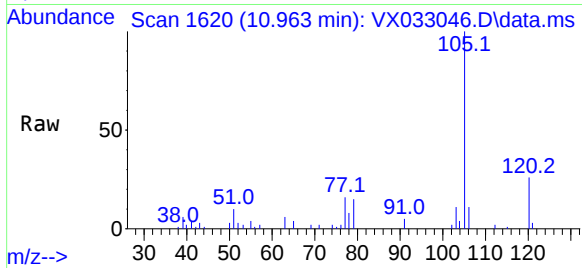

#74
N-ethyl acetate
Concen: 0.212 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.013 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 43 Resp: 459
Ion Ratio Lower Upper
43 100
70 17.9 33.6 50.4#
55 0.0 19.4 29.2#
61 0.0 18.8 28.2#


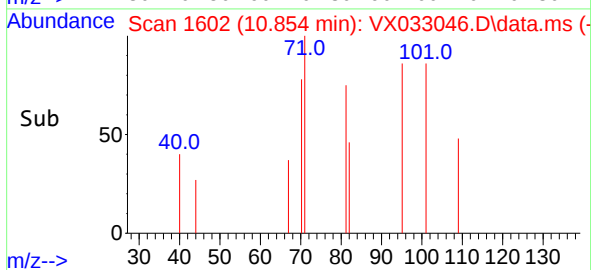

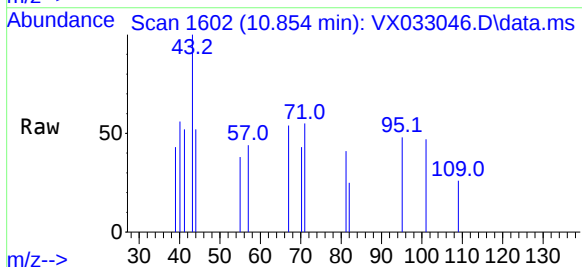




#76
1,2,3-Trichloropropane
Concen: 22.594 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 38116
Ion Ratio Lower Upper
75 100
77 1.2 20.0 60.0#

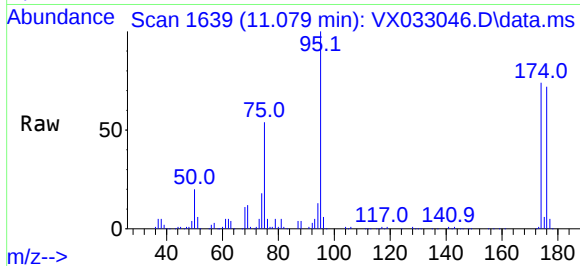

#78
n-propylbenzene
Concen: 0.200 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 91 Resp: 1458
Ion Ratio Lower Upper
91 100
120 21.8 11.6 34.8


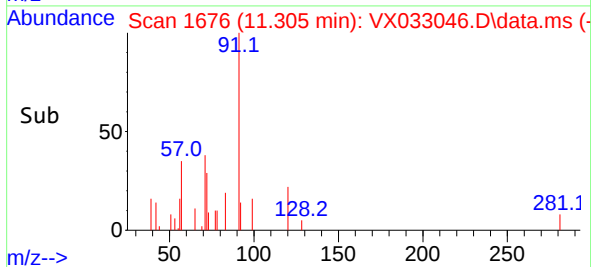

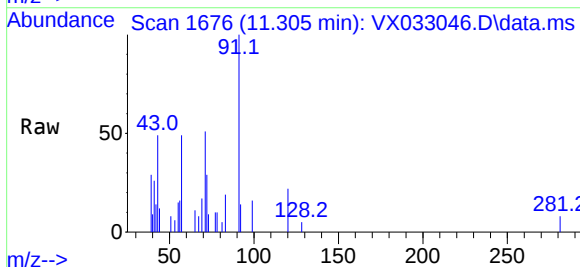




#80
1,3,5-Trimethylbenzene
Concen: 0.629 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:105 Resp: 3362
Ion Ratio Lower Upper
105 100
120 43.0 23.6 71.0

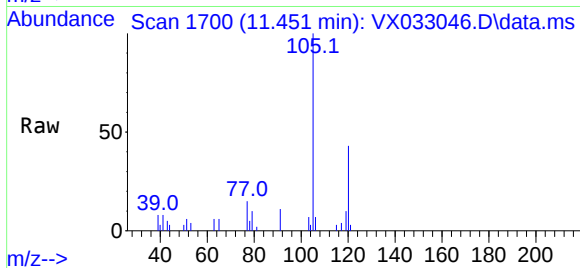

#81
trans-1,4-Dichloro-2-butene
Concen: 73.442 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 75 Resp: 38116
Ion Ratio Lower Upper
75 100
53 0.1 86.9 130.3#
89 0.0 38.3 57.5#


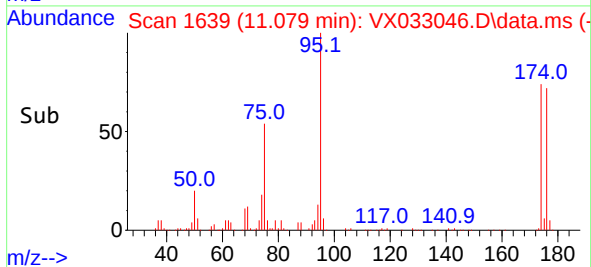

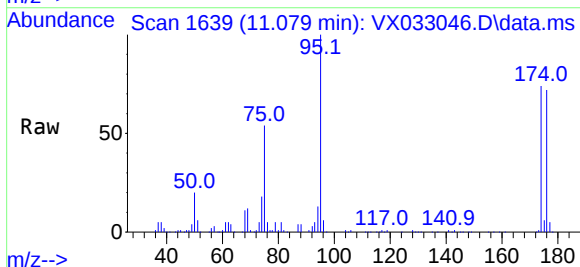




#84
1,2,4-Trimethylbenzene
Concen: 1.137 ug/l
RT: 11.750 min Scan# 11749
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:105 Resp: 6060
Ion Ratio Lower Upper
105 100
120 42.1 21.9 65.5

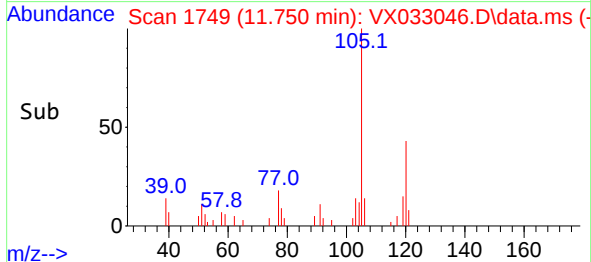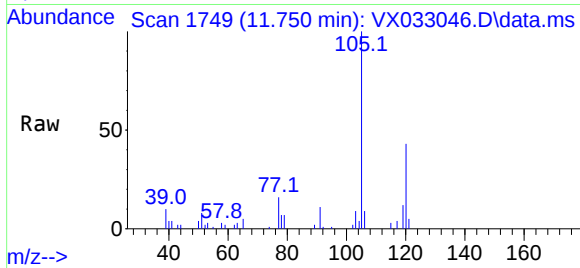

#85
sec-Butylbenzene
Concen: 0.261 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.006 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion:105 Resp: 1661
Ion Ratio Lower Upper
105 100
134 14.3 9.9 29.7


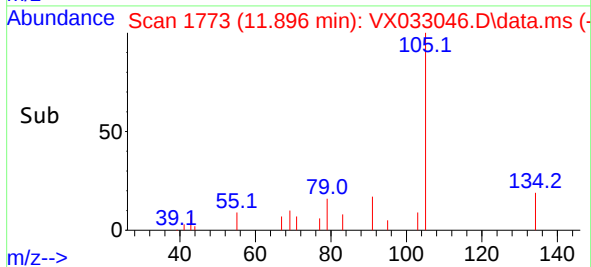

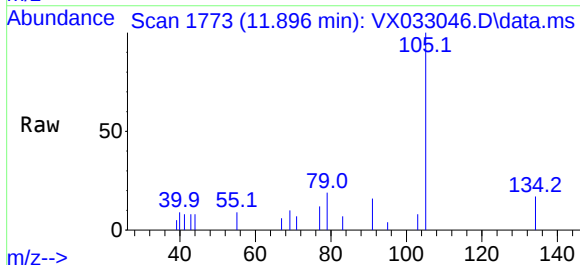




#86
p-Isopropyltoluene
Concen: 0.225 ug/l
RT: 12.177 min Scan# 1819
Delta R.T. 0.165 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:119 Resp: 1216
Ion Ratio Lower Upper
119 100
134 23.6 12.9 38.7
91 27.1 12.5 37.5

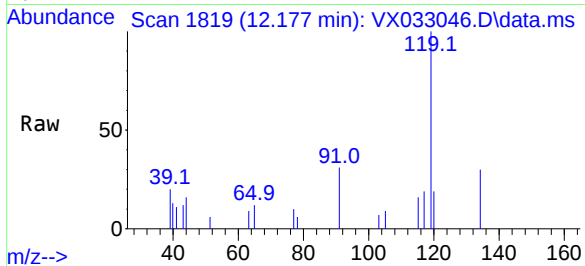

#90
Hexachloroethane
Concen: 0.288 ug/l
RT: 12.615 min Scan# 1891
Delta R.T. 0.073 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion:117 Resp: 255
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#



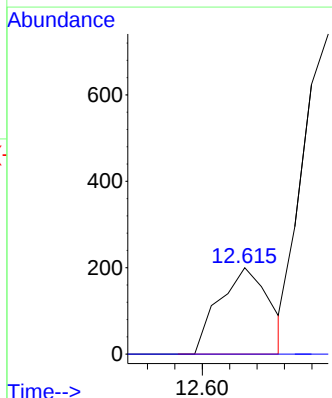
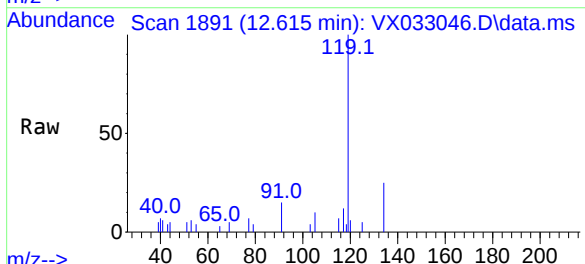




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.316 ug/l
RT: 12.695 min Scan# 1945
Delta R.T. -0.250 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Tgt Ion: 75 Resp: 121
Ion Ratio Lower Upper
75 100
155 0.0 41.6 124.8#
157 0.0 54.1 162.4#

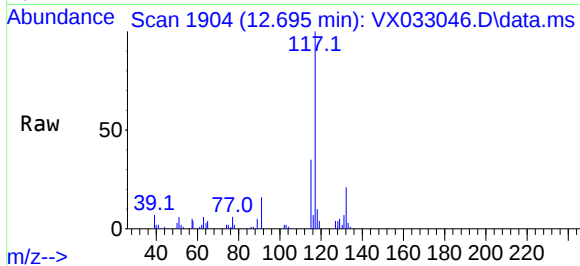

#95
Naphthalene
Concen: 0.240 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX033046.D
Acq: 24 Nov 2022 07:59

Tgt Ion: 128 Resp: 1366
Ion Ratio Lower Upper
128 100
127 11.6 10.2 15.4
129 8.8 8.9 13.3#

