

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112322\  
 Data File : VX033049.D  
 Acq On : 24 Nov 2022 09:07  
 Operator : JC/MD  
 Sample : N5742-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-43

Quant Time: Nov 25 06:38:51 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Nov 22 13:58:46 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc      | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|--------|----------|
| -----                         |        |       |          |           |        |          |
| Internal Standards            |        |       |          |           |        |          |
| 1) Pentafluorobenzene         | 5.556  | 168   | 131348   | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763  | 114   | 212817   | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 189983   | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 89312    | 50.000    | ug/l   | 0.00     |
| System Monitoring Compounds   |        |       |          |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958  | 65    | 70801    | 55.509    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 78 - 117 | Recovery  | =      | 111.020% |
| 35) Dibromofluoromethane      | 5.385  | 113   | 56464    | 47.062    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery  | =      | 94.120%  |
| 50) Toluene-d8                | 8.647  | 98    | 192706   | 53.535    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 92 - 112 | Recovery  | =      | 107.060% |
| 62) 4-Bromofluorobenzene      | 11.079 | 95    | 69743    | 44.252    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery  | =      | 88.500%  |
| Target Compounds              |        |       |          |           |        |          |
|                               |        |       |          |           | Qvalue |          |
| 3) Chloromethane              | 1.246  | 50    | 1888     | 1.743     | ug/l # | 43       |
| 11) Tert butyl alcohol        | 2.977  | 59    | 214      | 1.055     | ug/l # | 72       |
| 14) Allyl chloride            | 2.782  | 41    | 1060     | 0.573     | ug/l # | 65       |
| 16) Acetone                   | 2.392  | 43    | 1606     | 2.688     | ug/l   | 97       |
| 18) Methyl Acetate            | 2.782  | 43    | 2371     | 1.434     | ug/l # | 51       |
| 19) Methyl tert-butyl Ether   | 3.111  | 73    | 1845     | 0.464     | ug/l # | 1        |
| 20) Methylene Chloride        | 2.788  | 84    | 44       | Below Cal | #      | 56       |
| 25) 2-Butanone                | 4.599  | 43    | 343      | 0.416     | ug/l # | 47       |
| 31) Cyclohexane               | 5.477  | 56    | 1370     | 0.661     | ug/l   | 96       |
| 36) 1,1-Dichloropropene       | 5.556  | 75    | 10622    | 5.537     | ug/l # | 51       |
| 37) Ethyl Acetate             | 4.599  | 43    | 343      | 0.205     | ug/l # | 67       |
| 38) Carbon Tetrachloride      | 5.556  | 117   | 13384    | 6.289     | ug/l # | 16       |
| 39) Methylcyclohexane         | 7.385  | 83    | 614      | 0.281     | ug/l # | 86       |
| 40) Benzene                   | 6.038  | 78    | 3266     | 0.607     | ug/l   | 95       |
| 55) 1,1,2-Trichloroethane     | 9.104  | 97    | 425      | 0.295     | ug/l # | 15       |
| 67) Ethyl Benzene             | 10.195 | 91    | 1527     | 0.227     | ug/l # | 88       |
| 73) Isopropylbenzene          | 10.964 | 105   | 2368     | 0.371     | ug/l   | 99       |
| 76) 1,2,3-Trichloropropane    | 11.079 | 75    | 38195    | 22.582    | ug/l # | 37       |
| 78) n-propylbenzene           | 11.305 | 91    | 3326     | 0.456     | ug/l   | 96       |
| 79) 2-Chlorotoluene           | 11.305 | 91    | 3326     | 0.750     | ug/l # | 41       |
| 80) 1,3,5-Trimethylbenzene    | 11.616 | 105   | 2174     | 0.405     | ug/l   | 76       |
| 81) trans-1,4-Dichloro-2-b... | 11.079 | 75    | 38195    | 73.400    | ug/l # | 6        |
| 82) 4-Chlorotoluene           | 11.305 | 91    | 3326     | 0.640     | ug/l # | 45       |
| 84) 1,2,4-Trimethylbenzene    | 11.756 | 105   | 2446     | 0.458     | ug/l   | 94       |
| 89) n-Butylbenzene            | 12.329 | 91    | 1075     | 0.231     | ug/l # | 65       |
| 90) Hexachloroethane          | 12.616 | 117   | 365      | 0.411     | ug/l # | 12       |
| 95) Naphthalene               | 13.780 | 128   | 1862     | 0.326     | ug/l # | 94       |
| -----                         |        |       |          |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112322\  
Data File : VX033049.D  
Acq On : 24 Nov 2022 09:07  
Operator : JC/MD  
Sample : N5742-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 44 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43

Quant Time: Nov 25 06:38:51 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Quant Title : SW846 8260  
QLast Update : Tue Nov 22 13:58:46 2022  
Response via : Initial Calibration




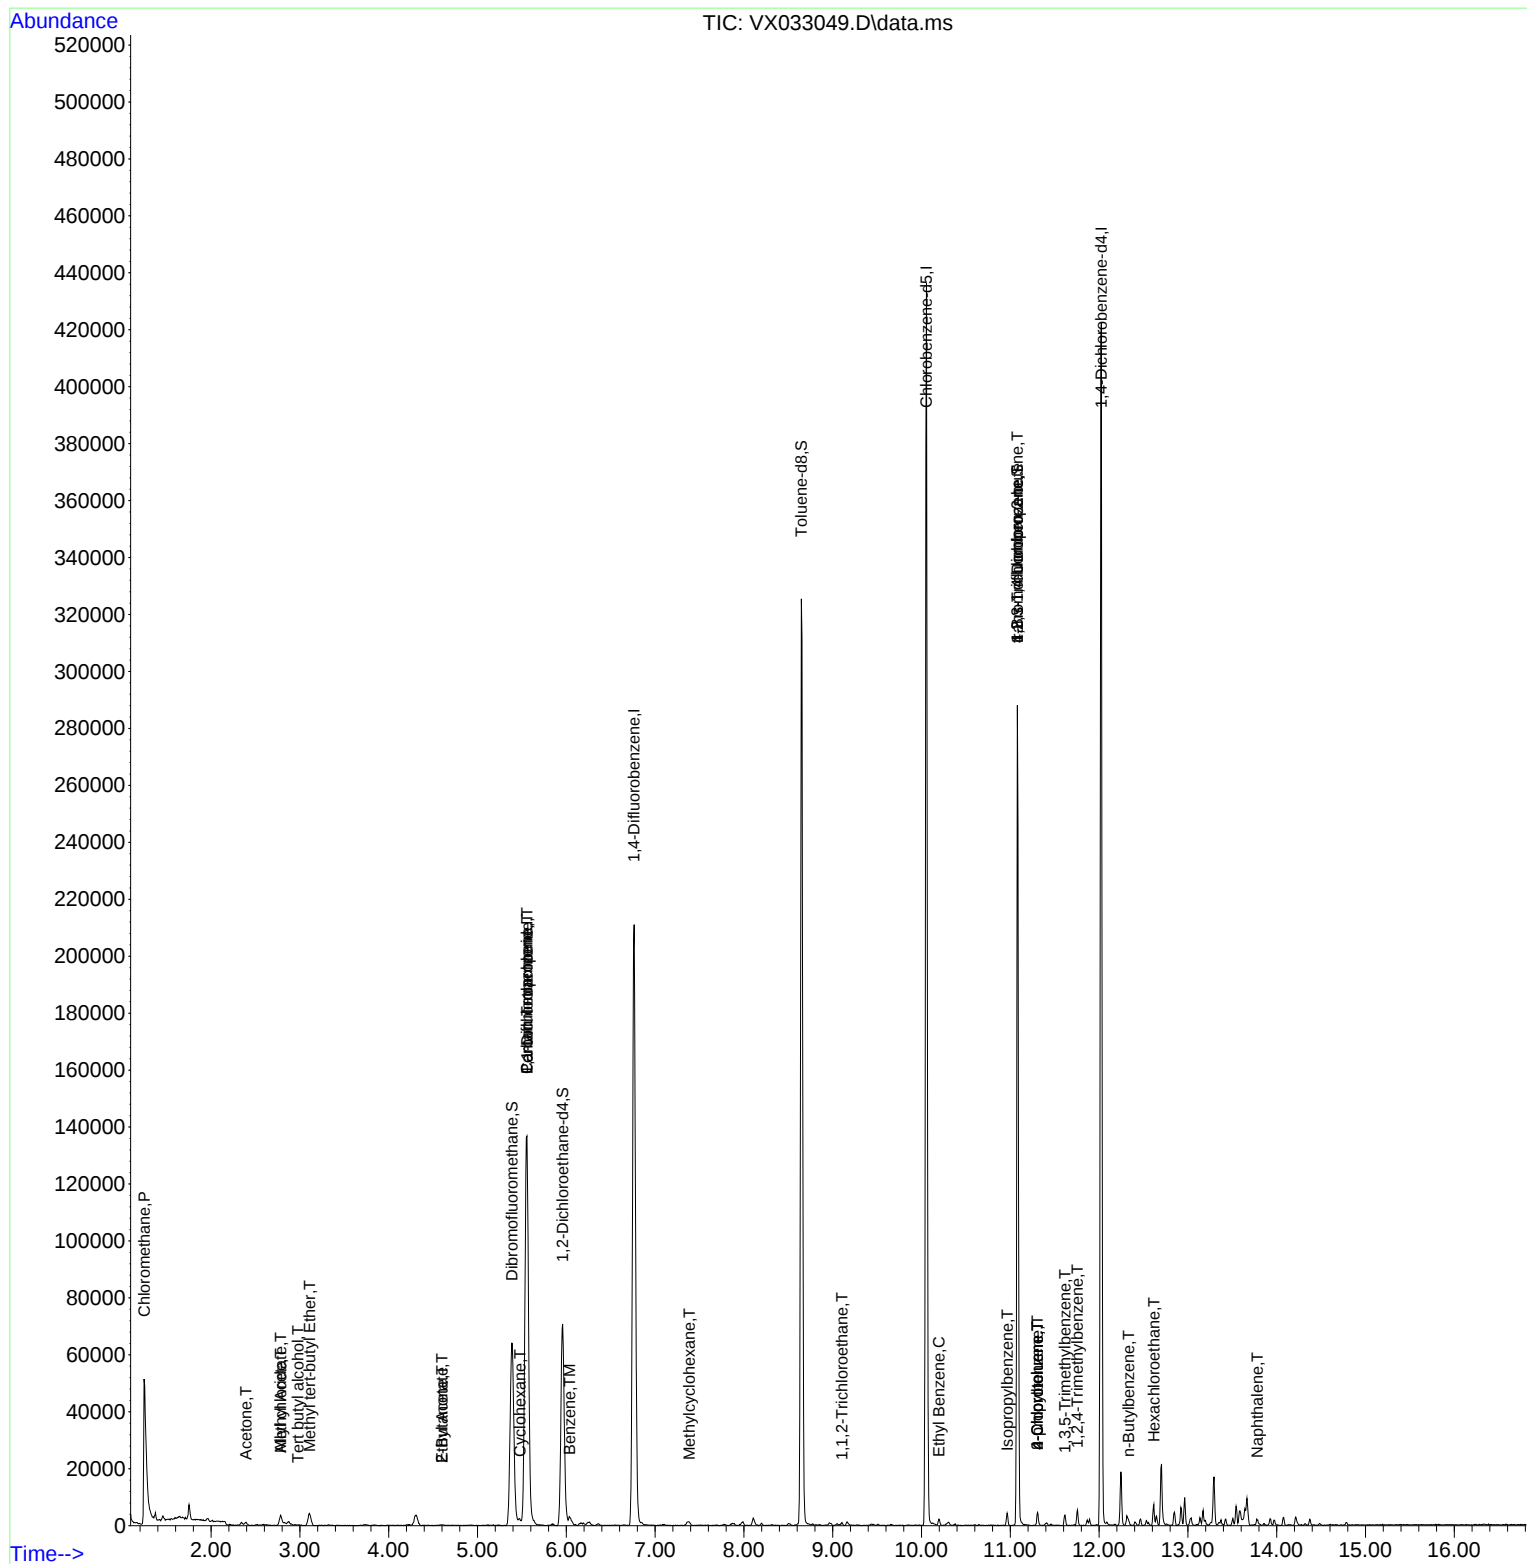


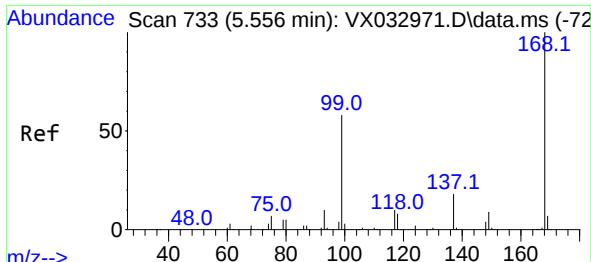

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.556 min Scan# 71  
Delta R.T. 0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion:168 Resp: 131348  
Ion Ratio Lower Upper  
168 100  
99 57.3 46.1 69.1

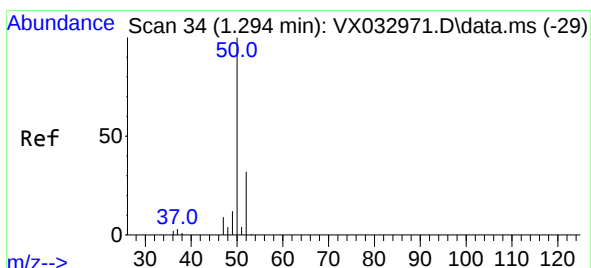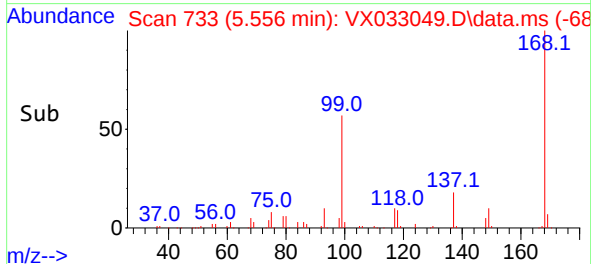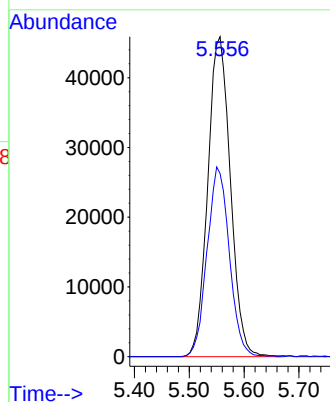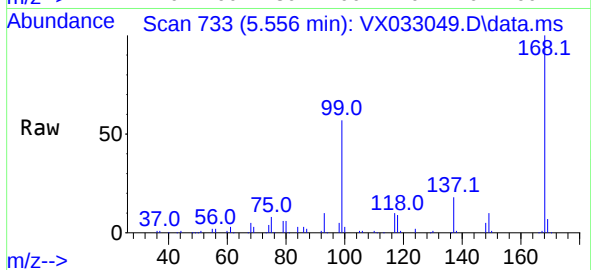

#3  
Chloromethane  
Concen: 1.743 ug/l  
RT: 1.246 min Scan# 26  
Delta R.T. -0.048 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 50 Resp: 1888  
Ion Ratio Lower Upper  
50 100  
52 0.0 25.4 38.2#


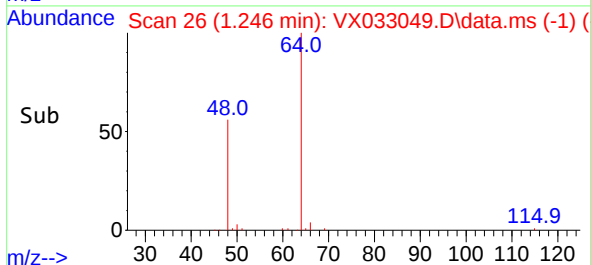

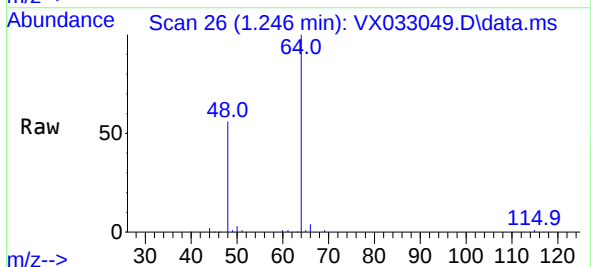




#11  
Tert butyl alcohol  
Concen: 1.055 ug/l  
RT: 2.977 min Scan# 31  
Delta R.T. 0.012 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 59 Resp: 214  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.2 12.4#

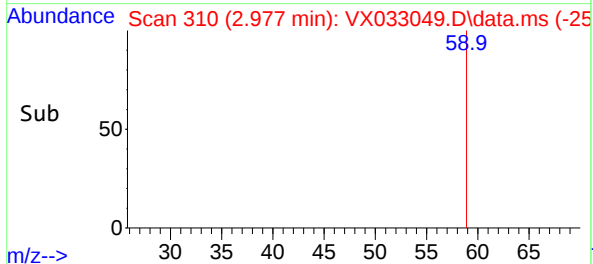

#14  
Allyl chloride  
Concen: 0.573 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.116 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 41 Resp: 1060  
Ion Ratio Lower Upper  
41 100  
39 57.5 61.4 92.2#  
76 0.0 29.2 43.8#


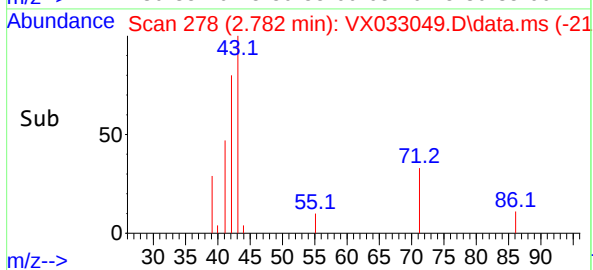

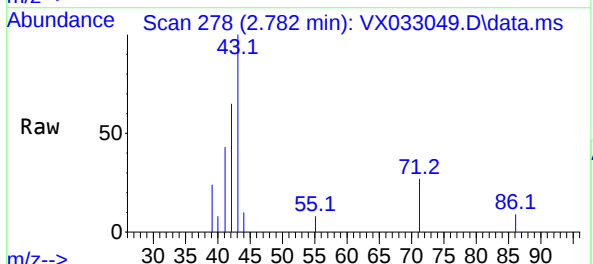




#16  
Acetone  
Concen: 2.688 ug/l  
RT: 2.392 min Scan# 214  
Delta R.T. 0.012 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 43 Resp: 1606  
Ion Ratio Lower Upper  
43 100  
58 31.3 23.8 35.8

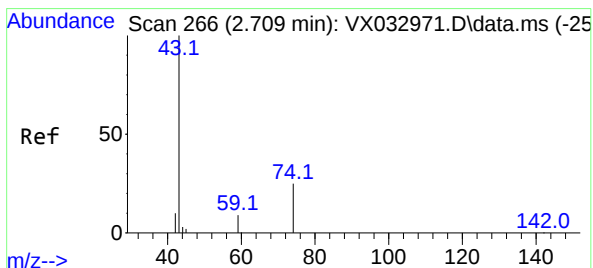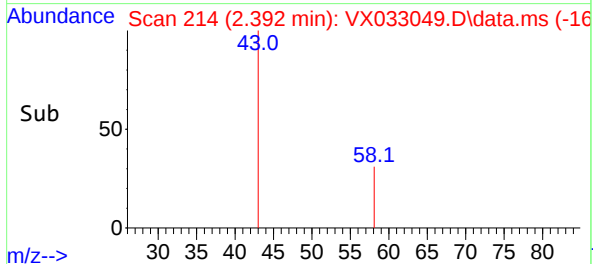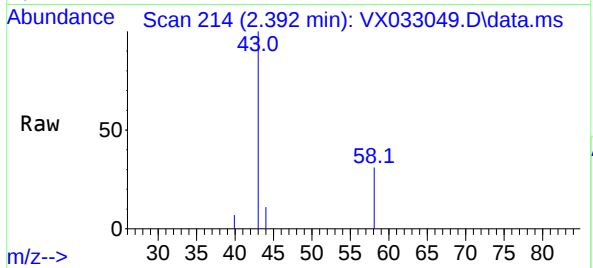

#18  
Methyl Acetate  
Concen: 1.434 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.079 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 43 Resp: 2371  
Ion Ratio Lower Upper  
43 100  
74 0.0 19.4 29.0#

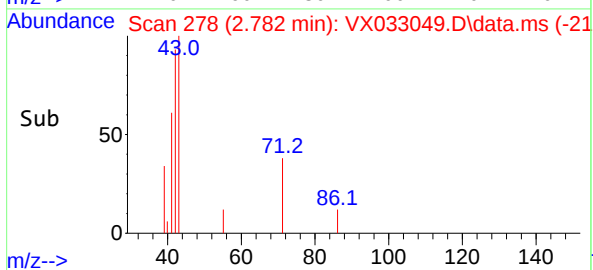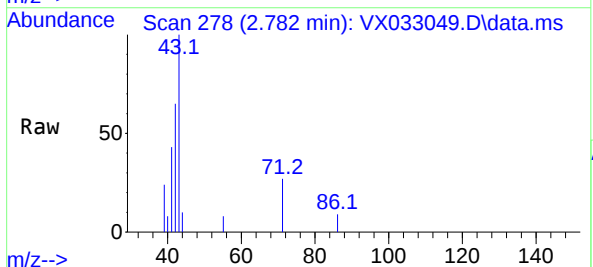



#19

Methyl tert-butyl Ether

Concen: 0.464 ug/l

RT: 3.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :





MW-43

Tgt Ion: 73 Resp: 1845

Ion Ratio Lower Upper

73 100

57 94.9 16.6 25.0#

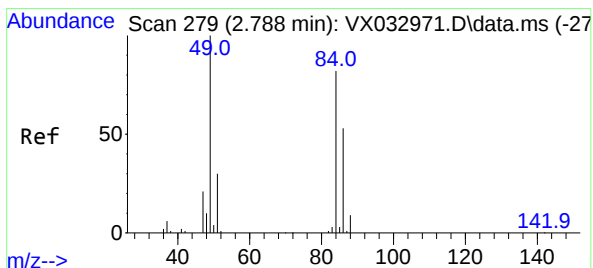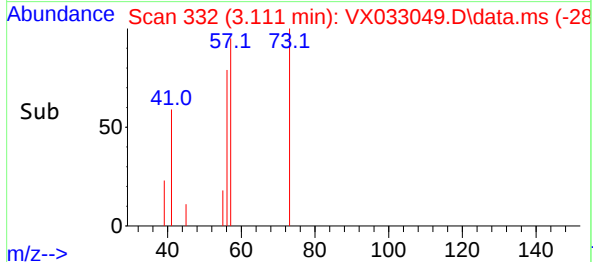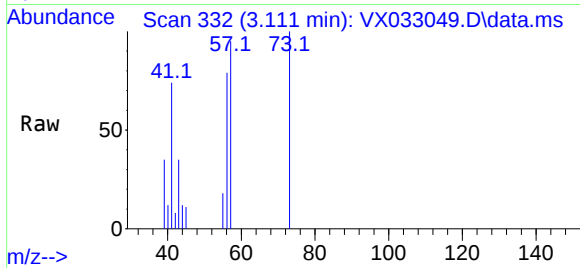

#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Tgt Ion: 84 Resp: 44




Ion Ratio Lower Upper


84 100

49 83.3 101.0 151.6#

51 91.7 31.1 46.7#

86 40.0 52.3 78.5#

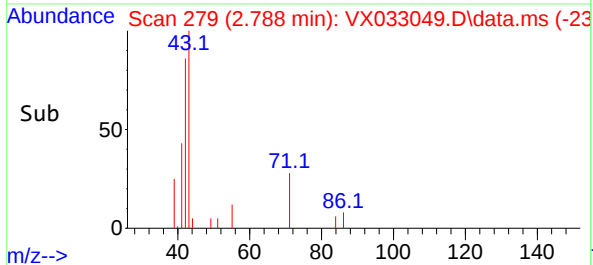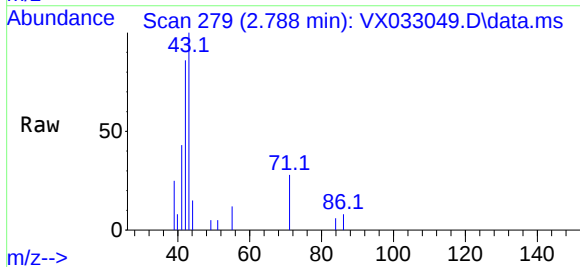



#25

2-Butanone

Concen: 0.416 ug/l

RT: 4.599 min Scan# 51

Delta R.T. 0.043 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :





MW-43

Tgt Ion: 43 Resp: 343

Ion Ratio Lower Upper

43 100

72 0.0 22.2 33.2#

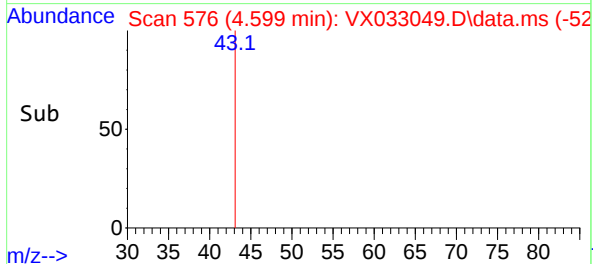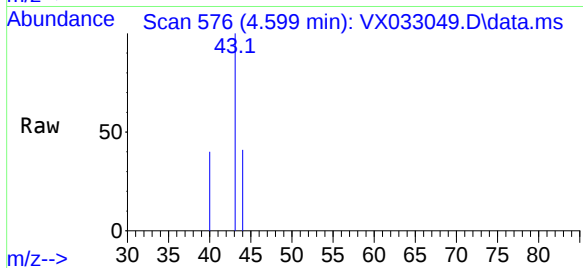

#31

Cyclohexane

Concen: 0.661 ug/l

RT: 5.477 min Scan# 720

Delta R.T. 0.007 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07




Tgt Ion: 56 Resp: 1370


Ion Ratio Lower Upper

56 100

69 32.8 24.1 36.1

84 80.0 66.9 100.3

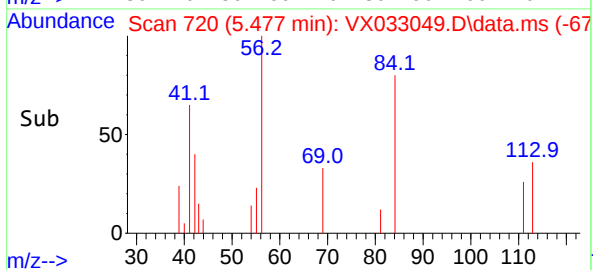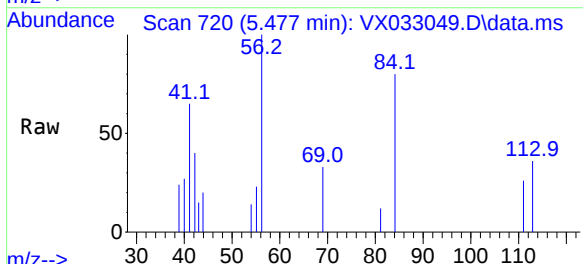



#33

1,2-Dichloroethane-d4

Concen: 55.509 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :





MW-43

Tgt Ion: 65 Resp: 70801

Ion Ratio Lower Upper

65 100

67 51.1 0.0 101.8

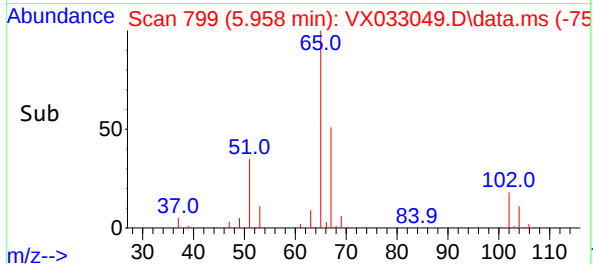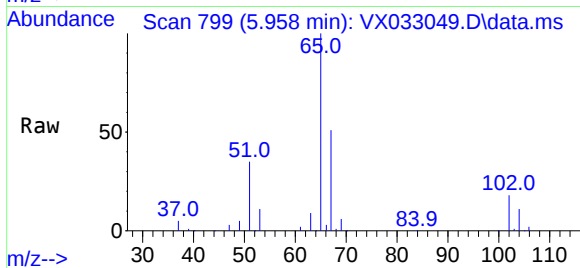

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07




Tgt Ion: 114 Resp: 212817


Ion Ratio Lower Upper

114 100

63 19.7 0.0 41.6

88 15.9 0.0 33.4


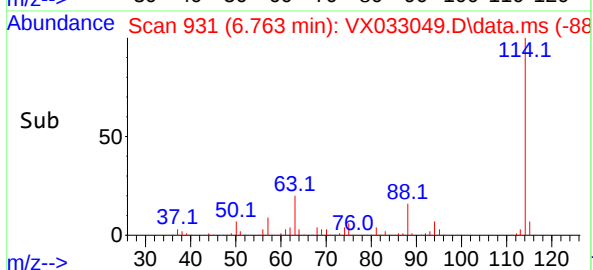
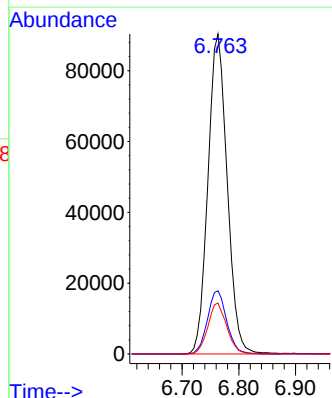
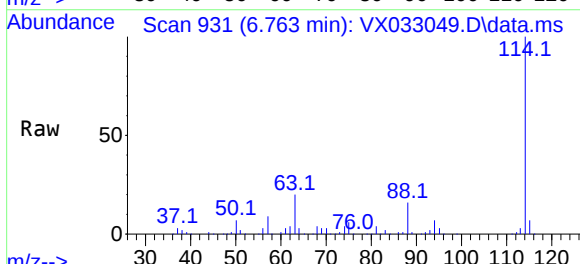


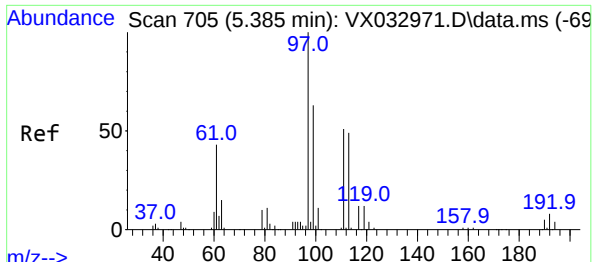

#35  
Dibromofluoromethane  
Concen: 47.062 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion:113 Resp: 56464  
Ion Ratio Lower Upper  
113 100  
111 102.9 82.4 123.6  
192 17.9 15.4 23.2

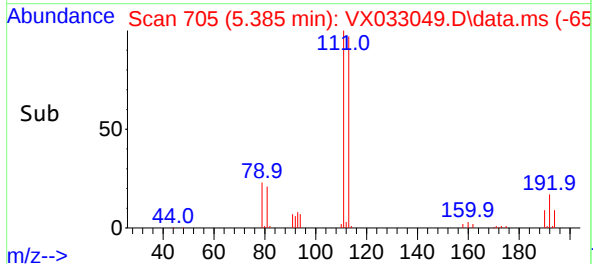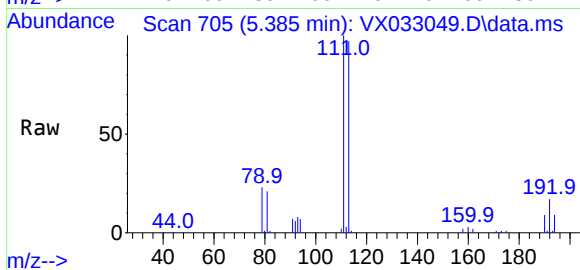

#36  
1,1-Dichloropropene  
Concen: 5.537 ug/l  
RT: 5.556 min Scan# 733  
Delta R.T. -0.140 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 75 Resp: 10622  
Ion Ratio Lower Upper  
75 100  
110 10.6 18.4 55.2#  
77 0.0 24.5 36.7#

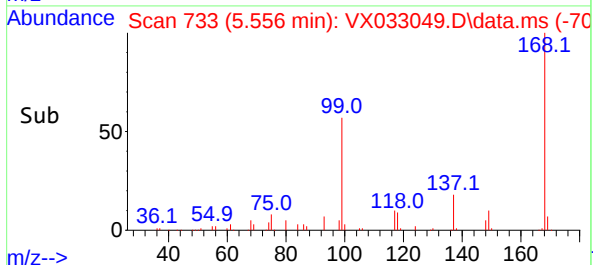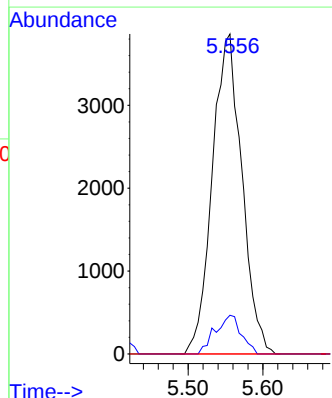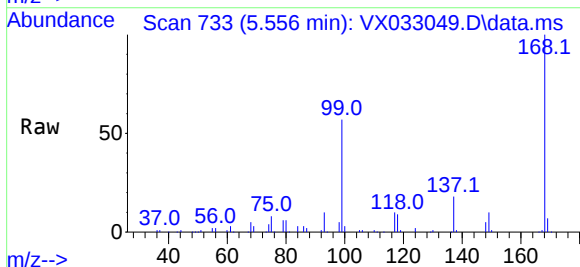



#37

Ethyl Acetate

Concen: 0.205 ug/l

RT: 4.599 min Scan# 51

Delta R.T. -0.116 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :

MW-43





Tgt Ion: 43 Resp: 343

Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#

70 0.0 9.1 13.7#

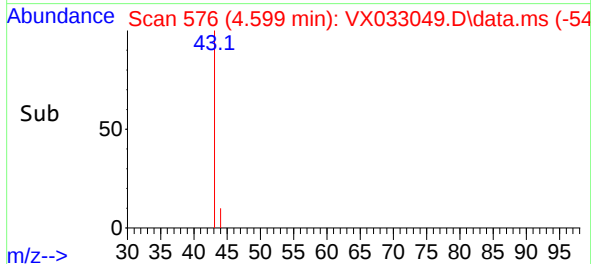

#38

Carbon Tetrachloride

Concen: 6.289 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07




Tgt Ion: 117 Resp: 13384


Ion Ratio Lower Upper

117 100

119 5.2 77.2 115.8#

121 0.0 25.8 38.6#

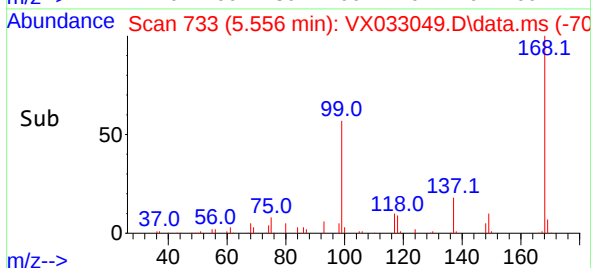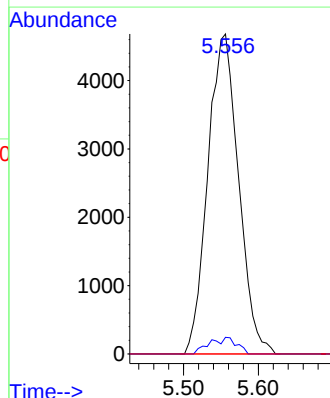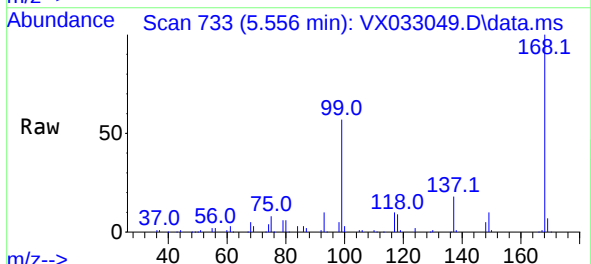



#39

Methylcyclohexane

Concen: 0.281 ug/l

RT: 7.385 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :

MW-43





Tgt Ion: 83 Resp: 614

Ion Ratio Lower Upper

83 100

55 57.4 58.4 87.6#

98 42.0 37.2 55.8

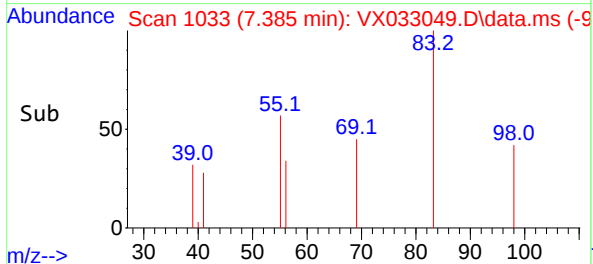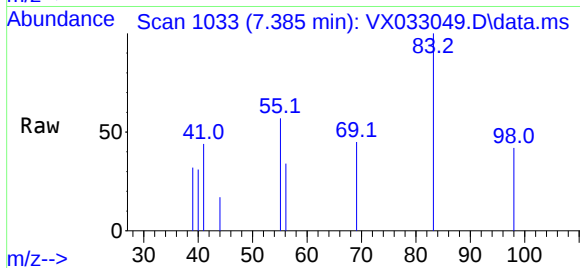

#40

Benzene

Concen: 0.607 ug/l

RT: 6.038 min Scan# 812

Delta R.T. 0.001 min

Lab File: VX033049.D




Acq: 24 Nov 2022 09:07


Tgt Ion: 78 Resp: 3266

Ion Ratio Lower Upper

78 100

77 25.9 19.0 28.4


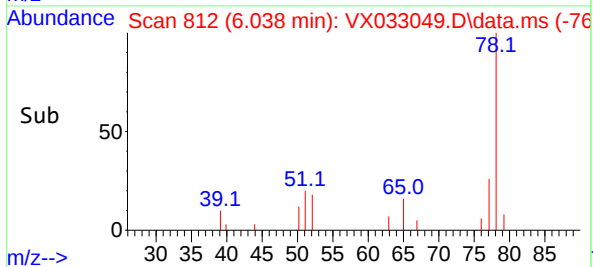

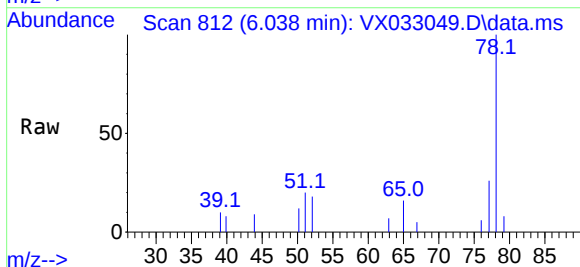




#50  
Toluene-d8  
Concen: 53.535 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 98 Resp: 192706  
Ion Ratio Lower Upper  
98 100  
100 64.4 50.9 76.3

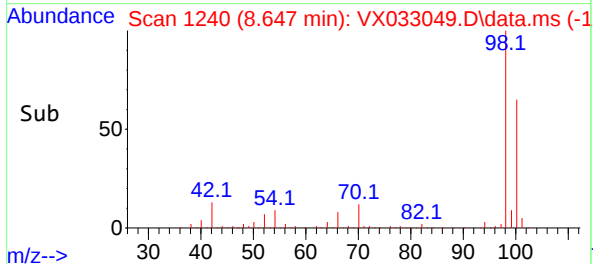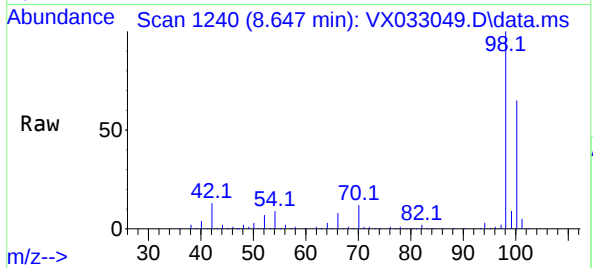

#55  
1,1,2-Trichloroethane  
Concen: 0.295 ug/l  
RT: 9.104 min Scan# 1315  
Delta R.T. -0.049 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 97 Resp: 425  
Ion Ratio Lower Upper  
97 100  
83 0.0 68.1 102.1#  
85 0.0 43.3 64.9#  
99 0.0 50.4 75.6#

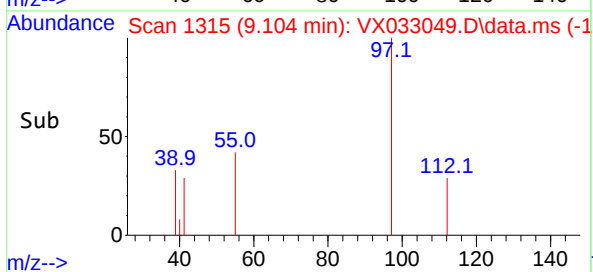



#62

4-Bromofluorobenzene

Concen: 44.252 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :

MW-43





Tgt Ion: 95 Resp: 69743

Ion Ratio Lower Upper

95 100

174 83.8 0.0 164.0

176 80.0 0.0 154.4

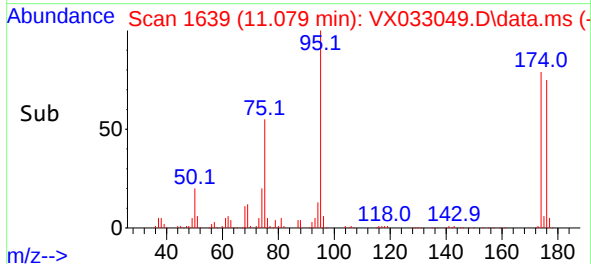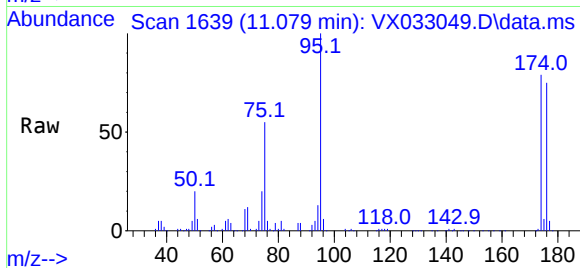

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07




Tgt Ion: 117 Resp: 189983


Ion Ratio Lower Upper

117 100

82 55.3 44.3 66.5

119 32.8 25.7 38.5


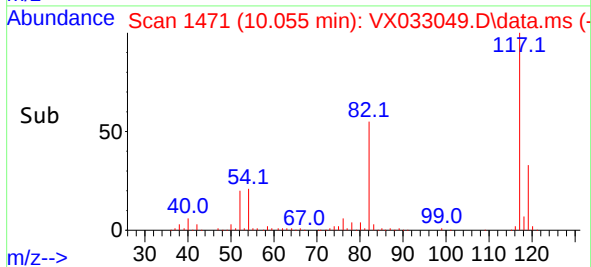

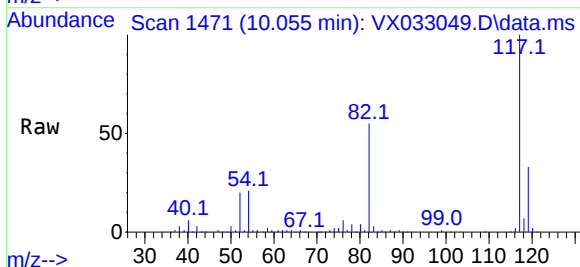




#67  
Ethyl Benzene  
Concen: 0.227 ug/l  
RT: 10.195 min Scan# 1494  
Delta R.T. 0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 91 Resp: 1527  
Ion Ratio Lower Upper  
91 100  
106 38.0 25.0 37.6#

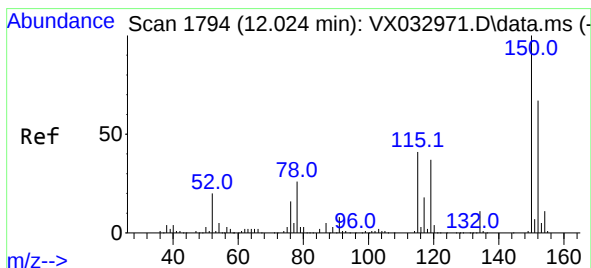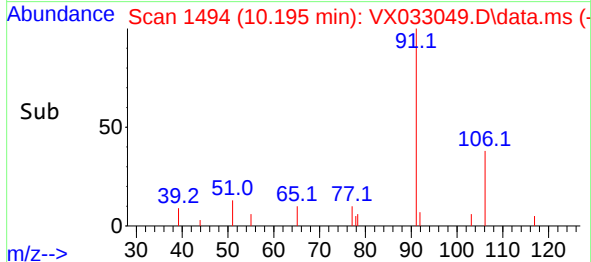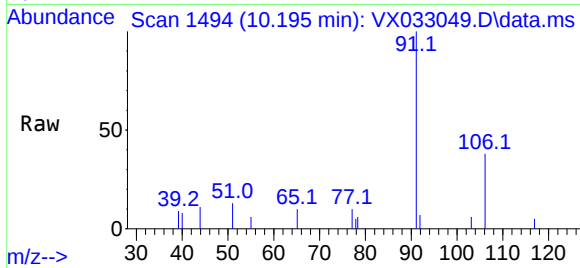

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 152 Resp: 89312  
Ion Ratio Lower Upper  
152 100  
115 60.1 44.0 132.0  
150 157.7 0.0 351.8


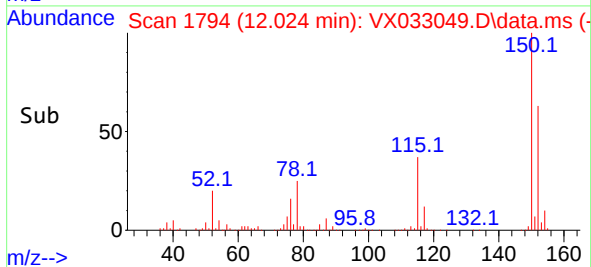

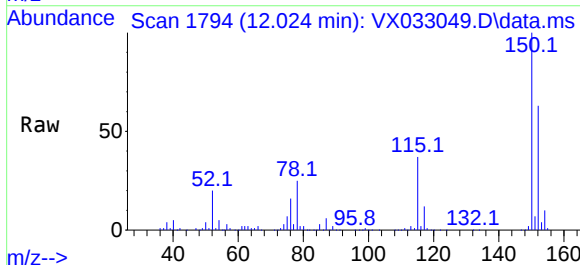




#73  
Isopropylbenzene  
Concen: 0.371 ug/l  
RT: 10.964 min Scan# 1639  
Delta R.T. 0.001 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion:105 Resp: 2368  
Ion Ratio Lower Upper  
105 100  
120 26.5 13.1 39.3

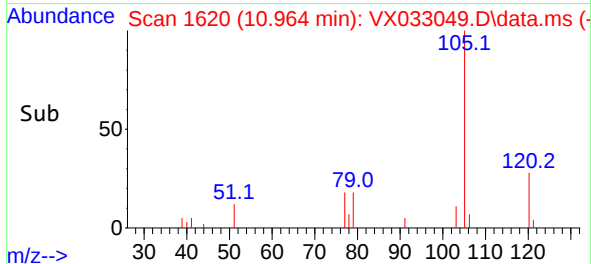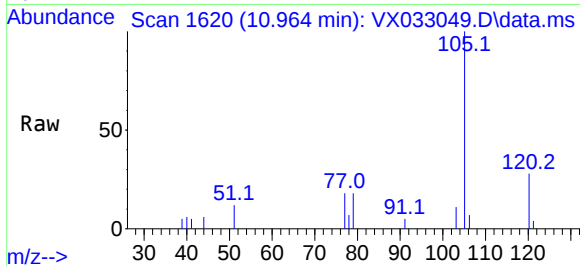

#76  
1,2,3-Trichloropropane  
Concen: 22.582 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.165 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 75 Resp: 38195  
Ion Ratio Lower Upper  
75 100  
77 0.8 20.0 60.0#


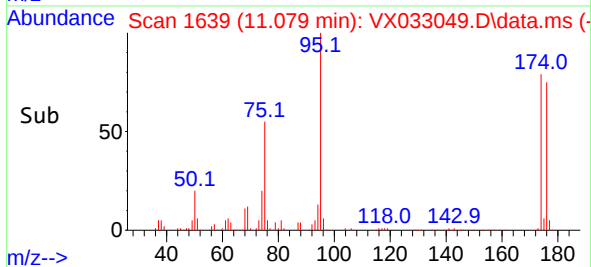

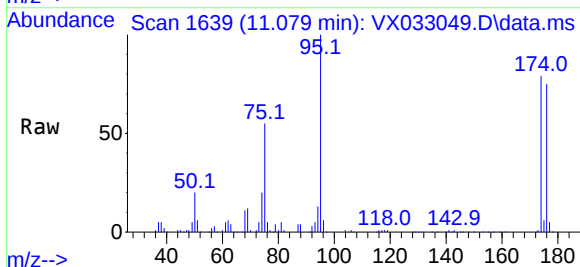




#78  
n-propylbenzene  
Concen: 0.456 ug/l  
RT: 11.305 min Scan# 1676  
Delta R.T. -0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 91 Resp: 3326  
Ion Ratio Lower Upper  
91 100  
120 21.0 11.6 34.8

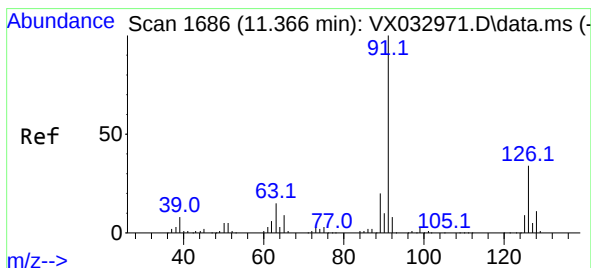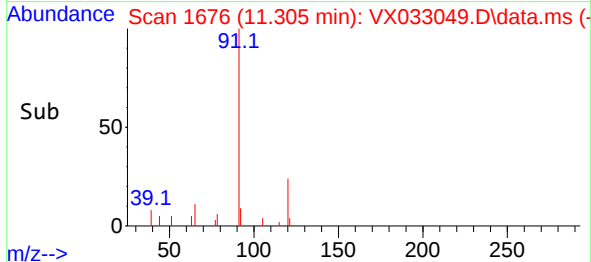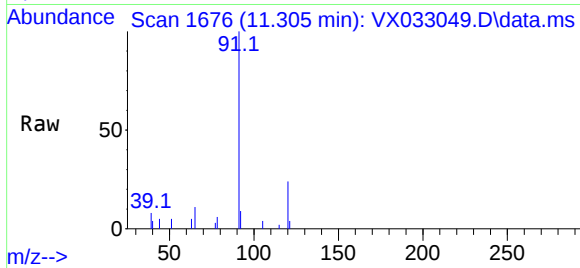

#79  
2-Chlorotoluene  
Concen: 0.750 ug/l  
RT: 11.305 min Scan# 1676  
Delta R.T. -0.061 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 91 Resp: 3326  
Ion Ratio Lower Upper  
91 100  
126 0.0 17.1 51.2#


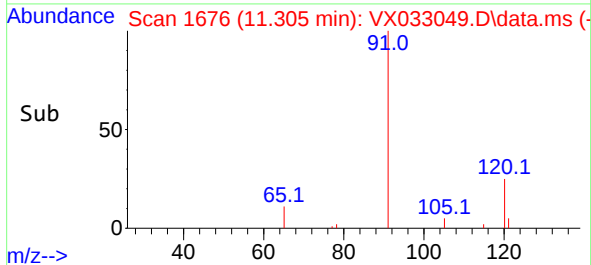

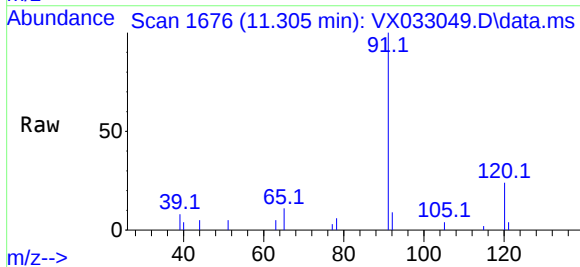




#80  
1,3,5-Trimethylbenzene  
Concen: 0.405 ug/l  
RT: 11.616 min Scan# 11  
Delta R.T. 0.165 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion:105 Resp: 2174  
Ion Ratio Lower Upper  
105 100  
120 31.5 23.6 71.0

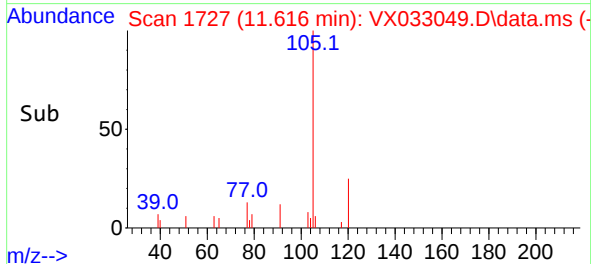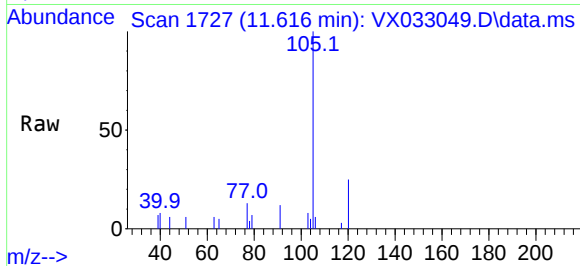

#81  
trans-1,4-Dichloro-2-butene  
Concen: 73.400 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.061 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 75 Resp: 38195  
Ion Ratio Lower Upper  
75 100  
53 0.0 86.9 130.3#  
89 0.0 38.3 57.5#


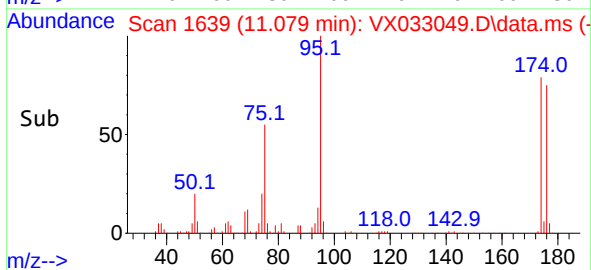

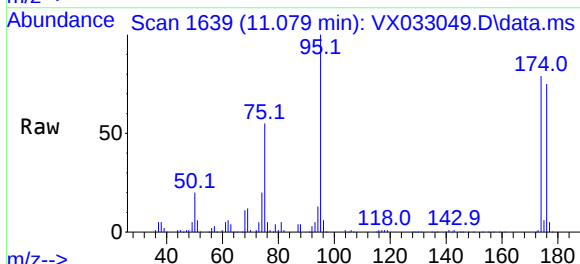




#82  
4-Chlorotoluene  
Concen: 0.640 ug/l  
RT: 11.305 min Scan# 11  
Delta R.T. -0.152 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43


Tgt Ion: 91 Resp: 3326  
Ion Ratio Lower Upper  
91 100  
126 0.0 14.8 44.4#

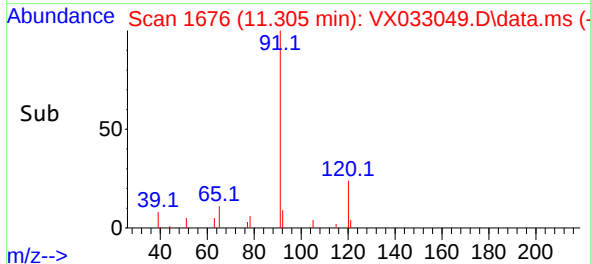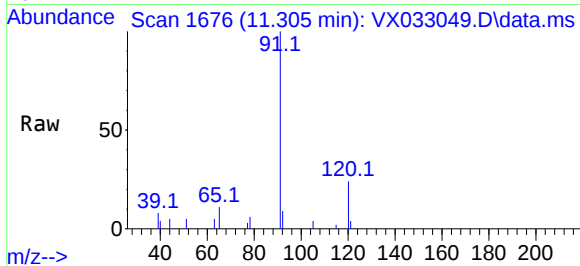

#84  
1,2,4-Trimethylbenzene  
Concen: 0.458 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. 0.006 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Tgt Ion: 105 Resp: 2446  
Ion Ratio Lower Upper  
105 100  
120 47.7 21.9 65.5

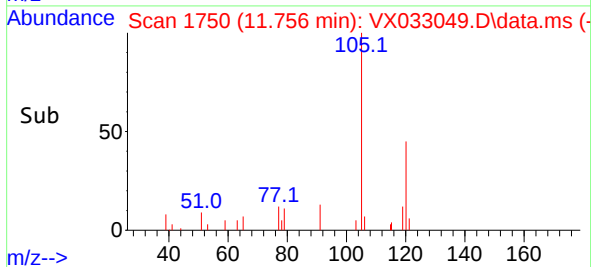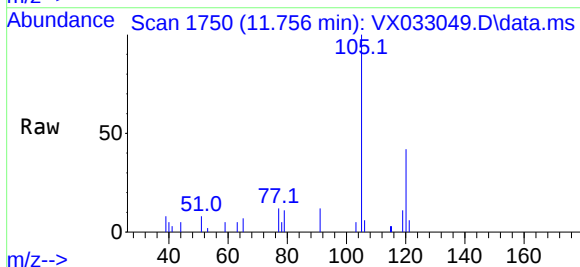



#89

n-Butylbenzene

Concen: 0.231 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX033049.D

Acq: 24 Nov 2022 09:07

Instrument :

MSVOA\_X

ClientSampleId :

MW-43





Tgt Ion: 91 Resp: 1075

Ion Ratio Lower Upper

91 100

92 42.0 26.2 78.6

134 64.3 12.9 38.6#

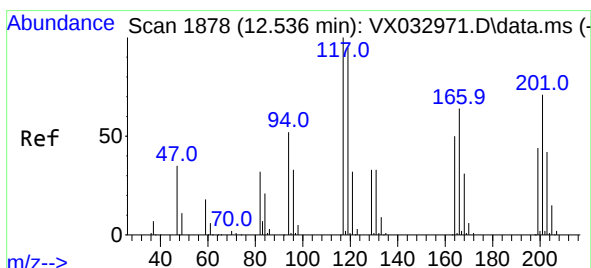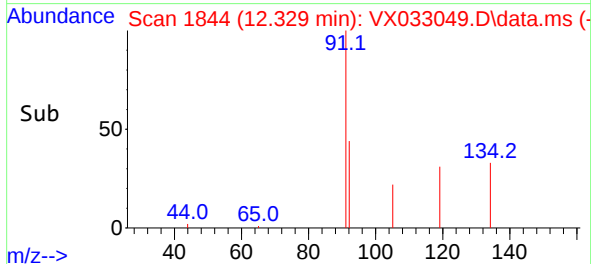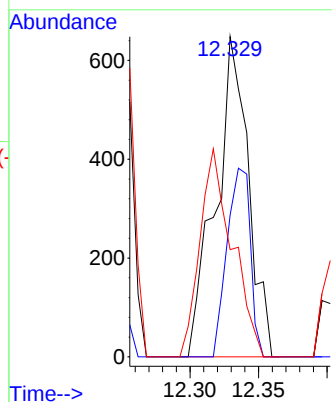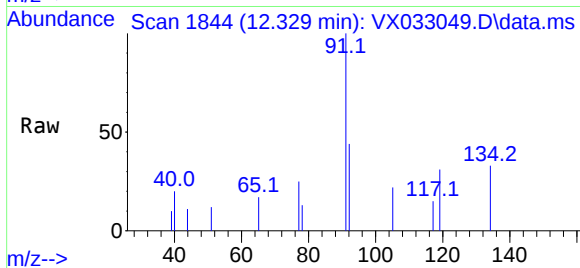

#90

Hexachloroethane

Concen: 0.411 ug/l

RT: 12.616 min Scan# 1891

Delta R.T. 0.074 min

Lab File: VX033049.D




Acq: 24 Nov 2022 09:07


Tgt Ion:117 Resp: 365

Ion Ratio Lower Upper

117 100


201 0.0 37.6 112.9#

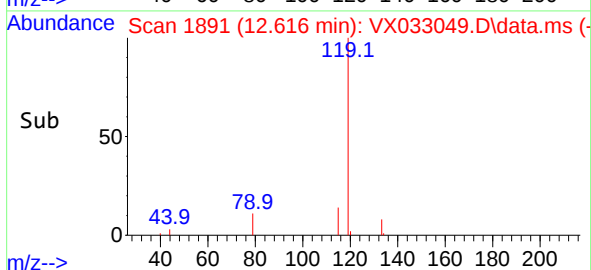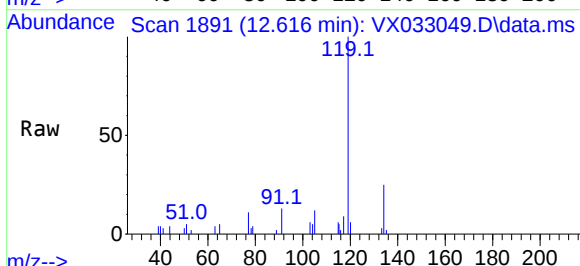

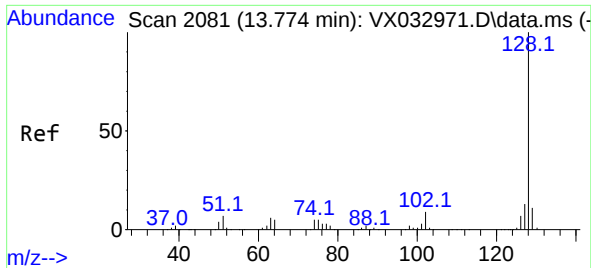

#95  
Naphthalene  
Concen: 0.326 ug/l  
RT: 13.780 min Scan# 2081  
Delta R.T. 0.000 min  
Lab File: VX033049.D  
Acq: 24 Nov 2022 09:07

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-43

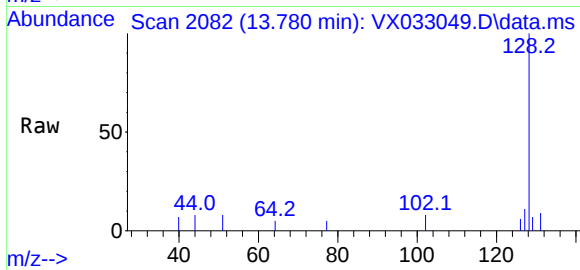

Tgt Ion:128 Resp: 1862  
Ion Ratio Lower Upper  
128 100  
127 11.0 10.2 15.4  
129 8.2 8.9 13.3#

