

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033025.D
 Acq On : 23 Nov 2022 17:20
 Operator : JC/MD
 Sample : N5744-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Nov 24 04:07:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 22 13:58:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	122253	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	199970	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177075	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82652	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	66403	55.960	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	111.920%
35) Dibromofluoromethane	5.391	113	53126	47.124	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.240%
50) Toluene-d8	8.647	98	180485	53.354	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.700%
62) 4-Bromofluorobenzene	11.079	95	64902	43.826	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.660%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033025.D
Acq On : 23 Nov 2022 17:20
Operator : JC/MD
Sample : N5744-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Nov 24 04:07:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration




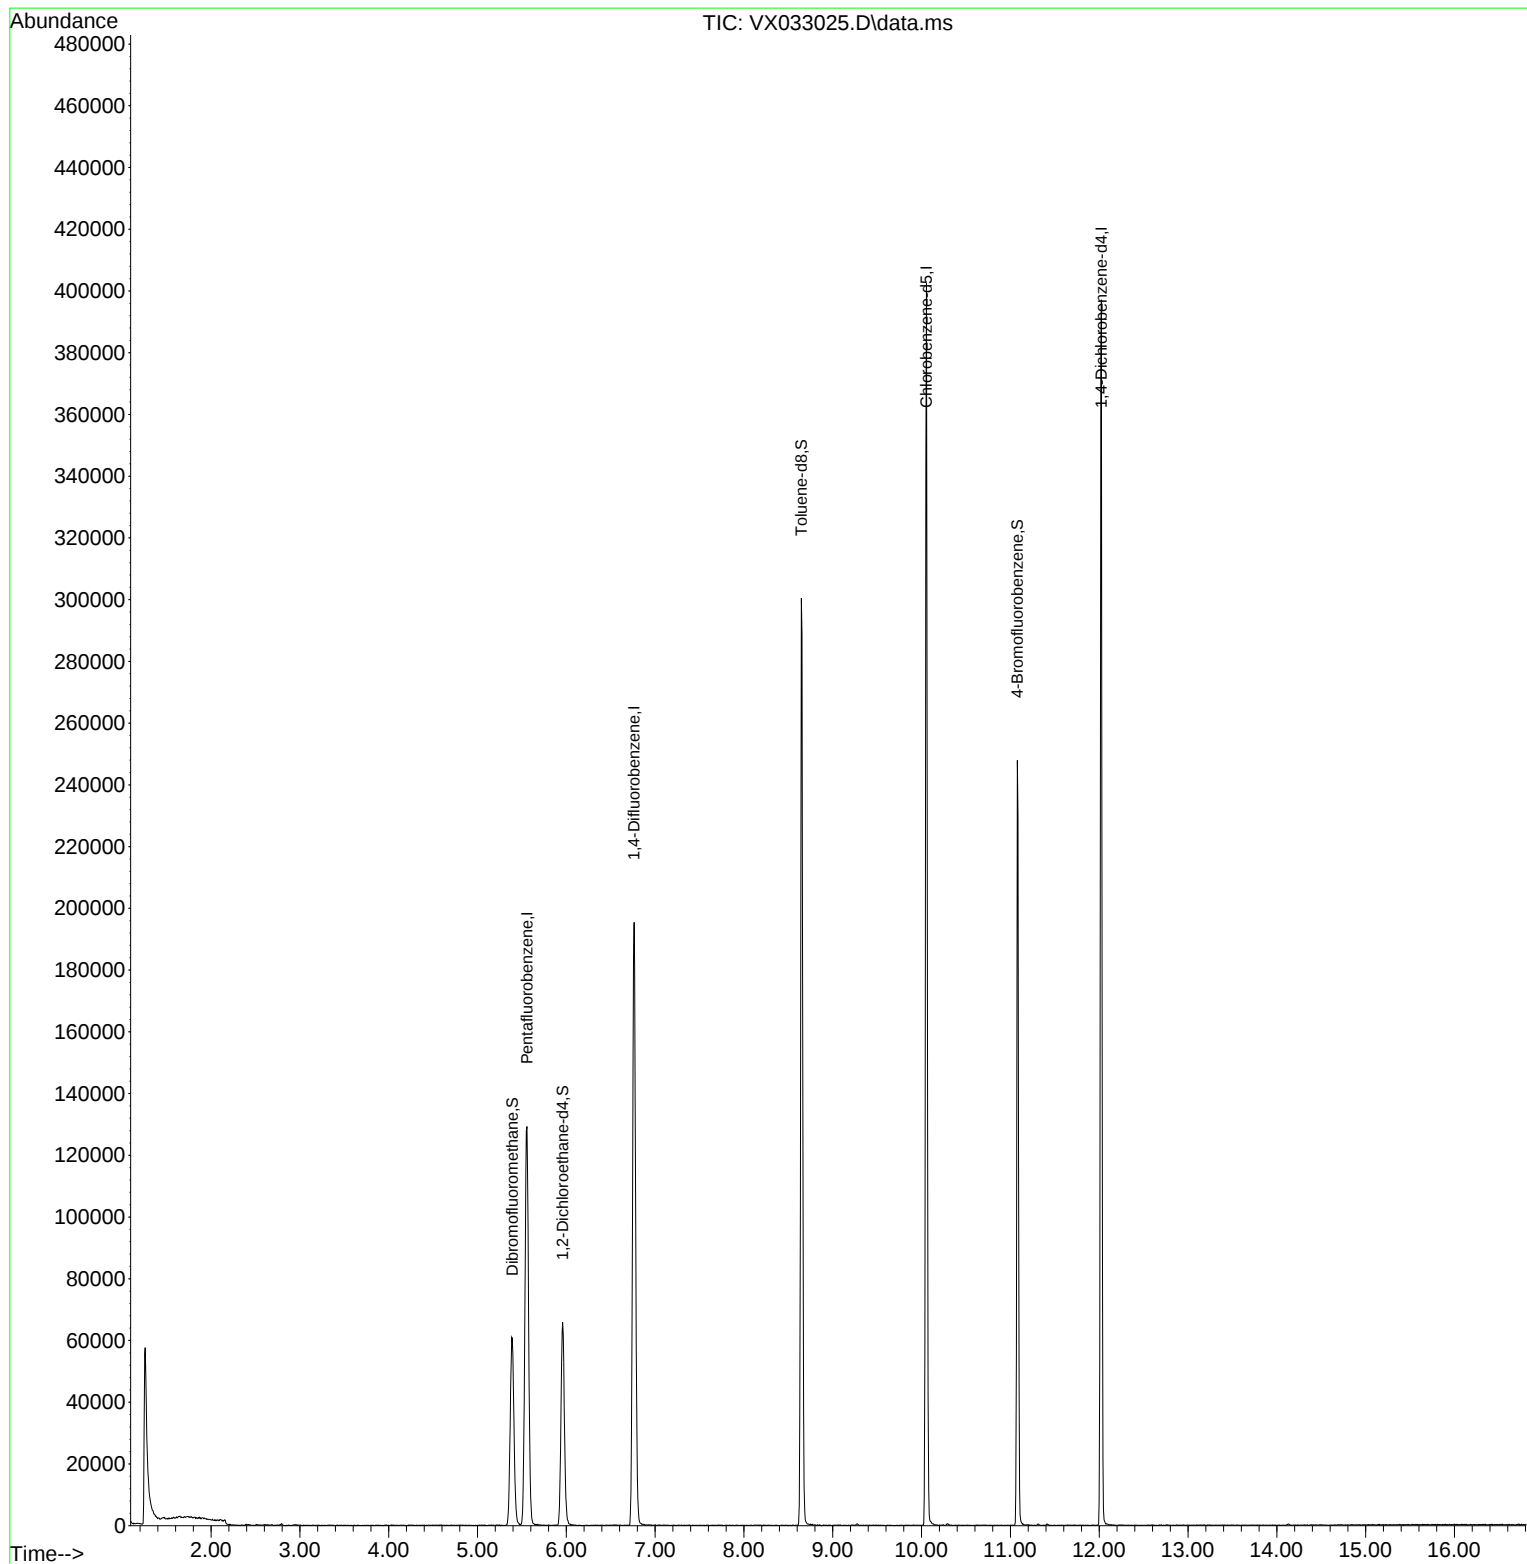




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:168 Resp: 122253
Ion Ratio Lower Upper
168 100
99 57.4 46.1 69.1

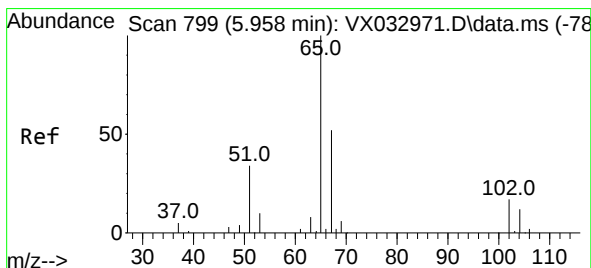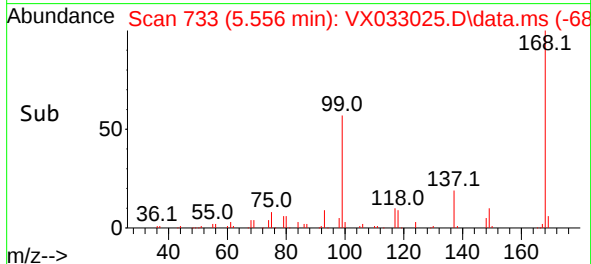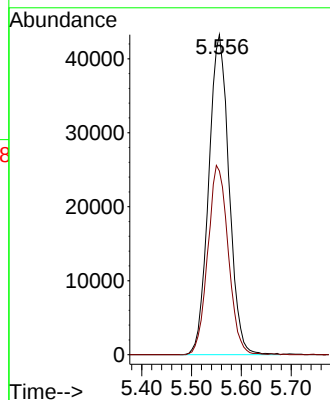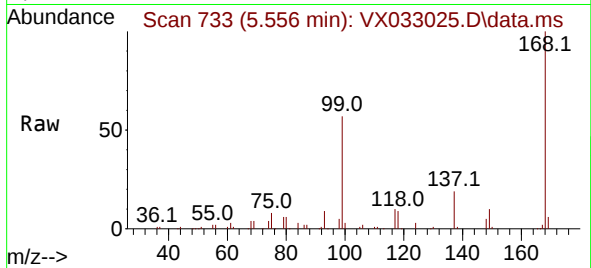

#33
1,2-Dichloroethane-d4
Concen: 55.960 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20

Tgt Ion: 65 Resp: 66403
Ion Ratio Lower Upper
65 100
67 49.7 0.0 101.8

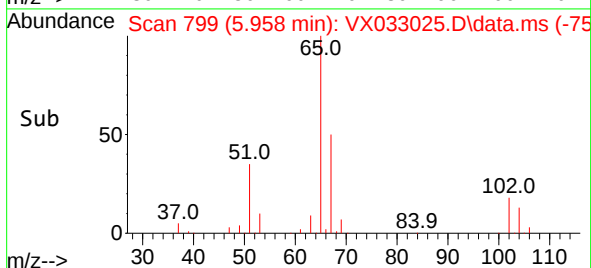
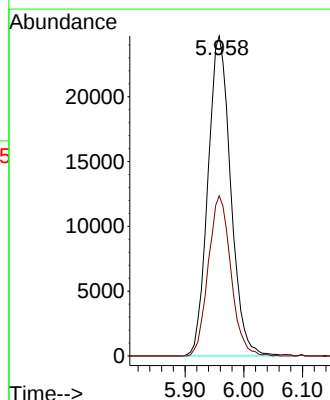
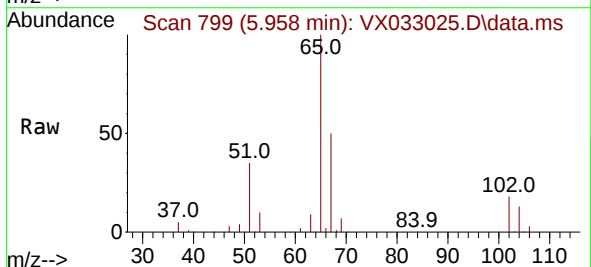




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 199970
Ion Ratio Lower Upper
114 100
63 19.7 0.0 41.6
88 14.8 0.0 33.4

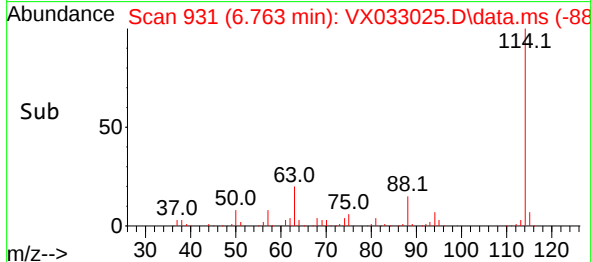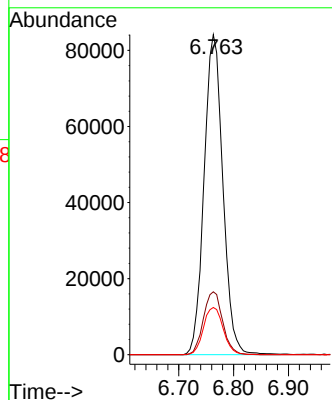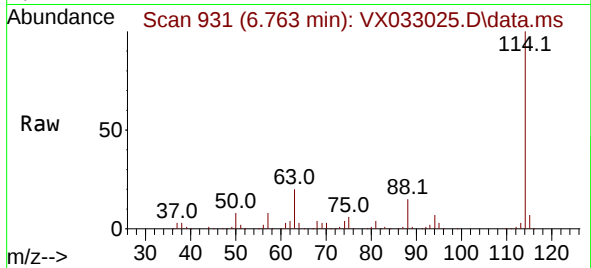

#35
Dibromofluoromethane
Concen: 47.124 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20

Tgt Ion:113 Resp: 53126
Ion Ratio Lower Upper
113 100
111 101.8 82.4 123.6
192 18.9 15.4 23.2


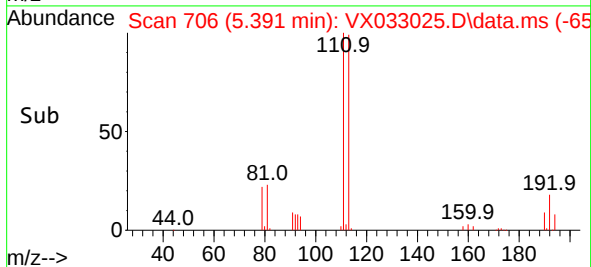
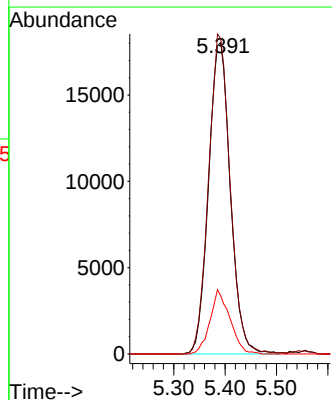
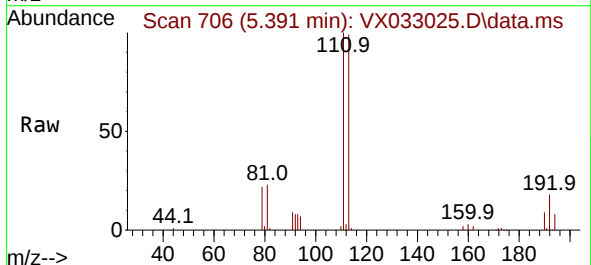


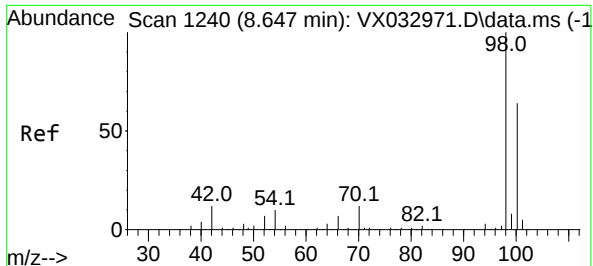

#50
Toluene-d8
Concen: 53.354 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 180485
Ion Ratio Lower Upper
98 100
100 63.2 50.9 76.3

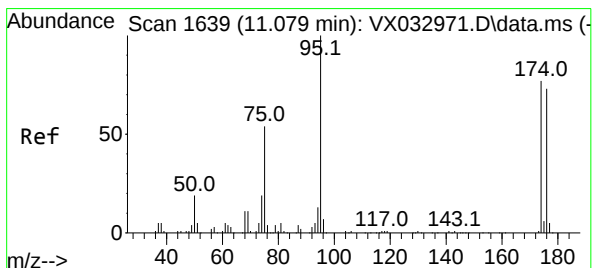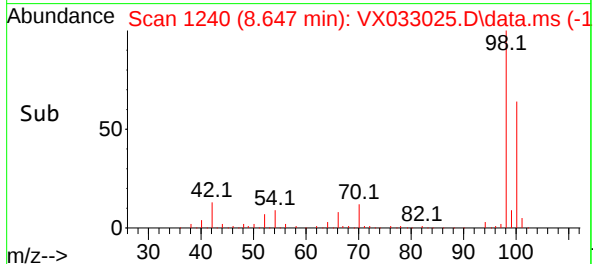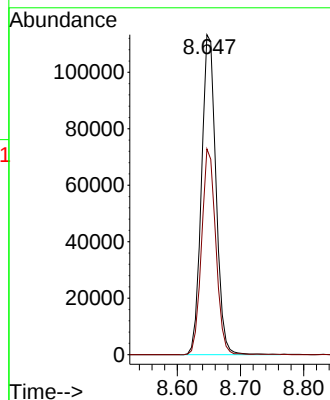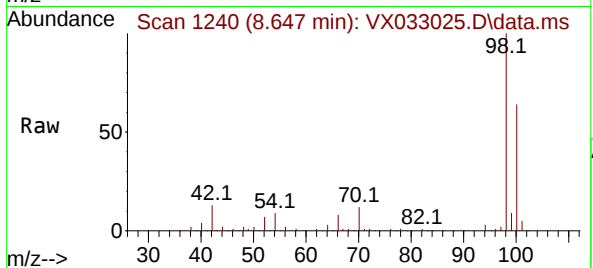

#62
4-Bromofluorobenzene
Concen: 43.826 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20

Tgt Ion: 95 Resp: 64902
Ion Ratio Lower Upper
95 100
174 80.3 0.0 164.0
176 77.7 0.0 154.4


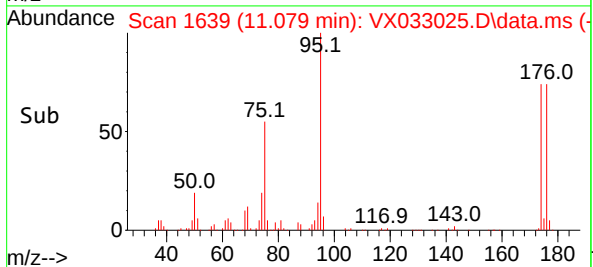
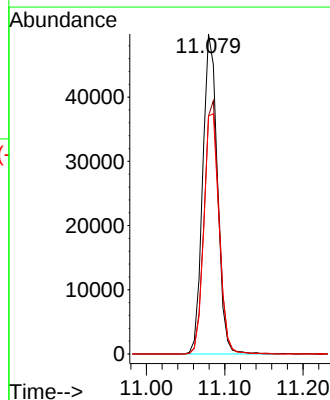
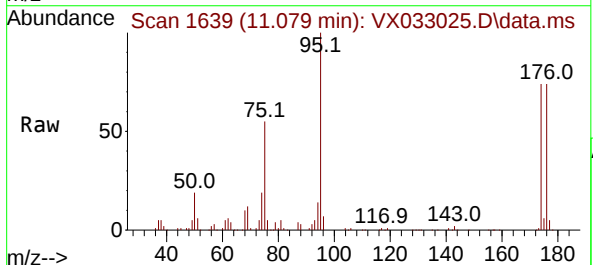


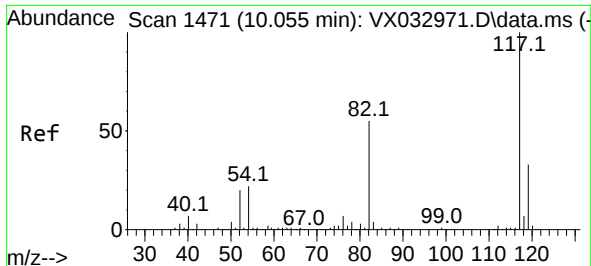

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 177075
Ion Ratio Lower Upper
117 100
82 56.7 44.3 66.5
119 32.3 25.7 38.5

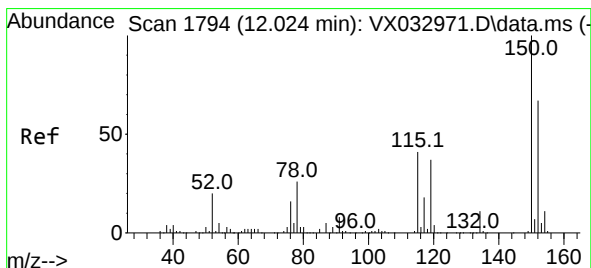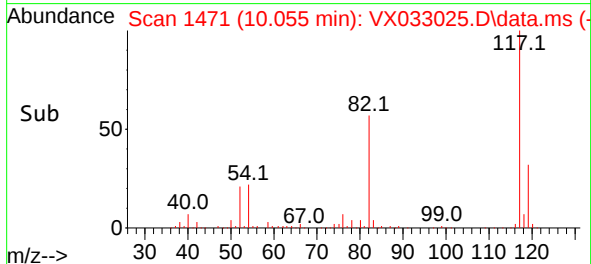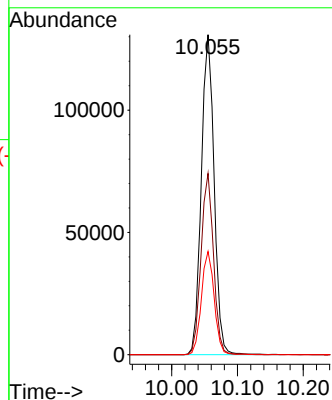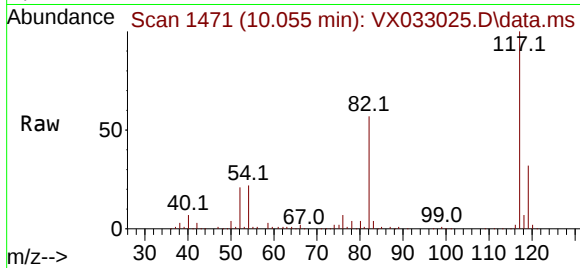

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033025.D
Acq: 23 Nov 2022 17:20

Tgt Ion:152 Resp: 82652
Ion Ratio Lower Upper
152 100
115 59.6 44.0 132.0
150 156.0 0.0 351.8

