

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033010.D
 Acq On : 23 Nov 2022 11:31
 Operator : JC/MD
 Sample : VX1123MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1123MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	298	305	312	rVB3	3007	6839	1.14%	0.197%
2	5.385	694	705	718	rBV	73597	210342	35.19%	6.062%
3	5.550	722	732	747	rVV	149915	418095	69.95%	12.049%
4	5.958	789	799	816	rBV	75998	204551	34.22%	5.895%
5	6.763	920	931	942	rBV	216816	517528	86.58%	14.914%
6	8.647	1232	1240	1251	rBV	358598	563070	94.20%	16.227%
7	10.055	1465	1471	1481	rBV	439268	597747	100.00%	17.226%
8	11.079	1634	1639	1651	rBV	303341	384054	64.25%	11.068%
9	12.024	1788	1794	1803	rBV	454174	560602	93.79%	16.156%
10	13.725	2069	2073	2077	rBV2	6465	7210	1.21%	0.208%




Sum of corrected areas: 3470038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033010.D
Acq On : 23 Nov 2022 11:31
Operator : JC/MD
Sample : VX1123MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1123MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

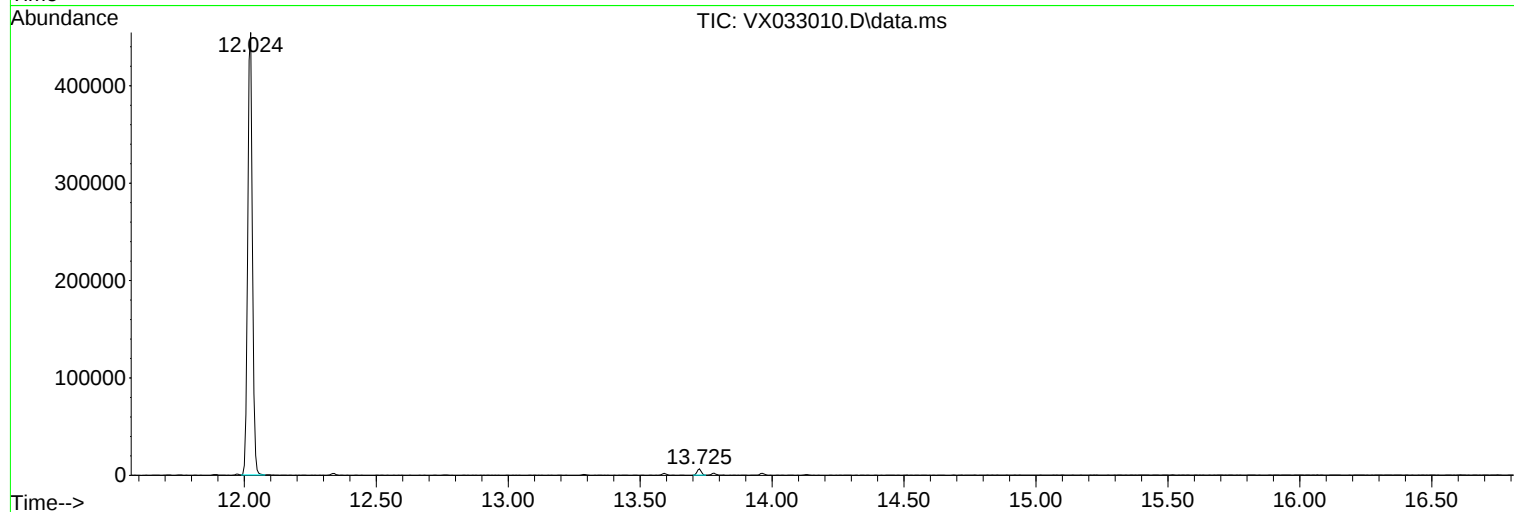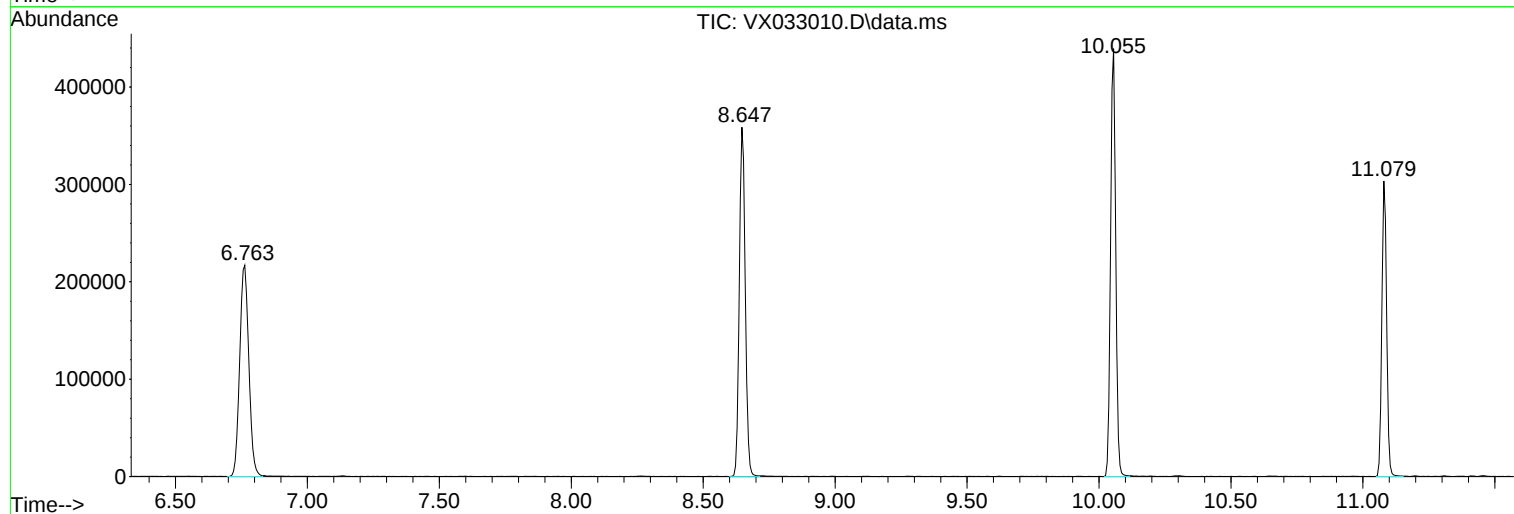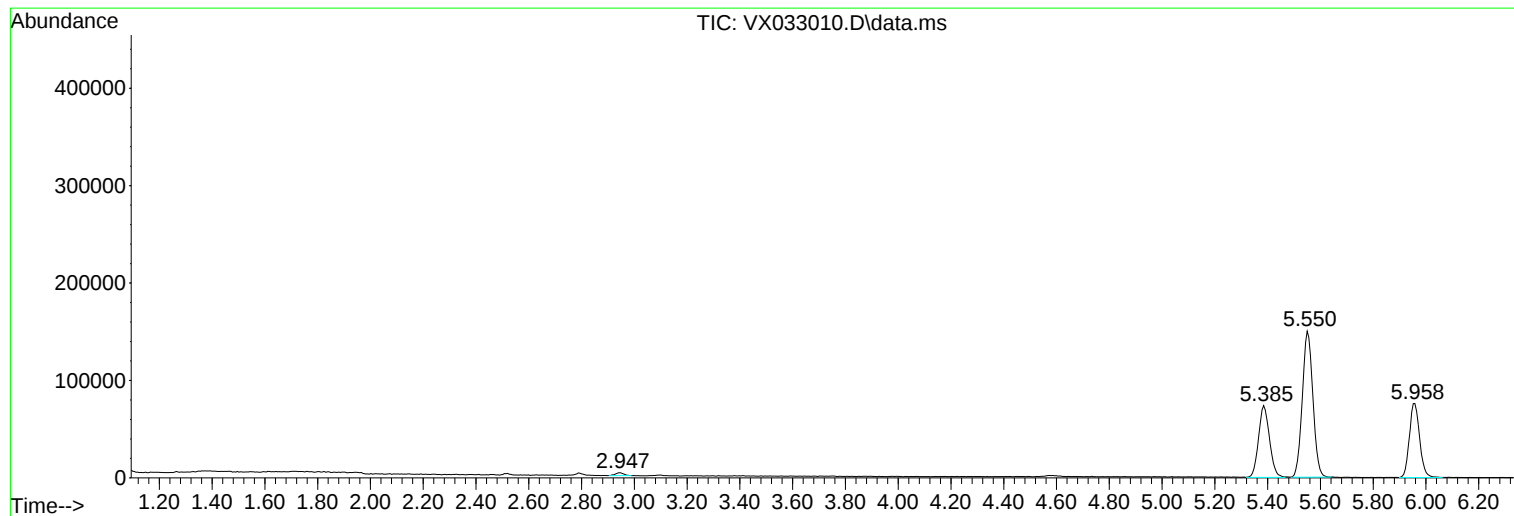

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033010.D
Acq On : 23 Nov 2022 11:31
Operator : JC/MD
Sample : VX1123MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1123MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033010.D
Acq On : 23 Nov 2022 11:31
Operator : JC/MD
Sample : VX1123MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1123MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc