

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033023.D
 Acq On : 23 Nov 2022 16:34
 Operator : JC/MD
 Sample : N5741-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-24

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	47	rBV	247100	375350	67.64%	10.385%
2	2.124	168	170	178	rVB	3068	5654	1.02%	0.156%
3	3.117	323	333	341	rBV	25521	60504	10.90%	1.674%
4	5.391	693	706	720	rBV	62712	181170	32.65%	5.013%
5	5.556	722	733	747	rVB2	128764	368696	66.44%	10.201%
6	5.958	786	799	811	rBV	67286	179105	32.28%	4.955%
7	6.763	920	931	944	rBV	202071	468367	84.40%	12.959%
8	8.647	1234	1240	1250	rBV	307463	488550	88.04%	13.517%
9	10.055	1465	1471	1480	rBV	412281	554923	100.00%	15.353%
10	11.079	1634	1639	1649	rBV	256982	333501	60.10%	9.227%
11	12.024	1789	1794	1802	rVV	411625	518192	93.38%	14.337%
12	12.244	1824	1830	1838	rBV2	18021	24664	4.44%	0.682%
13	12.701	1900	1905	1910	rVB	12224	15218	2.74%	0.421%
14	12.920	1936	1941	1945	rBV	15313	18370	3.31%	0.508%
15	13.548	2039	2044	2046	rBV	4910	6685	1.20%	0.185%
16	13.664	2060	2063	2068	rVB2	4720	7166	1.29%	0.198%
17	14.079	2126	2131	2137	rBV	6892	8209	1.48%	0.227%




Sum of corrected areas: 3614324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033023.D
Acq On : 23 Nov 2022 16:34
Operator : JC/MD
Sample : N5741-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

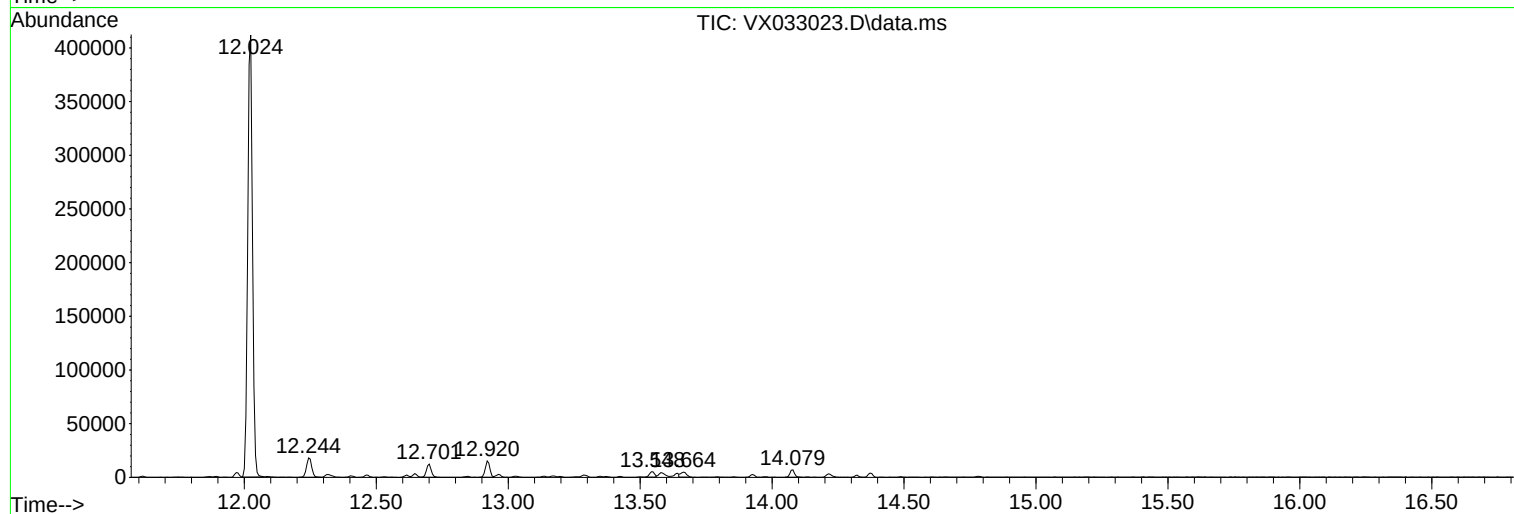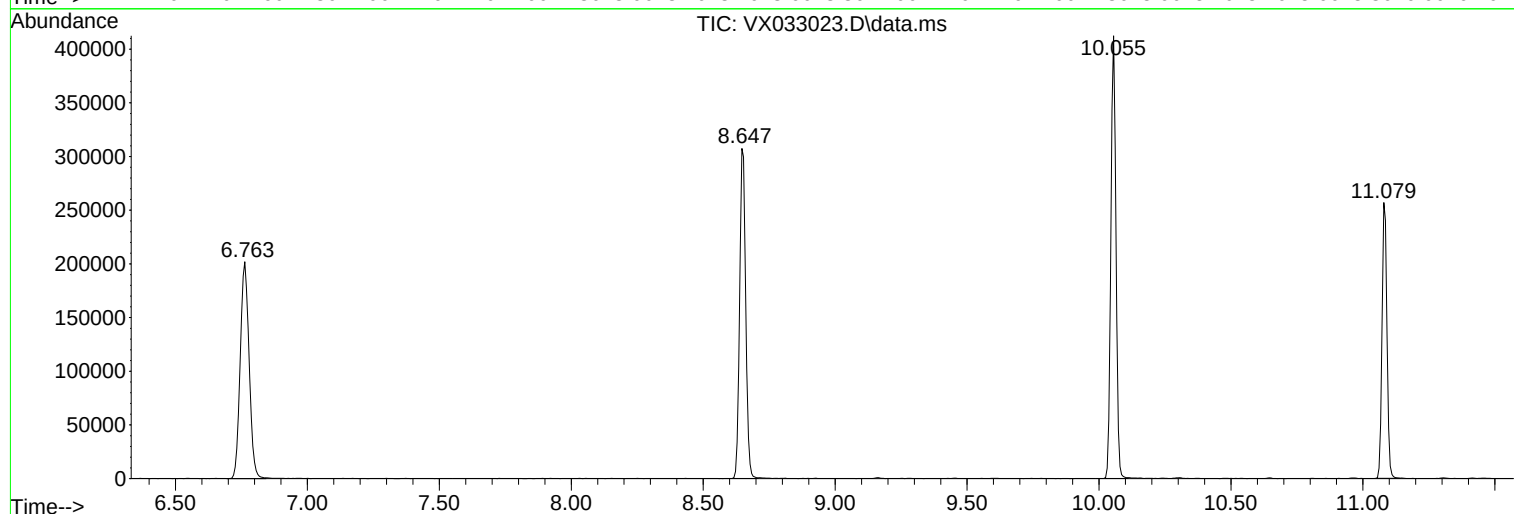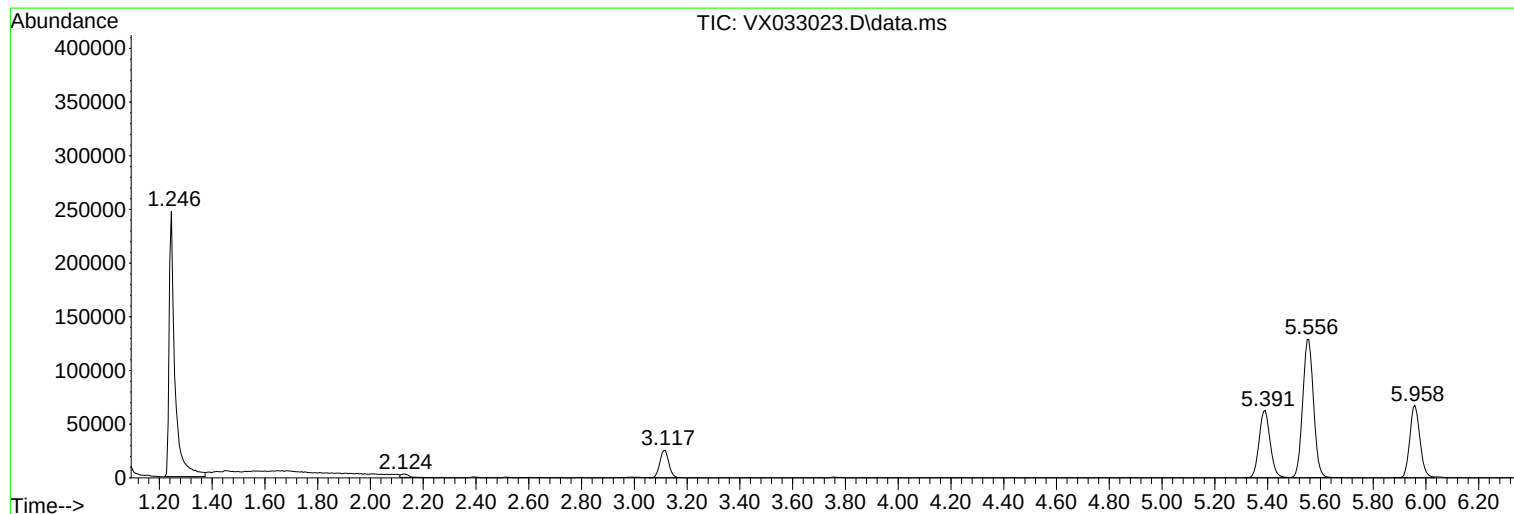

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033023.D
Acq On : 23 Nov 2022 16:34
Operator : JC/MD
Sample : N5741-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033023.D
Acq On : 23 Nov 2022 16:34
Operator : JC/MD
Sample : N5741-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------