

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033024.D
 Acq On : 23 Nov 2022 16:57
 Operator : JC/MD
 Sample : N5730-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP06-20221118

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	50	rBV	207378	337165	59.88%	9.567%
2	2.947	294	305	315	rBB2	9737	23198	4.12%	0.658%
3	3.611	406	414	422	rVB3	2822	6374	1.13%	0.181%
4	4.587	559	574	584	rBV2	2952	11296	2.01%	0.321%
5	5.391	695	706	721	rBV	62749	183595	32.61%	5.209%
6	5.556	721	733	745	rBV	133330	378241	67.18%	10.732%
7	5.958	790	799	816	rBV2	66657	180701	32.09%	5.127%
8	6.763	921	931	945	rBV	205817	481835	85.58%	13.671%
9	8.647	1234	1240	1249	rBV	312107	495969	88.09%	14.072%
10	10.055	1465	1471	1486	rBV	426767	563050	100.00%	15.976%
11	11.079	1634	1639	1657	rVB	265689	338071	60.04%	9.592%
12	12.024	1789	1794	1807	rVB	418100	524899	93.22%	14.893%




Sum of corrected areas: 3524394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033024.D
Acq On : 23 Nov 2022 16:57
Operator : JC/MD
Sample : N5730-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

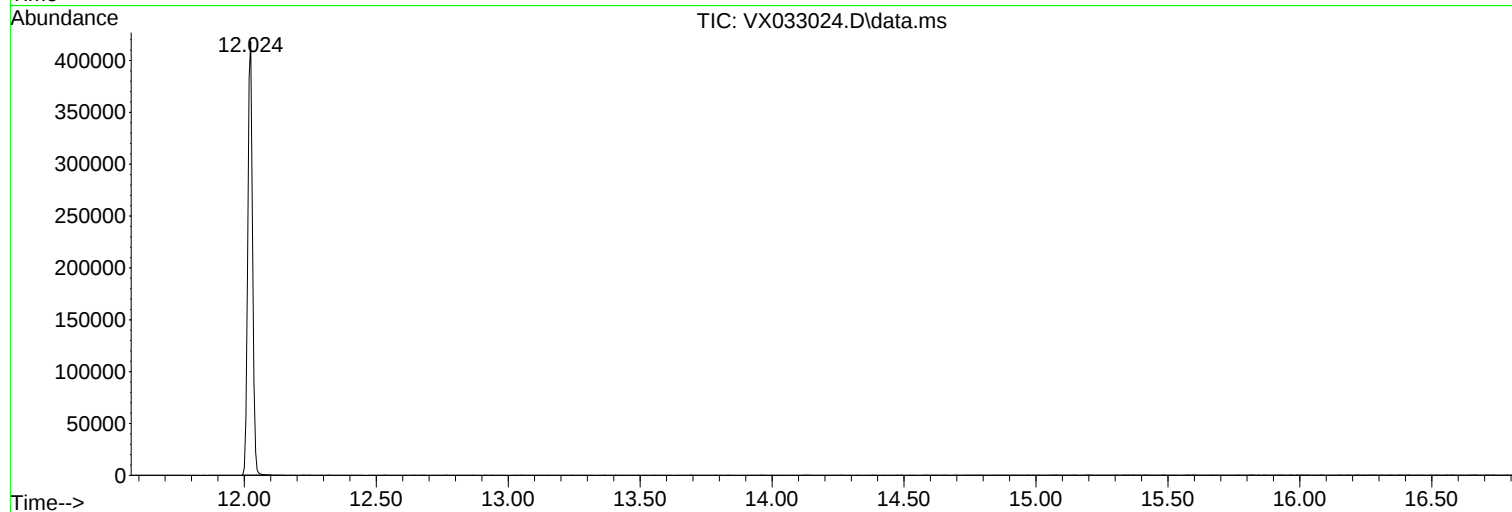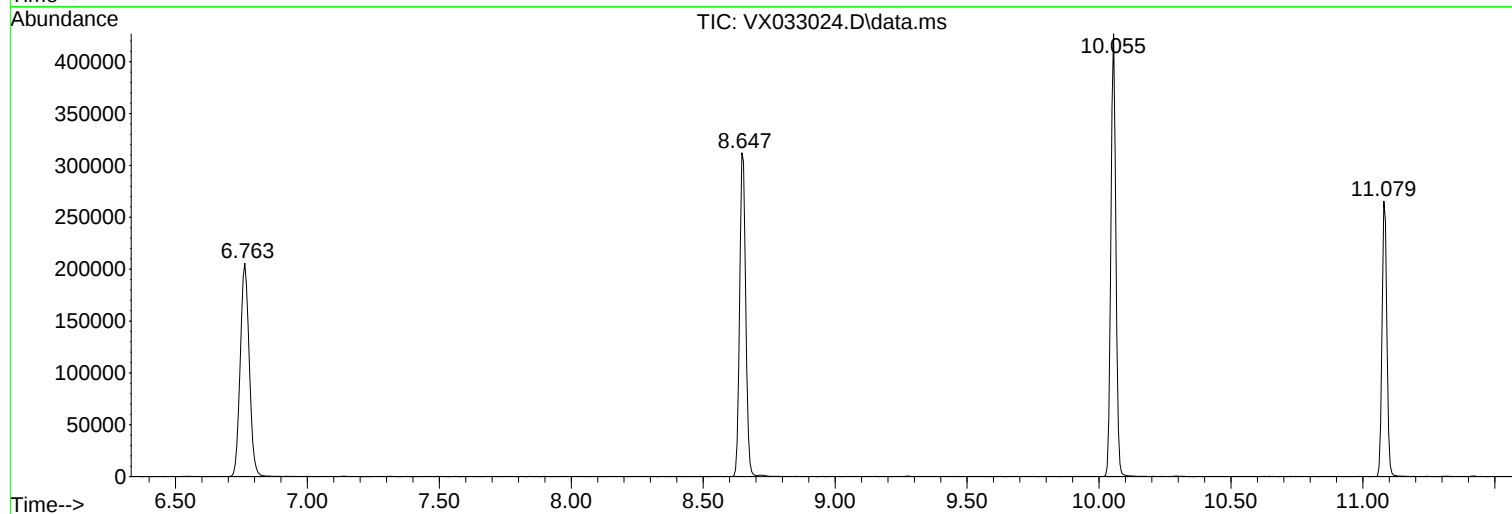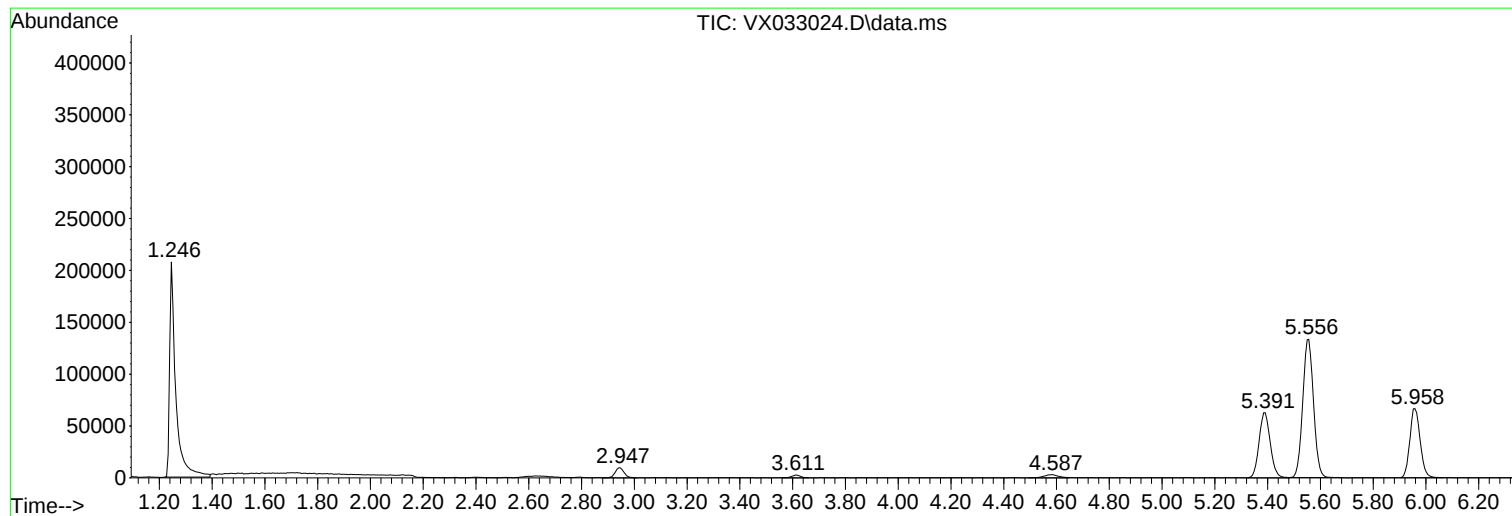

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033024.D
Acq On : 23 Nov 2022 16:57
Operator : JC/MD
Sample : N5730-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033024.D
Acq On : 23 Nov 2022 16:57
Operator : JC/MD
Sample : N5730-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20221118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc