

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
 Data File : VX033039.D
 Acq On : 24 Nov 2022 05:18
 Operator : JC/MD
 Sample : N5741-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-31

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.154	7	11	18	rVB2	15200	19697	1.43%	0.340%
2	1.301	30	35	43	rBV	9828	25212	1.83%	0.435%
3	3.002	300	314	323	rVV2	10187	42941	3.12%	0.741%
4	3.111	323	332	352	rVB	598135	1376403	100.00%	23.742%
5	3.758	428	438	447	rBV2	9590	25513	1.85%	0.440%
6	4.306	518	528	537	rVB2	5140	14101	1.02%	0.243%
7	5.385	694	705	716	rBV	68413	201825	14.66%	3.481%
8	5.550	723	732	756	rVB	144353	408565	29.68%	7.047%
9	5.958	789	799	806	rBV	74193	197593	14.36%	3.408%
10	6.038	806	812	826	rVB2	59451	158343	11.50%	2.731%
11	6.763	922	931	942	rBV	217409	516151	37.50%	8.903%
12	8.647	1234	1240	1249	rBV	343011	539485	39.20%	9.306%
13	8.958	1283	1291	1300	rBV	15265	24431	1.77%	0.421%
14	9.049	1300	1306	1312	rBV	14741	23853	1.73%	0.411%
15	10.055	1465	1471	1482	rBV	442957	596982	43.37%	10.297%
16	10.195	1489	1494	1500	rBV	76463	99962	7.26%	1.724%
17	10.305	1506	1512	1518	rVB	21733	29328	2.13%	0.506%
18	10.640	1563	1567	1573	rVB	20450	27269	1.98%	0.470%
19	10.964	1615	1620	1625	rBV	24817	31239	2.27%	0.539%
20	11.079	1634	1639	1650	rBV	293093	378441	27.49%	6.528%
21	11.305	1672	1676	1685	rVB	18960	23129	1.68%	0.399%
22	11.616	1721	1727	1736	rVB	29610	37790	2.75%	0.652%
23	11.756	1745	1750	1757	rVB	12757	16642	1.21%	0.287%
24	12.024	1788	1794	1800	rBV	446367	577435	41.95%	9.960%
25	12.085	1800	1804	1811	rVB	21461	28467	2.07%	0.491%
26	12.244	1823	1830	1835	rBV	112124	140472	10.21%	2.423%
27	12.701	1900	1905	1912	rVB2	30013	43691	3.17%	0.754%
28	12.920	1934	1941	1945	rBV	13282	17829	1.30%	0.308%
29	13.286	1997	2001	2006	rVV2	23770	33097	2.40%	0.571%
30	13.341	2006	2010	2017	rVV2	16734	22338	1.62%	0.385%
31	13.427	2019	2024	2030	rVB2	9947	14629	1.06%	0.252%
32	13.548	2040	2044	2047	rBV	12288	16763	1.22%	0.289%
33	13.774	2074	2081	2090	rVB	25609	37451	2.72%	0.646%
34	14.371	2175	2179	2184	rVB2	17173	21438	1.56%	0.370%
35	14.780	2241	2246	2250	rBV2	19263	28892	2.10%	0.498%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033039.D
Acq On : 24 Nov 2022 05:18
Operator : JC/MD
Sample : N5741-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-31

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260




Sum of corrected areas: 5797397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033039.D
Acq On : 24 Nov 2022 05:18
Operator : JC/MD
Sample : N5741-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

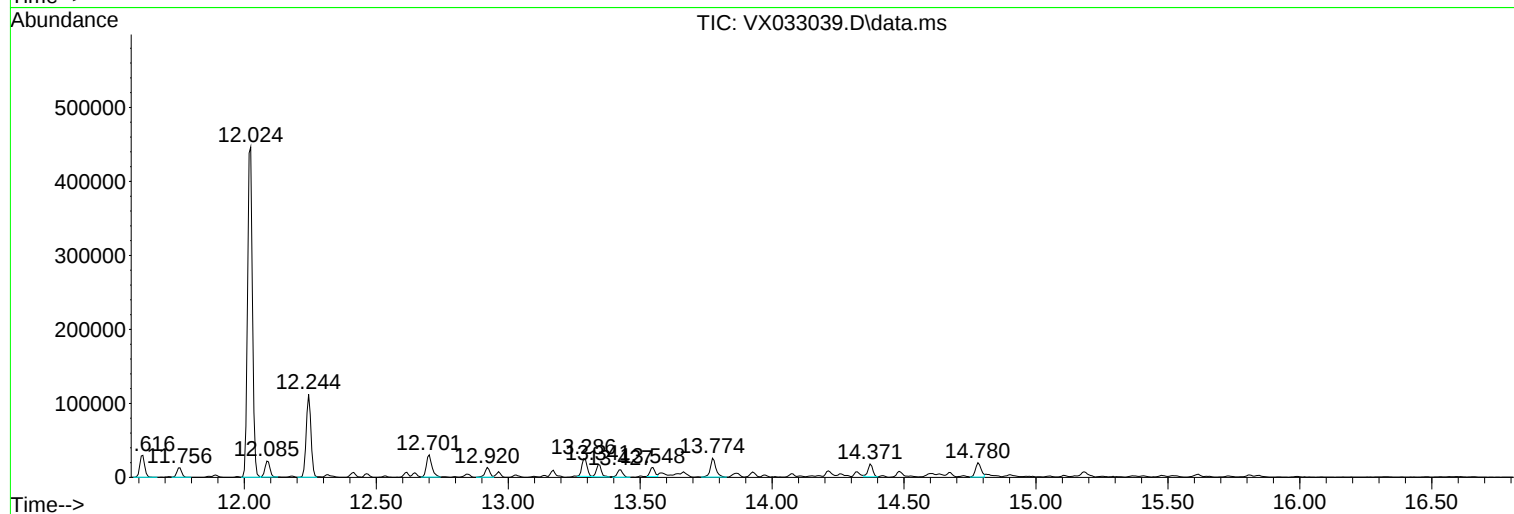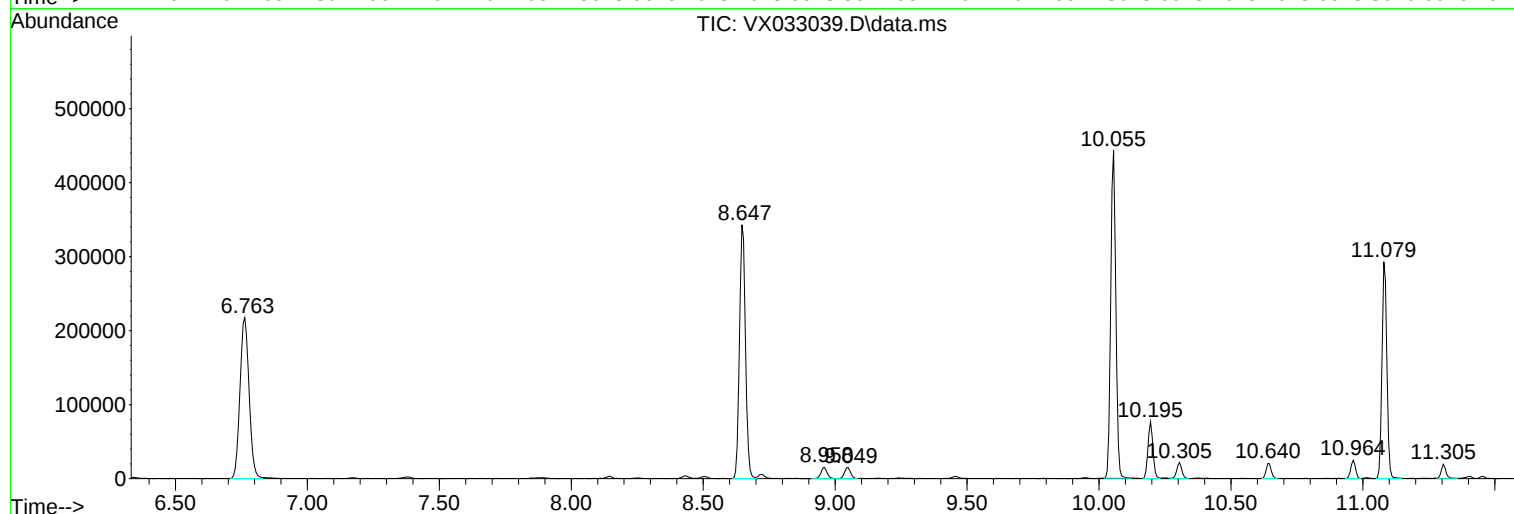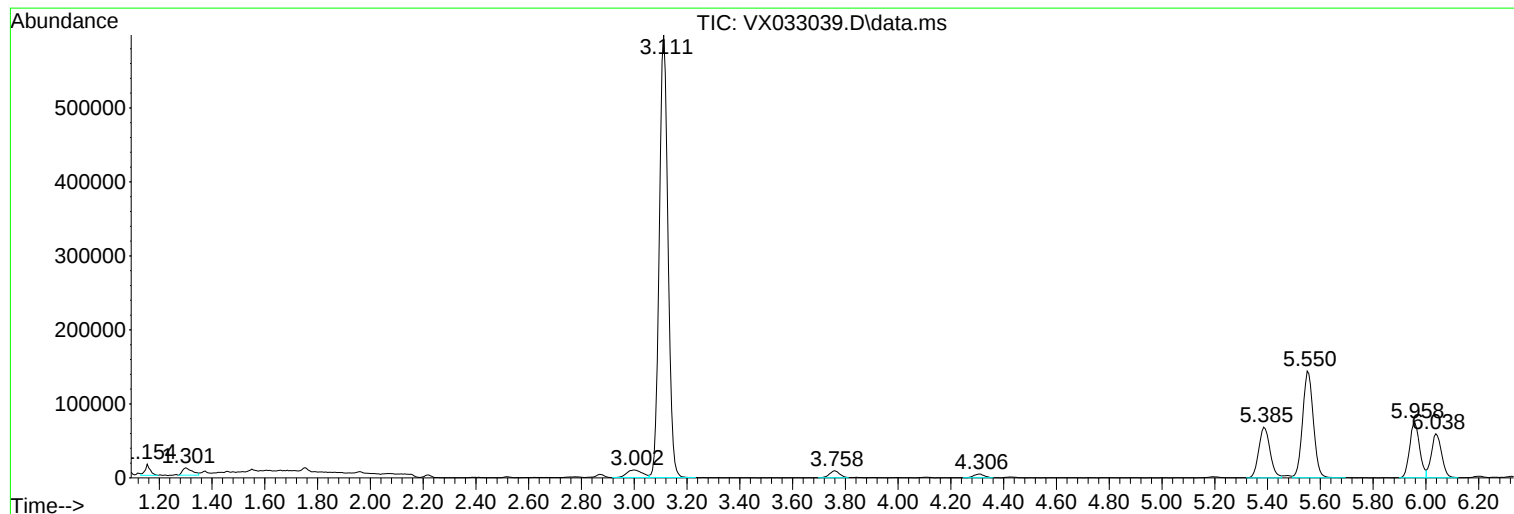

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033039.D
Acq On : 24 Nov 2022 05:18
Operator : JC/MD
Sample : N5741-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-31










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.244	12.16 ug/l	140472	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	87
2			Benzene, 1-ethenyl-4-methyl-	118	C9H10	000622-97-9	83
3			Benzene, 1-ethenyl-2-methyl-	118	C9H10	000611-15-4	81
4			Delatacyclene	118	C9H10	007785-10-6	64
5			Benzene, cyclopropyl-	118	C9H10	000873-49-4	59

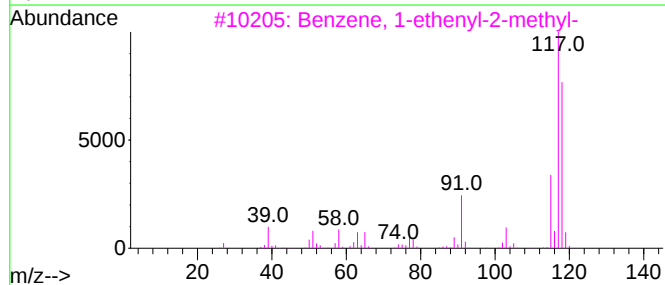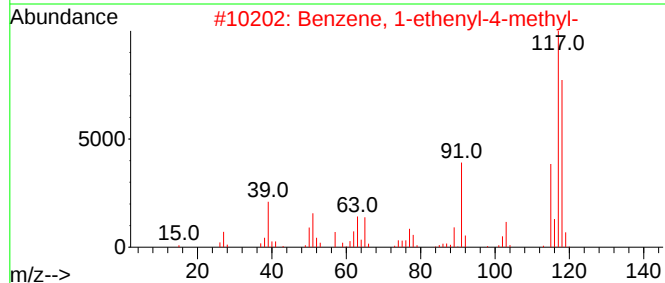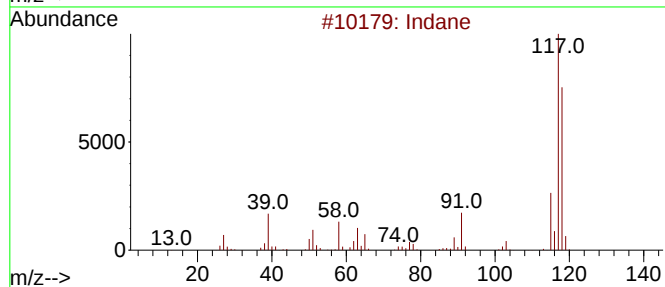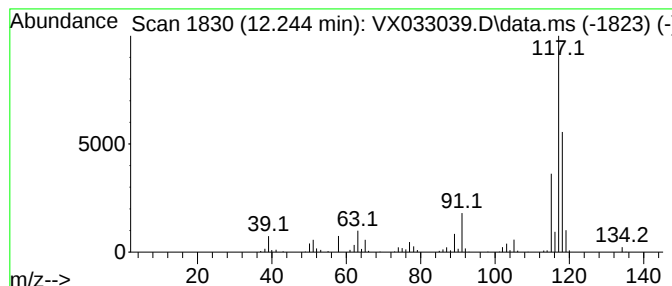

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033039.D
Acq On : 24 Nov 2022 05:18
Operator : JC/MD
Sample : N5741-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.244	12.2	ug/l	140472	4	12.024	577435	50.0