



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033008.D
Acq On : 23 Nov 2022 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260
Last Update : Tue Nov 22 13:58:46 2022

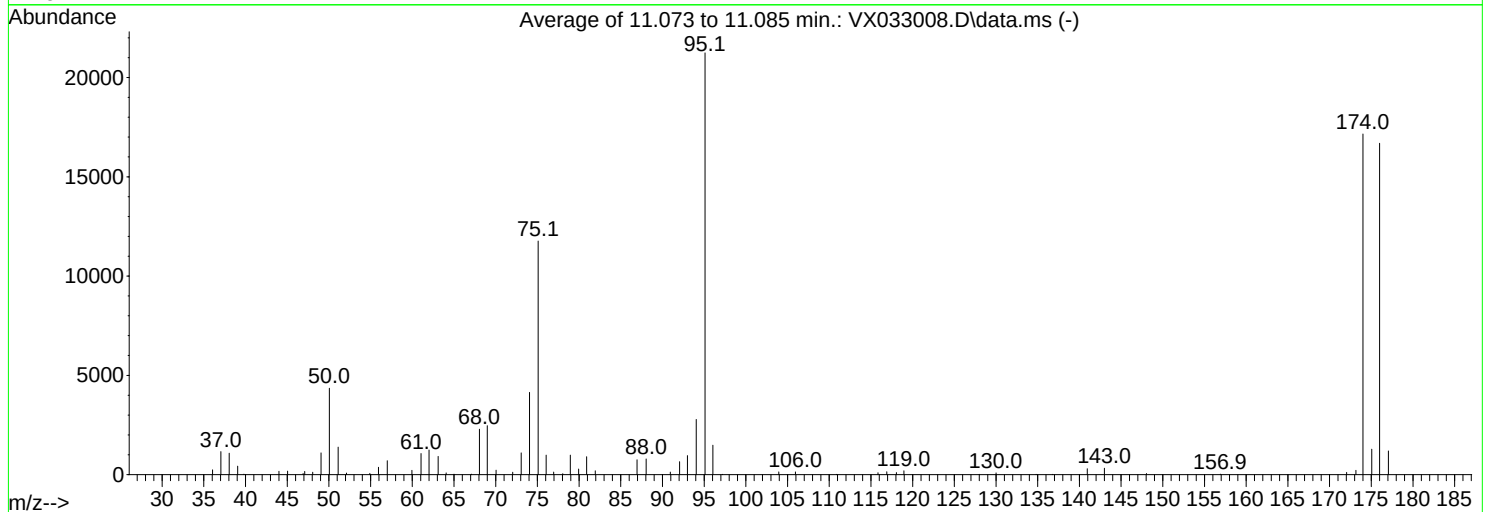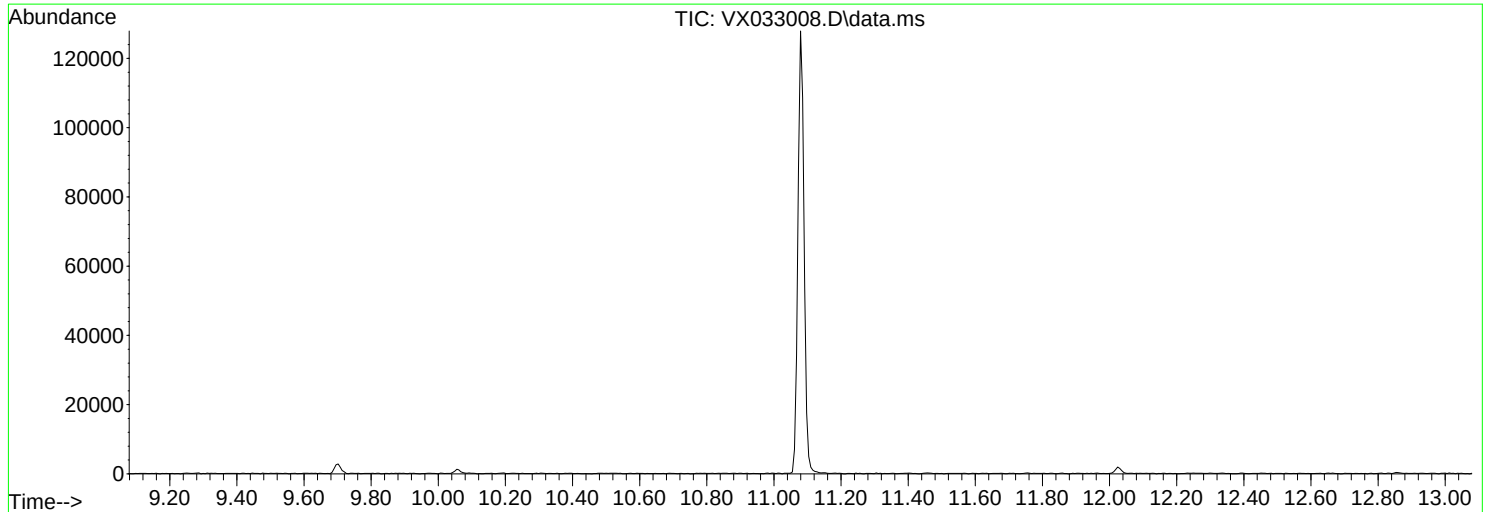

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	4353	PASS
75	95	30	60	55.4	11762	PASS
95	95	100	100	100.0	21243	PASS
96	95	5	9	7.0	1479	PASS
173	174	0.00	2	1.3	219	PASS
174	95	50	100	80.8	17156	PASS
175	174	5	9	7.5	1280	PASS
176	174	95	101	97.3	16689	PASS
177	176	5	9	7.2	1196	PASS