
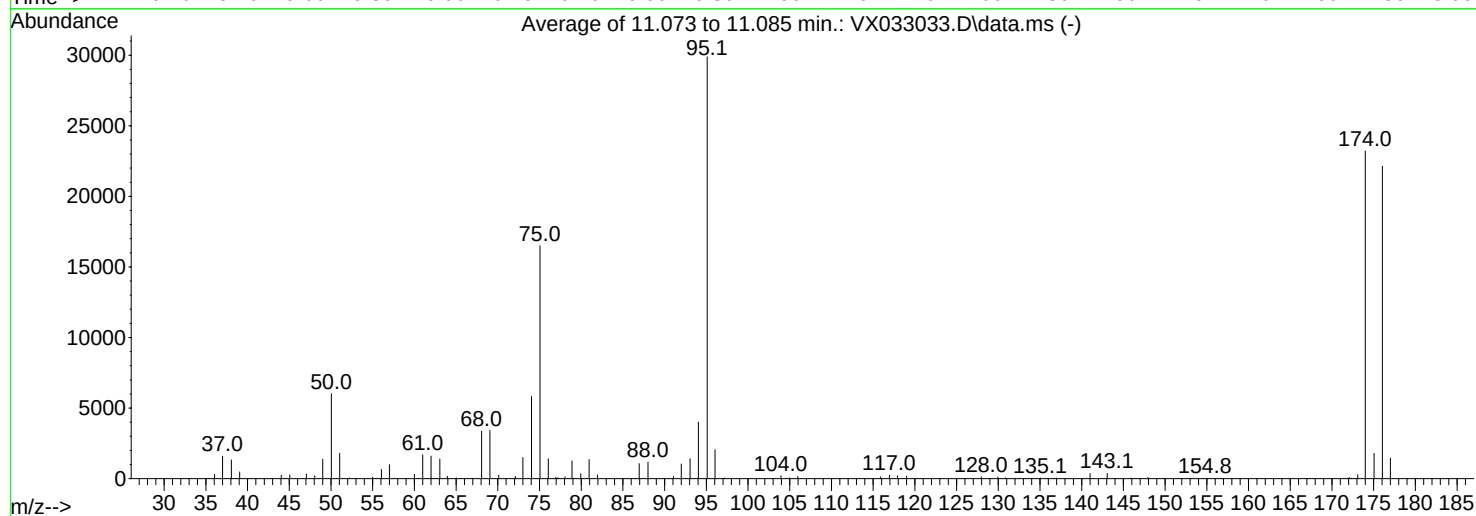


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112322\
Data File : VX033033.D
Acq On : 24 Nov 2022 01:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260
Last Update : Tue Nov 22 13:58:46 2022

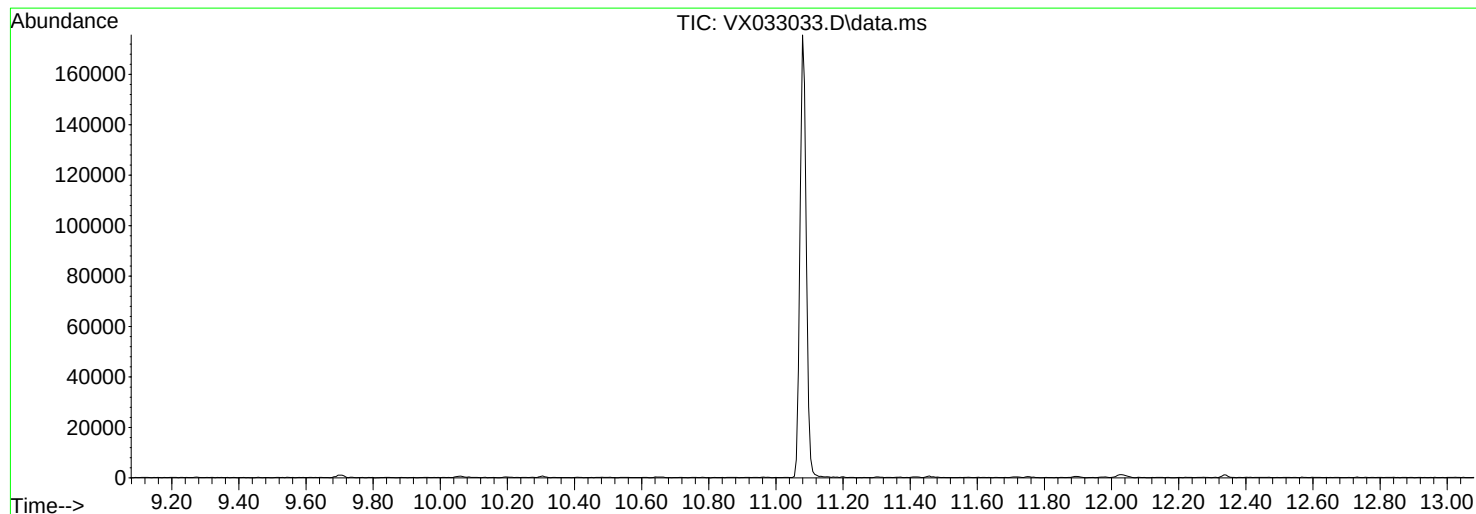

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6018	PASS
75	95	30	60	55.2	16495	PASS
95	95	100	100	100.0	29885	PASS
96	95	5	9	6.9	2054	PASS
173	174	0.00	2	1.2	270	PASS
174	95	50	100	77.7	23222	PASS
175	174	5	9	7.7	1793	PASS
176	174	95	101	95.3	22132	PASS
177	176	5	9	6.5	1447	PASS