

Data File : VX019614.D
Acq On : 24 Nov 2020 18:38
Operator : JC/MD
Sample : L4597-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BU-03-112320

Quant Time: Nov 25 04:05:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	324400	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	540466	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	491732	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	200050	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	203330	48.34	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.68%
35) Dibromofluoromethane	5.46	113	161447	47.59	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.18%
50) Toluene-d8	8.70	98	657258	49.86	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.72%
62) 4-Bromofluorobenzene	11.12	95	224142	47.26	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.52%

Target Compounds


					Qvalue	
5) Bromomethane	1.62	94	314	0.213	ug/l #	42
6) Chloroethane	1.70	64	1869	Below	Cal #	59
11) Tert butyl alcohol	3.00	59	4596	5.774	ug/l #	76
13) Acrolein	2.28	56	305	0.570	ug/l #	15
16) Acetone	2.42	43	12427	7.640	ug/l	97
18) Methyl Acetate	2.75	43	4729	1.805	ug/l	98
20) Methylene Chloride	2.83	84	10295	2.532	ug/l	91
25) 2-Butanone	4.63	43	1910	0.782	ug/l	98
29) Tetrahydrofuran	5.10	42	1326	0.851	ug/l #	82
31) Cyclohexane	5.63	56	6259	1.144	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	24627	4.860	ug/l #	50
38) Carbon Tetrachloride	5.62	117	31785	6.481	ug/l #	17
43) Isopropyl Acetate	6.41	43	76110	9.518	ug/l	100
48) Methyl methacrylate	7.65	41	4215	1.126	ug/l #	9
49) 1,4-Dioxane	7.85	88	248	2.917	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	73836	15.835	ug/l #	48
54) cis-1,3-Dichloropropene	8.59	75	38241	6.269	ug/l #	61
56) Ethyl methacrylate	9.29	69	1175	0.214	ug/l #	1
57) 1,3-Dichloropropane	9.52	76	6284	0.968	ug/l #	43
59) 2-Hexanone	9.52	43	79859	22.582	ug/l #	47
70) Styrene	10.70	104	120	1.656	ug/l #	40
74) N-amyl acetate	10.80	43	3161	0.610	ug/l #	43
76) 1,2,3-Trichloropropane	11.12	75	109409	25.061	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	109409	66.190	ug/l #	12
95) Naphthalene	13.82	128	1153	2.253	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX019614.D
Acq On : 24 Nov 2020 18:38
Operator : JC/MD
Sample : L4597-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BU-03-112320

Quant Time: Nov 25 04:05:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

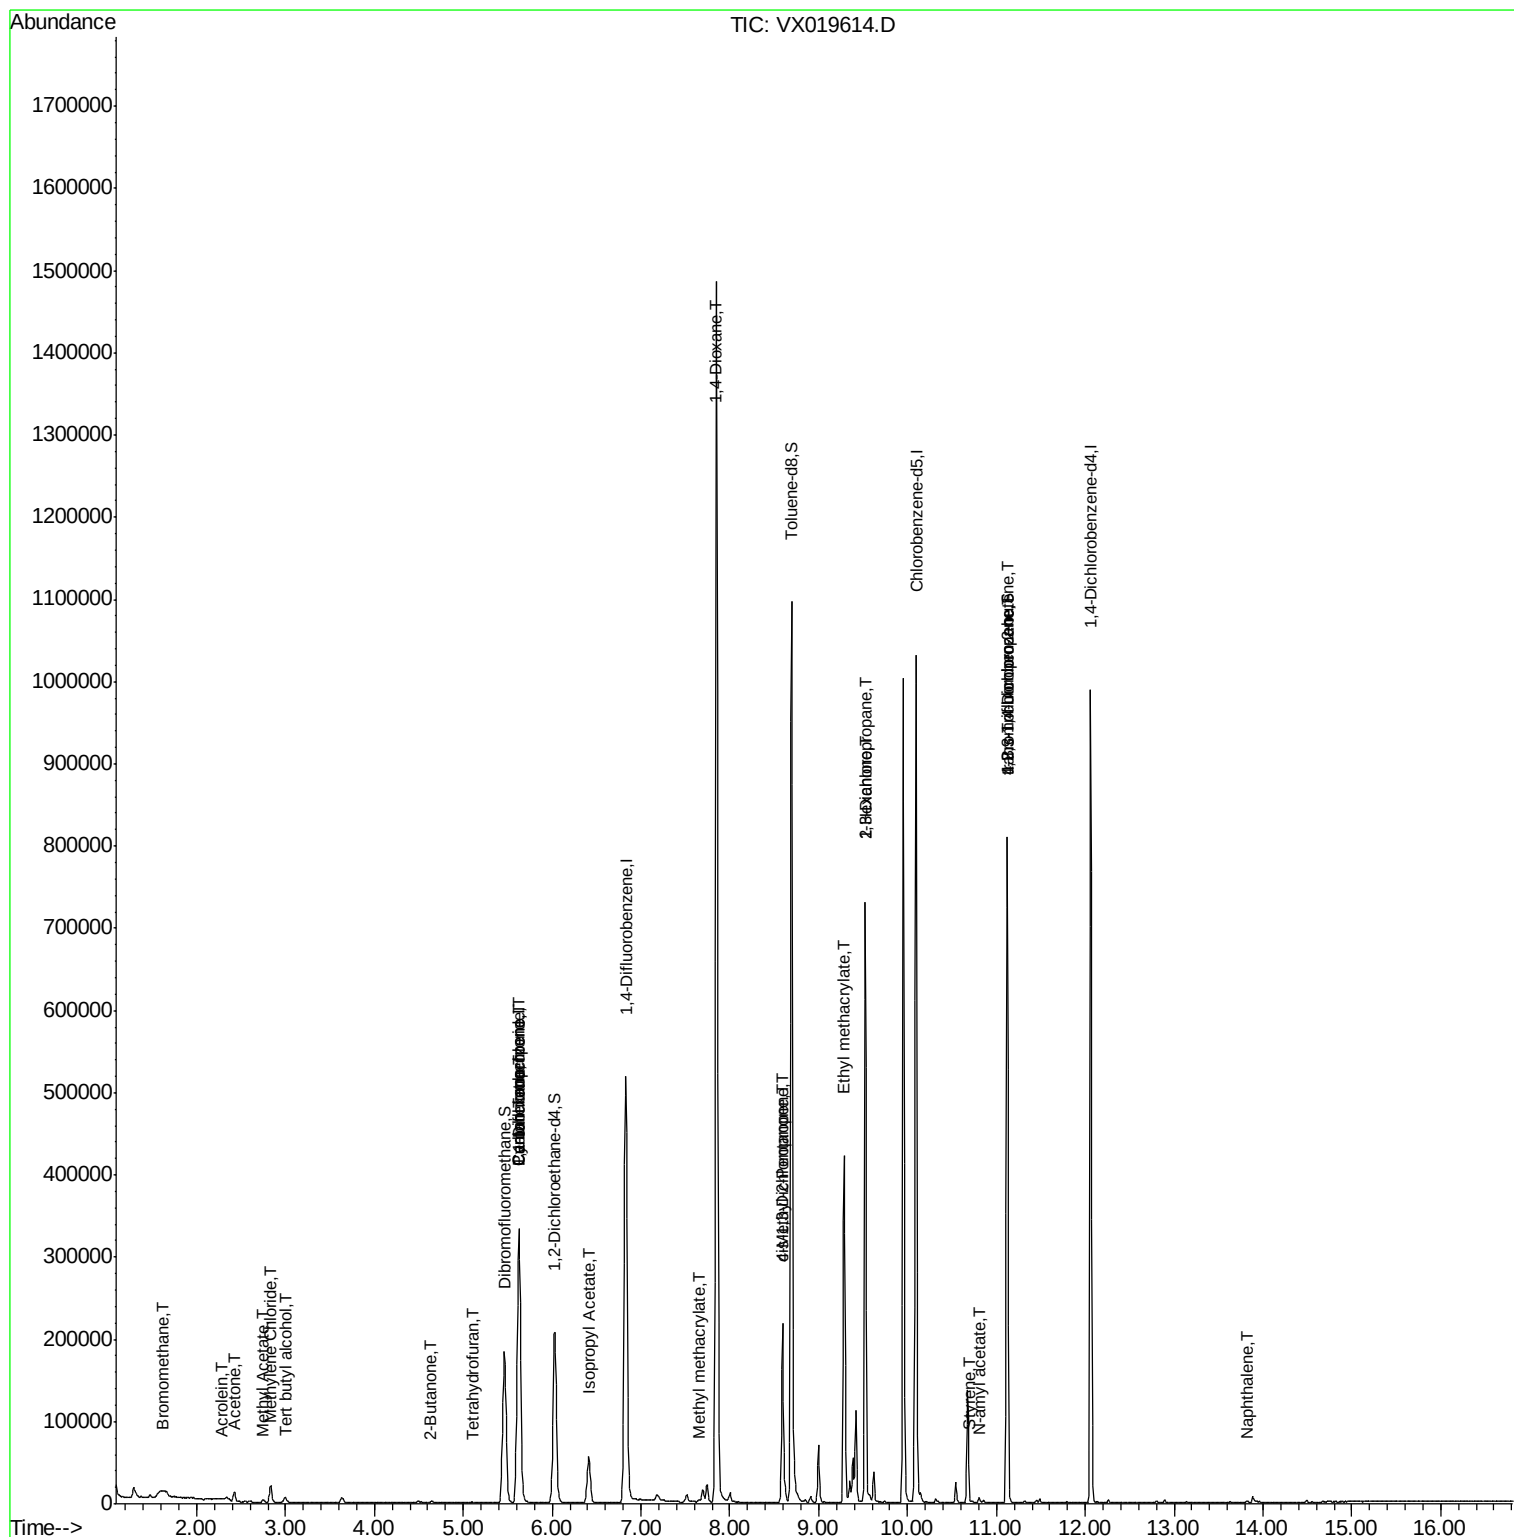

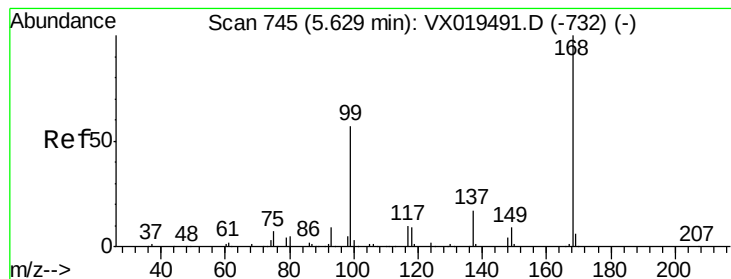

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :


BU-03-112320

Tgt Ion:168 Resp: 324400

Ion Ratio Lower Upper

168 100

99 53.9 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

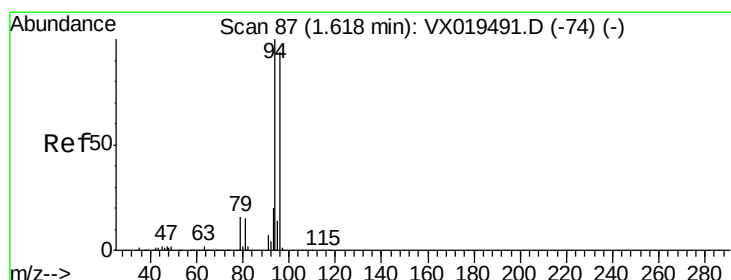

#5

Bromomethane

Concen: 0.213 ug/l

RT: 1.62 min Scan# 88

Delta R.T. 0.01 min

Lab File: VX019614.D


Acq: 24 Nov 2020 18:38

Tgt Ion: 94 Resp: 314

Ion Ratio Lower Upper

94 100

96 38.6 75.6 113.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.62

250

200

150


100


50

0

Time-->

1.60 1.62 1.64



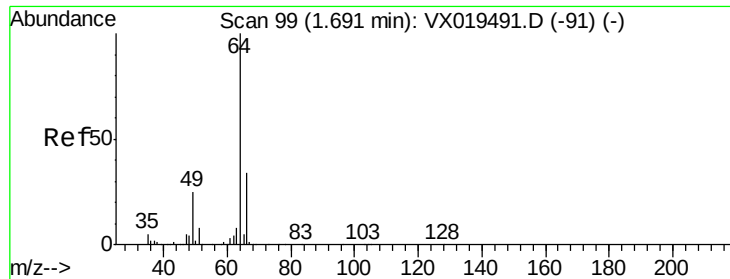

#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 100

Delta R.T. 0.01 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampled :





BU-03-112320

Tgt Ion: 64 Resp: 1869

Ion Ratio Lower Upper

64 100

66 10.6 27.1 40.7#

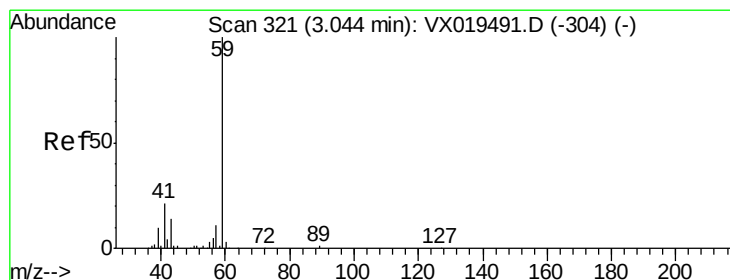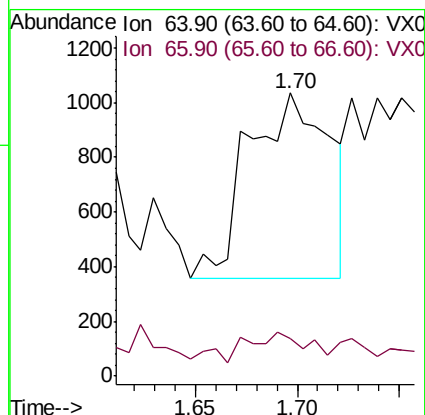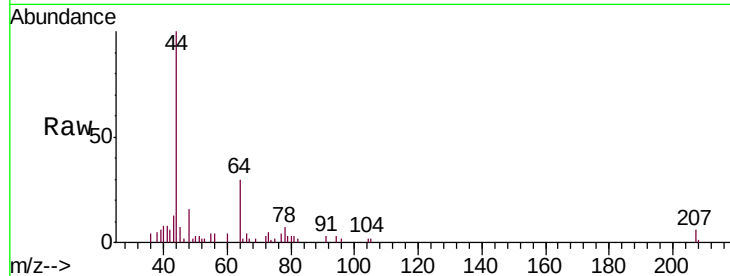

#11

Tert butyl alcohol

Concen: 5.774 ug/l

RT: 3.00 min Scan# 313

Delta R.T. -0.05 min

Lab File: VX019614.D




Acq: 24 Nov 2020 18:38


Tgt Ion: 59 Resp: 4596

Ion Ratio Lower Upper

59 100

57 0.9 7.9 11.9#

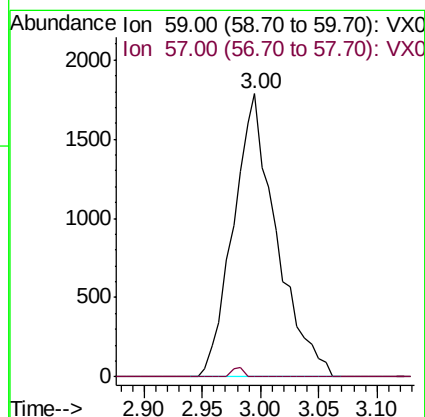



#13

Acrolein

Concen: 0.570 ug/l

RT: 2.28 min Scan# 196

Delta R.T. 0.01 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :


BU-03-112320

Tgt Ion: 56 Resp: 305

Ion Ratio Lower Upper




56 100

55 0.0 55.5 83.3#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

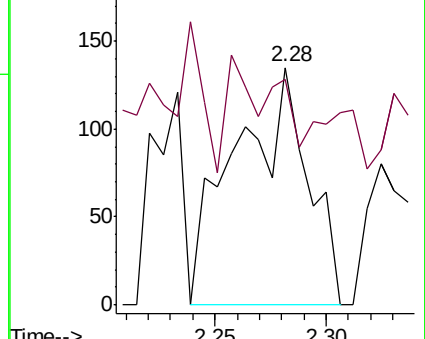

#16

Acetone

Concen: 7.640 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.01 min

Lab File: VX019614.D


Acq: 24 Nov 2020 18:38

Tgt Ion: 43 Resp: 12427

Ion Ratio Lower Upper



43 100


58 32.4 27.4 41.2



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




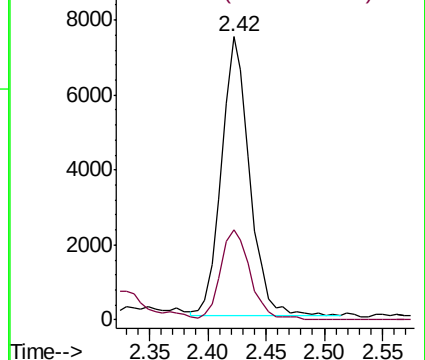


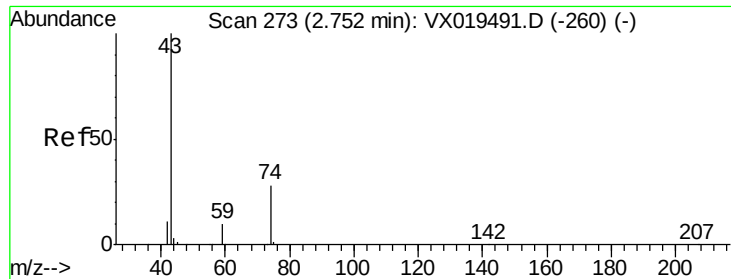

#18
Methyl Acetate
Concen: 1.805 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.00 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38




Instrument :
MSVOA_X
ClientSampled :
BU-03-112320


Tgt Ion: 43 Resp: 4729
Ion Ratio Lower Upper
43 100
74 26.7 22.2 33.4

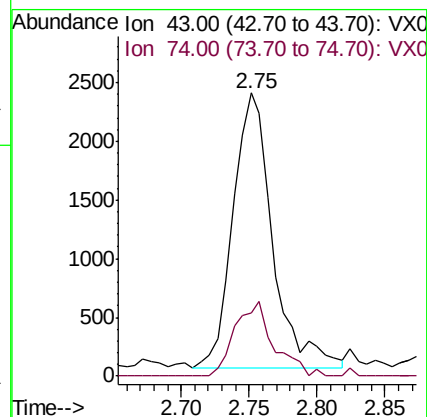

#20
Methylene Chloride
Concen: 2.532 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38

Tgt Ion: 84 Resp: 10295
Ion Ratio Lower Upper
84 100
49 98.8 88.5 132.7
51 31.6 28.0 42.0
86 59.4 53.0 79.4

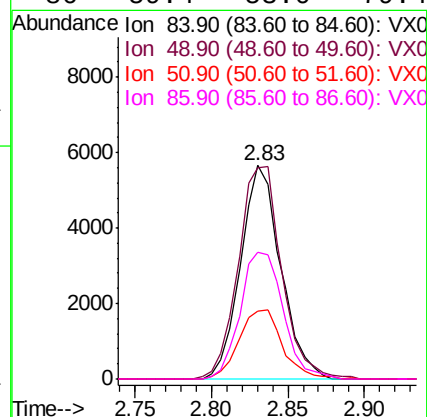

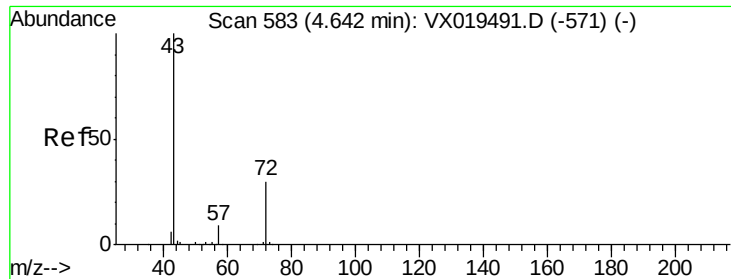

#25

2-Butanone

Concen: 0.782 ug/l

RT: 4.63 min Scan# 582

Delta R.T. -0.01 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :


BU-03-112320

Tgt Ion: 43 Resp: 1910

Ion Ratio Lower Upper




43 100

72 31.0 24.0 36.0

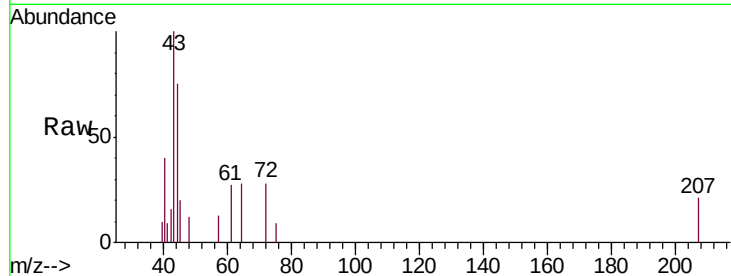

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

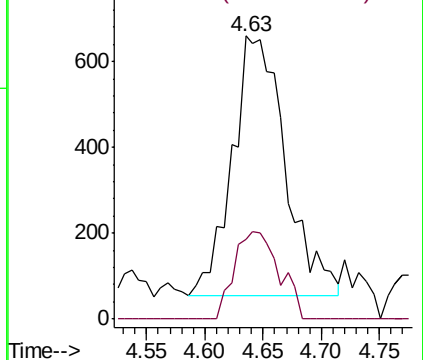

#29

Tetrahydrofuran

Concen: 0.851 ug/l

RT: 5.10 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38


Tgt Ion: 42 Resp: 1326

Ion Ratio Lower Upper

42 100

72 42.0 42.6 63.8#



71 34.2 39.0 58.6#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

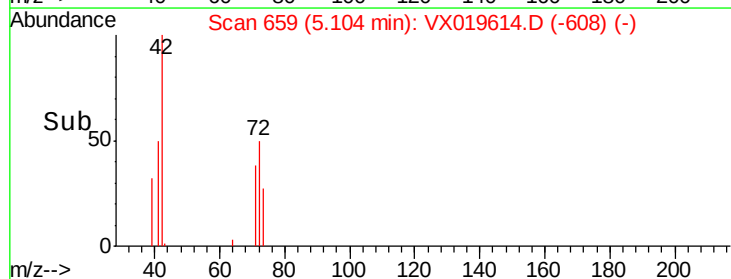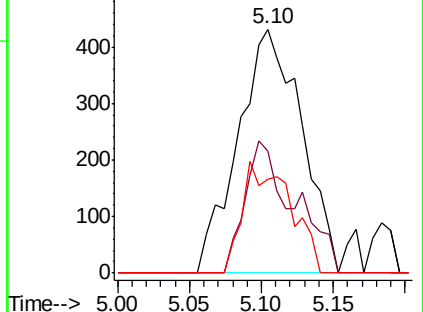

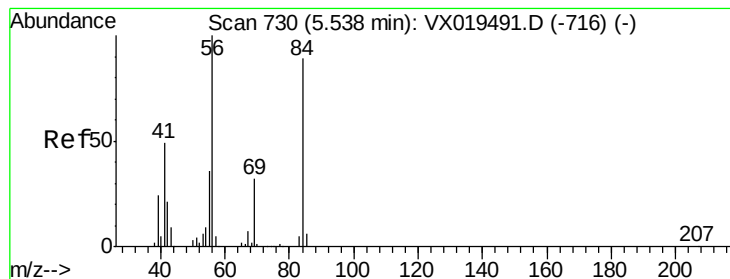

#31

Cyclohexane

Concen: 1.144 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.09 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320


Tgt Ion: 56 Resp: 6259

Ion Ratio Lower Upper

56 100

69 193.2 25.5 38.3#




84 172.7 71.1 106.7#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

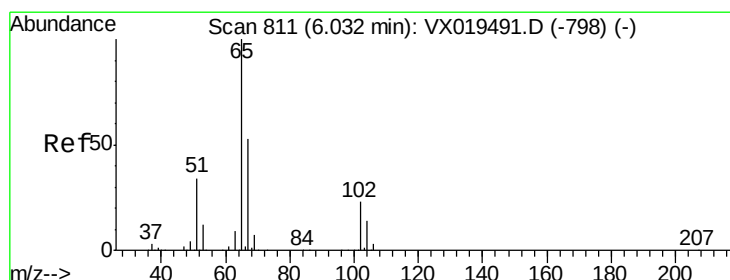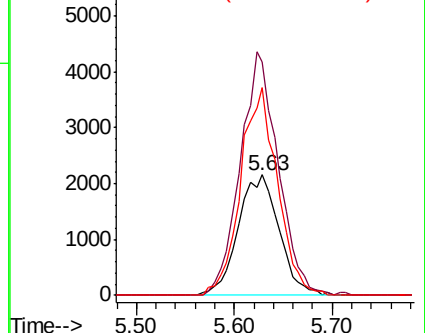

#33

1,2-Dichloroethane-d4

Concen: 48.341 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX019614.D


Acq: 24 Nov 2020 18:38

Tgt Ion: 65 Resp: 203330

Ion Ratio Lower Upper



65 100


67 52.0 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

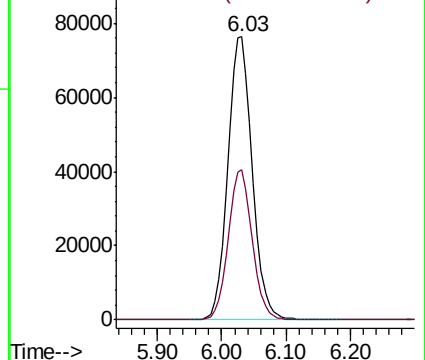

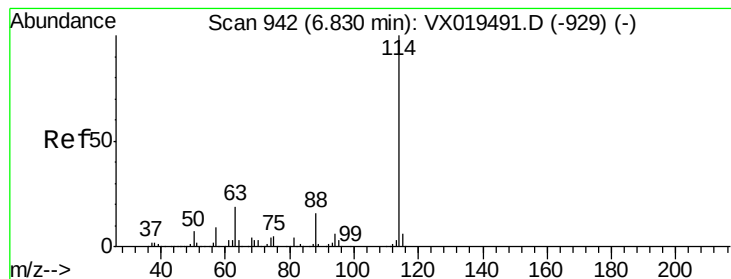

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320


Tgt Ion:114 Resp: 540466

Ion Ratio Lower Upper

114 100

63 19.6 0.0 38.8




88 15.5 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

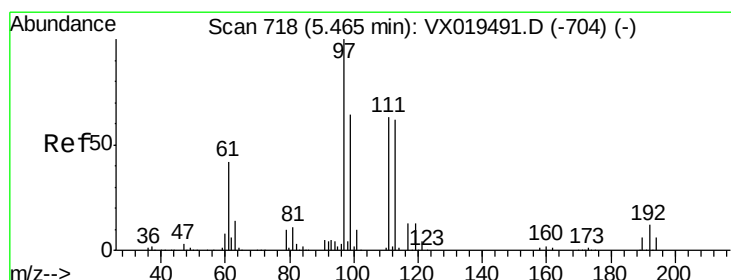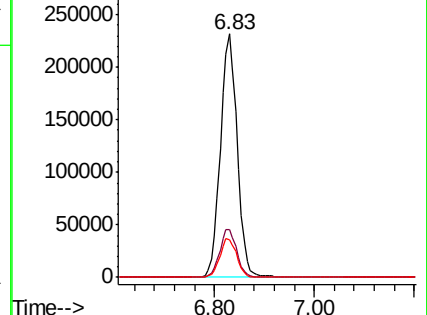

#35

Dibromofluoromethane

Concen: 47.589 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38


Tgt Ion:113 Resp: 161447

Ion Ratio Lower Upper

113 100

111 101.3 81.5 122.3



192 20.2 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



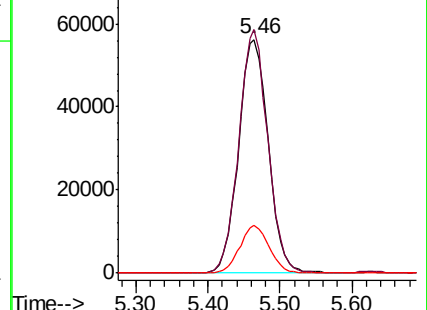



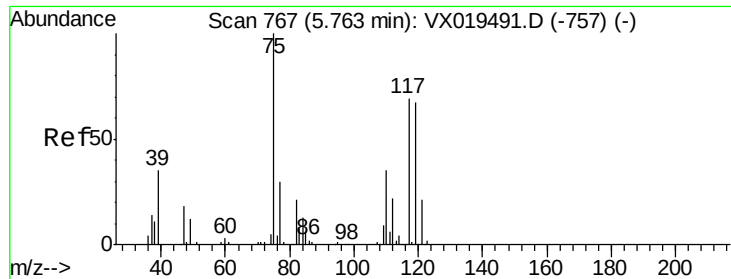

#36
 1,1-Dichloropropene
 Concen: 4.860 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX019614.D
 Acq: 24 Nov 2020 18:38




Instrument :
 MSVOA_X
 ClientSampled :
 BU-03-112320


Tgt Ion: 75 Resp: 24627
 Ion Ratio Lower Upper
 75 100
 110 9.1 18.1 54.3#
 77 0.0 24.2 36.4#

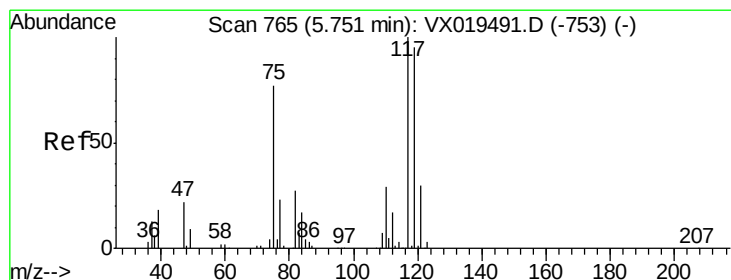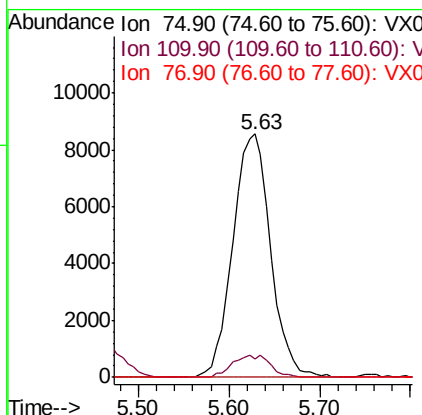

#38
 Carbon Tetrachloride
 Concen: 6.481 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.13 min
 Lab File: VX019614.D
 Acq: 24 Nov 2020 18:38

Tgt Ion: 117 Resp: 31785
 Ion Ratio Lower Upper
 117 100
 119 5.5 75.9 113.9#
 121 0.0 24.0 36.0#

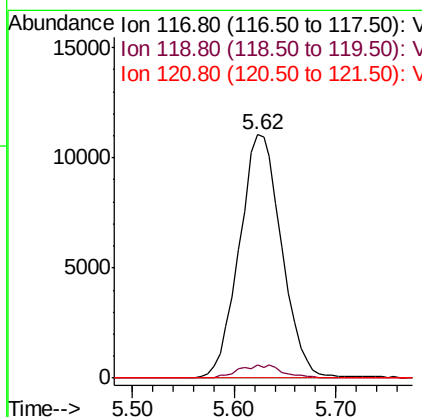

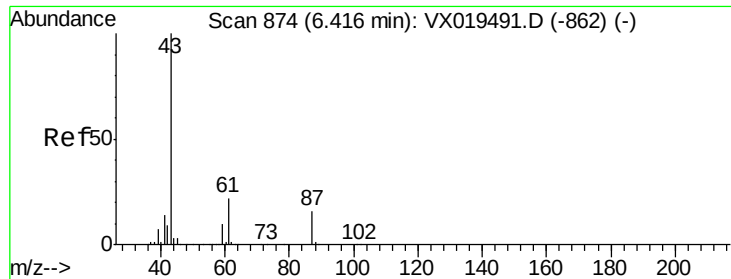

#43

Isopropyl Acetate

Concen: 9.518 ug/l

RT: 6.41 min Scan# 873

Delta R.T. -0.01 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320


Tgt Ion: 43 Resp: 76110

Ion Ratio Lower Upper




43 100

61 22.5 18.2 27.2

87 15.7 12.6 18.8

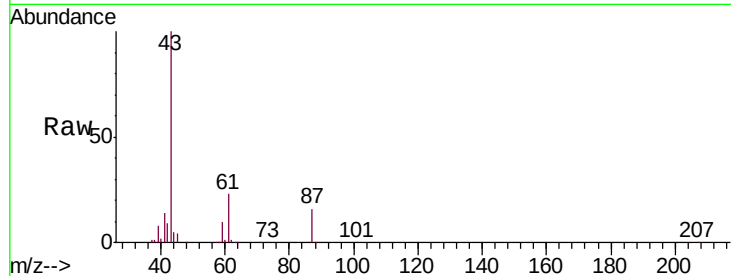

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

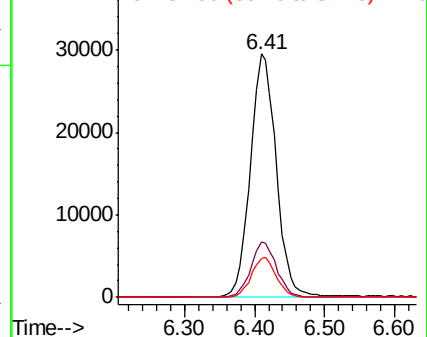

#48

Methyl methacrylate

Concen: 1.126 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38


Tgt Ion: 41 Resp: 4215

Ion Ratio Lower Upper



41 100


69 0.0 77.0 115.6#

39 0.0 45.6 68.4#



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

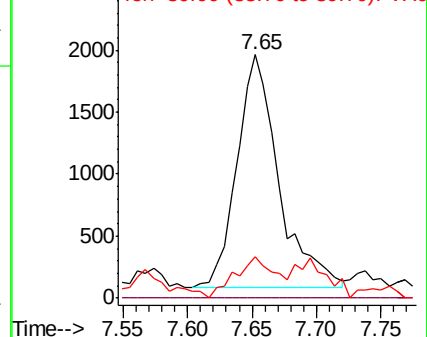

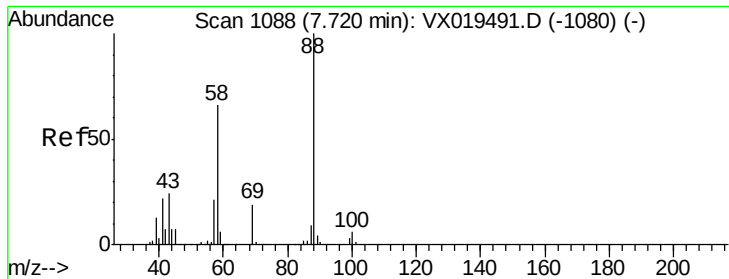

#49

1,4-Dioxane

Concen: 2.917 ug/l

RT: 7.85 min Scan# 1109

Delta R.T. 0.13 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320


Tgt Ion: 88 Resp: 248

Ion Ratio Lower Upper

88 100

43 526146.0 23.8 35.6#




58 2553.6 54.2 81.2#

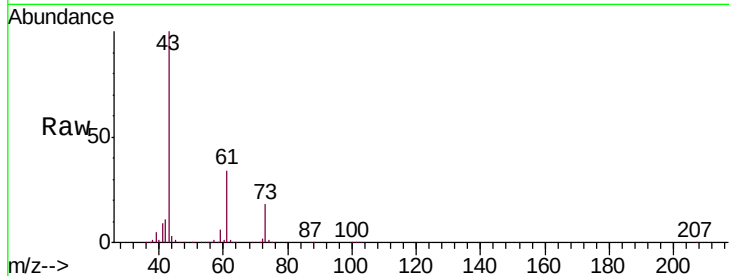

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

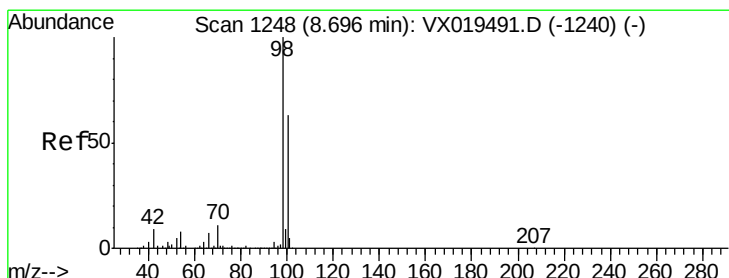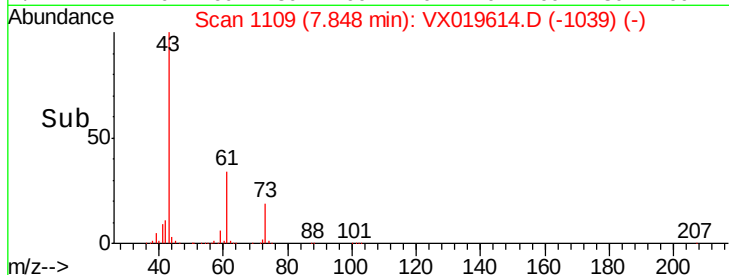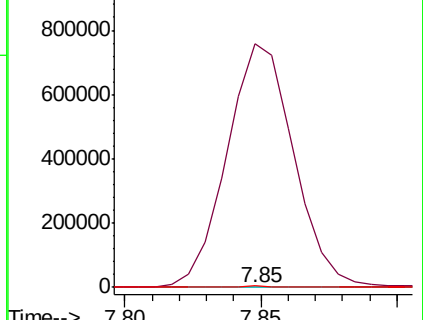

#50

Toluene-d8

Concen: 49.857 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019614.D


Acq: 24 Nov 2020 18:38

Tgt Ion: 98 Resp: 657258

Ion Ratio Lower Upper



98 100


100 66.1 52.4 78.6

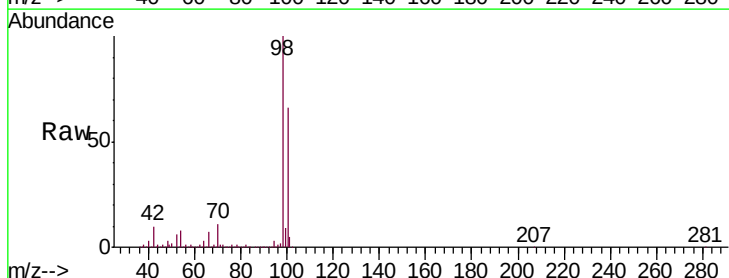

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

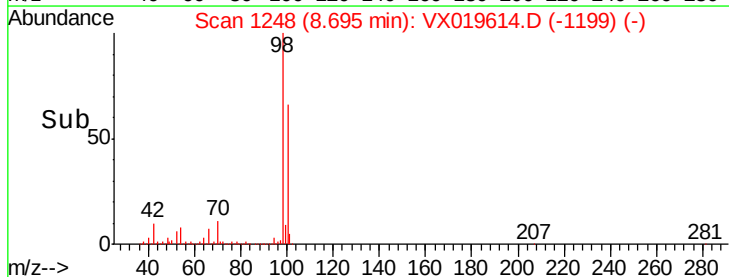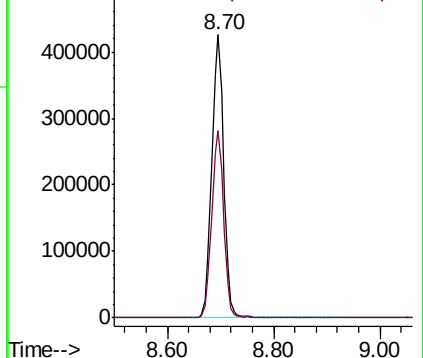



#51

4-Methyl-2-Pentanone

Concen: 15.835 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :


BU-03-112320

Tgt Ion: 43 Resp: 73836

Ion Ratio Lower Upper

43 100

58 10.0 35.1 52.7#

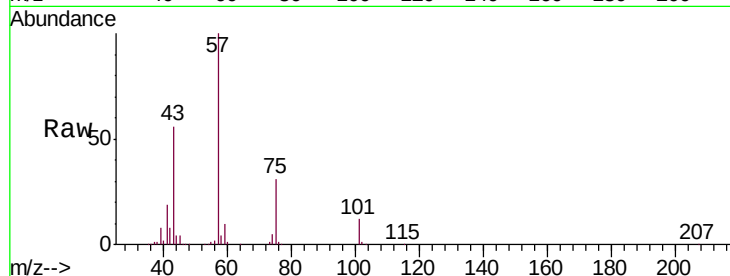

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

8.59

50000

40000

30000



20000

10000

0

Time-->

8.50 8.60 8.70



#54

cis-1,3-Dichloropropene

Concen: 6.269 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38


Tgt Ion: 75 Resp: 38241

Ion Ratio Lower Upper

75 100

77 0.7 25.8 38.6#

39 26.6 34.6 51.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0

8.59

30000


20000


10000

0

Time-->

8.50 8.55 8.60 8.65





#56

Ethyl methacrylate

Concen: 0.214 ug/l

RT: 9.29 min Scan# 1345

Delta R.T. 0.13 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320





Tgt Ion: 69 Resp: 1175

Ion Ratio Lower Upper

69 100

41 5090.1 46.2 69.2#

39 2069.6 25.5 38.3#

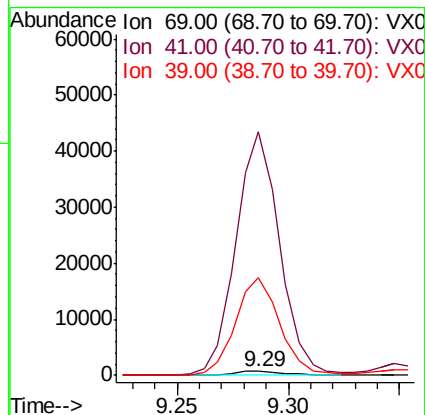

#57

1,3-Dichloropropane

Concen: 0.968 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019614.D




Acq: 24 Nov 2020 18:38


Tgt Ion: 76 Resp: 6284

Ion Ratio Lower Upper

76 100

78 0.3 25.7 38.5#



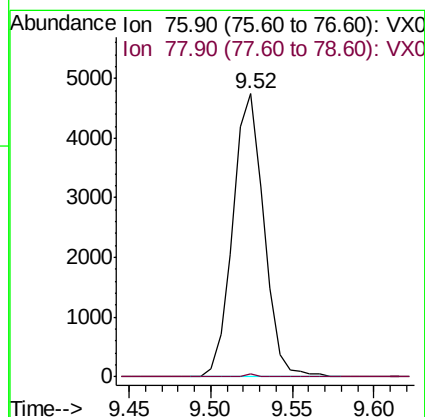



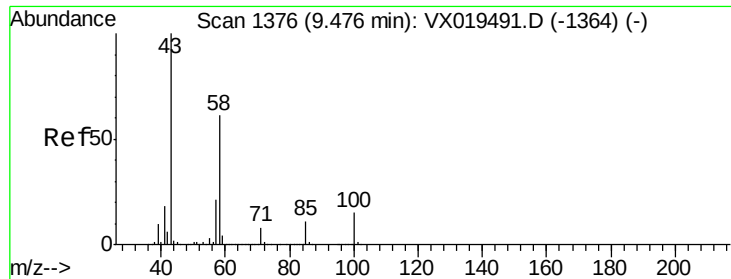

#59
2-Hexanone
Concen: 22.582 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38




Instrument :
MSVOA_X
ClientSampleId :
BU-03-112320


Tgt Ion: 43 Resp: 79859
Ion Ratio Lower Upper
43 100
58 20.3 30.6 91.6#

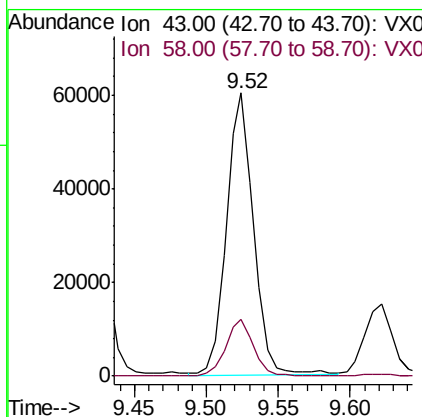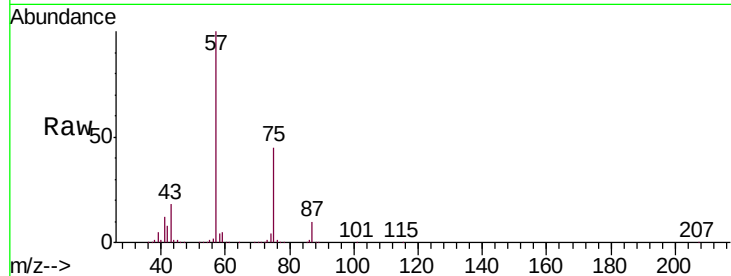

#62
4-Bromofluorobenzene
Concen: 47.257 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38

Tgt Ion: 95 Resp: 224142
Ion Ratio Lower Upper
95 100
174 75.8 0.0 156.2
176 76.0 0.0 151.4



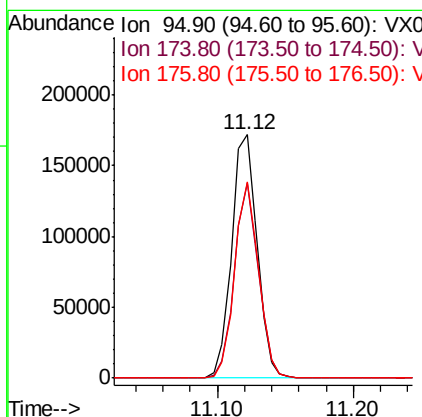





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38




Instrument :
MSVOA_X
ClientSampleId :
BU-03-112320


Tgt Ion:117 Resp: 491732
Ion Ratio Lower Upper
117 100
82 55.0 43.0 64.4
119 33.3 25.6 38.4

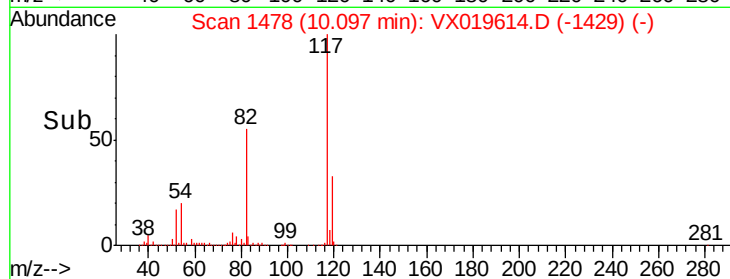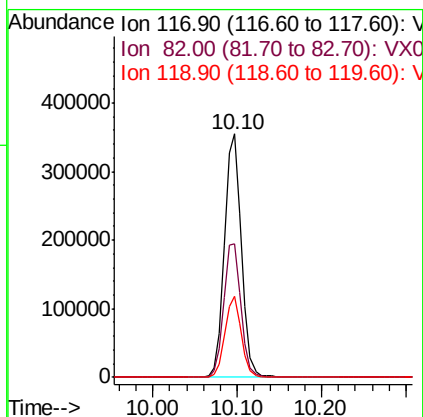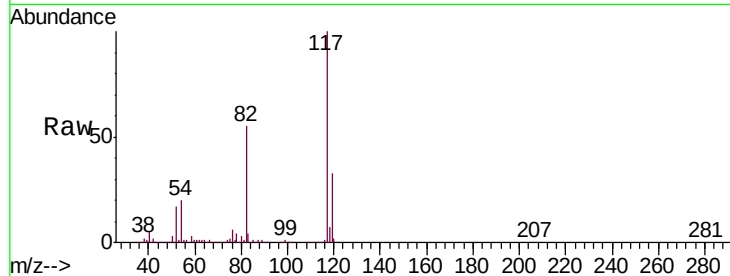

#70
Styrene
Concen: 1.656 ug/l
RT: 10.70 min Scan# 1577
Delta R.T. 0.01 min
Lab File: VX019614.D
Acq: 24 Nov 2020 18:38

Tgt Ion:104 Resp: 120
Ion Ratio Lower Upper
104 100
78 20.0 39.5 59.3#
103 0.0 43.6 65.4#

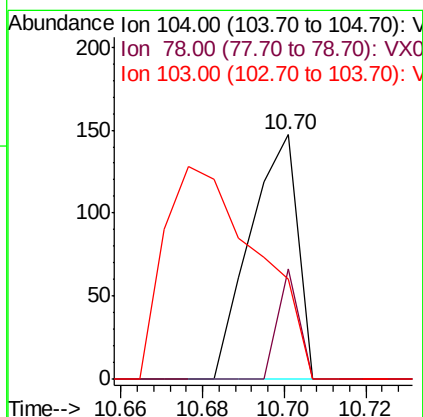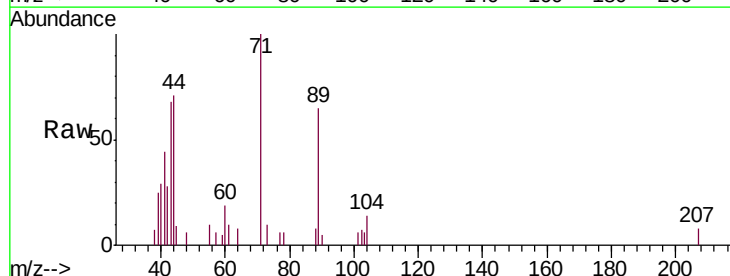



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320


Tgt Ion:152 Resp: 200050

Ion Ratio Lower Upper

152 100

115 59.6 41.8 125.4




150 156.1 0.0 348.2

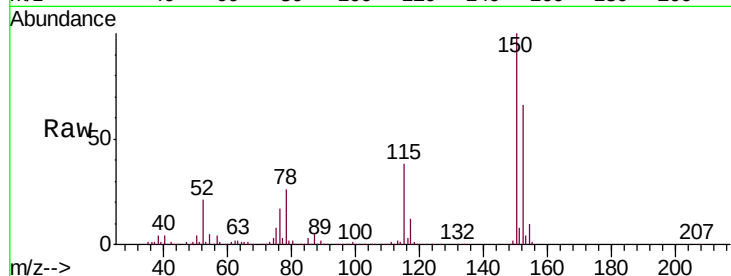

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

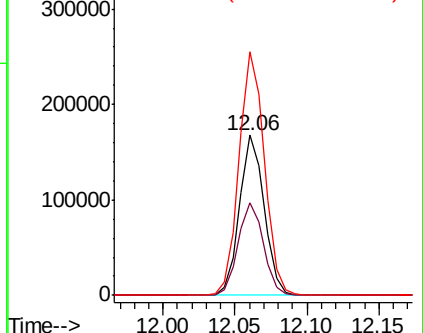

#74

N-ethyl acetate

Concen: 0.610 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Tgt Ion: 43 Resp: 3161


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 9.6 21.8 32.6#

61 0.0 22.2 33.4#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0



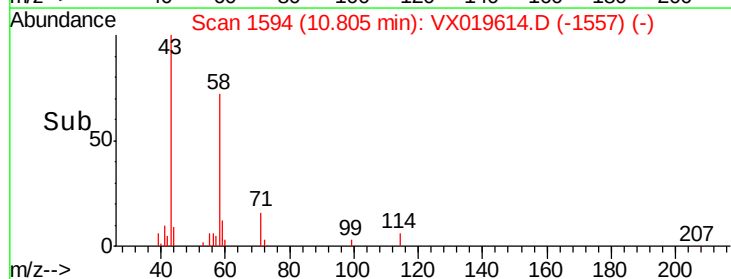
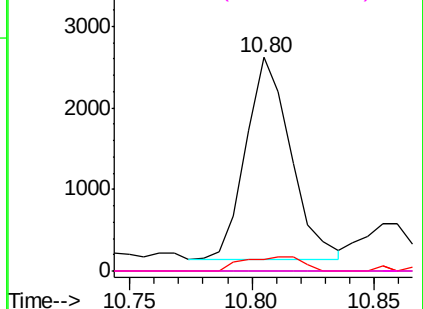




#76
 1,2,3-Trichloropropane
 Concen: 25.061 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. -0.16 min
 Lab File: VX019614.D
 Acq: 24 Nov 2020 18:38




Instrument :
 MSVOA_X
 ClientSampleId :
 BU-03-112320


Tgt Ion: 75 Resp: 109409
 Ion Ratio Lower Upper
 75 100
 77 1.2 20.0 60.0#

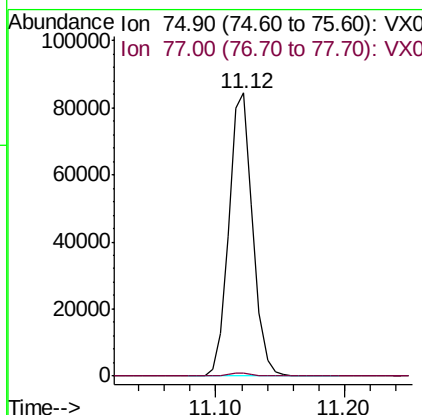

#81
 trans-1,4-Dichloro-2-butene
 Concen: 66.190 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. 0.07 min
 Lab File: VX019614.D
 Acq: 24 Nov 2020 18:38

Tgt Ion: 75 Resp: 109409
 Ion Ratio Lower Upper
 75 100
 53 0.0 73.9 110.9#
 89 0.0 37.3 55.9#

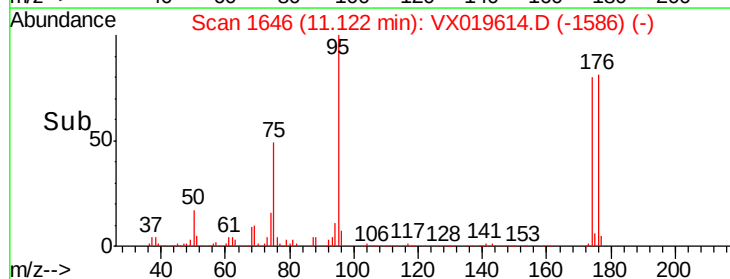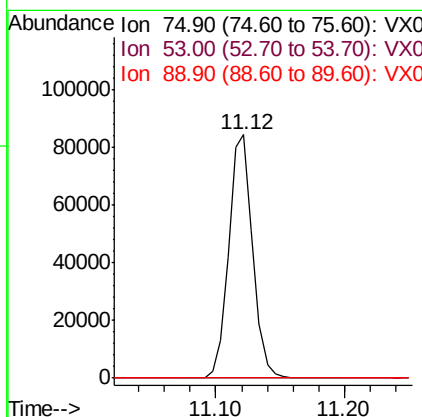



#95

Naphthalene

Concen: 2.253 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019614.D

Acq: 24 Nov 2020 18:38

Instrument :

MSVOA_X

ClientSampleId :

BU-03-112320

Tgt Ion:128 Resp: 1153

Ion Ratio Lower Upper

128 100

127 12.5 10.3 15.5

129 13.7 8.7 13.1#

