

Data File : VX019630.D
Acq On : 25 Nov 2020 01:36
Operator : JC/MD
Sample : L4835-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119

Quant Time: Nov 25 04:11:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.62	168	310563	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	506078	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	461998	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	191581	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	189761	47.13	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.26%
35) Dibromofluoromethane	5.46	113	150113	47.26	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.52%
50) Toluene-d8	8.70	98	602426	48.80	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.60%
62) 4-Bromofluorobenzene	11.12	95	215970	48.63	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.26%

Target Compounds


						Qvalue
2) Dichlorodifluoromethane	1.18	85	7034	2.329	ug/l	98
4) Vinyl Chloride	1.39	62	8591	2.303	ug/l	93
5) Bromomethane	1.64	94	609	0.431	ug/l #	10
6) Chloroethane	1.67	64	950	Below Cal	#	49
7) Trichlorofluoromethane	1.91	101	1523	0.283	ug/l	100
9) 1,1,2-Trichlorotrifluoroet	2.36	101	6499	2.163	ug/l	98
11) Tert butyl alcohol	3.03	59	431	0.566	ug/l #	73
12) 1,1-Dichloroethene	2.36	96	20325	6.592	ug/l	94
13) Acrolein	2.28	56	165	0.322	ug/l #	1
16) Acetone	2.42	43	2311	1.484	ug/l	92
18) Methyl Acetate	2.75	43	682	0.811	ug/l #	62
21) trans-1,2-Dichloroethene	3.14	96	25346	7.256	ug/l	98
27) cis-1,2-Dichloroethene	4.56	96	1366411	340.522	ug/l	90
31) Cyclohexane	5.62	56	6038	1.153	ug/l #	1
36) 1,1-Dichloropropene	5.62	75	23276	4.906	ug/l #	50
38) Carbon Tetrachloride	5.63	117	30204	6.577	ug/l #	17
39) Methylcyclohexane	7.19	83	56185	10.171	ug/l #	1
44) Trichloroethene	7.19	130	4747685	1243.371	ug/l	95
49) 1,4-Dioxane	7.72	88	20	0.251	ug/l #	1
60) Dibromochloromethane	9.31	129	1477	0.415	ug/l #	10
64) Tetrachloroethene	9.32	164	1614	0.444	ug/l	92
70) Styrene	10.70	104	93	1.654	ug/l #	52
76) 1,2,3-Trichloropropane	11.12	75	105679	25.276	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	105679	66.723	ug/l #	12
95) Naphthalene	13.82	128	1381	2.272	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX019630.D
Acq On : 25 Nov 2020 01:36
Operator : JC/MD
Sample : L4835-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119

Quant Time: Nov 25 04:11:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

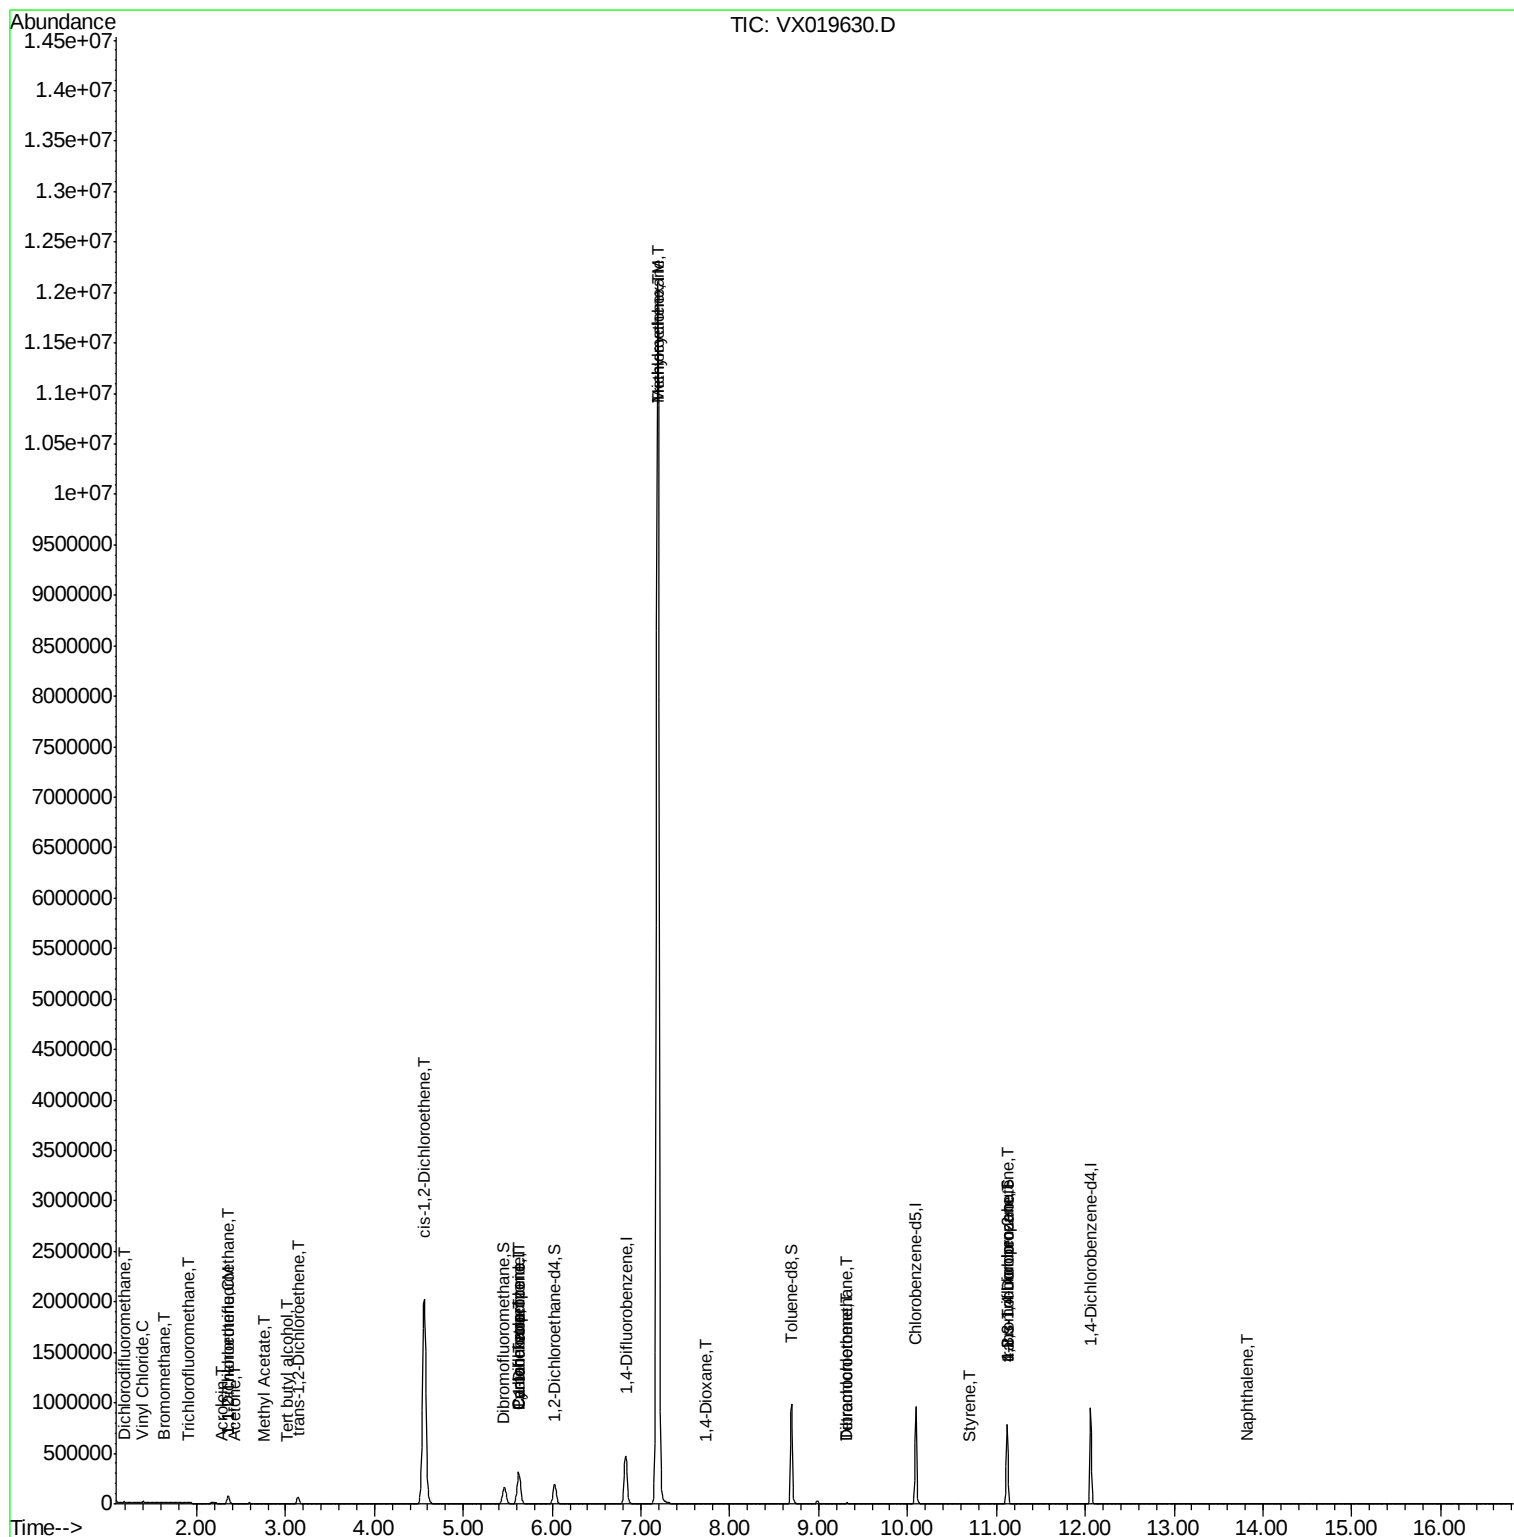



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.01 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :


INTERCEPTOR-20201119

Tgt Ion:168 Resp: 310563

Ion Ratio Lower Upper




168 100

99 57.0 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

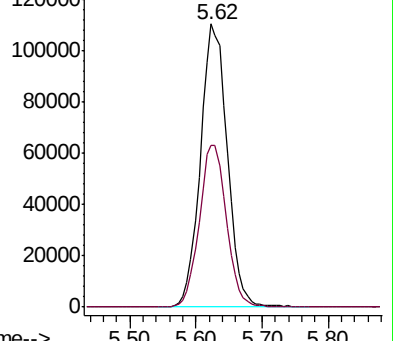

#2

Dichlorodifluoromethane

Concen: 2.329 ug/l

RT: 1.18 min Scan# 16

Delta R.T. -0.00 min

Lab File: VX019630.D


Acq: 25 Nov 2020 01:36

Tgt Ion: 85 Resp: 7034

Ion Ratio Lower Upper



85 100


87 31.1 16.0 47.9



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

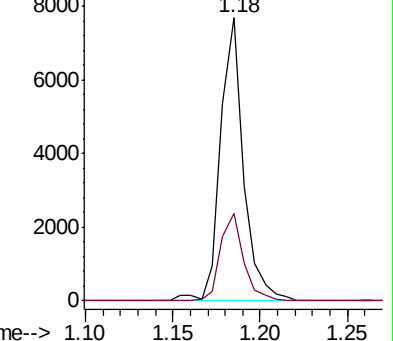



#4

Vinyl Chloride

Concen: 2.303 ug/l

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :





INTERCEPTOR-20201119

Tgt Ion: 62 Resp: 8591

Ion Ratio Lower Upper

62 100

64 35.5 25.4 38.2

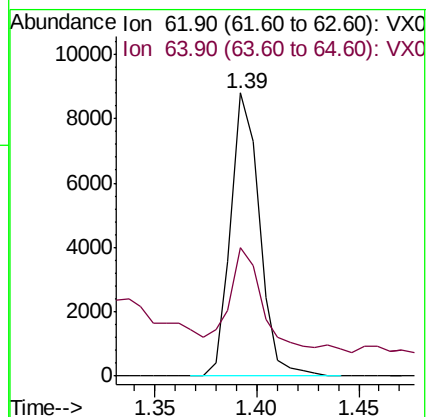

#5

Bromomethane

Concen: 0.431 ug/l

RT: 1.64 min Scan# 90

Delta R.T. 0.02 min

Lab File: VX019630.D




Acq: 25 Nov 2020 01:36


Tgt Ion: 94 Resp: 609

Ion Ratio Lower Upper

94 100

96 6.9 75.6 113.4#

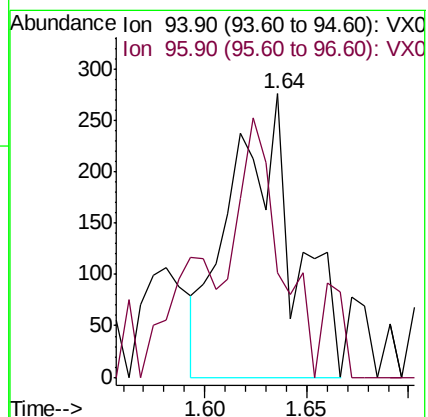



#6

Chloroethane

Concen: Below Cal

RT: 1.67 min Scan# 95

Delta R.T. -0.02 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36





Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119

Tgt Ion: 64 Resp: 950

Ion Ratio Lower Upper

64 100

66 4.8 27.1 40.7#

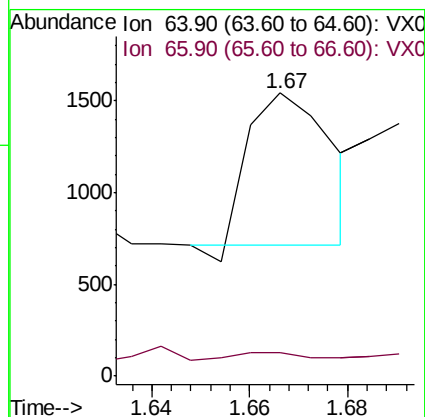

#7

Trichlorofluoromethane

Concen: 0.283 ug/l

RT: 1.91 min Scan# 135

Delta R.T. 0.01 min

Lab File: VX019630.D




Acq: 25 Nov 2020 01:36


Tgt Ion: 101 Resp: 1523

Ion Ratio Lower Upper

101 100

103 63.9 50.9 76.3

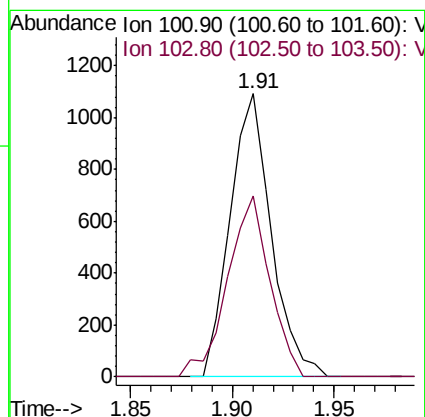

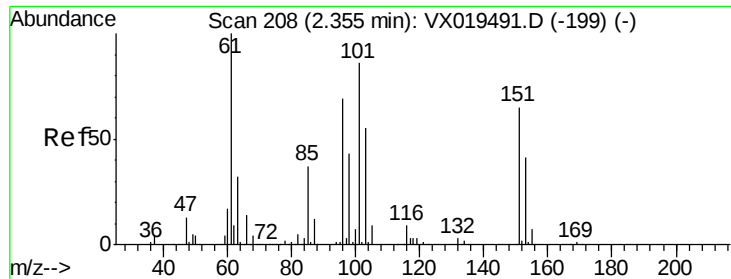

#9

1,1,2-Trichlorotrifluoroethane

Concen: 2.163 ug/l

RT: 2.36 min Scan# 209

Delta R.T. 0.01 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :

INTERCEPTOR-20201119


Tgt Ion:101 Resp: 6499

Ion Ratio Lower Upper

101 100

85 43.8 33.9 50.9




151 78.0 60.9 91.3

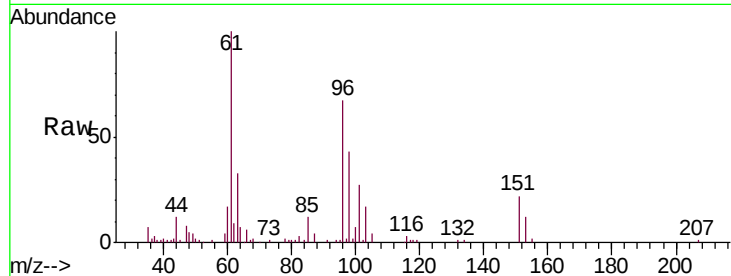

Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

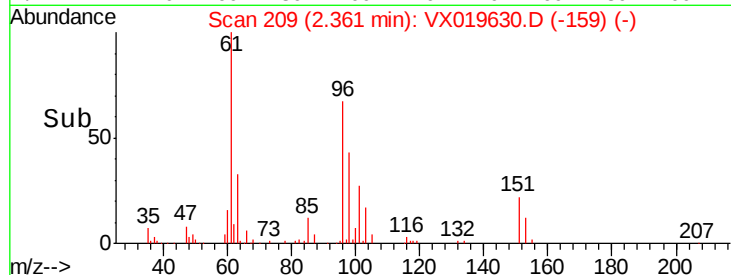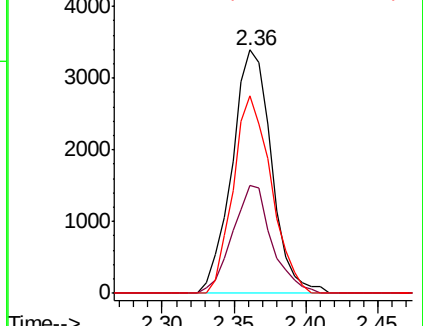

#11

Tert butyl alcohol

Concen: 0.566 ug/l

RT: 3.03 min Scan# 318

Delta R.T. -0.02 min

Lab File: VX019630.D


Acq: 25 Nov 2020 01:36

Tgt Ion: 59 Resp: 431

Ion Ratio Lower Upper



59 100


57 0.0 7.9 11.9#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0




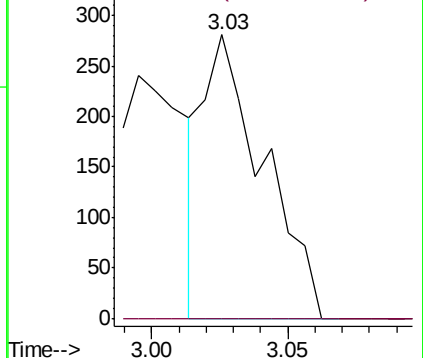


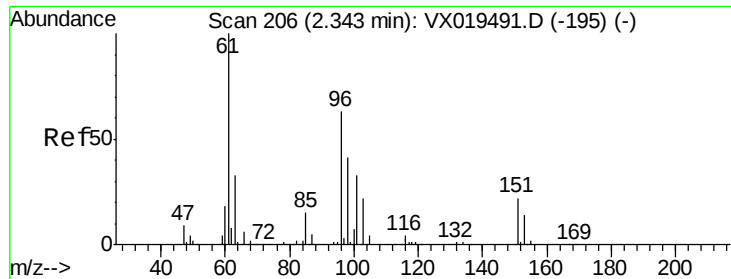

#12
 1,1-Dichloroethene
 Concen: 6.592 ug/l
 RT: 2.36 min Scan# 208
 Delta R.T. 0.01 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36




Instrument :
 MSVOA_X
 ClientSampleId :
 INTERCEPTOR-20201119


Tgt Ion: 96 Resp: 20325
 Ion Ratio Lower Upper
 96 100
 61 148.2 126.0 189.0
 98 62.2 52.0 78.0

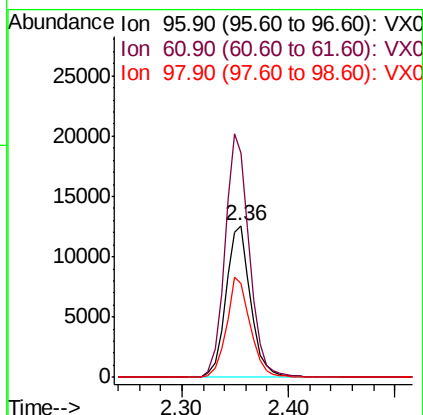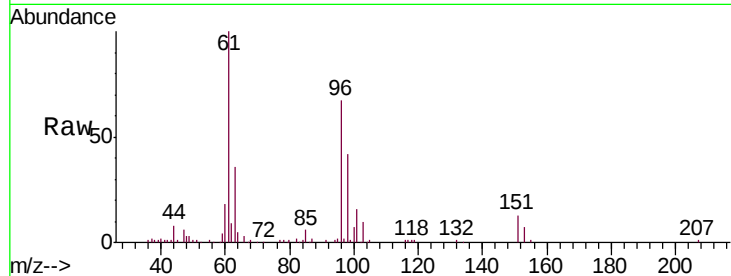

#13
 Acrolein
 Concen: 0.322 ug/l
 RT: 2.28 min Scan# 196
 Delta R.T. 0.01 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36

Tgt Ion: 56 Resp: 165
 Ion Ratio Lower Upper
 56 100
 55 169.7 55.5 83.3#

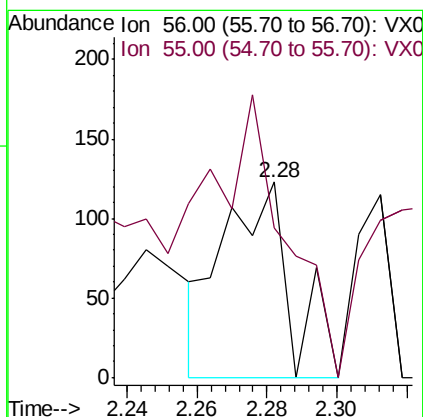

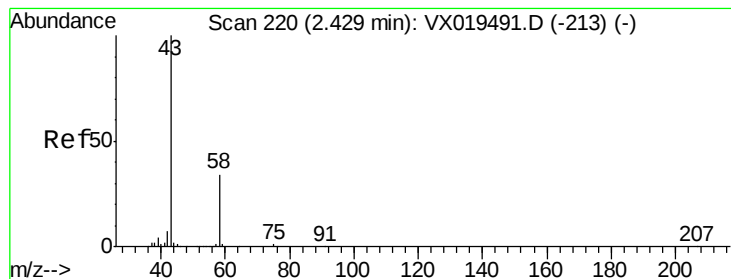

#16

Acetone

Concen: 1.484 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.01 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :


INTERCEPTOR-20201119

Tgt Ion: 43 Resp: 2311

Ion Ratio Lower Upper




43 100

58 29.8 27.4 41.2



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

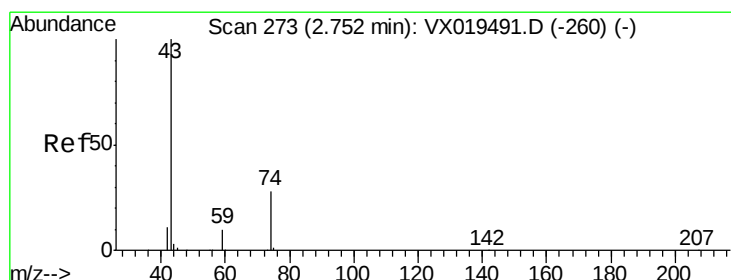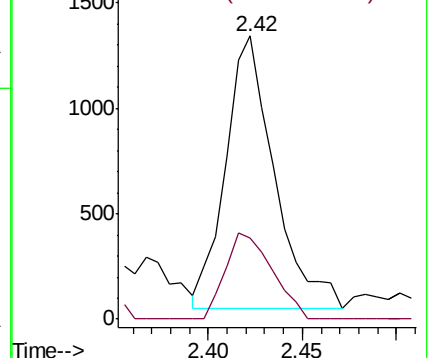

#18

Methyl Acetate

Concen: 0.811 ug/l

RT: 2.75 min Scan# 273

Delta R.T. 0.00 min

Lab File: VX019630.D


Acq: 25 Nov 2020 01:36

Tgt Ion: 43 Resp: 682

Ion Ratio Lower Upper



43 100


74 7.9 22.2 33.4#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

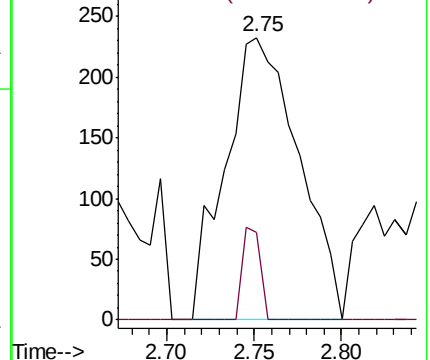

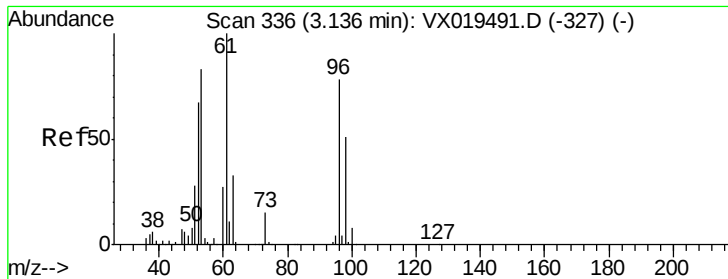

#21

trans-1,2-Dichloroethene

Concen: 7.256 ug/l

RT: 3.14 min Scan# 337

Delta R.T. 0.01 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :

INTERCEPTOR-20201119





Tgt Ion: 96 Resp: 25346

Ion Ratio Lower Upper

96 100

61 130.8 102.9 154.3

98 63.4 52.1 78.1

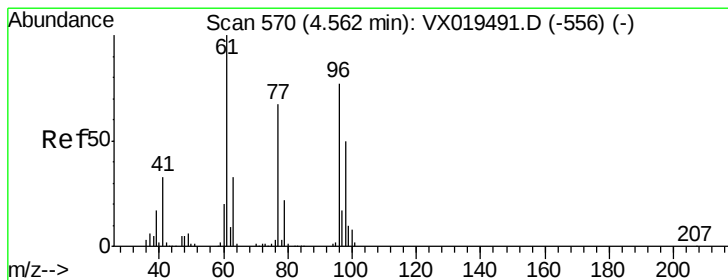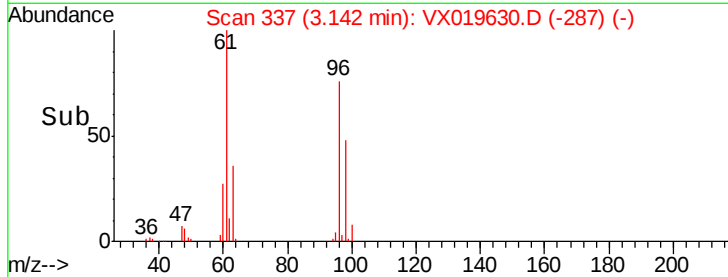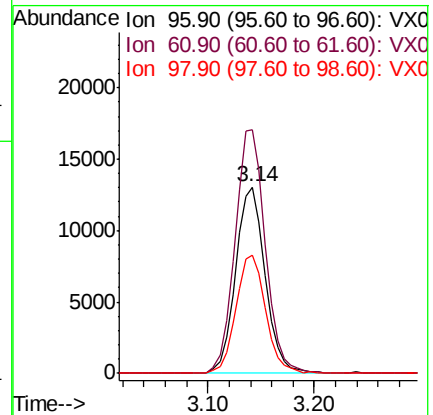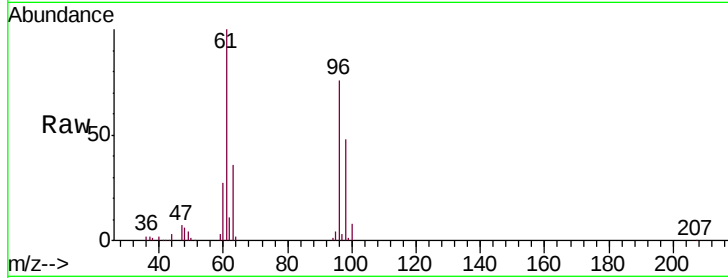

#27

cis-1,2-Dichloroethene

Concen: 340.522 ug/l

RT: 4.56 min Scan# 570

Delta R.T. -0.00 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36




Tgt Ion: 96 Resp: 1366411


Ion Ratio Lower Upper

96 100

61 121.6 0.0 279.2

98 64.3 0.0 129.8

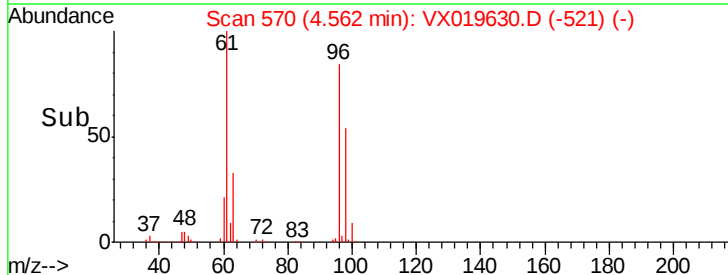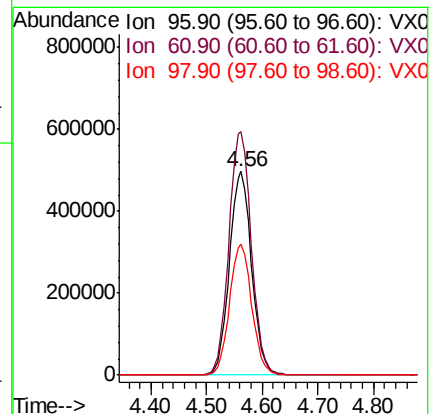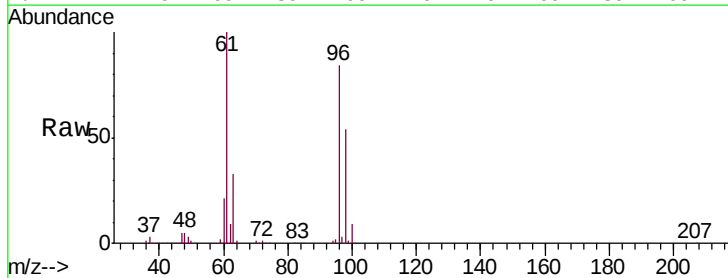

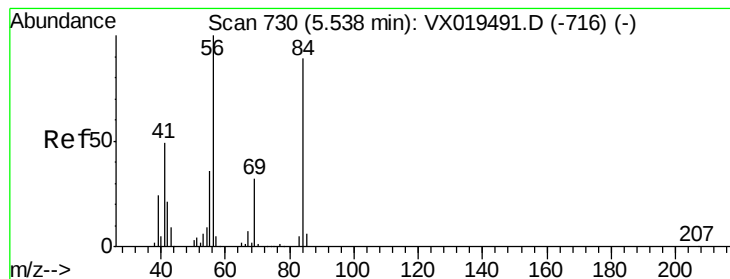

#31

Cyclohexane

Concen: 1.153 ug/l

RT: 5.62 min Scan# 744

Delta R.T. 0.09 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :

INTERCEPTOR-20201119


Tgt Ion: 56 Resp: 6038

Ion Ratio Lower Upper

56 100

69 189.8 25.5 38.3#




84 145.9 71.1 106.7#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

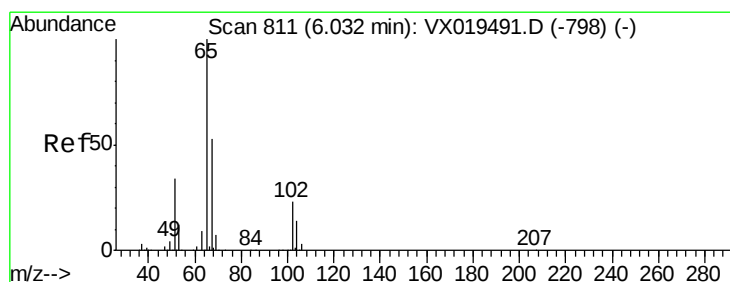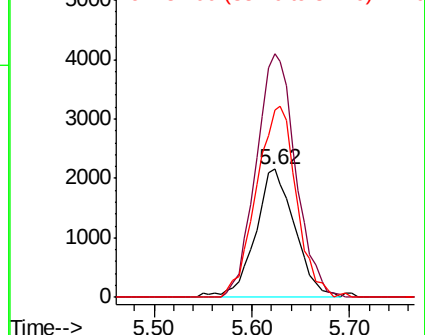

#33

1,2-Dichloroethane-d4

Concen: 47.126 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX019630.D


Acq: 25 Nov 2020 01:36

Tgt Ion: 65 Resp: 189761

Ion Ratio Lower Upper



65 100


67 52.2 0.0 105.0

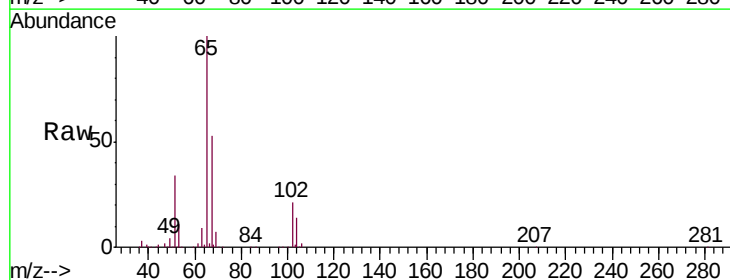

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0




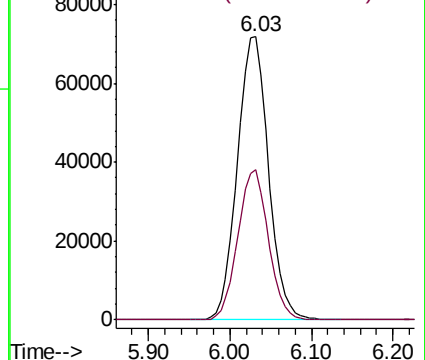




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36




Instrument :
 MSVOA_X
 ClientSampleId :
 INTERCEPTOR-20201119


Tgt Ion:114 Resp: 506078
 Ion Ratio Lower Upper
 114 100
 63 20.0 0.0 38.8
 88 16.3 0.0 31.6

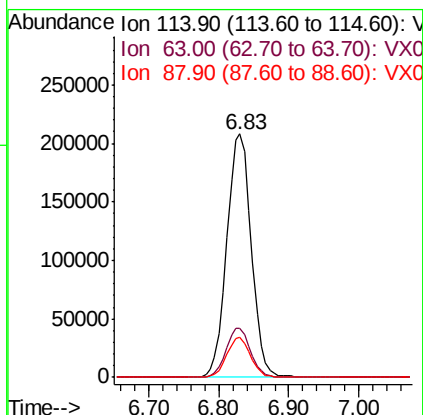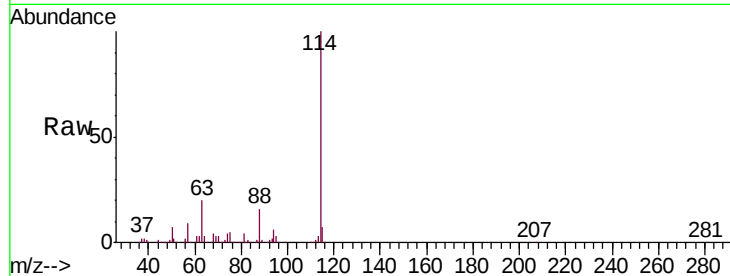

#35
 Dibromofluoromethane
 Concen: 47.255 ug/l
 RT: 5.46 min Scan# 717
 Delta R.T. -0.01 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36

Tgt Ion:113 Resp: 150113
 Ion Ratio Lower Upper
 113 100
 111 102.6 81.5 122.3
 192 20.3 16.2 24.2

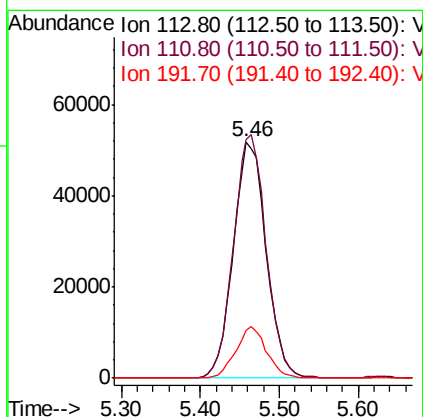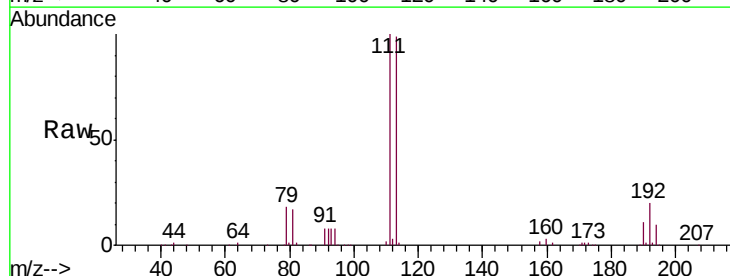

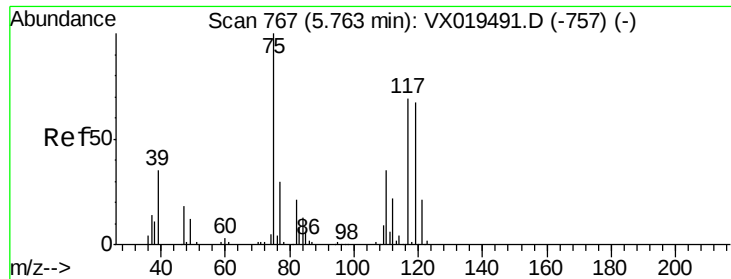

#36

1,1-Dichloropropene

Concen: 4.906 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.14 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :

INTERCEPTOR-20201119


Tgt Ion: 75 Resp: 23276

Ion Ratio Lower Upper

75 100

110 9.1 18.1 54.3#




77 0.0 24.2 36.4#

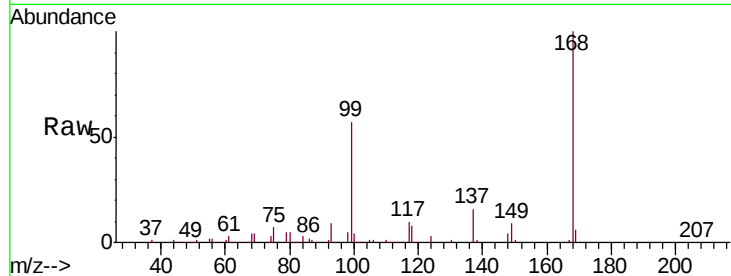

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

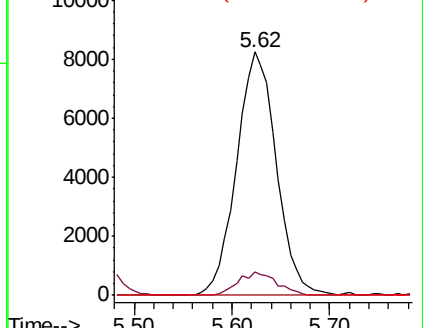

#38

Carbon Tetrachloride

Concen: 6.577 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36


Tgt Ion: 117 Resp: 30204

Ion Ratio Lower Upper

117 100

119 5.7 75.9 113.9#



121 0.0 24.0 36.0#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V



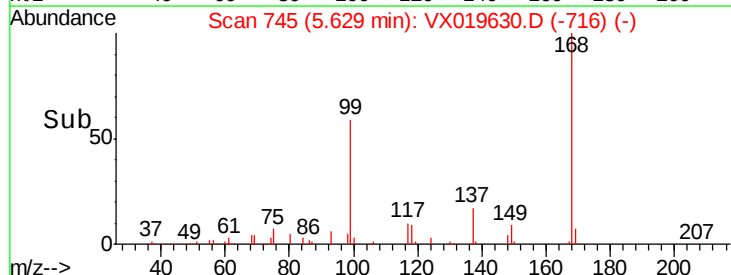
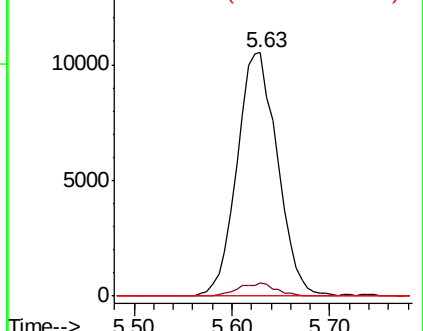




#39
Methylcyclohexane
Concen: 10.171 ug/l
RT: 7.19 min Scan# 1001
Delta R.T. -0.25 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36




Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119


Tgt Ion: 83 Resp: 56185
Ion Ratio Lower Upper
83 100
55 0.3 58.3 87.5#
98 208.5 38.9 58.3#

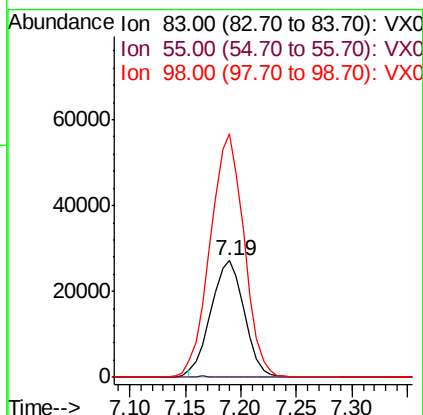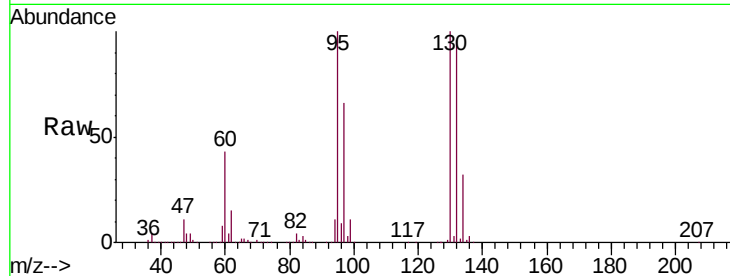

#44
Trichloroethene
Concen: 1243.371 ug/l
RT: 7.19 min Scan# 1001
Delta R.T. 0.01 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36

Tgt Ion:130 Resp: 4747685
Ion Ratio Lower Upper
130 100
95 100.2 0.0 191.2

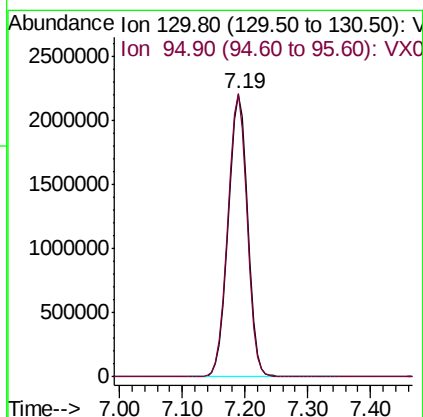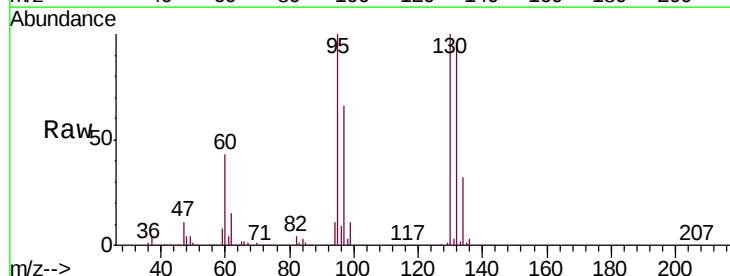







#49
1,4-Dioxane
Concen: 0.251 ug/l
RT: 7.72 min Scan# 1088
Delta R.T. -0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119

Tgt Ion: 88 Resp: 20
Ion Ratio Lower Upper
88 100
43 1135.0 23.8 35.6#
58 0.0 54.2 81.2#

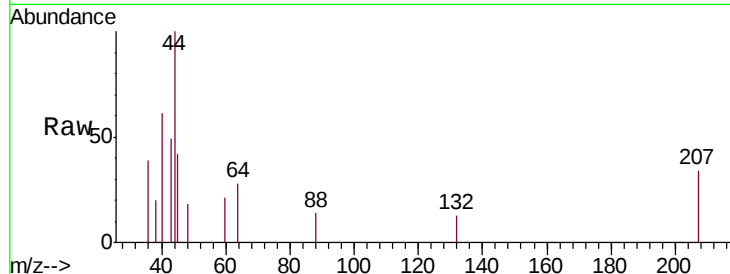


Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0


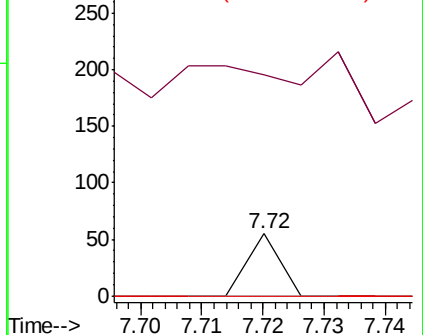



#50
Toluene-d8
Concen: 48.803 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36

Tgt Ion: 98 Resp: 602426
Ion Ratio Lower Upper
98 100
100 67.1 52.4 78.6

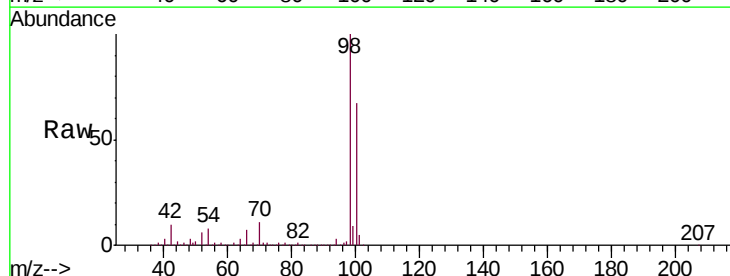

Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

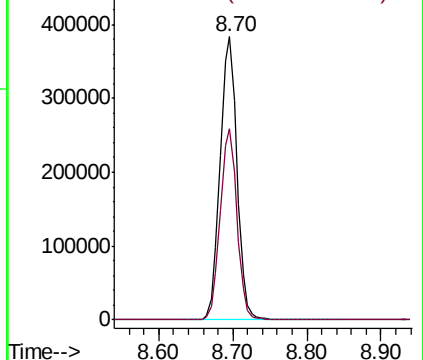



#60

Dibromochloromethane

Concen: 0.415 ug/l

RT: 9.31 min Scan# 1349

Delta R.T. -0.26 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :


INTERCEPTOR-20201119

Tgt Ion:129 Resp: 1477

Ion Ratio Lower Upper

129 100

127 0.0 39.0 116.9#

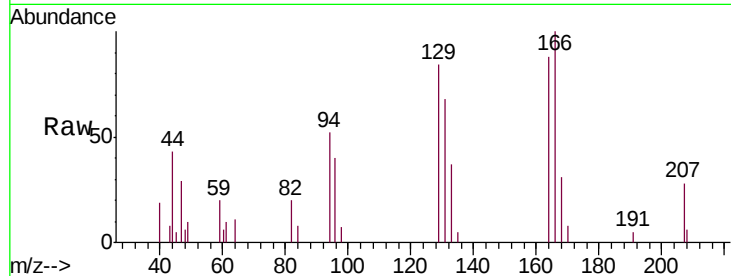

Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

9.31

1000

800

600



400

200

0

9.30 9.35

Time-->

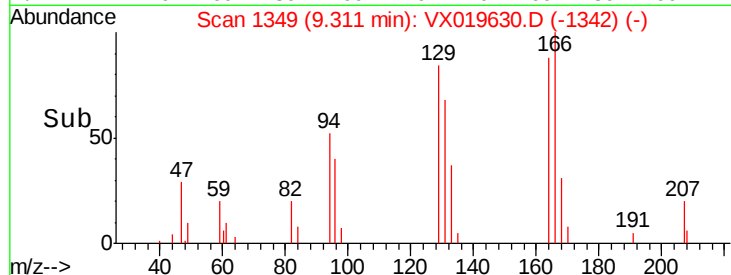

#62

4-Bromofluorobenzene

Concen: 48.628 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36


Tgt Ion: 95 Resp: 215970

Ion Ratio Lower Upper

95 100

174 77.7 0.0 156.2

176 75.5 0.0 151.4



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

200000

150000


100000


50000

0

11.10 11.20

Time-->







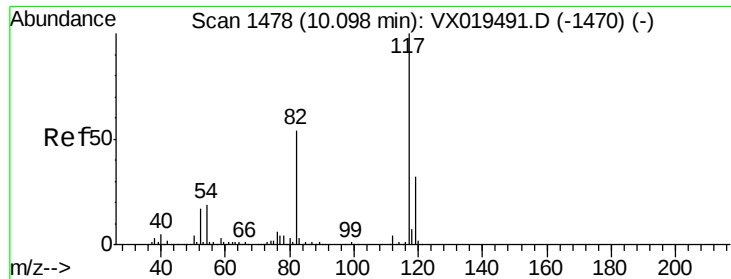

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36




Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119


Tgt Ion:117 Resp: 461998
Ion Ratio Lower Upper
117 100
82 53.4 43.0 64.4
119 32.5 25.6 38.4

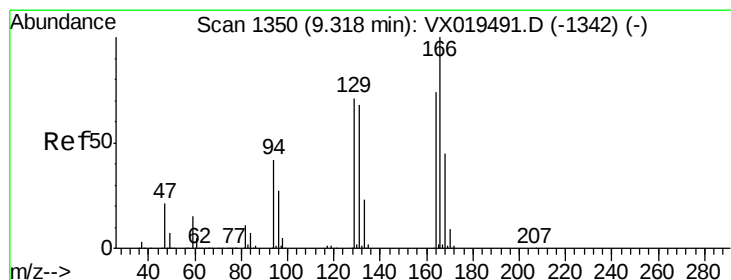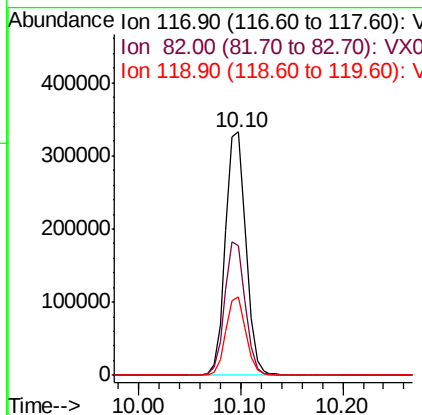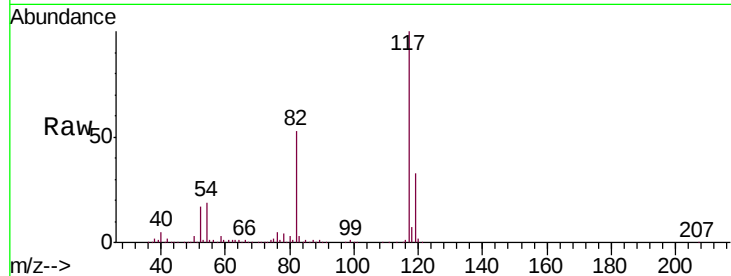

#64
Tetrachloroethene
Concen: 0.444 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36

Tgt Ion:164 Resp: 1614
Ion Ratio Lower Upper
164 100
166 121.2 107.4 161.0
129 88.6 76.6 114.8
131 87.4 72.6 108.8


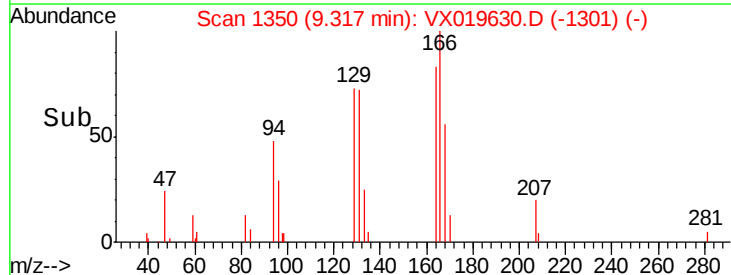
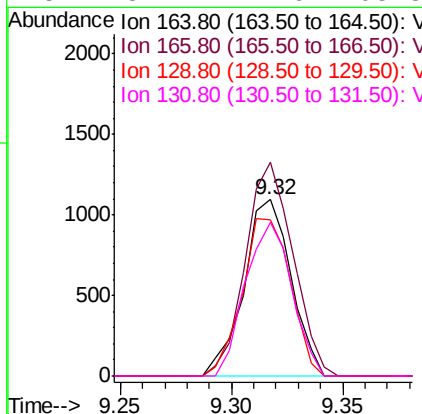



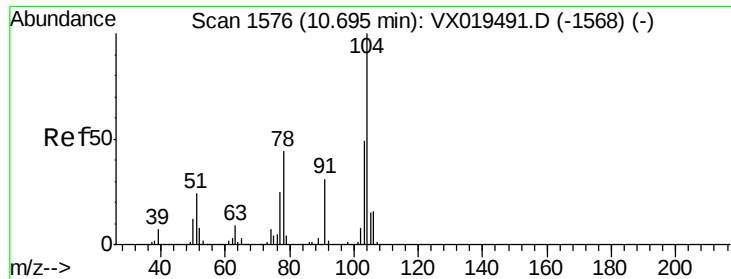

#70
Styrene
Concen: 1.654 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. 0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36




Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-20201119


Tgt Ion:104 Resp: 93
Ion Ratio Lower Upper
104 100
78 73.1 39.5 59.3#
103 97.8 43.6 65.4#

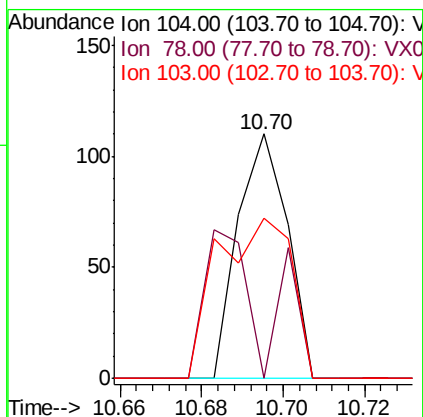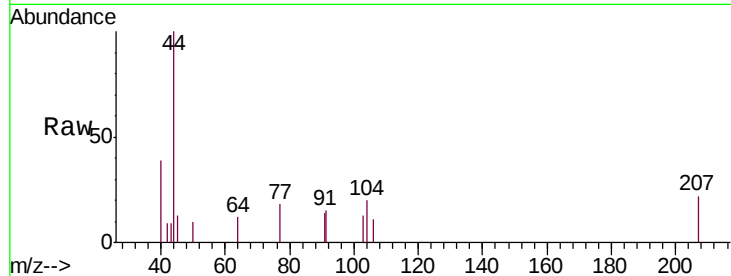

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX019630.D
Acq: 25 Nov 2020 01:36

Tgt Ion:152 Resp: 191581
Ion Ratio Lower Upper
152 100
115 60.7 41.8 125.4
150 158.0 0.0 348.2



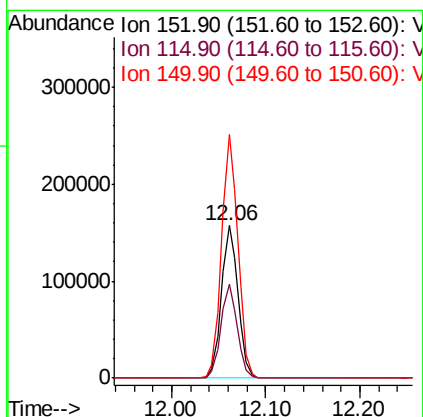





#76
 1,2,3-Trichloropropane
 Concen: 25.276 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. -0.16 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36




Instrument :
 MSVOA_X
 ClientSampleId :
 INTERCEPTOR-20201119


Tgt Ion: 75 Resp: 105679
 Ion Ratio Lower Upper
 75 100
 77 1.2 20.0 60.0#

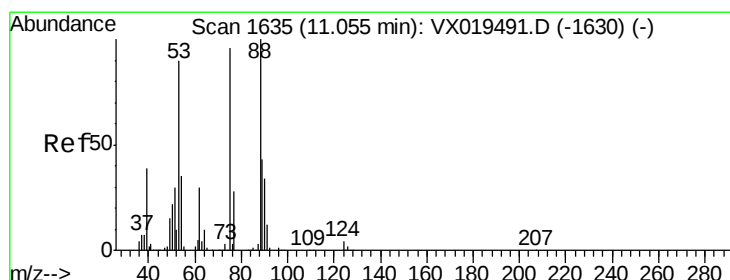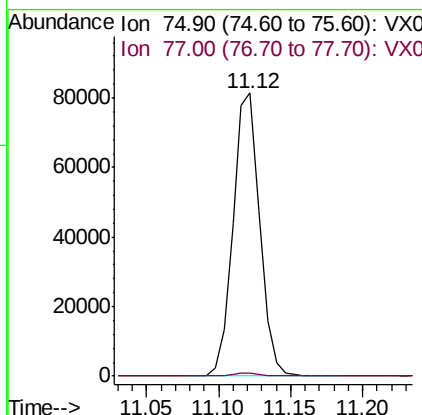

#81
 trans-1,4-Dichloro-2-butene
 Concen: 66.723 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. 0.07 min
 Lab File: VX019630.D
 Acq: 25 Nov 2020 01:36

Tgt Ion: 75 Resp: 105679
 Ion Ratio Lower Upper
 75 100
 53 0.0 73.9 110.9#
 89 0.0 37.3 55.9#

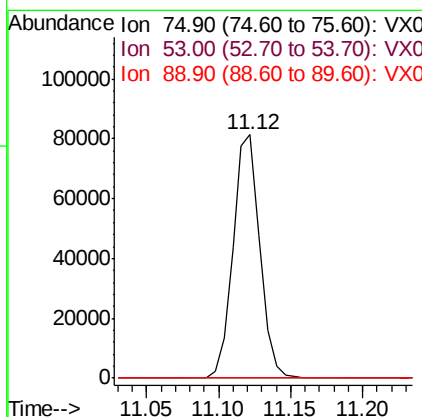

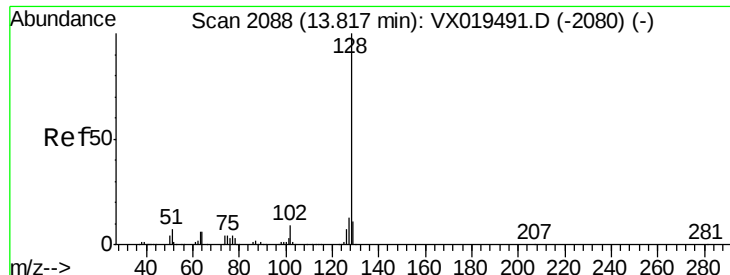

#95

Naphthalene

Concen: 2.272 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019630.D

Acq: 25 Nov 2020 01:36

Instrument :

MSVOA_X

ClientSampleId :

INTERCEPTOR-20201119


Tgt Ion:128 Resp: 1381

Ion Ratio Lower Upper

128 100

127 12.2 10.3 15.5

129 12.1 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

