

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112421\
 Data File : VX025322.D
 Acq On : 24 Nov 2021 13:28
 Operator : JC/MD
 Sample : M4784-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Nov 26 10:33:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	96041	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	173977	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	170289	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	75116	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	58186	57.477	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	114.960%
35) Dibromofluoromethane	5.391	113	56030	52.489	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.980%
50) Toluene-d8	8.653	98	207054	51.589	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	103.180%
62) 4-Bromofluorobenzene	11.079	95	77441	51.003	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112421\
Data File : VX025322.D
Acq On : 24 Nov 2021 13:28
Operator : JC/MD
Sample : M4784-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Nov 26 10:33:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration




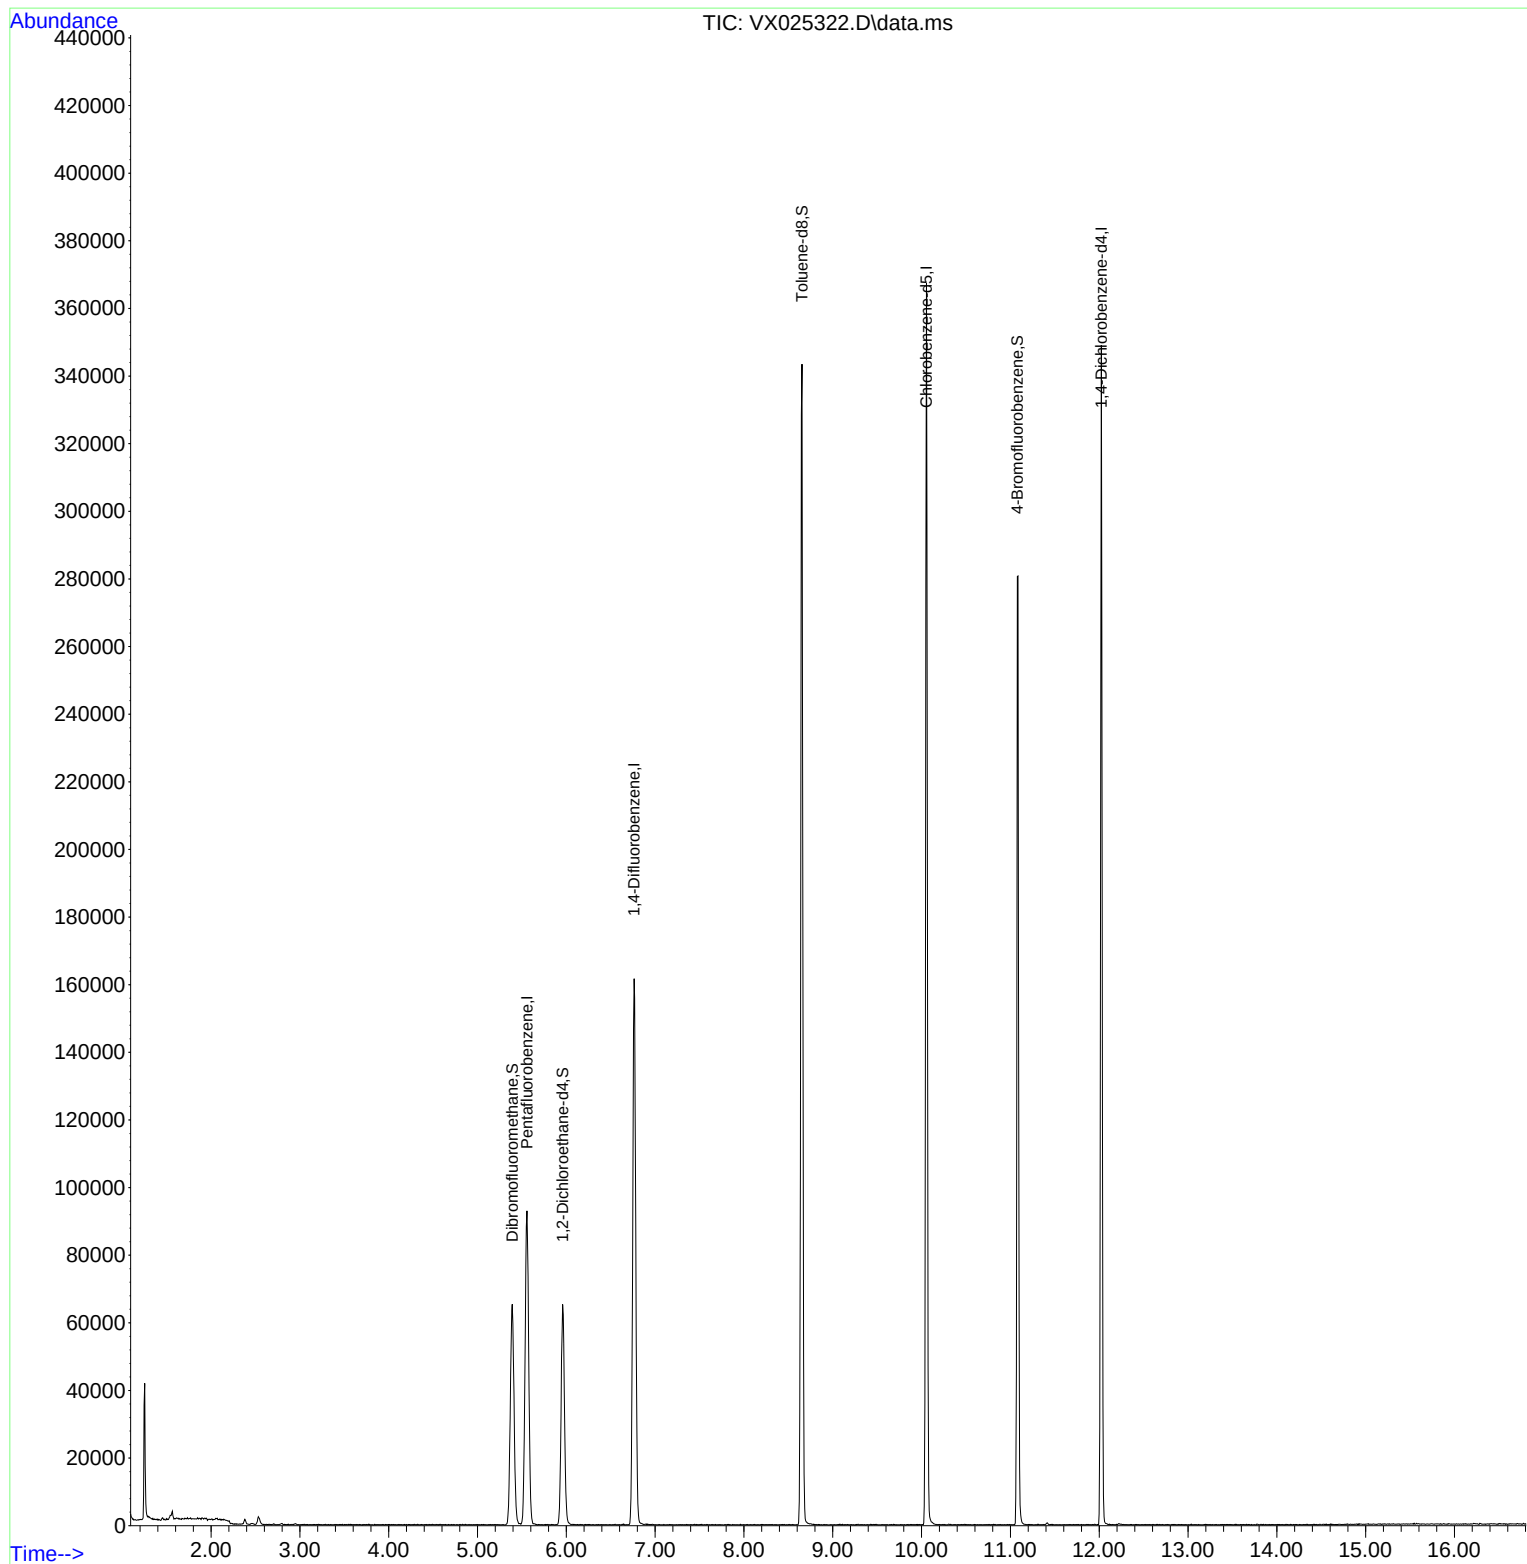


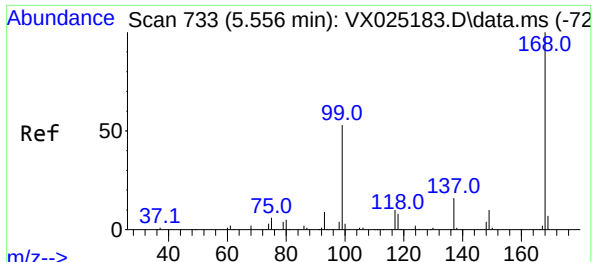

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 96041
Ion Ratio Lower Upper
168 100
99 51.6 46.4 69.6

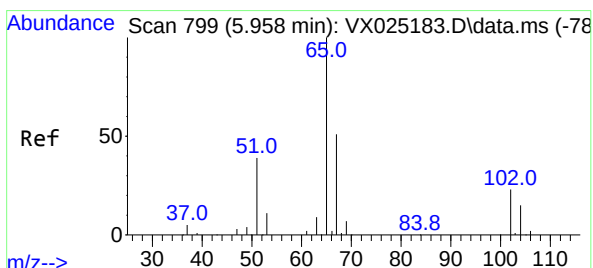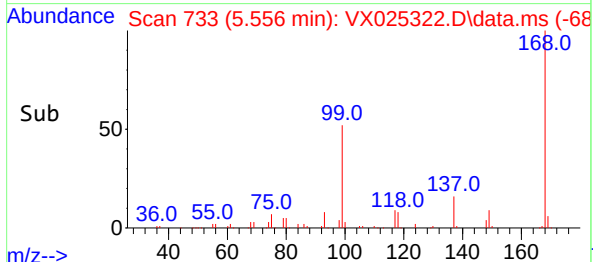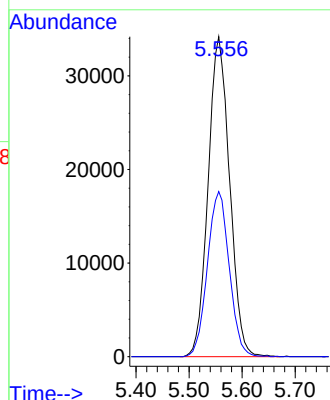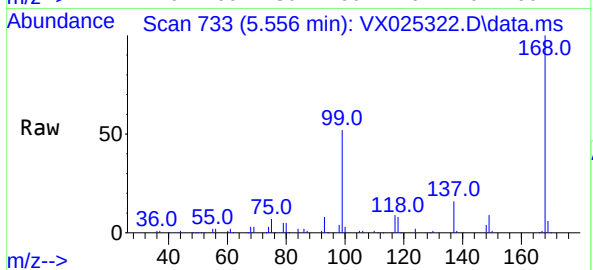

#33
1,2-Dichloroethane-d4
Concen: 57.477 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28

Tgt Ion: 65 Resp: 58186
Ion Ratio Lower Upper
65 100
67 53.2 0.0 101.0


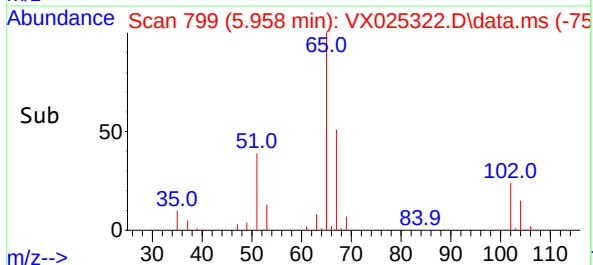
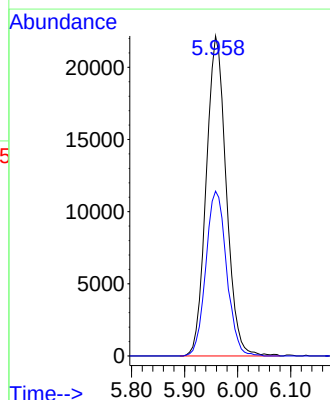
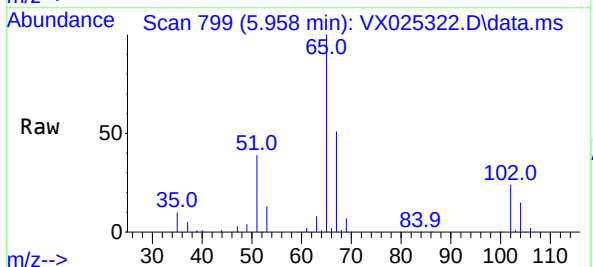


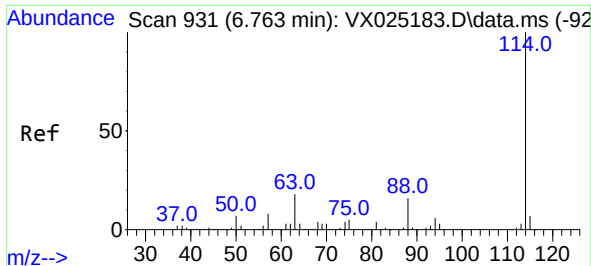

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 173977
Ion Ratio Lower Upper
114 100
63 18.5 0.0 41.0
88 15.5 0.0 34.8

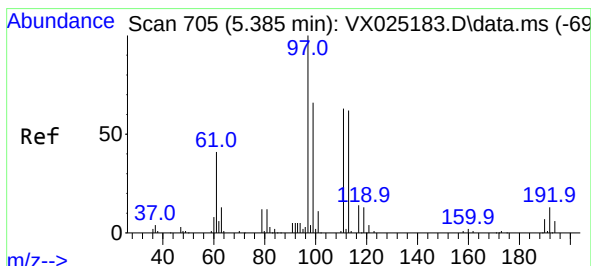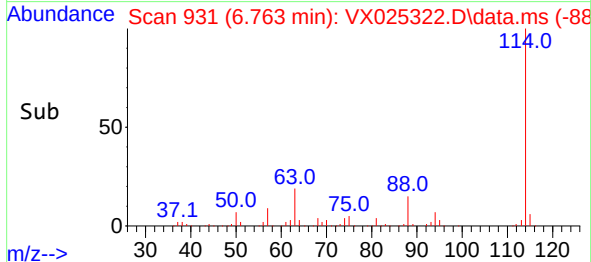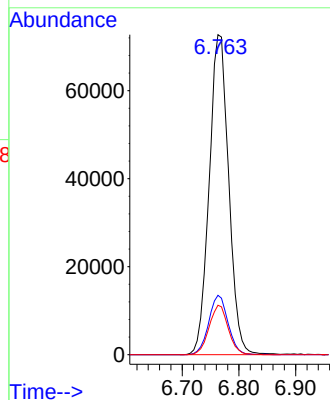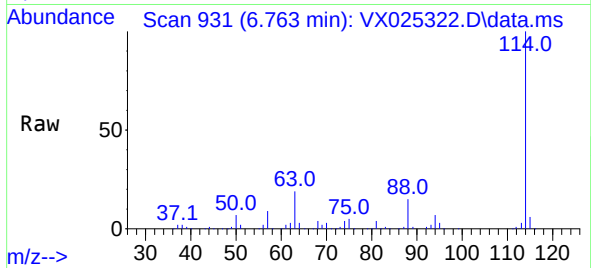

#35
Dibromofluoromethane
Concen: 52.489 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28

Tgt Ion:113 Resp: 56030
Ion Ratio Lower Upper
113 100
111 103.2 82.1 123.1
192 21.8 15.6 23.4

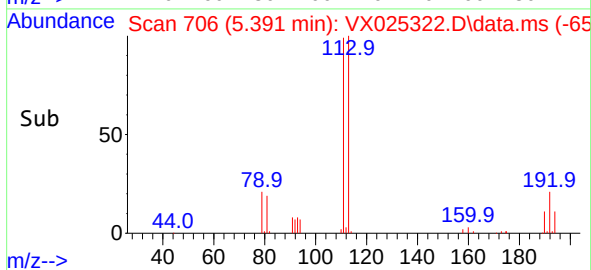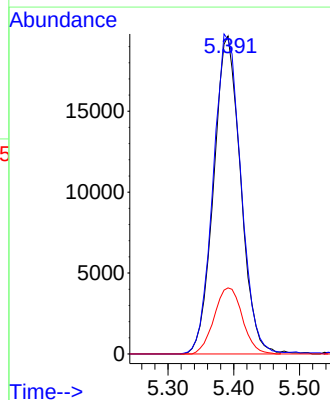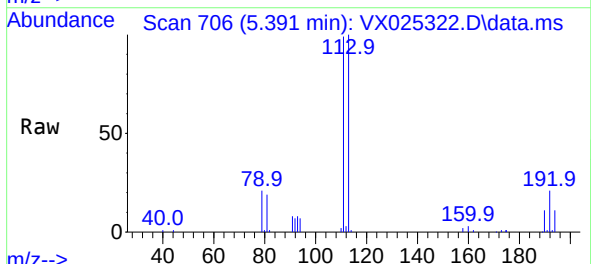

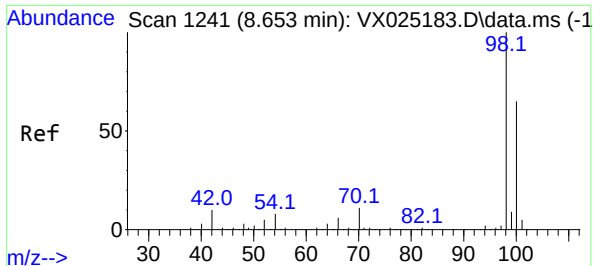

#50

Toluene-d8

Concen: 51.589 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX025322.D

Acq: 24 Nov 2021 13:28

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-WATER-REF-5

Tgt Ion: 98 Resp: 207054

Ion Ratio Lower Upper

98 100

100 66.9 51.4 77.0

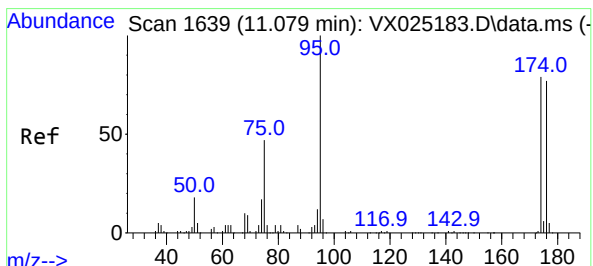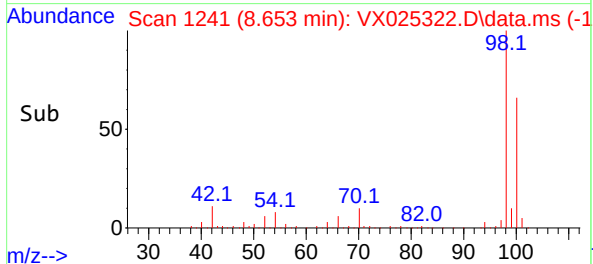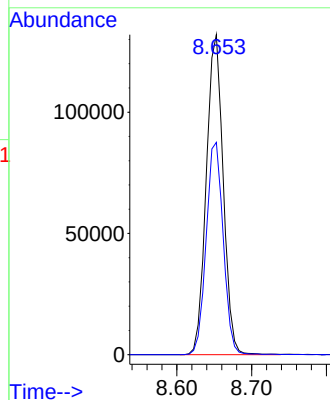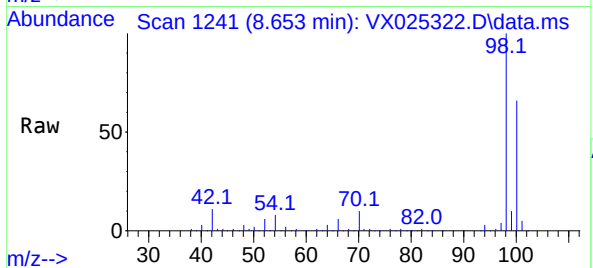

#62

4-Bromofluorobenzene

Concen: 51.003 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX025322.D

Acq: 24 Nov 2021 13:28




Tgt Ion: 95 Resp: 77441


Ion Ratio Lower Upper

95 100

174 86.9 0.0 158.0

176 82.3 0.0 153.6


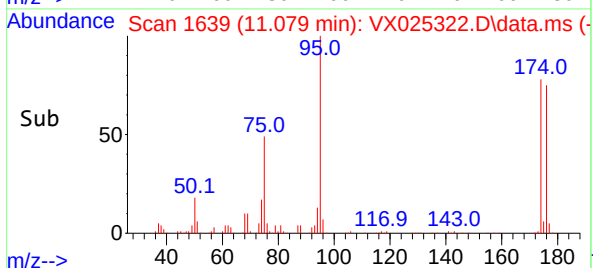
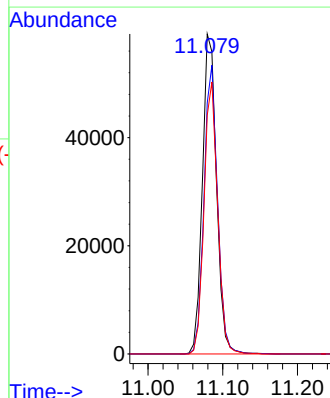
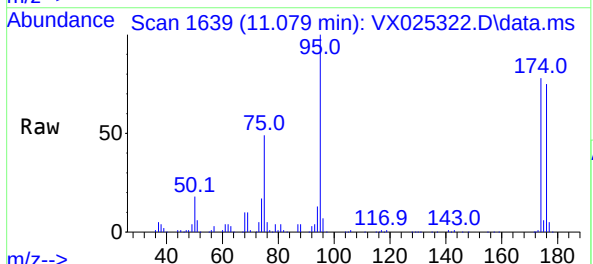


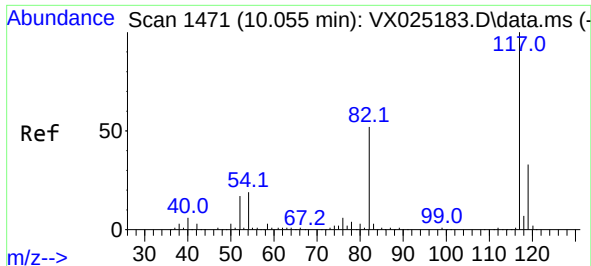

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 170289
Ion Ratio Lower Upper
117 100
82 51.7 44.6 67.0
119 31.6 24.8 37.2

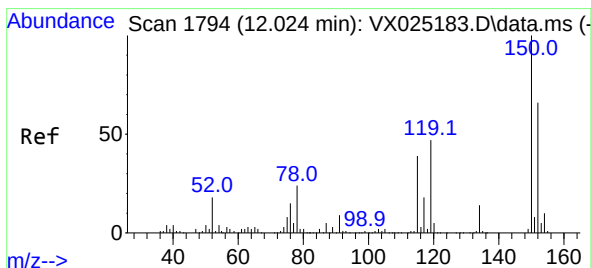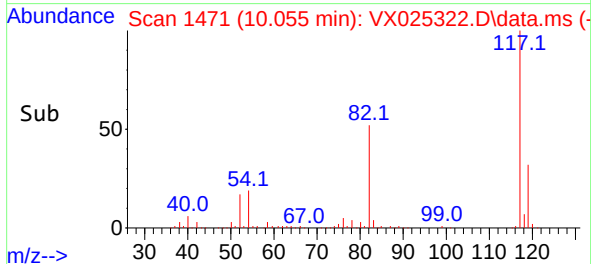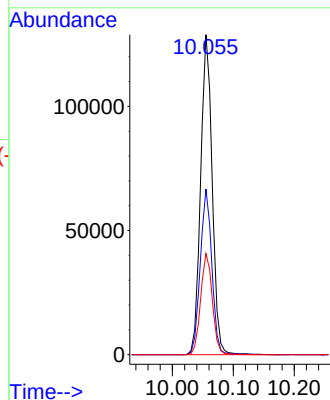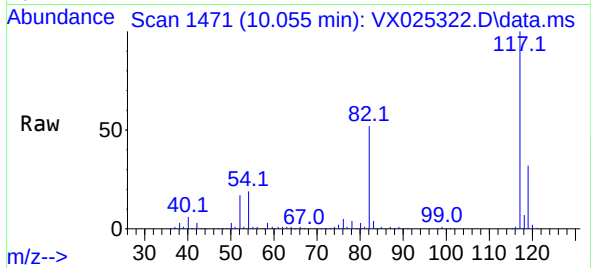

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX025322.D
Acq: 24 Nov 2021 13:28

Tgt Ion:152 Resp: 75116
Ion Ratio Lower Upper
152 100
115 56.5 43.3 129.8
150 156.6 0.0 351.2

