

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112423\
 Data File : VX039025.D
 Acq On : 24 Nov 2023 15:32
 Operator : JC/MD
 Sample : VX1124WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1124WBL02

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX039025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.544	70	75	82	rVB5	2732	4907	1.57%	0.375%
2	2.947	300	305	312	rVB5	1490	3436	1.10%	0.263%
3	4.556	560	569	577	rBV2	4482	14593	4.66%	1.116%
4	4.897	616	625	642	rVB3	23618	71047	22.70%	5.431%
5	5.952	788	798	812	rBV	44197	119644	38.23%	9.147%
6	6.763	922	931	943	rBV	77056	188032	60.08%	14.375%
7	8.647	1234	1240	1257	rBV	194184	312945	100.00%	23.924%
8	10.055	1465	1471	1483	rBV	213447	306337	97.89%	23.419%
9	11.079	1634	1639	1651	rBV	210497	280457	89.62%	21.441%
10	12.024	1790	1794	1801	rVB3	3591	6673	2.13%	0.510%




Sum of corrected areas: 1308071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112423\
Data File : VX039025.D
Acq On : 24 Nov 2023 15:32
Operator : JC/MD
Sample : VX1124WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

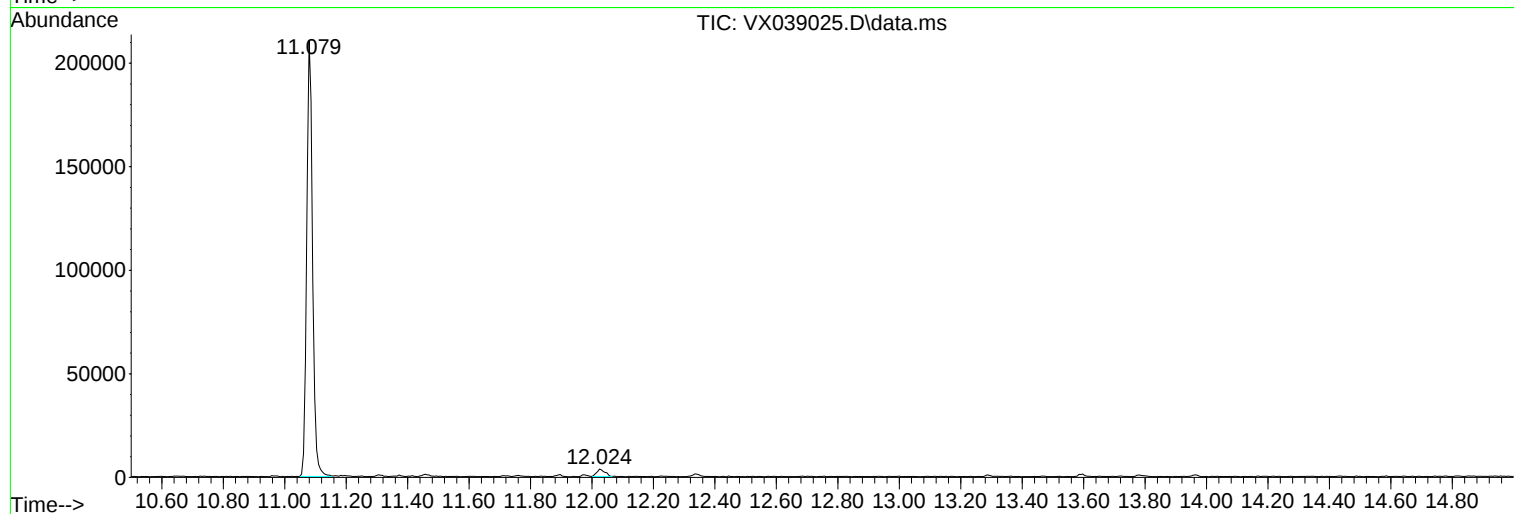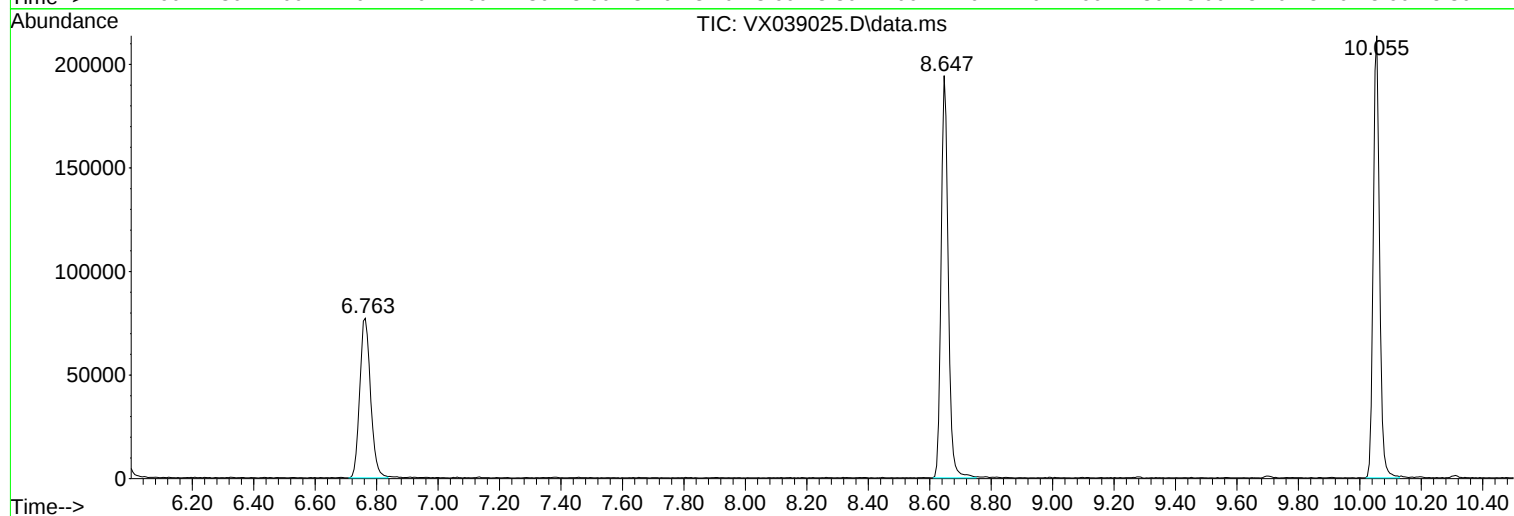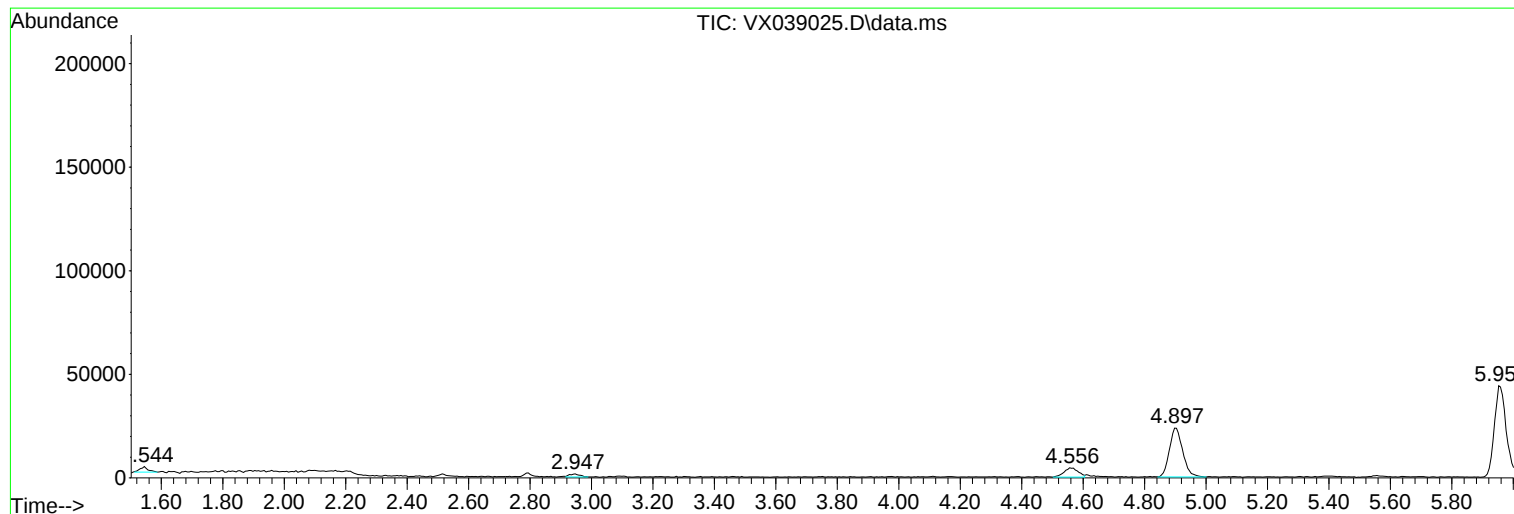

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112423\
Data File : VX039025.D
Acq On : 24 Nov 2023 15:32
Operator : JC/MD
Sample : VX1124WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112423\
Data File : VX039025.D
Acq On : 24 Nov 2023 15:32
Operator : JC/MD
Sample : VX1124WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------