
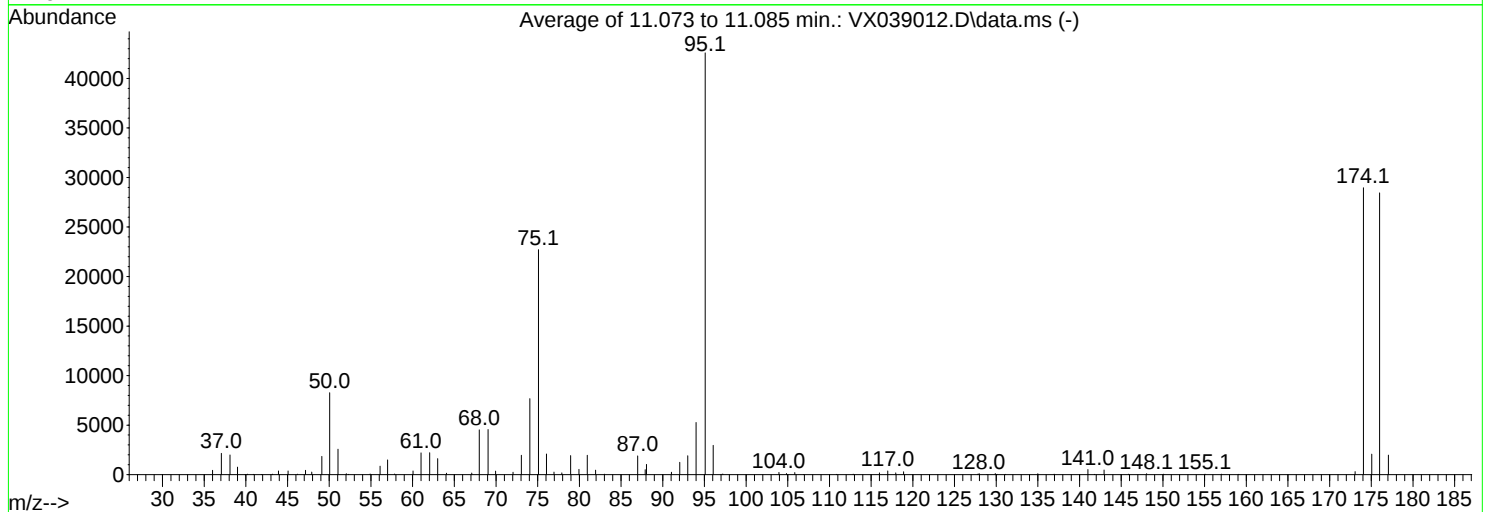


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112423\
Data File : VX039012.D
Acq On : 24 Nov 2023 08:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Nov 27 03:22:25 2023

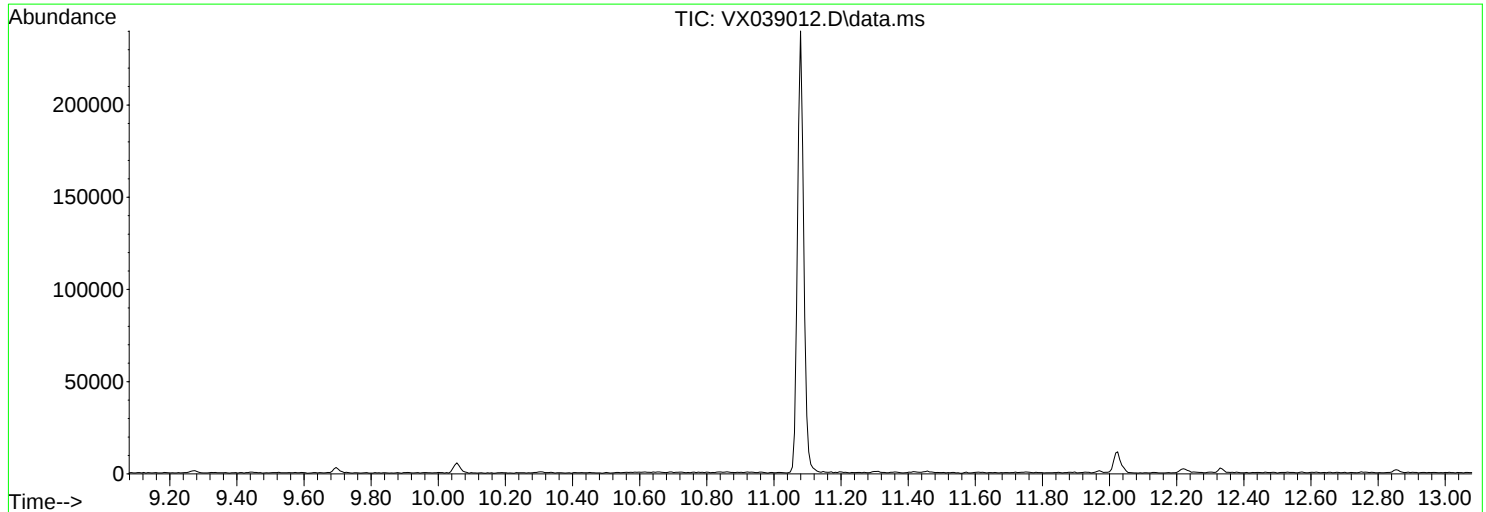

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	8265	PASS
75	95	30	60	53.3	22709	PASS
95	95	100	100	100.0	42587	PASS
96	95	5	9	7.0	2964	PASS
173	174	0.00	2	1.1	313	PASS
174	95	50	100	68.0	28965	PASS
175	174	5	9	7.1	2062	PASS
176	174	95	101	98.2	28451	PASS
177	176	5	9	6.9	1973	PASS