

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112425\
 Data File : VX048660.D
 Acq On : 24 Nov 2025 13:56
 Operator : JC/MD
 Sample : VX1124WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1124WBL01

Quant Time: Nov 26 00:24:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 08 05:08:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.537	168	214588	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	413236	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	436701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	231925	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	140122	46.862	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	93.720%
35) Dibromofluoromethane	5.373	113	133054	42.542	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	85.080%
50) Toluene-d8	8.634	98	462882	47.453	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.900%
62) 4-Bromofluorobenzene	11.061	95	199508	54.882	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112425\
Data File : VX048660.D
Acq On : 24 Nov 2025 13:56
Operator : JC/MD
Sample : VX1124WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL01

Quant Time: Nov 26 00:24:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 08 05:08:11 2025
Response via : Initial Calibration




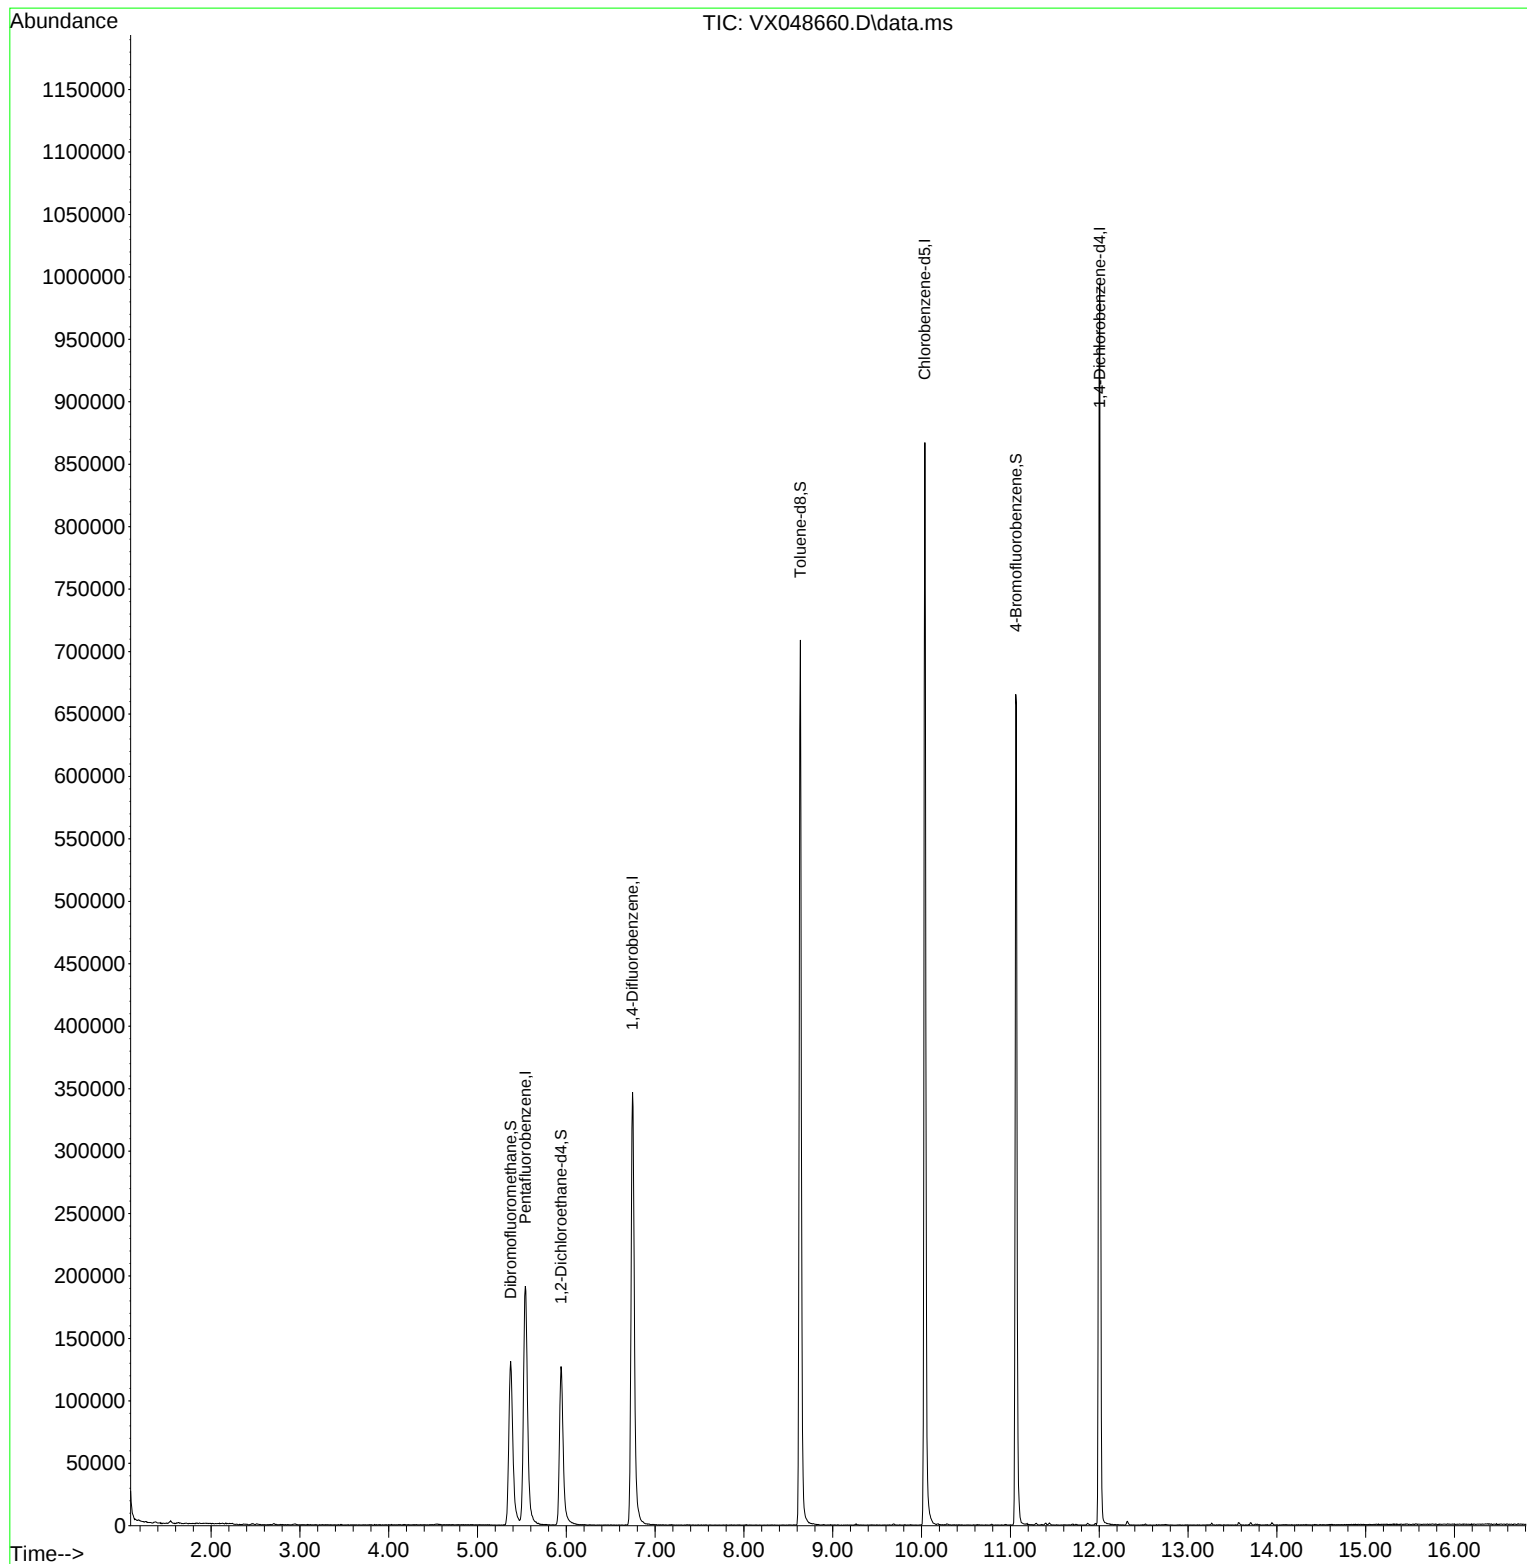


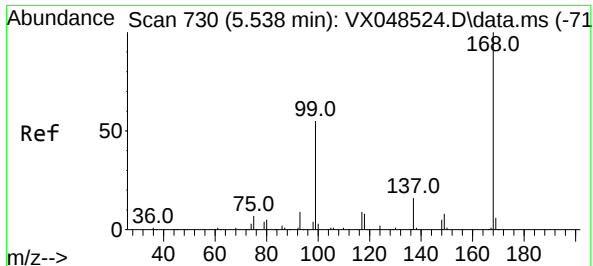

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.001 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56




Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL01


Tgt Ion:168 Resp: 214588
Ion Ratio Lower Upper
168 100
99 56.6 45.2 67.8

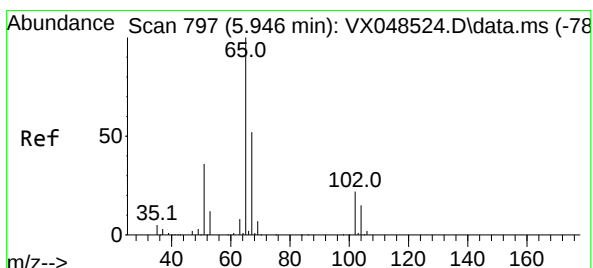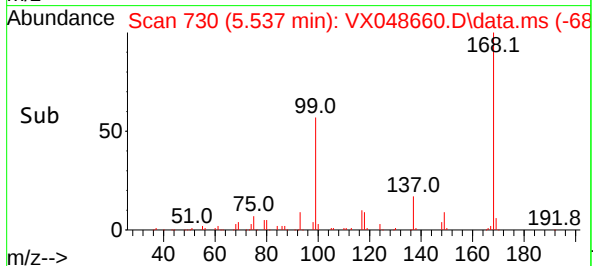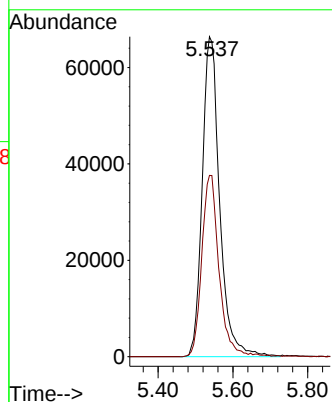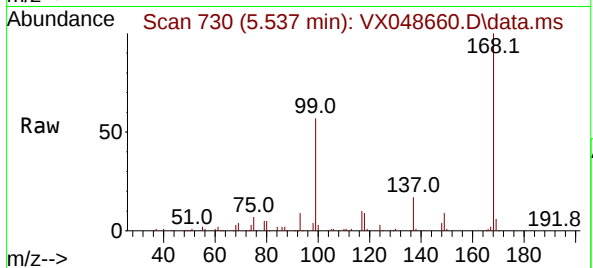

#33
1,2-Dichloroethane-d4
Concen: 46.862 ug/l
RT: 5.940 min Scan# 796
Delta R.T. -0.006 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56

Tgt Ion: 65 Resp: 140122
Ion Ratio Lower Upper
65 100
67 51.4 0.0 106.2

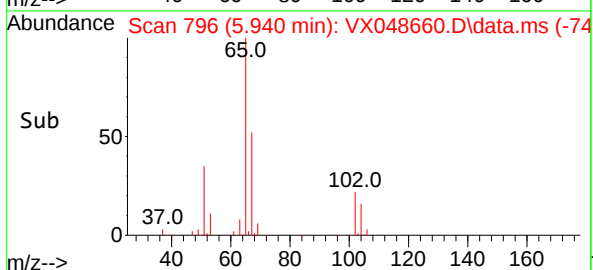
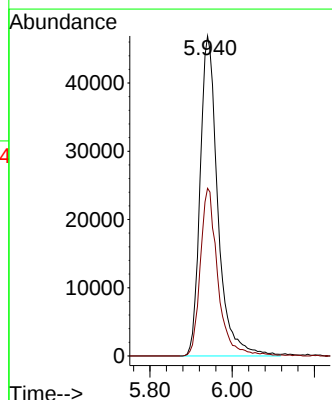
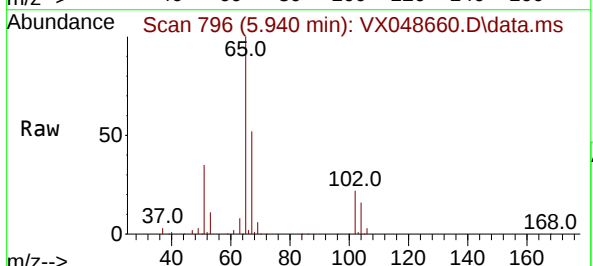


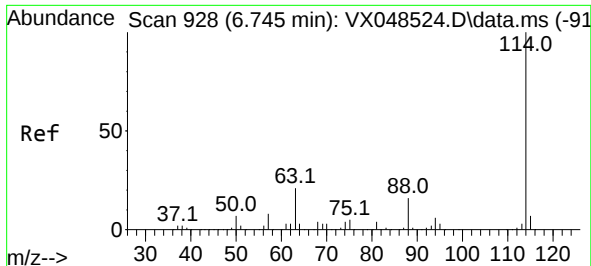

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56




Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL01


Tgt Ion:114 Resp: 413236
Ion Ratio Lower Upper
114 100
63 19.3 0.0 41.2
88 15.0 0.0 32.2

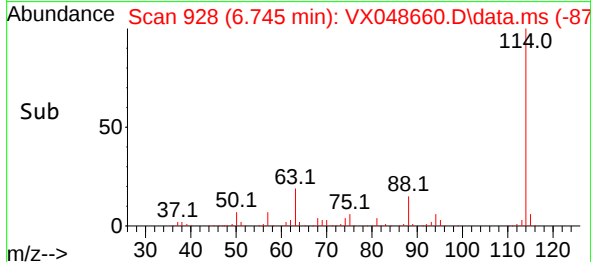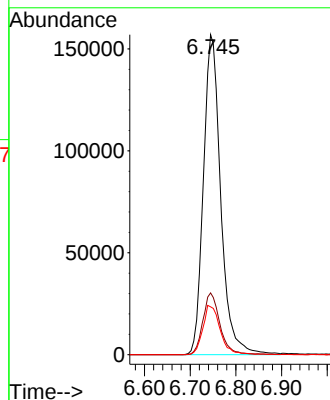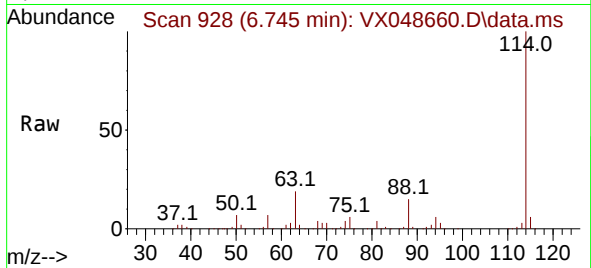

#35
Dibromofluoromethane
Concen: 42.542 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56

Tgt Ion:113 Resp: 133054
Ion Ratio Lower Upper
113 100
111 101.4 81.9 122.9
192 21.8 15.8 23.6


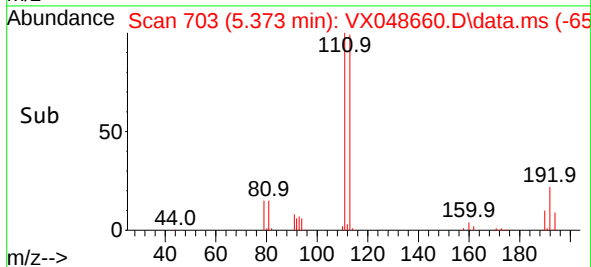
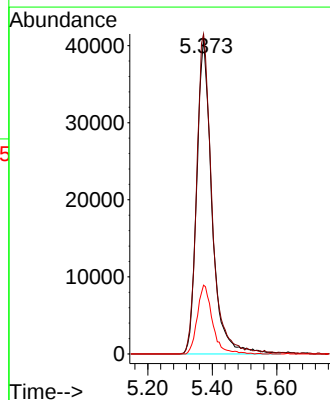
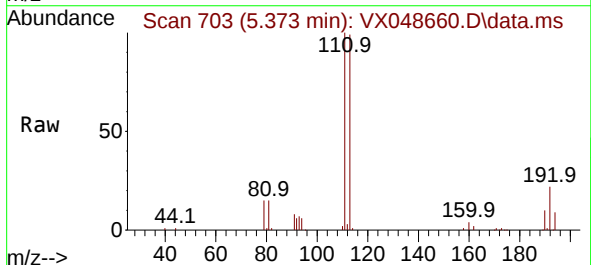


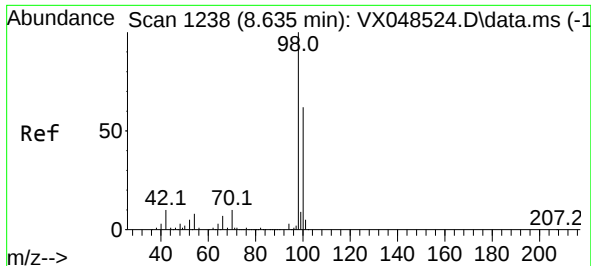

#50
Toluene-d8
Concen: 47.453 ug/l
RT: 8.634 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56




Instrument :
MSVOA_X
ClientSampleId :
VX1124WBL01


Tgt Ion: 98 Resp: 462882
Ion Ratio Lower Upper
98 100
100 66.3 53.6 80.4

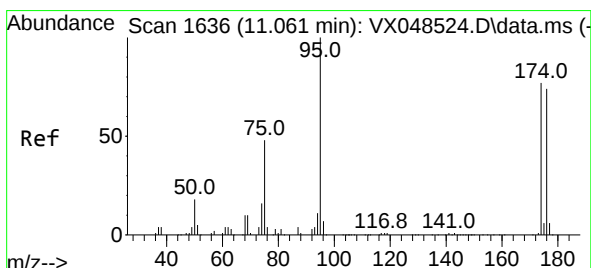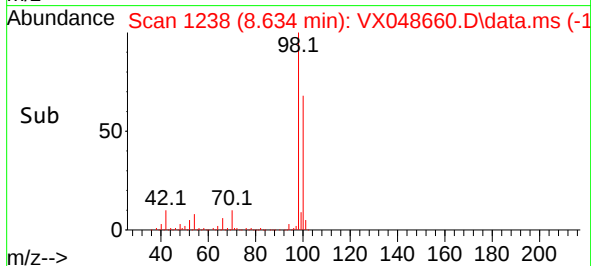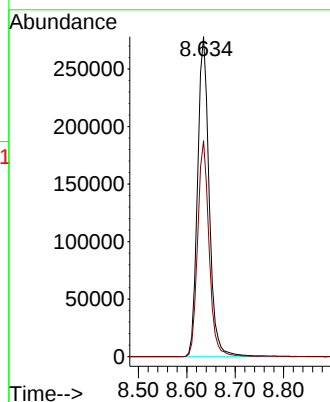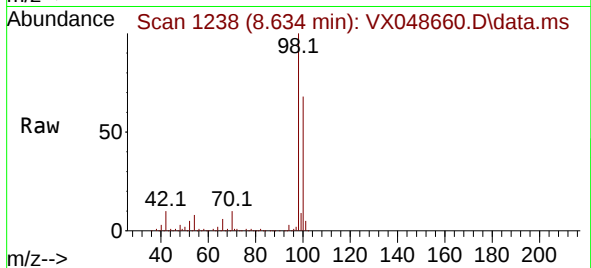

#62
4-Bromofluorobenzene
Concen: 54.882 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX048660.D
Acq: 24 Nov 2025 13:56

Tgt Ion: 95 Resp: 199508
Ion Ratio Lower Upper
95 100
174 84.5 0.0 161.8
176 81.4 0.0 153.6

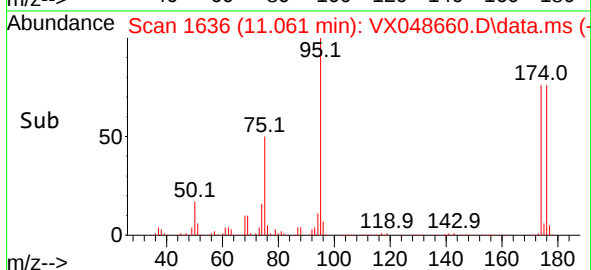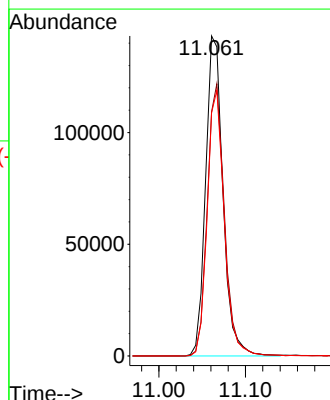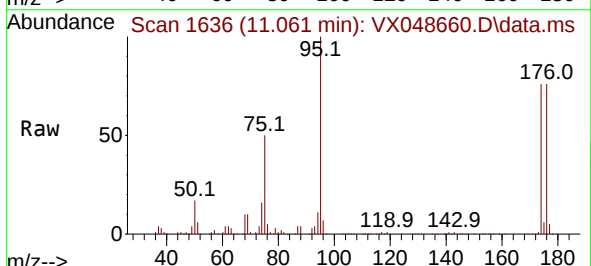

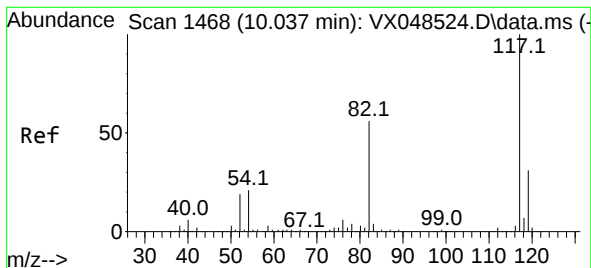

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VX048660.D

Acq: 24 Nov 2025 13:56

Instrument :

MSVOA_X

ClientSampleId :

VX1124WBL01





Tgt Ion:117 Resp: 436701

Ion Ratio Lower Upper

117 100

82 54.4 44.4 66.6

119 32.5 25.1 37.7

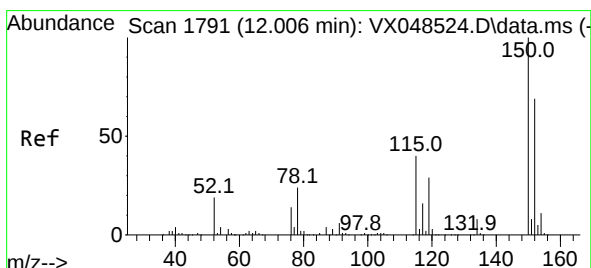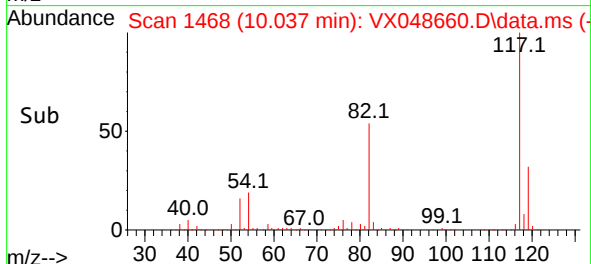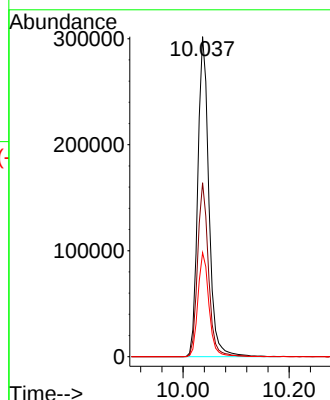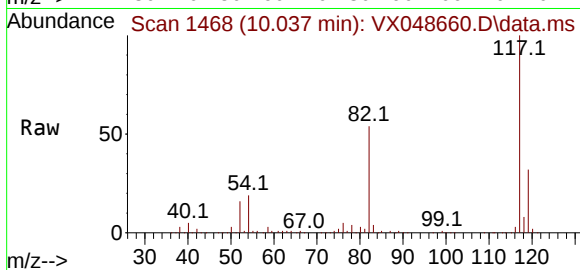

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX048660.D

Acq: 24 Nov 2025 13:56

Tgt Ion:152 Resp: 231925

Ion Ratio Lower Upper

152 100

115 59.0 39.2 117.6

150 157.5 0.0 347.0

