

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112425\  
Data File : VX048659.D  
Acq On : 24 Nov 2025 13:36  
Operator : JC/MD  
Sample : VX1124MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1124MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X110725W.M

Title : SW846 8260

Signal : TIC: VX048659.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.367       | 692           | 702         | 719          | rBV2     | 95210          | 311342        | 31.42%          | 5.901%        |
| 2         | 5.531       | 719           | 729         | 750          | rVB2     | 141365         | 443427        | 44.75%          | 8.405%        |
| 3         | 5.933       | 785           | 795         | 816          | rBV2     | 96970          | 296375        | 29.91%          | 5.618%        |
| 4         | 6.738       | 918           | 927         | 949          | rBV      | 268132         | 691884        | 69.83%          | 13.115%       |
| 5         | 8.628       | 1231          | 1237        | 1258         | rBV      | 529236         | 884411        | 89.26%          | 16.764%       |
| 6         | 10.036      | 1462          | 1468        | 1487         | rBV      | 648404         | 952535        | 96.13%          | 18.055%       |
| 7         | 11.061      | 1631          | 1636        | 1650         | rBV      | 489829         | 680925        | 68.72%          | 12.907%       |
| 8         | 12.006      | 1785          | 1791        | 1808         | rVB      | 729484         | 990868        | 100.00%         | 18.782%       |
| 9         | 12.316      | 1836          | 1842        | 1849         | rVB2     | 10271          | 13754         | 1.39%           | 0.261%        |
| 10        | 13.944      | 2103          | 2109        | 2115         | rBV2     | 7038           | 10152         | 1.02%           | 0.192%        |




Sum of corrected areas: 5275673

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112425\  
Data File : VX048659.D  
Acq On : 24 Nov 2025 13:36  
Operator : JC/MD  
Sample : VX1124MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1124MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X110725W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

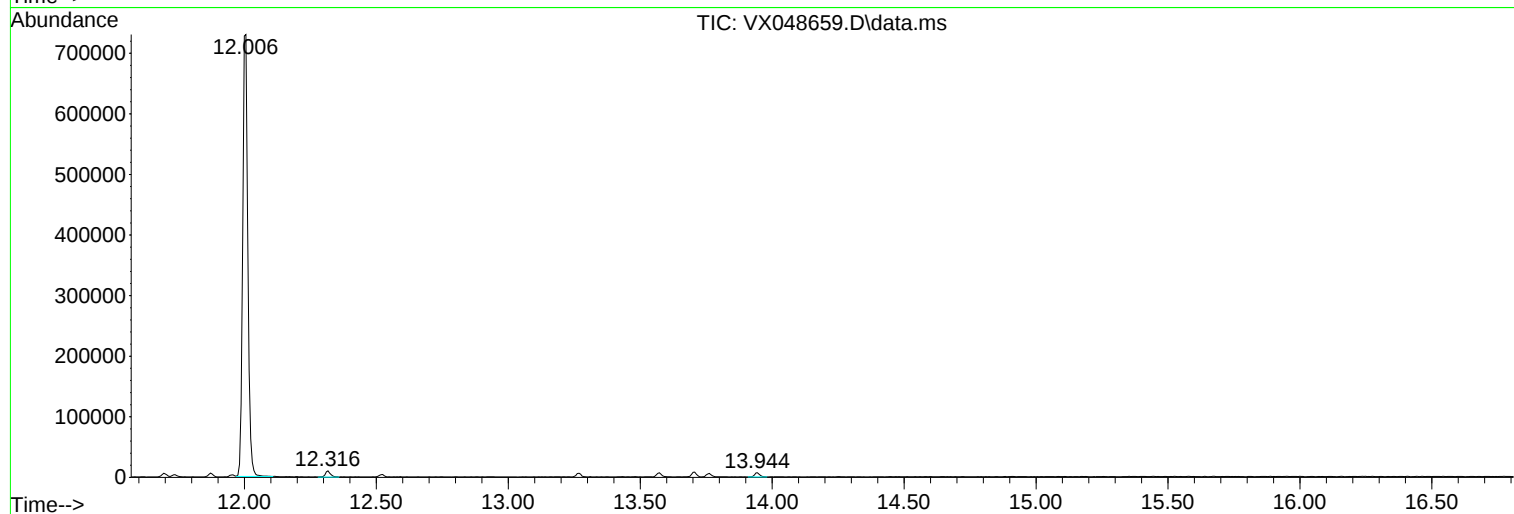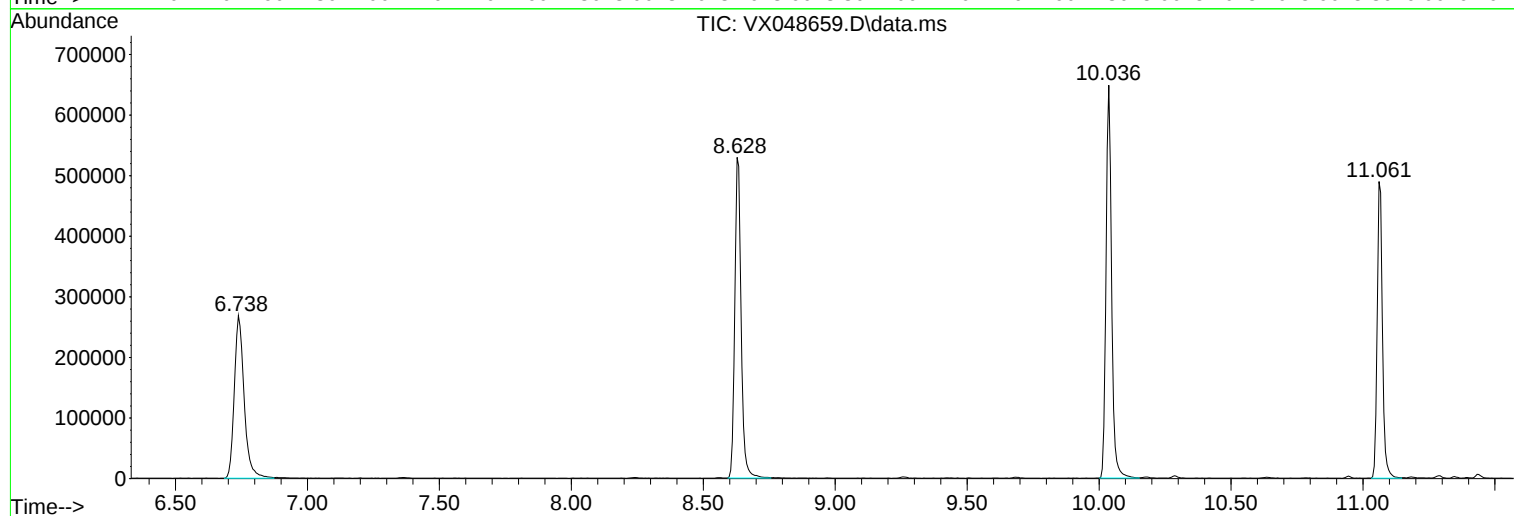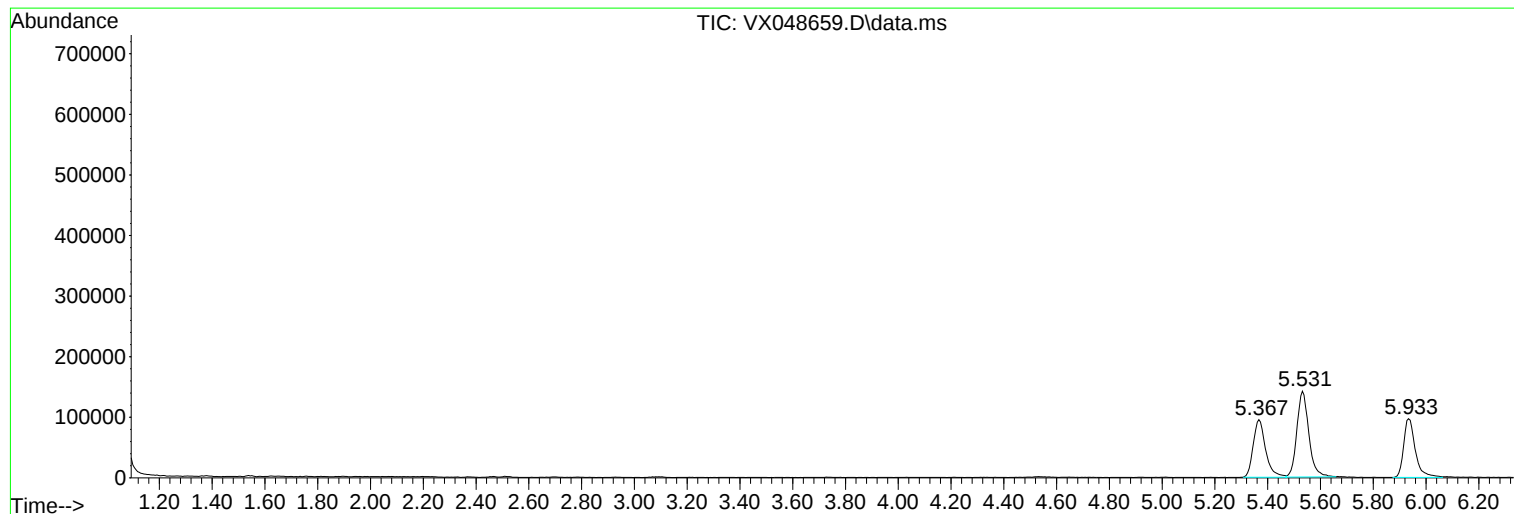

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112425\  
Data File : VX048659.D  
Acq On : 24 Nov 2025 13:36  
Operator : JC/MD  
Sample : VX1124MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1124MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X110725W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX112425\  
Data File : VX048659.D  
Acq On : 24 Nov 2025 13:36  
Operator : JC/MD  
Sample : VX1124MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1124MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X110725W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |