
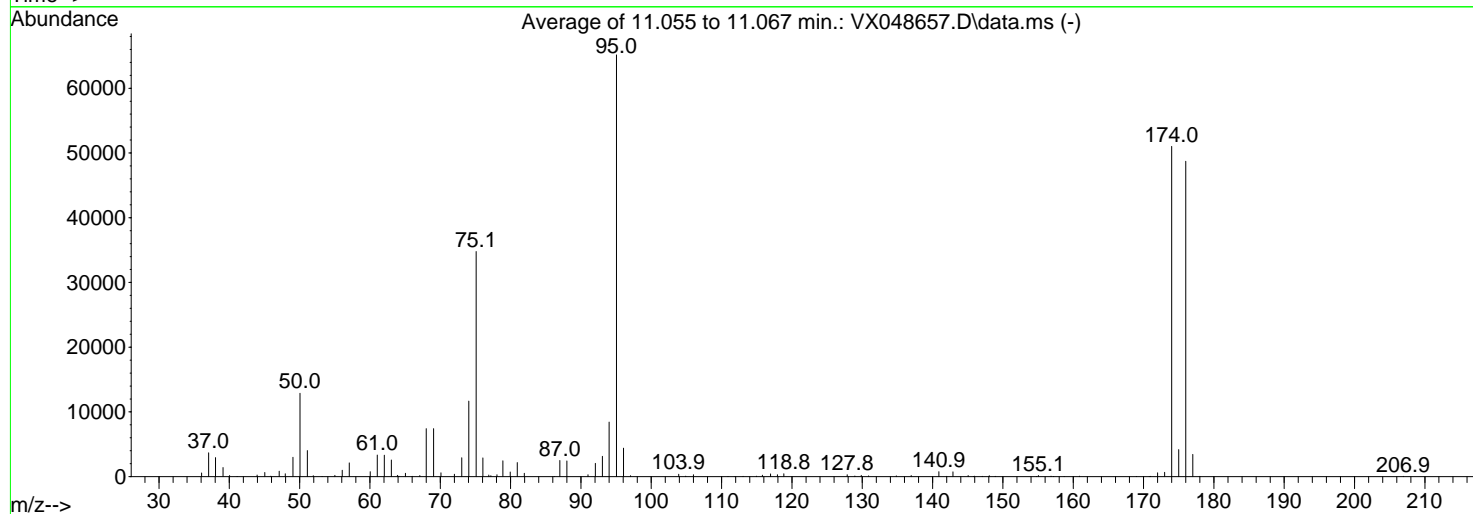


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112425\
 Data File : VX048657.D
 Acq On : 24 Nov 2025 12:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
 Title : SW846 8260
 Last Update : Sat Nov 08 05:08:11 2025

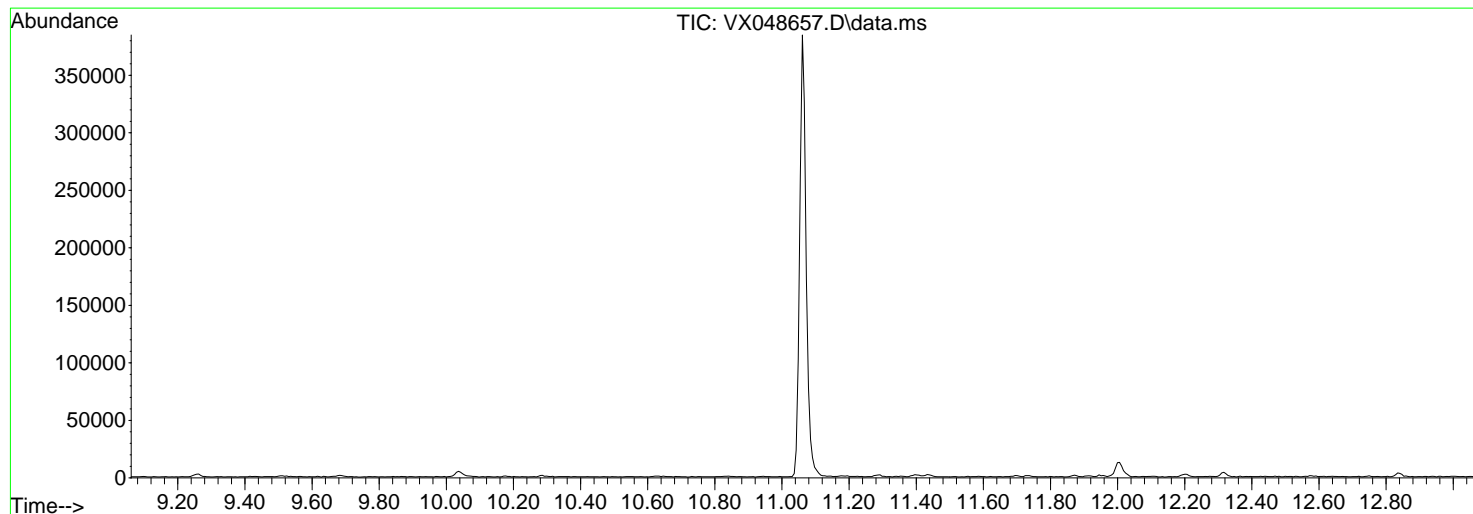

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12875	PASS
75	95	30	60	53.4	34781	PASS
95	95	100	100	100.0	65165	PASS
96	95	5	9	6.8	4407	PASS
173	174	0.00	2	1.3	668	PASS
174	95	50	100	78.3	51013	PASS
175	174	5	9	8.2	4182	PASS
176	174	95	101	95.5	48715	PASS
177	176	5	9	7.1	3451	PASS