

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112519\
 Data File : VX013591.D
 Acq On : 25 Nov 2019 19:07
 Operator : JC/SP
 Sample : K5968-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WEST-DITCH-IN-20191121

Quant Time: Nov 26 04:27:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 02 07:06:38 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	673599	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	1094877	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	987976	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	449263	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	404434	50.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.36%	
35) Dibromofluoromethane	5.49	113	327696	47.72	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.44%	
50) Toluene-d8	8.71	98	1302392	50.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.62%	
62) 4-Bromofluorobenzene	11.13	95	440142	47.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.22%	
Target Compounds						
44) Trichloroethene	7.20	130	4963	0.616	ug/l	Qvalue 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112519\
Data File : VX013591.D
Acq On : 25 Nov 2019 19:07
Operator : JC/SP
Sample : K5968-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WEST-DITCH-IN-20191121

Quant Time: Nov 26 04:27:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 02 07:06:38 2019
Response via : Initial Calibration

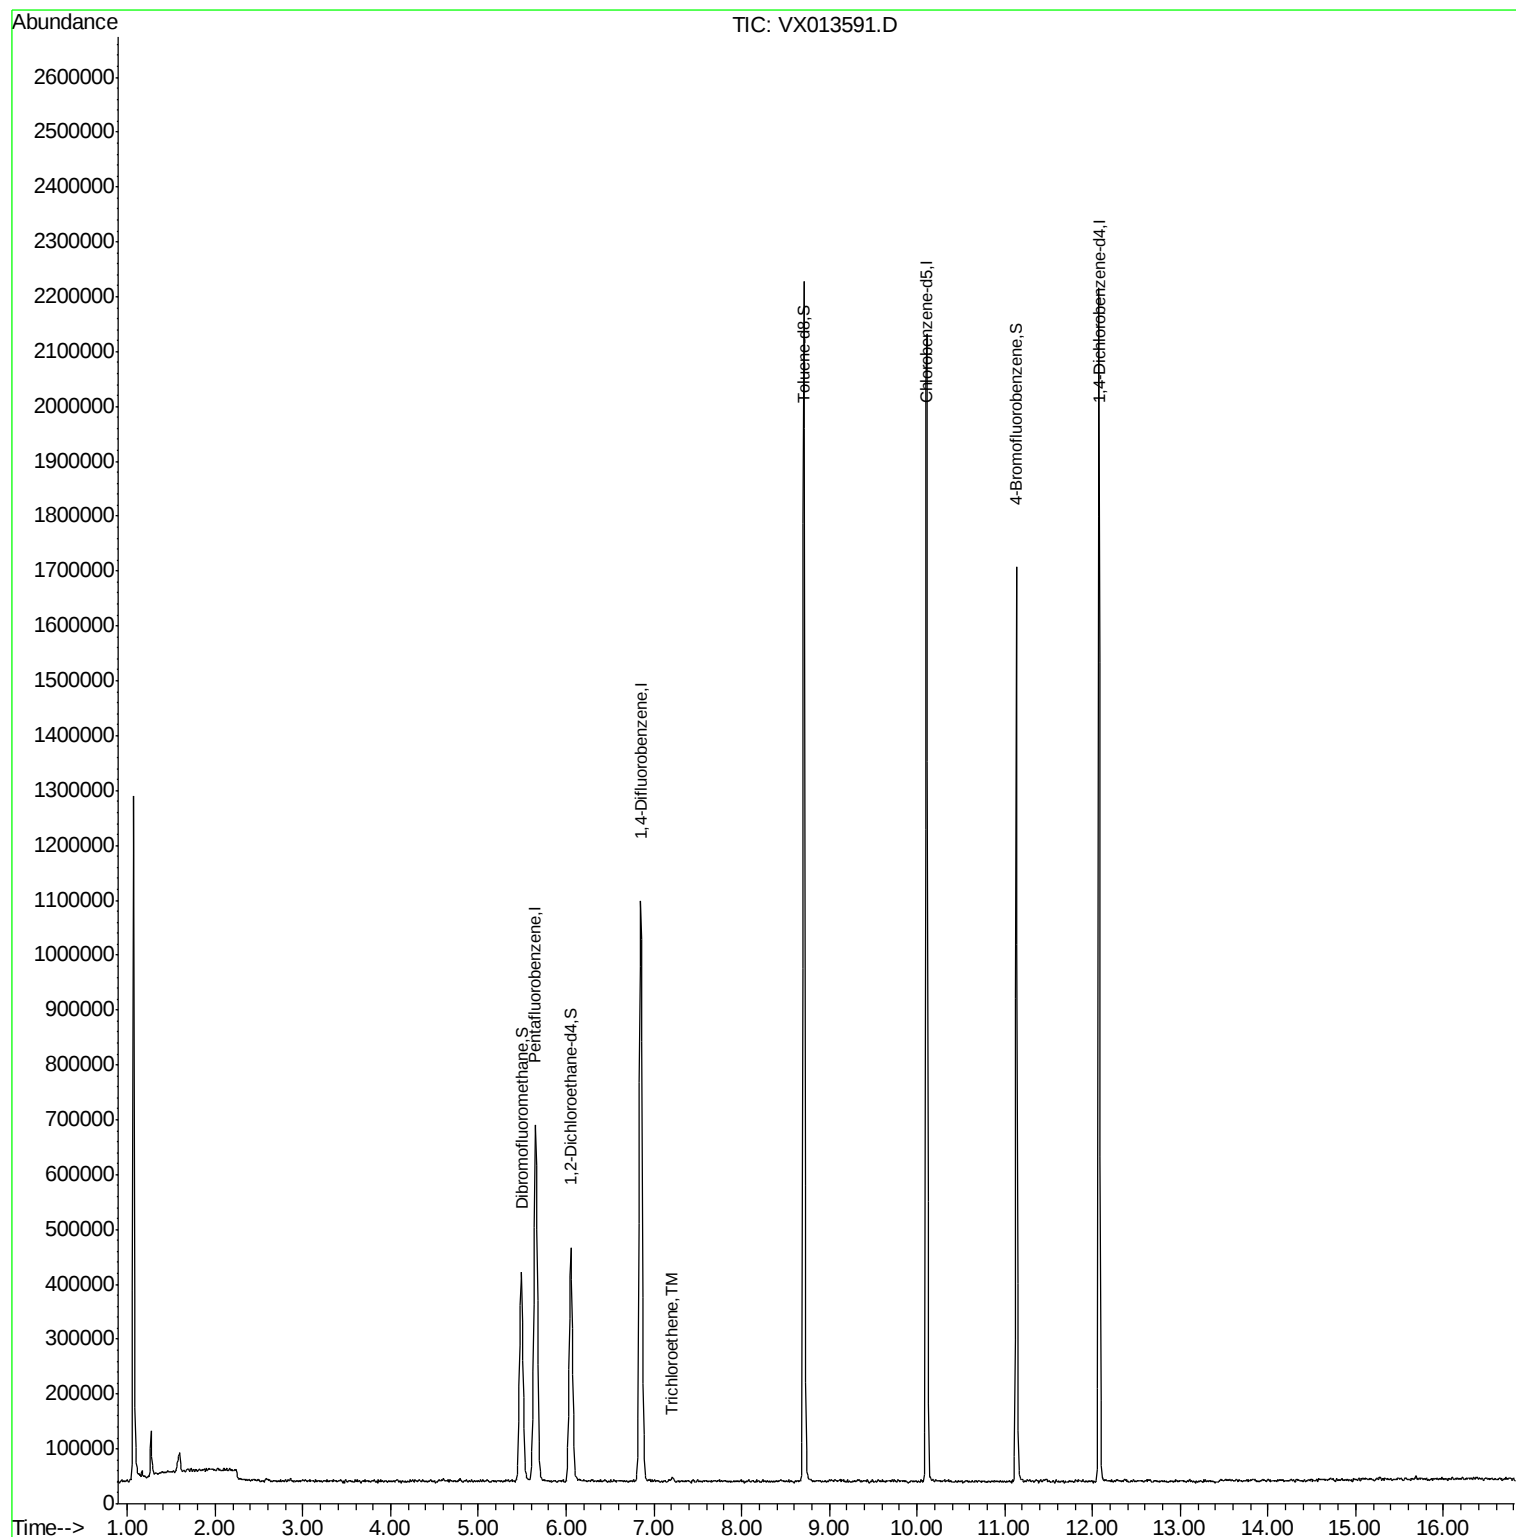

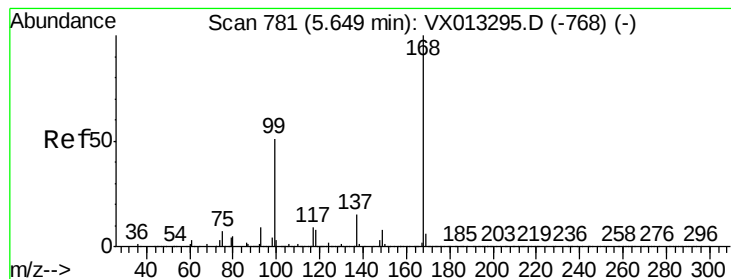

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07

Instrument :

MSVOA_X

ClientSampleId :


WEST-DITCH-IN-20191121

Tot Ion:168 Resp: 673599

Ion Ratio Lower Upper

168 100

99 49.9 40.8 61.2

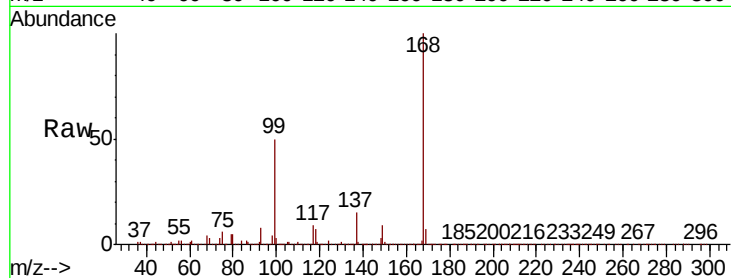

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

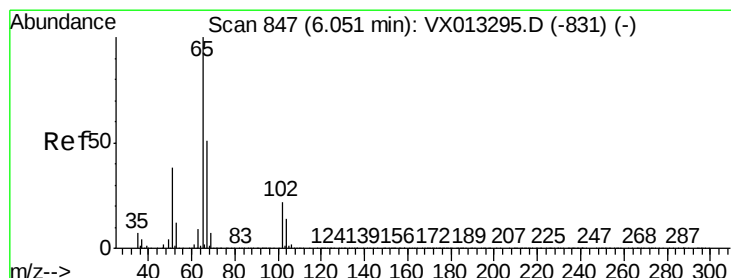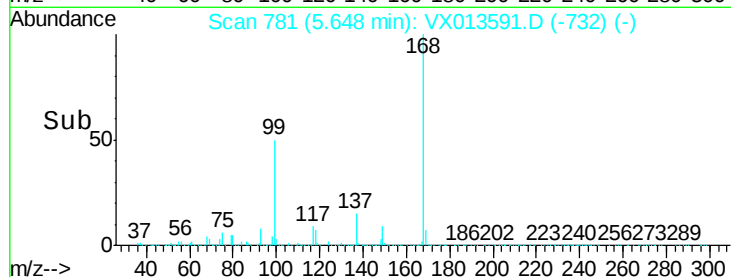

#33

1,2-Dichloroethane-d4

Concen: 50.680 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX013591.D


Acq: 25 Nov 2019 19:07

Tgt Ion: 65 Resp: 404434

Ion Ratio Lower Upper

65 100

67 52.2 0.0 104.2

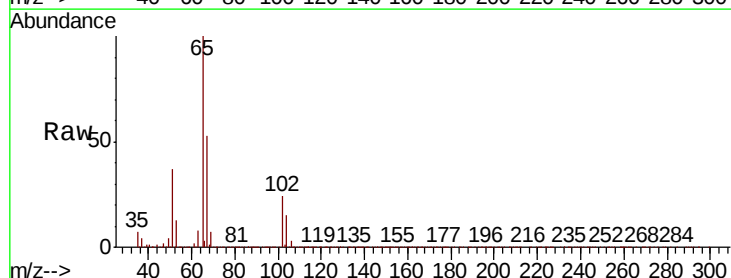

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05

150000


100000


50000

0

Time-->

5.90 6.00 6.10 6.20

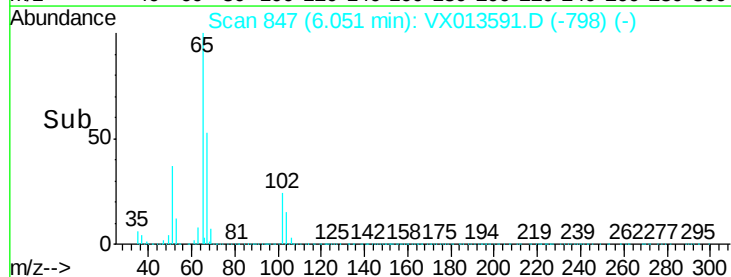

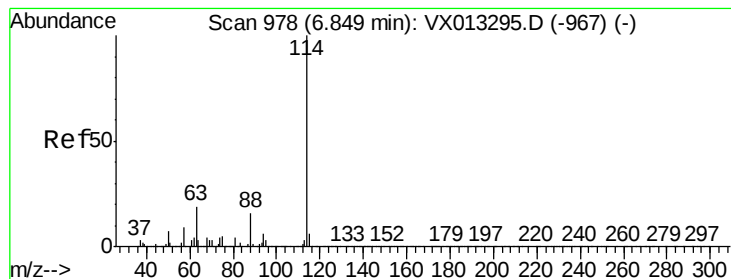

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07

Instrument :

MSVOA_X

ClientSampleId :

WEST-DITCH-IN-20191121


Tot Ion:114 Resp: 1094877

Ion Ratio Lower Upper

114 100

63 19.7 0.0 38.4




88 15.3 0.0 32.2

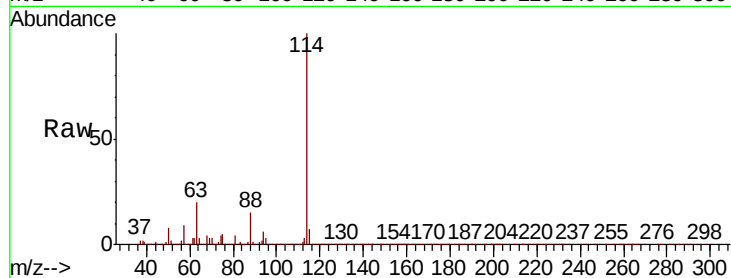

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

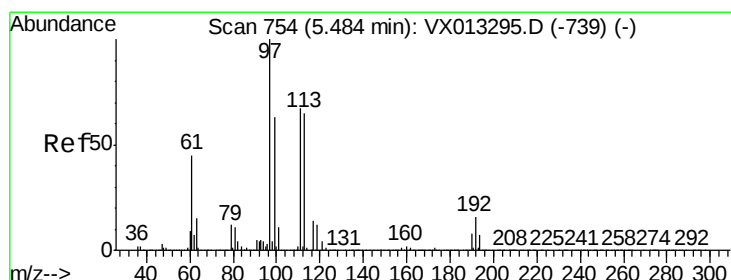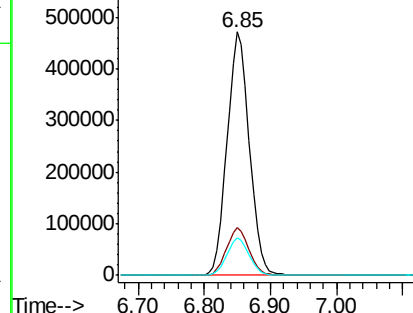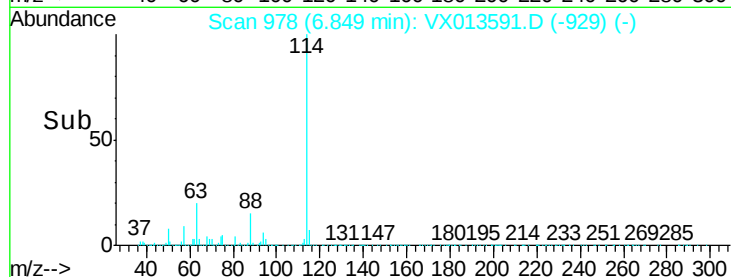

#35

Dibromofluoromethane

Concen: 47.719 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.01 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07


Tgt Ion:113 Resp: 327696

Ion Ratio Lower Upper

113 100

111 102.1 81.9 122.9



192 23.5 19.1 28.7

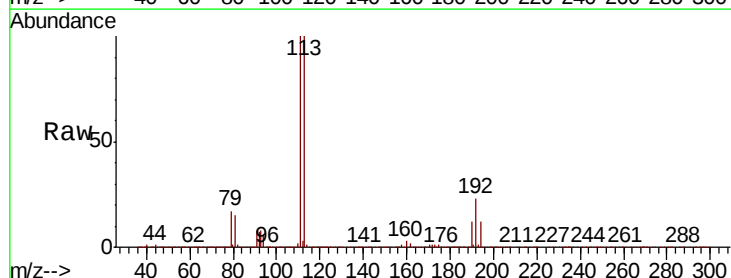


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

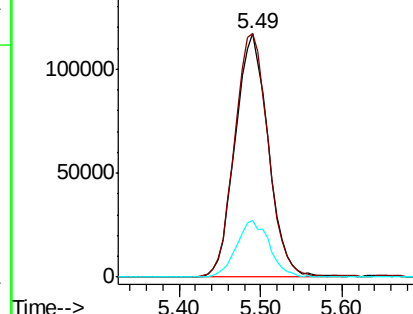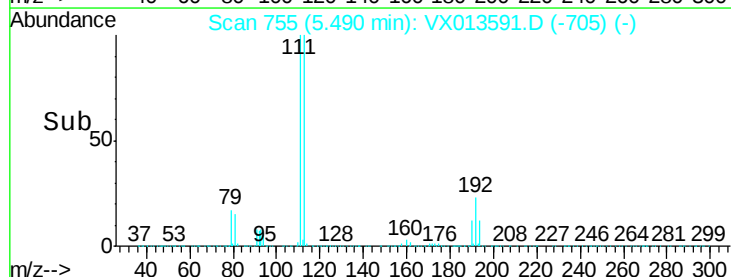

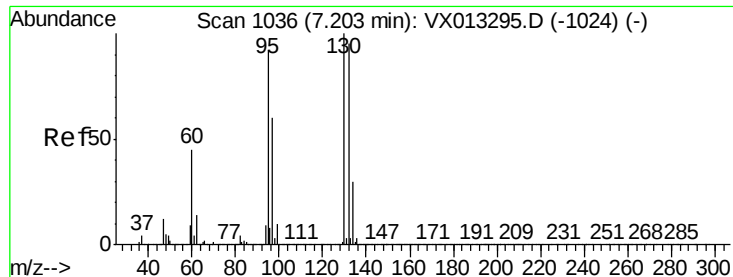

#44

Trichloroethene

Concen: 0.616 ug/l

RT: 7.20 min Scan# 1036

Delta R.T. -0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07

Instrument :

MSVOA_X

ClientSampleId :


WEST-DITCH-IN-20191121

Tot Ion:130 Resp: 4963

Ion Ratio Lower Upper




130 100

95 42.1 0.0 184.8

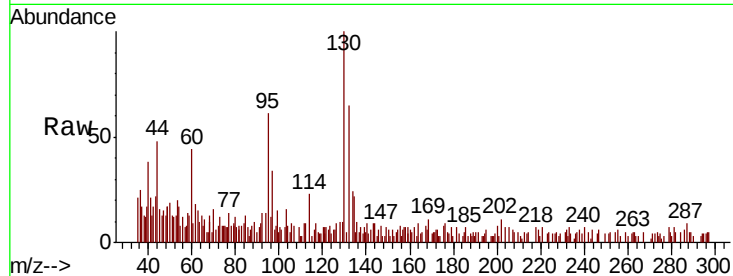

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

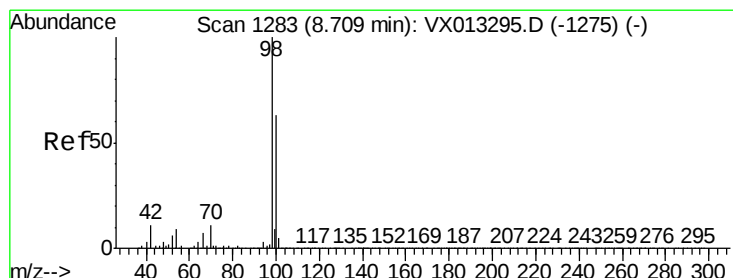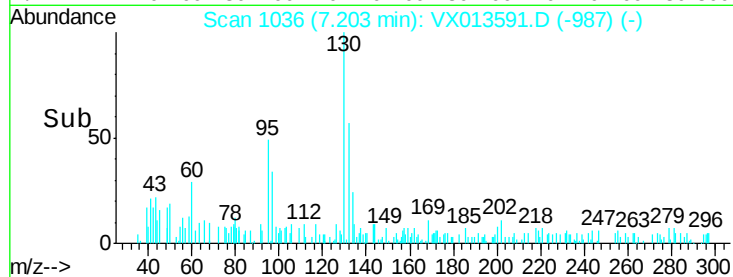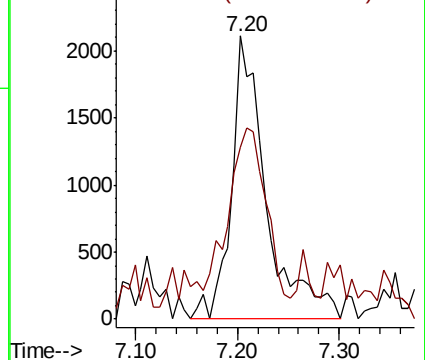

#50

Toluene-d8

Concen: 50.307 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX013591.D


Acq: 25 Nov 2019 19:07

Tgt Ion: 98 Resp: 1302392

Ion Ratio Lower Upper



98 100


100 65.8 52.2 78.2

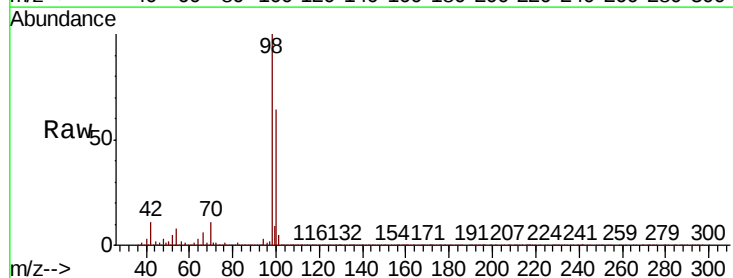

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

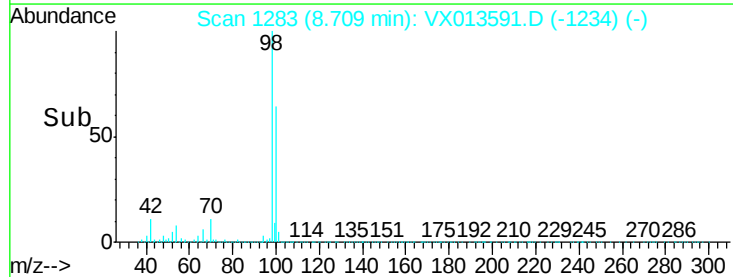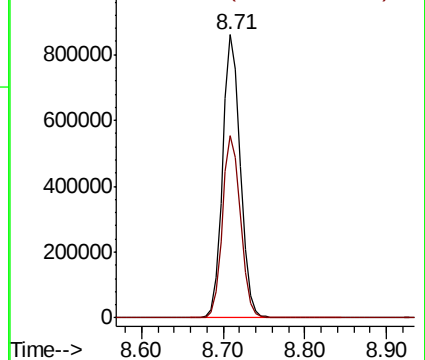

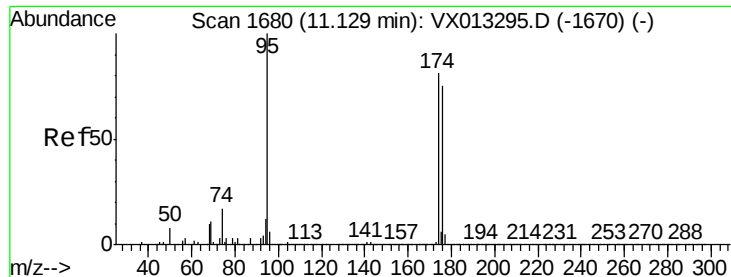

#62

4-Bromofluorobenzene

Concen: 47.107 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07

Instrument :

MSVOA_X

ClientSampleId :

WEST-DITCH-IN-20191121


Tot Ion: 95 Resp: 440142

Ion Ratio Lower Upper

95 100

174 89.1 0.0 179.8

176 86.2 0.0 173.0

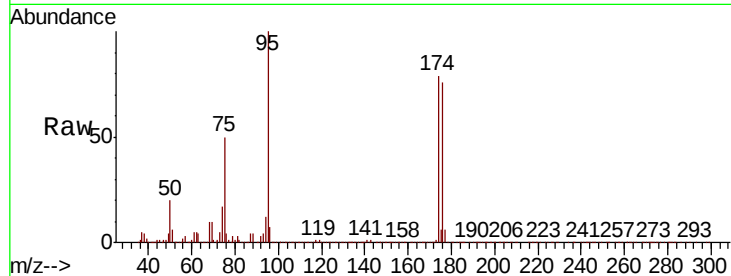


Abundance Ion 94.90 (94.60 to 95.60): VX0


Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

Time-->

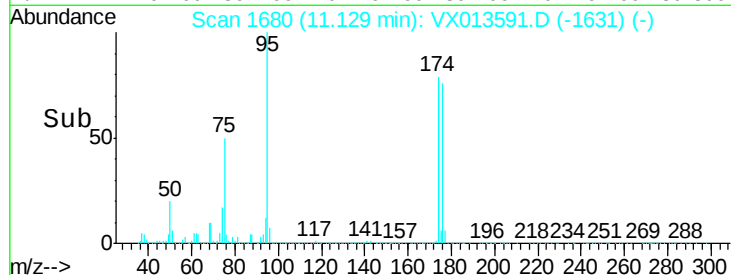

Time-->

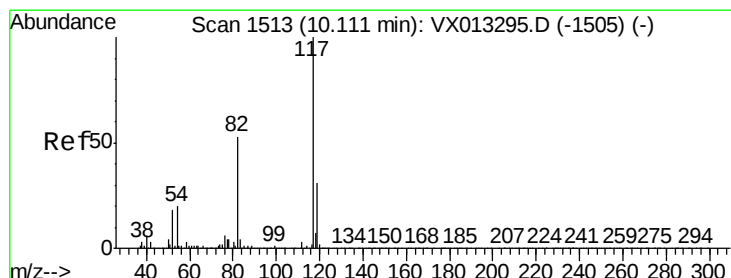

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1513

Delta R.T. -0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07


Tgt Ion: 117 Resp: 987976

Ion Ratio Lower Upper

117 100

82 52.9 42.6 64.0

119 32.2 24.8 37.2

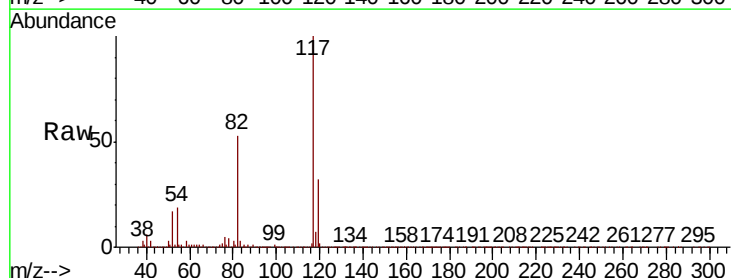


Abundance Ion 116.90 (116.60 to 117.60): V


Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

Time-->

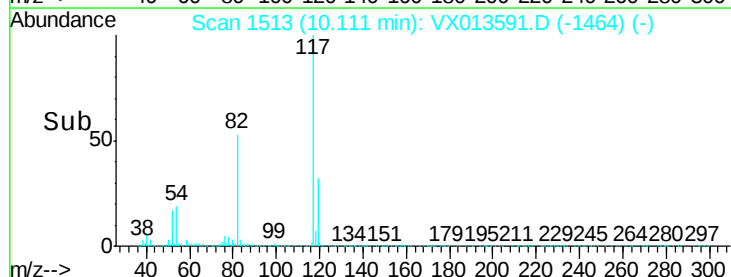

Time-->

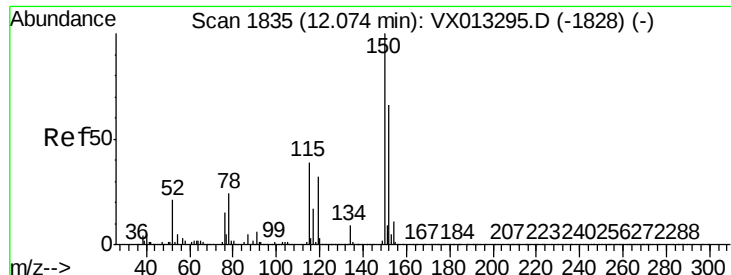

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX013591.D

Acq: 25 Nov 2019 19:07

Instrument :

MSVOA_X

ClientSampleId :

WEST-DITCH-IN-20191121

Tot Ion:152 Resp: 449263

Ion Ratio Lower Upper

152 100

115 56.2 39.5 118.3

150 157.6 0.0 344.4

