

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112520\
 Data File : VX019666.D
 Acq On : 25 Nov 2020 19:01
 Operator : JC/MD
 Sample : L4891-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PAV-B3-112420-0-1


Quant Time: Nov 26 05:01:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.62	168	312032	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	522720	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	459013	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	182919	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	197006	48.69	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.38%	
35) Dibromofluoromethane		5.46	113	155029	47.25	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.50%	
50) Toluene-d8		8.70	98	620609	48.67	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.34%	
62) 4-Bromofluorobenzene		11.12	95	208495	45.45	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	90.90%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.63	94	475	0.335	ug/l #	73
6) Chloroethane	1.69	64	1154	Below Cal	#	68
11) Tert butyl alcohol	3.00	59	5742	7.499	ug/l #	73
13) Acrolein	2.27	56	233	0.453	ug/l #	15
16) Acetone	2.42	43	14846	9.489	ug/l	99
18) Methyl Acetate	2.75	43	4265	1.732	ug/l	97
20) Methylene Chloride	2.83	84	19091	4.882	ug/l	95
25) 2-Butanone	4.64	43	2727	1.160	ug/l #	88
29) Tetrahydrofuran	5.11	42	1447	0.965	ug/l #	88
31) Cyclohexane	5.62	56	6020	1.144	ug/l #	1
36) 1,1-Dichloropropene	5.62	75	23719	4.840	ug/l #	50
38) Carbon Tetrachloride	5.63	117	30312	6.390	ug/l #	16
43) Isopropyl Acetate	6.41	43	75834	9.806	ug/l	100
48) Methyl methacrylate	7.65	41	3988	1.101	ug/l #	9
49) 1,4-Dioxane	7.85	88	265	3.222	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	68284	15.142	ug/l #	49
54) cis-1,3-Dichloropropene	8.59	75	35521	6.020	ug/l #	60
56) Ethyl methacrylate	9.29	69	1072	0.202	ug/l #	1
57) 1,3-Dichloropropane	9.52	76	5516	0.878	ug/l #	43
59) 2-Hexanone	9.52	43	64938	18.986	ug/l #	48
70) Styrene	10.70	104	77	1.653	ug/l #	1
74) N-amyl acetate	10.80	43	2742	0.578	ug/l #	43
76) 1,2,3-Trichloropropane	11.12	75	101045	25.312	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	101045	66.812	ug/l #	12
95) Naphthalene	13.81	128	432	2.209	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

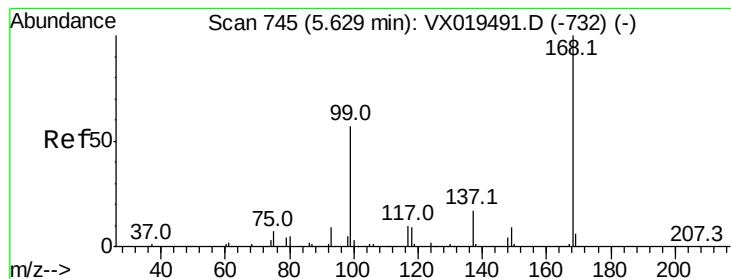

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.01 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :


PAV-B3-112420-0-1

Tot Ion:168 Resp: 312032

Ion Ratio Lower Upper

168 100

99 55.5 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.62

120000

100000

80000



60000

40000

20000

0

Time-->

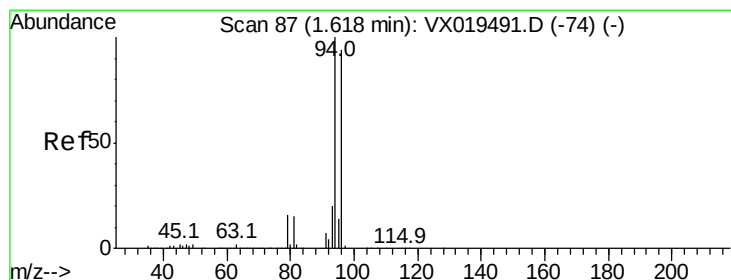

#5

Bromomethane

Concen: 0.335 ug/l

RT: 1.63 min Scan# 89

Delta R.T. 0.01 min

Lab File: VX019666.D


Acq: 25 Nov 2020 19:01

Tgt Ion: 94 Resp: 475

Ion Ratio Lower Upper

94 100

96 68.8 75.6 113.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.63

300

250

200


150


100

50

0

Time-->



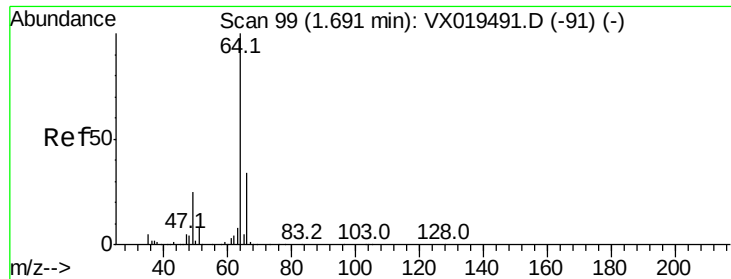

#6

Chloroethane

Concen: Below Cal

RT: 1.69 min Scan# 99

Delta R.T. 0.00 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :





PAV-B3-112420-0-1

Tot Ion: 64 Resp: 1154

Ion Ratio Lower Upper

64 100

66 15.7 27.1 40.7#

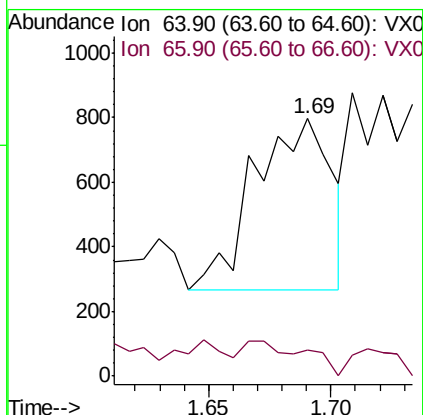

#11

Tert butyl alcohol

Concen: 7.499 ug/l

RT: 3.00 min Scan# 313

Delta R.T. -0.05 min

Lab File: VX019666.D




Acq: 25 Nov 2020 19:01


Tgt Ion: 59 Resp: 5742

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#

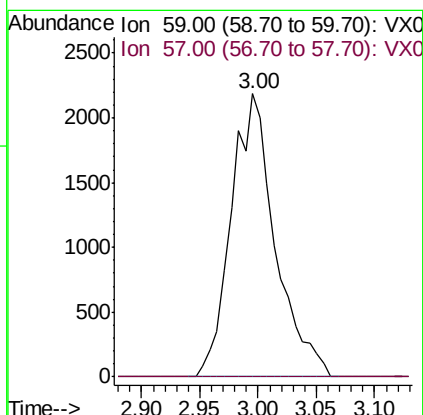

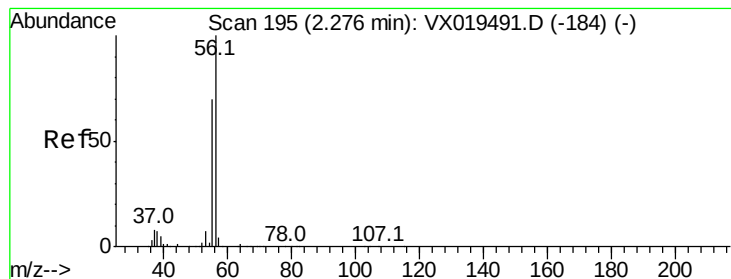

#13

Acrolein

Concen: 0.453 ug/l

RT: 2.27 min Scan# 194

Delta R.T. -0.01 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :





PAV-B3-112420-0-1

Tot Ion: 56 Resp: 233

Ion Ratio Lower Upper

56 100

55 0.0 55.5 83.3#

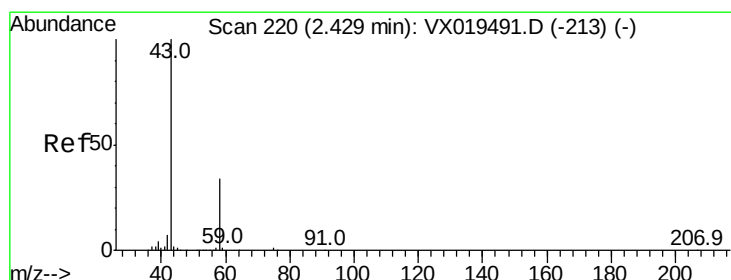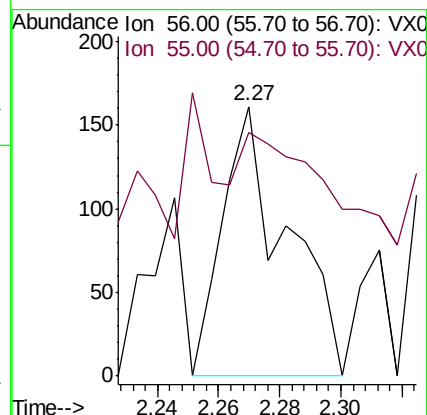

#16

Acetone

Concen: 9.489 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.01 min

Lab File: VX019666.D




Acq: 25 Nov 2020 19:01


Tgt Ion: 43 Resp: 14846

Ion Ratio Lower Upper

43 100

58 34.7 27.4 41.2



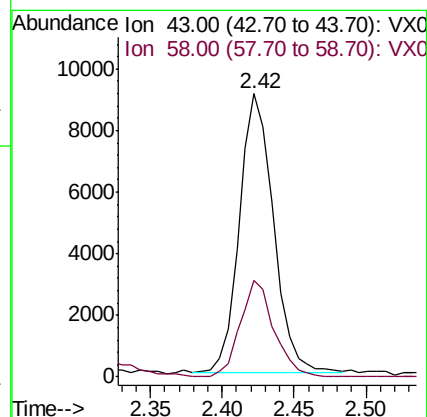



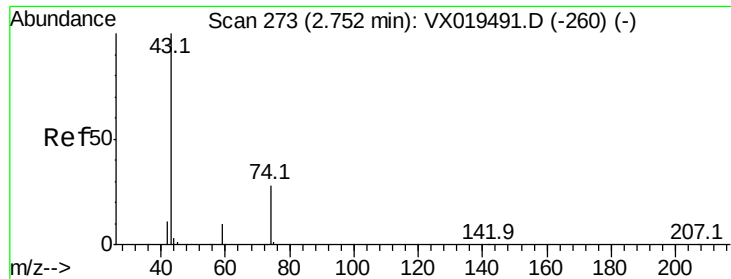

#18
Methvl Acetate
Concen: 1.732 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.00 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01




Instrument :
MSVOA_X
ClientSampleId :
PAV-B3-112420-0-1


Tot Ion: 43 Resp: 4265
Ion Ratio Lower Upper
43 100
74 29.6 22.2 33.4

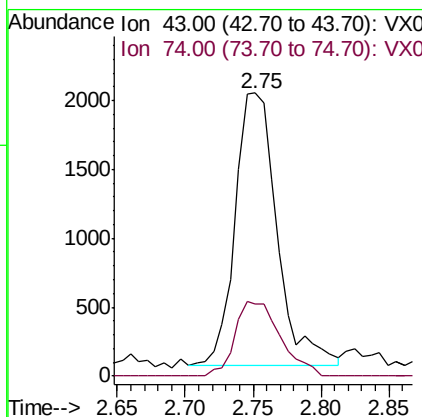

#20
Methylene Chloride
Concen: 4.882 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01

Tgt Ion: 84 Resp: 19091
Ion Ratio Lower Upper
84 100
49 103.2 88.5 132.7
51 32.8 28.0 42.0
86 63.3 53.0 79.4

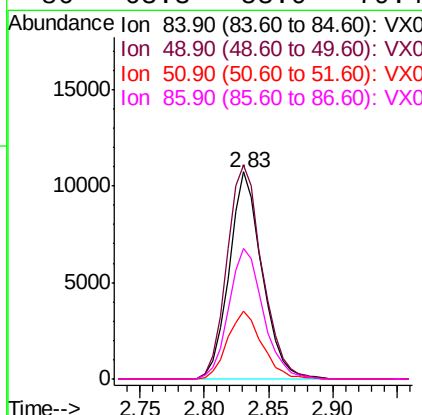

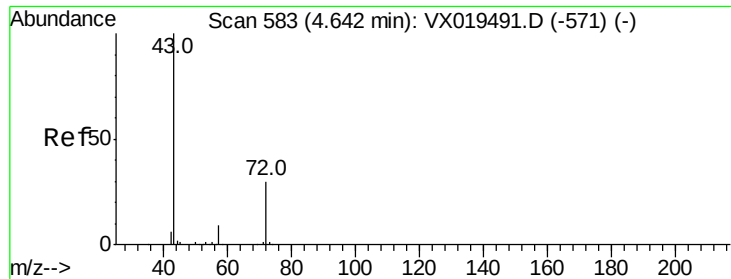

#25

2-Butanone

Concen: 1.160 ug/l

RT: 4.64 min Scan# 583

Delta R.T. -0.00 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :


PAV-B3-112420-0-1

Tot Ion: 43 Resp: 2727

Ion Ratio Lower Upper




43 100

72 23.3 24.0 36.0#

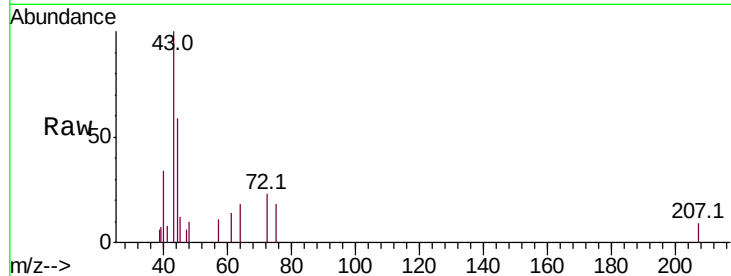

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

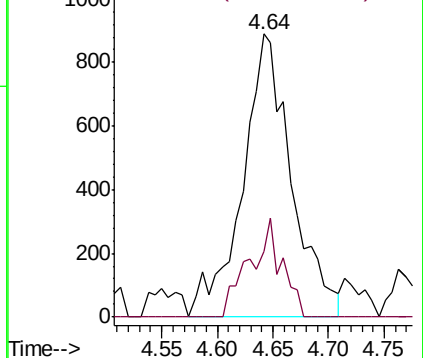

#29

Tetrahydrofuran

Concen: 0.965 ug/l

RT: 5.11 min Scan# 660

Delta R.T. 0.02 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01


Tgt Ion: 42 Resp: 1447

Ion Ratio Lower Upper

42 100

72 41.3 42.6 63.8#



71 44.0 39.0 58.6

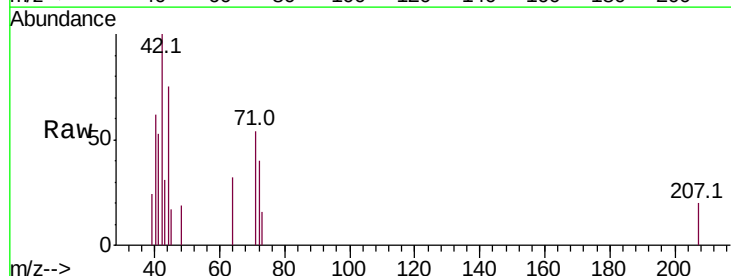


Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

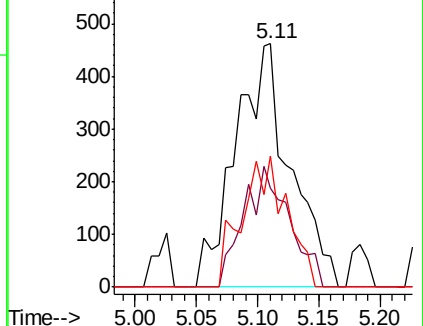

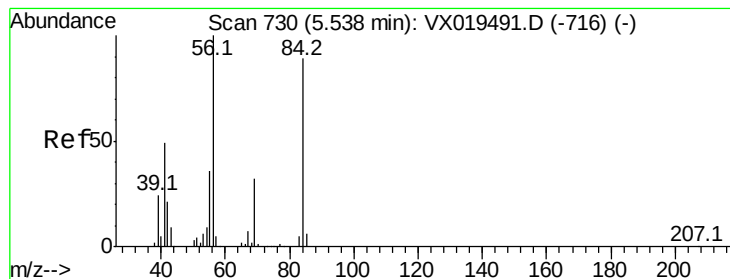

#31

Cyclohexane

Concen: 1.144 ug/l

RT: 5.62 min Scan# 744

Delta R.T. 0.09 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion: 56 Resp: 6020

Ion Ratio Lower Upper

56 100

69 190.8 25.5 38.3#




84 161.6 71.1 106.7#

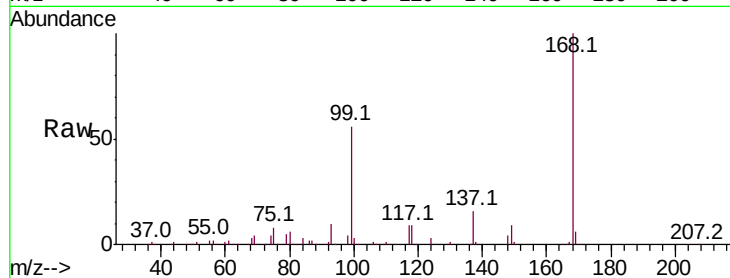

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

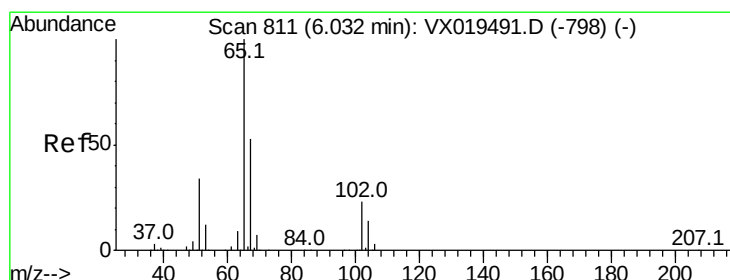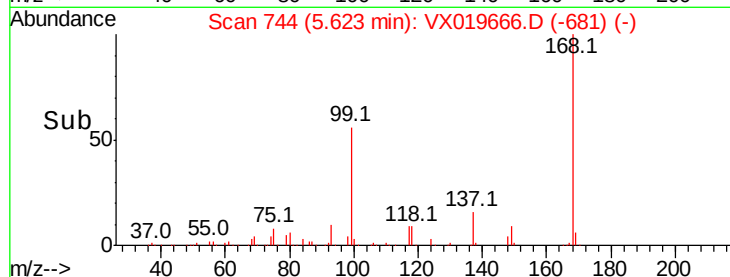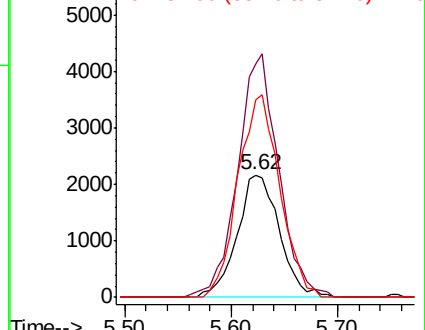

#33

1,2-Dichloroethane-d4

Concen: 48.694 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX019666.D


Acq: 25 Nov 2020 19:01

Tgt Ion: 65 Resp: 197006

Ion Ratio Lower Upper



65 100


67 52.4 0.0 105.0

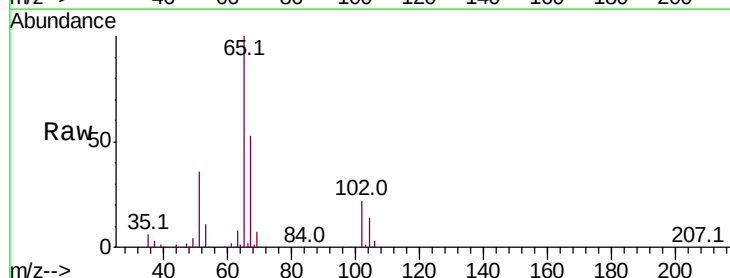

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

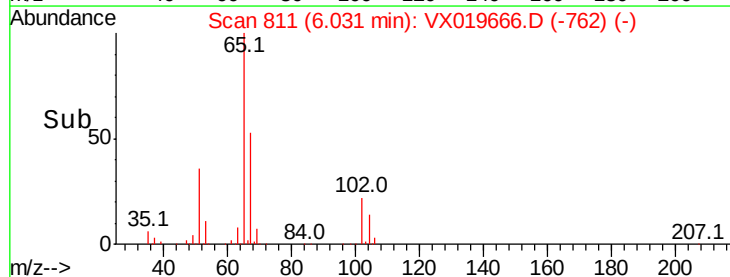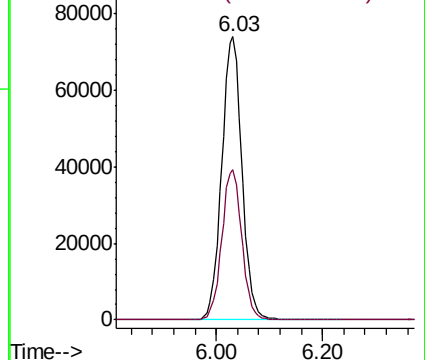



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion:114 Resp: 522720

Ion Ratio Lower Upper

114 100

63 19.9 0.0 38.8




88 15.6 0.0 31.6

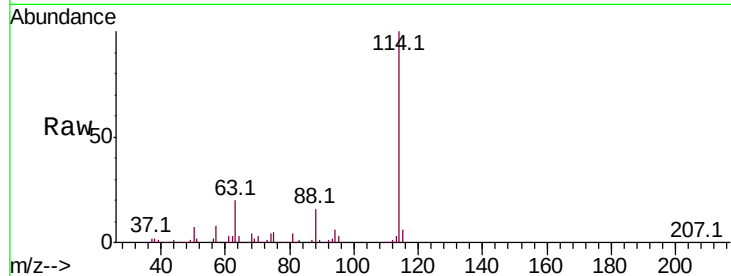

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

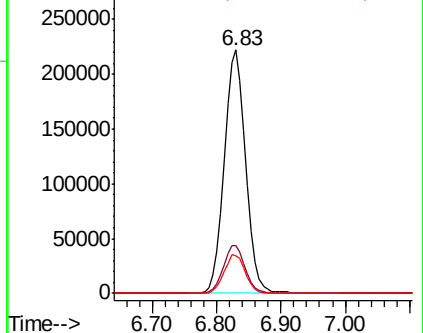

#35

Dibromofluoromethane

Concen: 47.249 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01


Tgt Ion:113 Resp: 155029

Ion Ratio Lower Upper

113 100

111 103.5 81.5 122.3



192 20.2 16.2 24.2

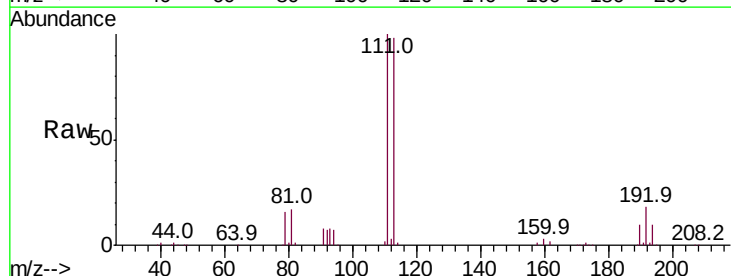


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

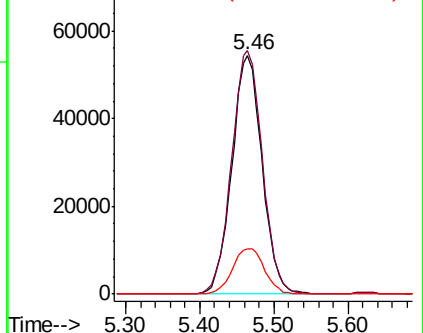

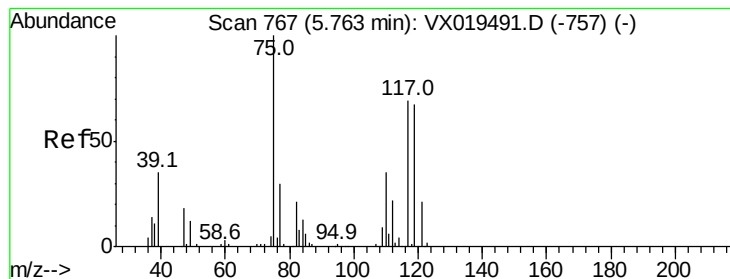

#36

1,1-Dichloropropene

Concen: 4.840 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.14 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion: 75 Resp: 23719

Ion Ratio Lower Upper

75 100

110 9.0 18.1 54.3#




77 0.0 24.2 36.4#

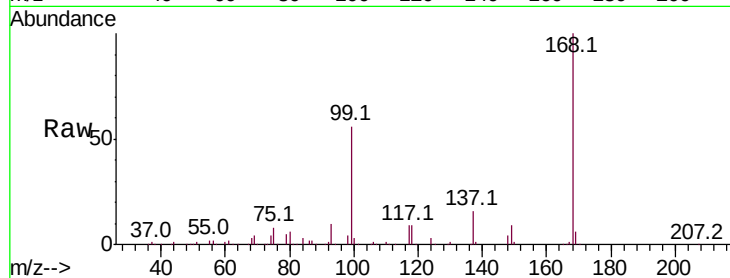

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

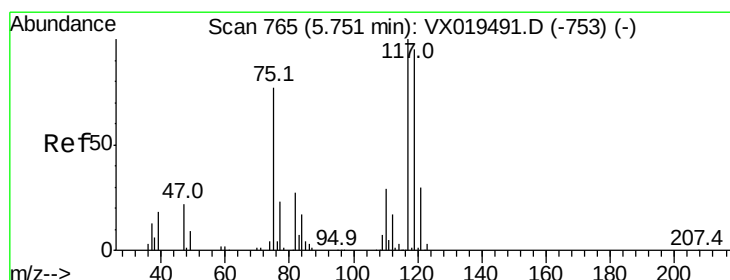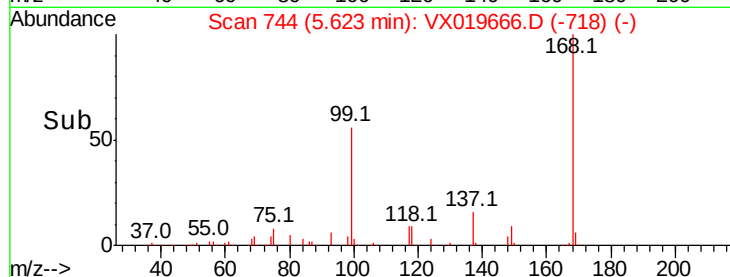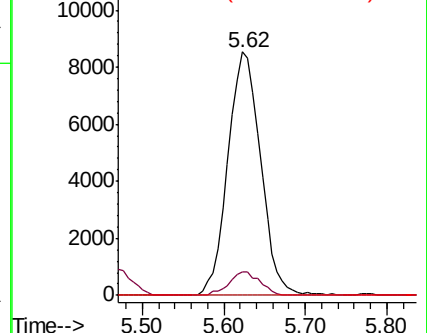

#38

Carbon Tetrachloride

Concen: 6.390 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01


Tgt Ion: 117 Resp: 30312

Ion Ratio Lower Upper

117 100

119 4.4 75.9 113.9#



121 0.0 24.0 36.0#

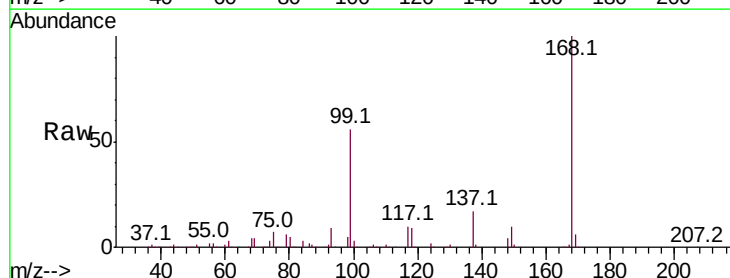


Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

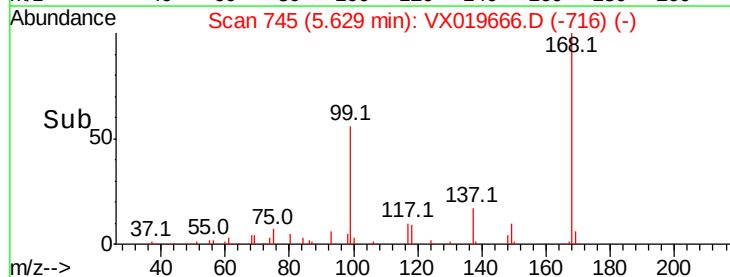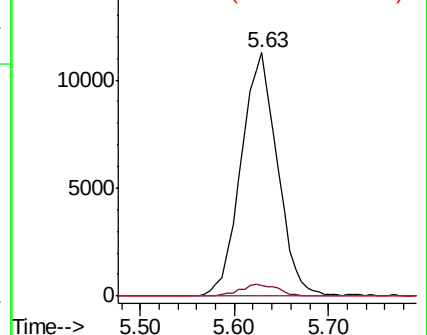

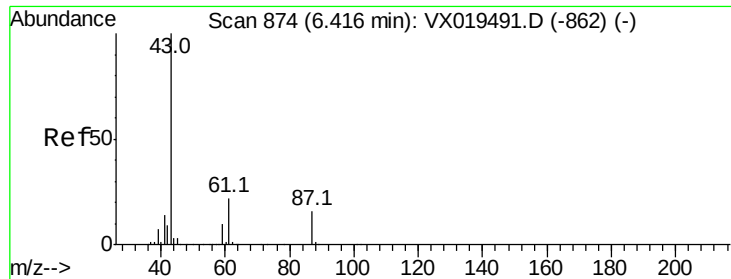

#43

Isopropyl Acetate

Concen: 9.806 ug/l

RT: 6.41 min Scan# 873

Delta R.T. -0.01 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion: 43 Resp: 75834

Ion Ratio Lower Upper

43 100

61 22.6 18.2 27.2




87 15.4 12.6 18.8

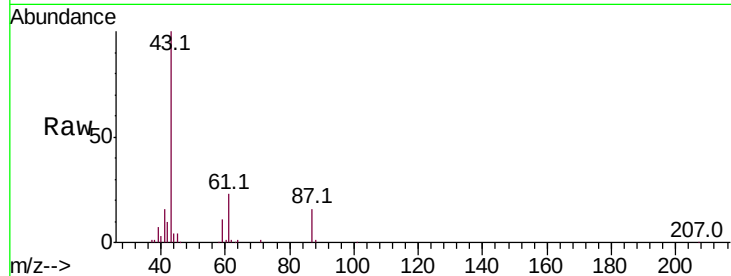

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

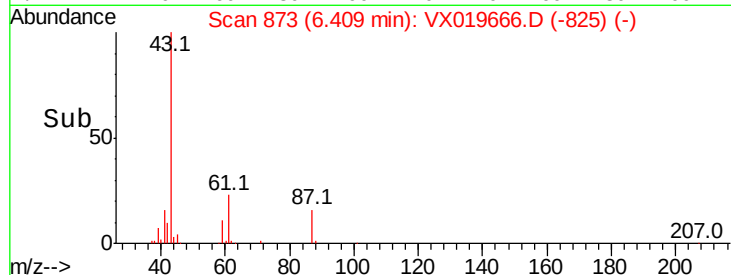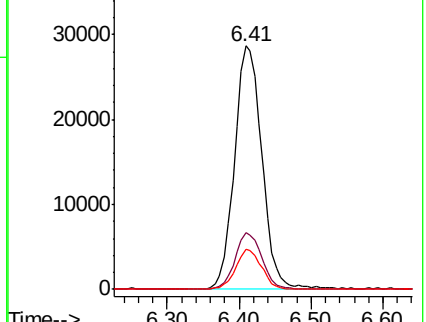

#48

Methyl methacrylate

Concen: 1.101 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01


Tgt Ion: 41 Resp: 3988

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#



39 0.0 45.6 68.4#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

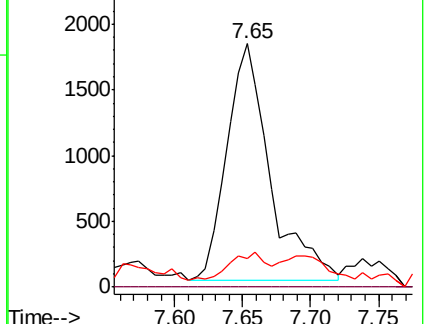

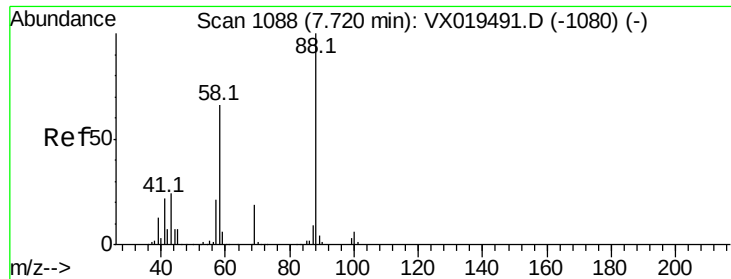

#49

1,4-Dioxane

Concen: 3.222 ug/l

RT: 7.85 min Scan# 1109

Delta R.T. 0.13 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion: 88 Resp: 265

Ion Ratio Lower Upper

88 100

43 459203.0 23.8 35.6#




58 2276.2 54.2 81.2#



Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

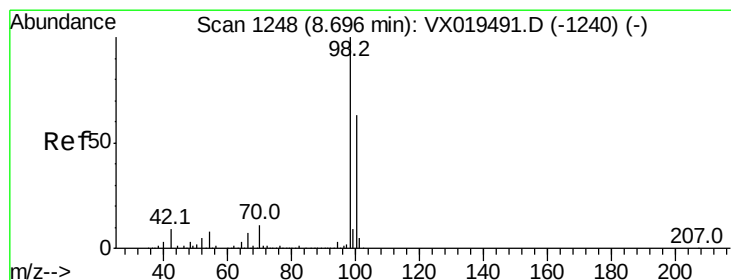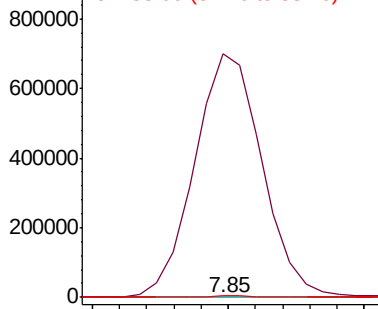

#50

Toluene-d8

Concen: 48.675 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019666.D


Acq: 25 Nov 2020 19:01

Tgt Ion: 98 Resp: 620609

Ion Ratio Lower Upper



98 100


100 66.5 52.4 78.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

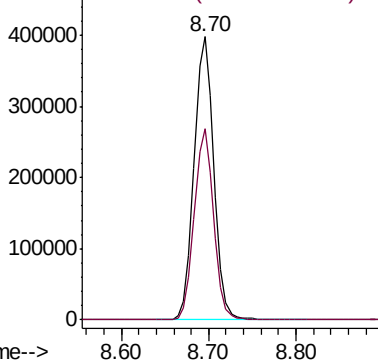



#51

4-Methyl-2-Pentanone

Concen: 15.142 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :





PAV-B3-112420-0-1

Tot Ion: 43 Resp: 68284

Ion Ratio Lower Upper

43 100

58 10.6 35.1 52.7#

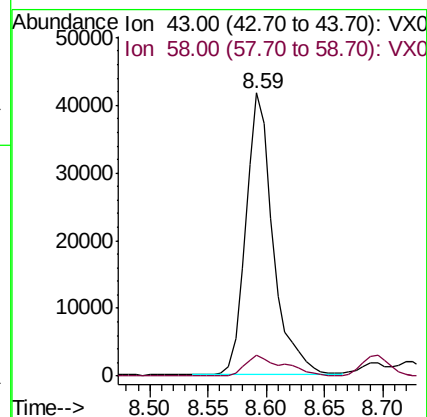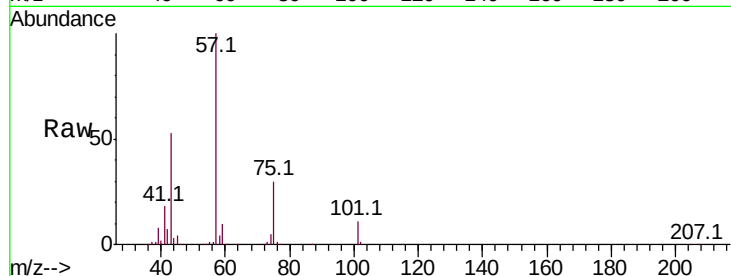

#54

cis-1,3-Dichloropropene

Concen: 6.020 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01




Tgt Ion: 75 Resp: 35521


Ion Ratio Lower Upper

75 100

77 0.6 25.8 38.6#

39 25.8 34.6 51.8#

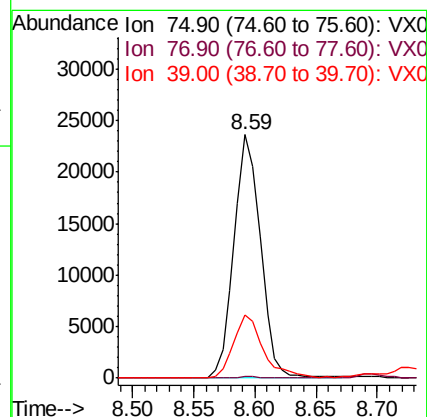

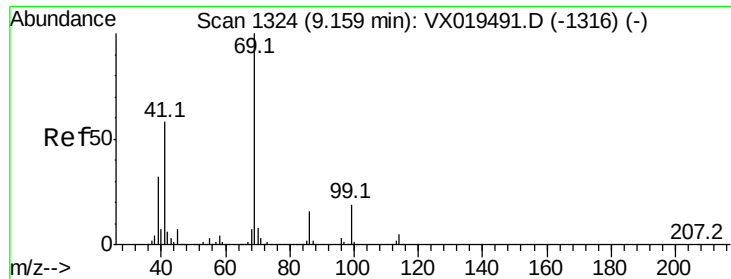

#56

Ethyl methacrylate

Concen: 0.202 ug/l

RT: 9.29 min Scan# 1345

Delta R.T. 0.13 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion: 69 Resp: 1072

Ion Ratio Lower Upper

69 100

41 4858.6 46.2 69.2#




39 2013.2 25.5 38.3#

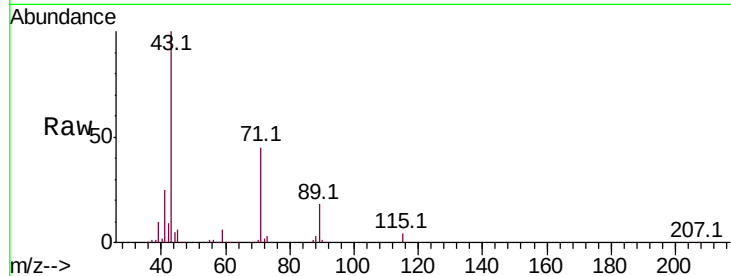

Abundance Ion 69.00 (68.70 to 69.70): VX0

Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

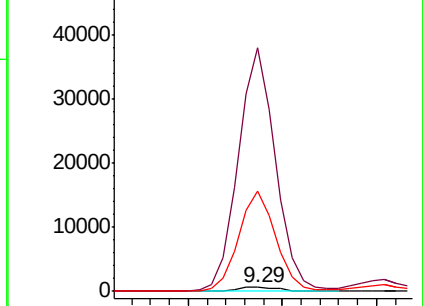

#57

1,3-Dichloropropane

Concen: 0.878 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019666.D


Acq: 25 Nov 2020 19:01

Tgt Ion: 76 Resp: 5516

Ion Ratio Lower Upper



76 100


78 0.3 25.7 38.5#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0




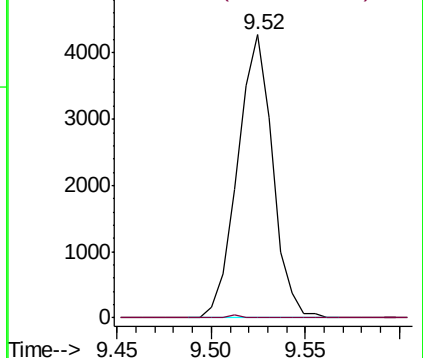


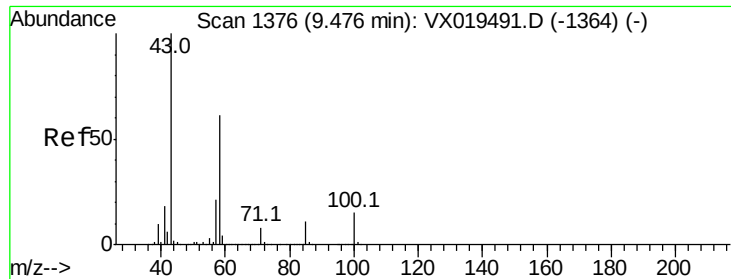

#59
2-Hexanone
Concen: 18.986 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01




Instrument :
MSVOA_X
ClientSampleId :
PAV-B3-112420-0-1


Tot Ion: 43 Resp: 64938
Ion Ratio Lower Upper
43 100
58 21.2 30.6 91.6#

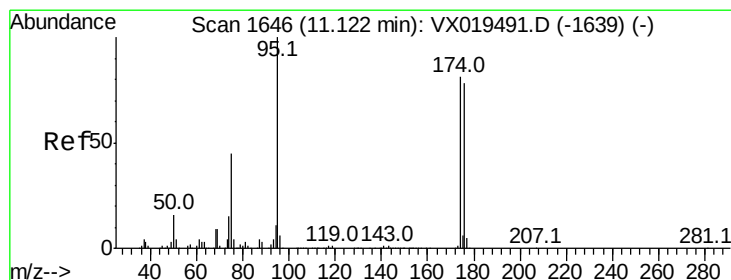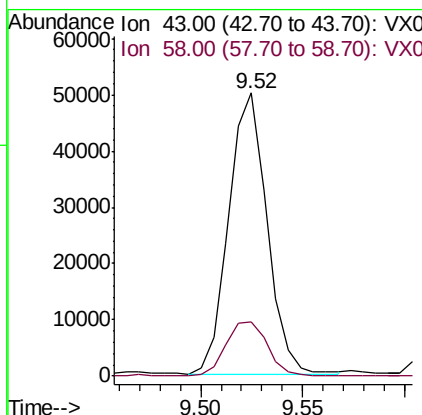

#62
4-Bromofluorobenzene
Concen: 45.450 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01

Tgt Ion: 95 Resp: 208495
Ion Ratio Lower Upper
95 100
174 76.8 0.0 156.2
176 74.0 0.0 151.4



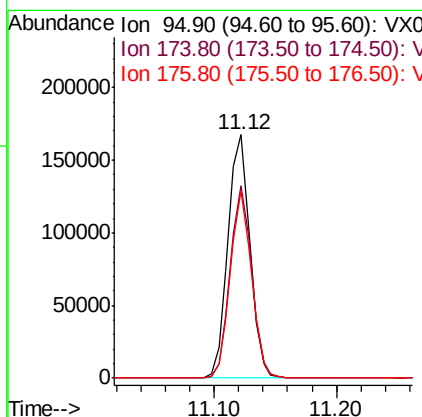





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01




Instrument :
MSVOA_X
ClientSampleId :
PAV-B3-112420-0-1


Tot Ion:117 Resp: 459013
Ion Ratio Lower Upper
117 100
82 53.0 43.0 64.4
119 31.8 25.6 38.4

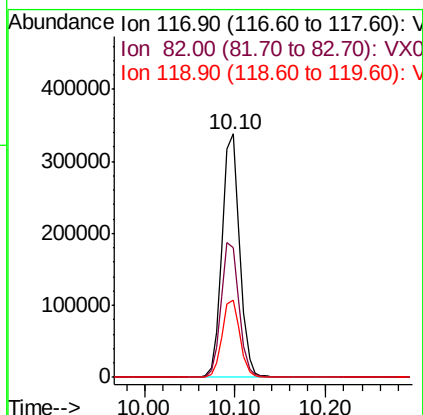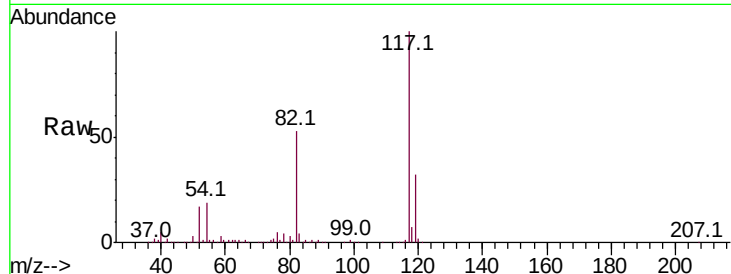

#70
Styrene
Concen: 1.653 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. 0.00 min
Lab File: VX019666.D
Acq: 25 Nov 2020 19:01

Tgt Ion:104 Resp: 77
Ion Ratio Lower Upper
104 100
78 87.0 39.5 59.3#
103 196.1 43.6 65.4#

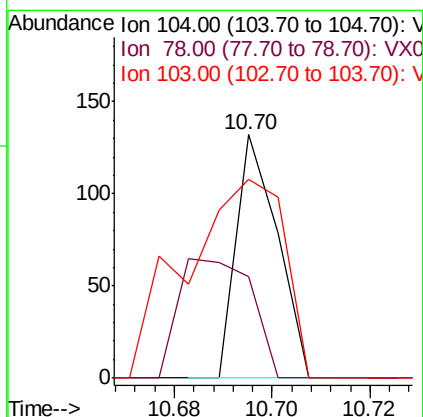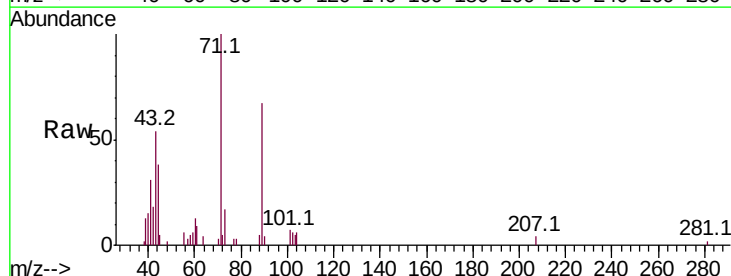



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1


Tot Ion:152 Resp: 182919

Ion Ratio Lower Upper

152 100

115 60.6 41.8 125.4




150 159.5 0.0 348.2

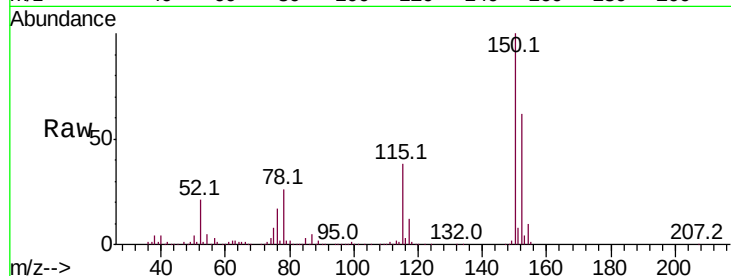

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

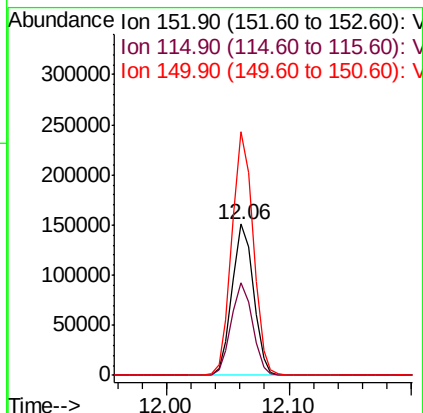

#74

N-ethyl acetate

Concen: 0.578 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Tgt Ion: 43 Resp: 2742


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 10.0 21.8 32.6#

61 0.0 22.2 33.4#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

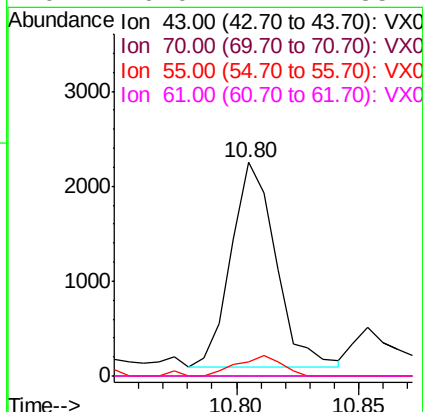

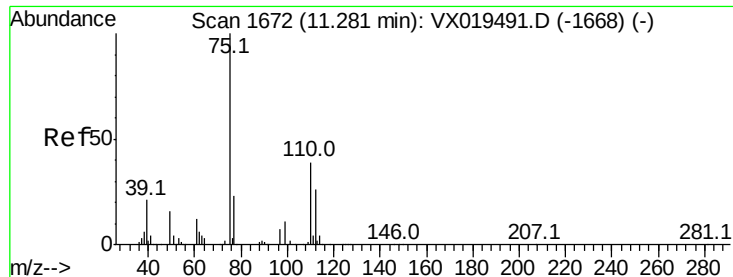

#76

1,2,3-Trichloropropane

Concen: 25.312 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :





PAV-B3-112420-0-1

Tot Ion: 75 Resp: 101045

Ion Ratio Lower Upper

75 100

77 1.2 20.0 60.0#

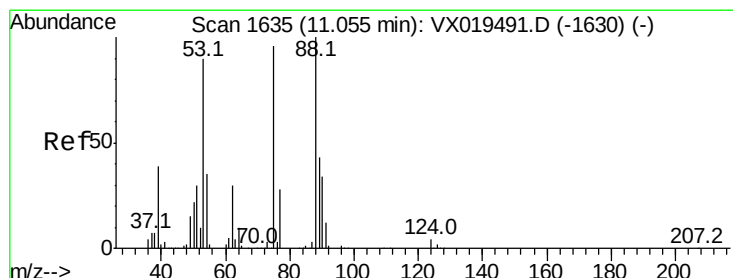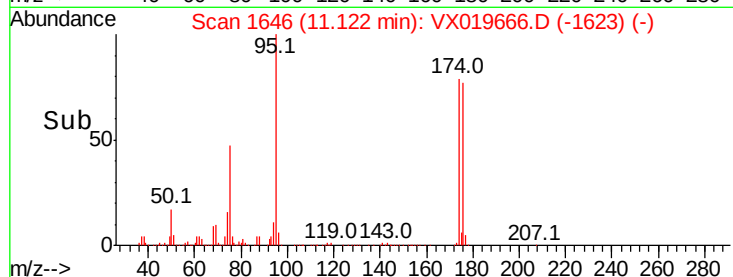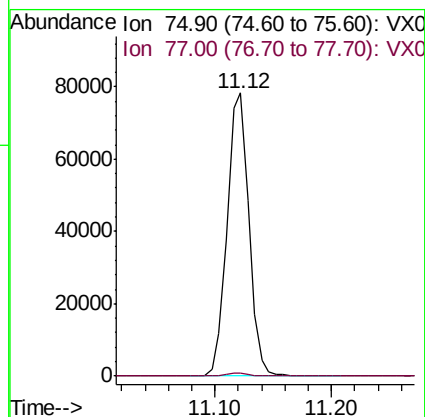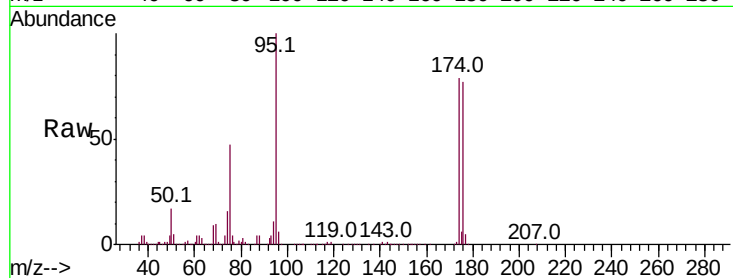

#81

trans-1,4-Dichloro-2-butene

Concen: 66.812 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01




Tgt Ion: 75 Resp: 101045


Ion Ratio Lower Upper

75 100

53 0.0 73.9 110.9#

89 0.0 37.3 55.9#

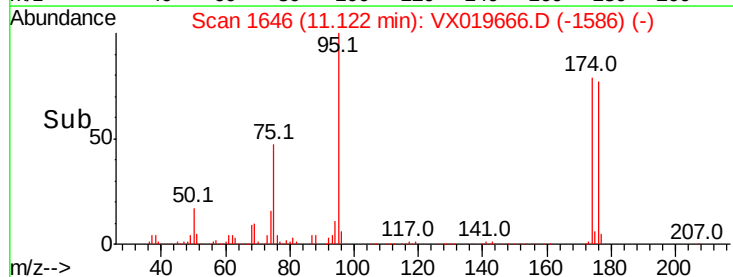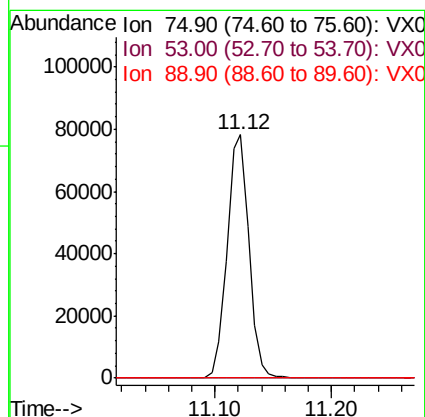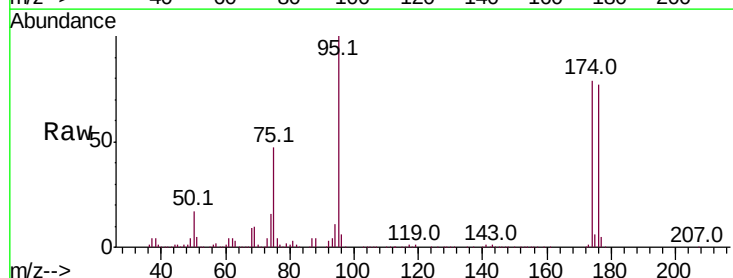

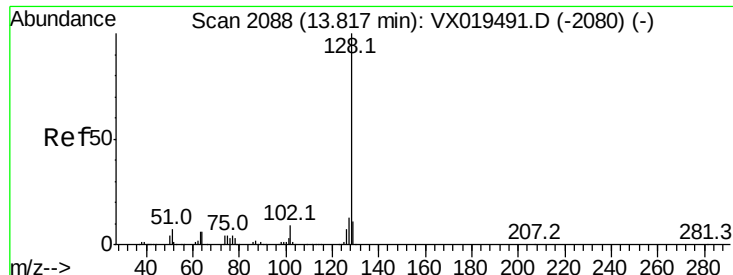

#95

Naphthalene

Concen: 2.209 ug/l

RT: 13.81 min Scan# 2087

Delta R.T. -0.01 min

Lab File: VX019666.D

Acq: 25 Nov 2020 19:01

Instrument :

MSVOA_X

ClientSampleId :

PAV-B3-112420-0-1

Tot Ion:128 Resp: 432

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.7 13.1#

