

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112520\
 Data File : VX019665.D
 Acq On : 25 Nov 2020 18:38
 Operator : JC/MD
 Sample : L4835-09
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ROOF-DRAIN-20201119

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	72	83	86	rBV7	8653	27954	1.79%	0.350%
2	4.562	563	570	579	rVB2	6221	16838	1.08%	0.211%
3	5.464	706	718	732	rBV	173605	493010	31.53%	6.180%
4	5.629	732	745	761	rVV	310331	870883	55.69%	10.917%
5	6.025	799	810	828	rBV	193276	516572	33.04%	6.475%
6	6.830	931	942	953	rBV	481562	1143598	73.13%	14.335%
7	7.183	993	1000	1009	rVB3	21219	49547	3.17%	0.621%
8	8.695	1240	1248	1272	rBV	993820	1563700	100.00%	19.602%
9	10.097	1471	1478	1494	rBV	929040	1304385	83.42%	16.351%
10	11.122	1640	1646	1657	rBV	749841	920260	58.85%	11.536%
11	12.060	1795	1800	1809	rBV	867163	1049832	67.14%	13.160%
12	13.414	2016	2022	2028	rBV	14034	20863	1.33%	0.262%


Sum of corrected areas: 7977442

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112520\
Data File : VX019665.D
Acq On : 25 Nov 2020 18:38
Operator : JC/MD
Sample : L4835-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20201119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

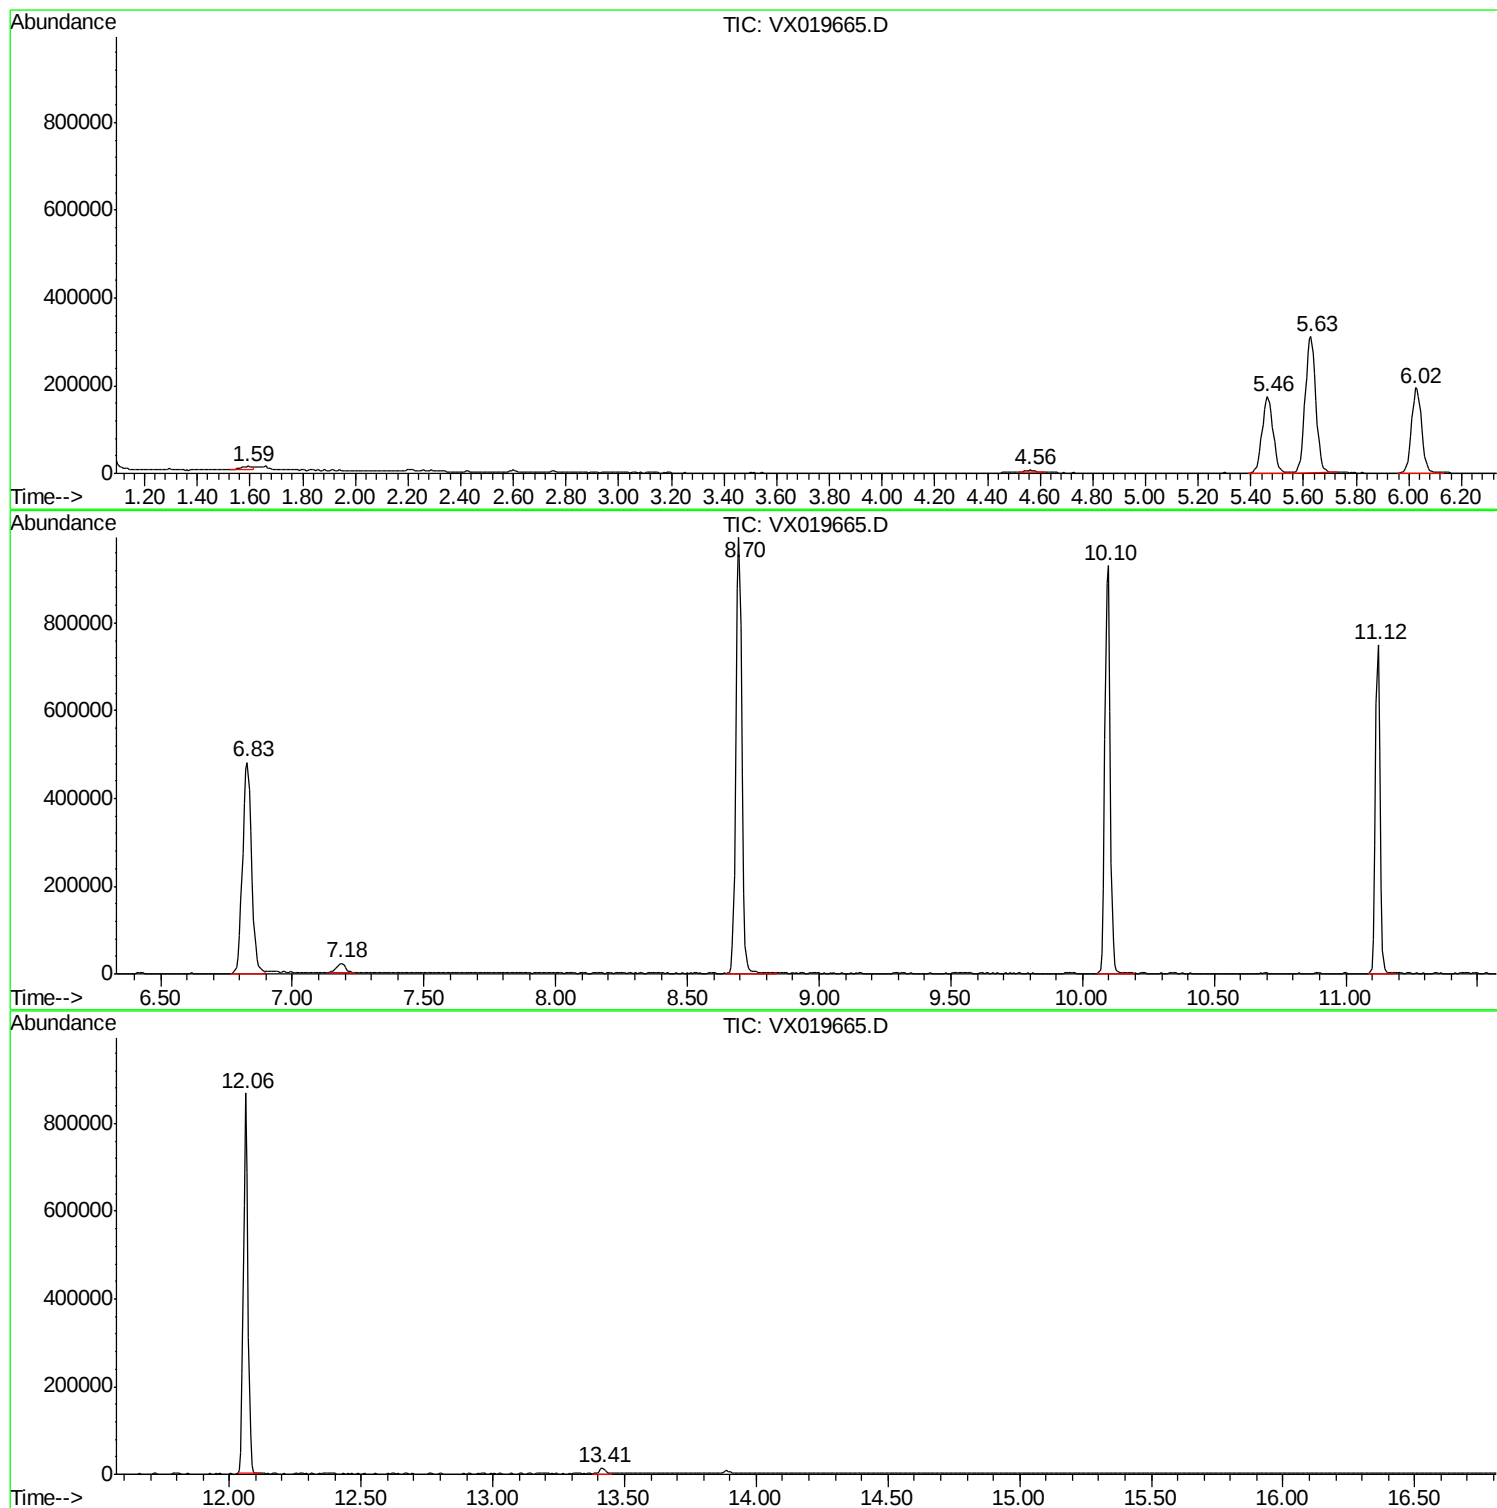

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112520\
Data File : VX019665.D
Acq On : 25 Nov 2020 18:38
Operator : JC/MD
Sample : L4835-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20201119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112520\
Data File : VX019665.D
Acq On : 25 Nov 2020 18:38
Operator : JC/MD
Sample : L4835-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20201119

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc