


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112520\
 Data File : VX019646.D
 Acq On : 25 Nov 2020 08:23
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Title : SW846 8260
 Last Update : Sat Nov 21 01:57:45 2020

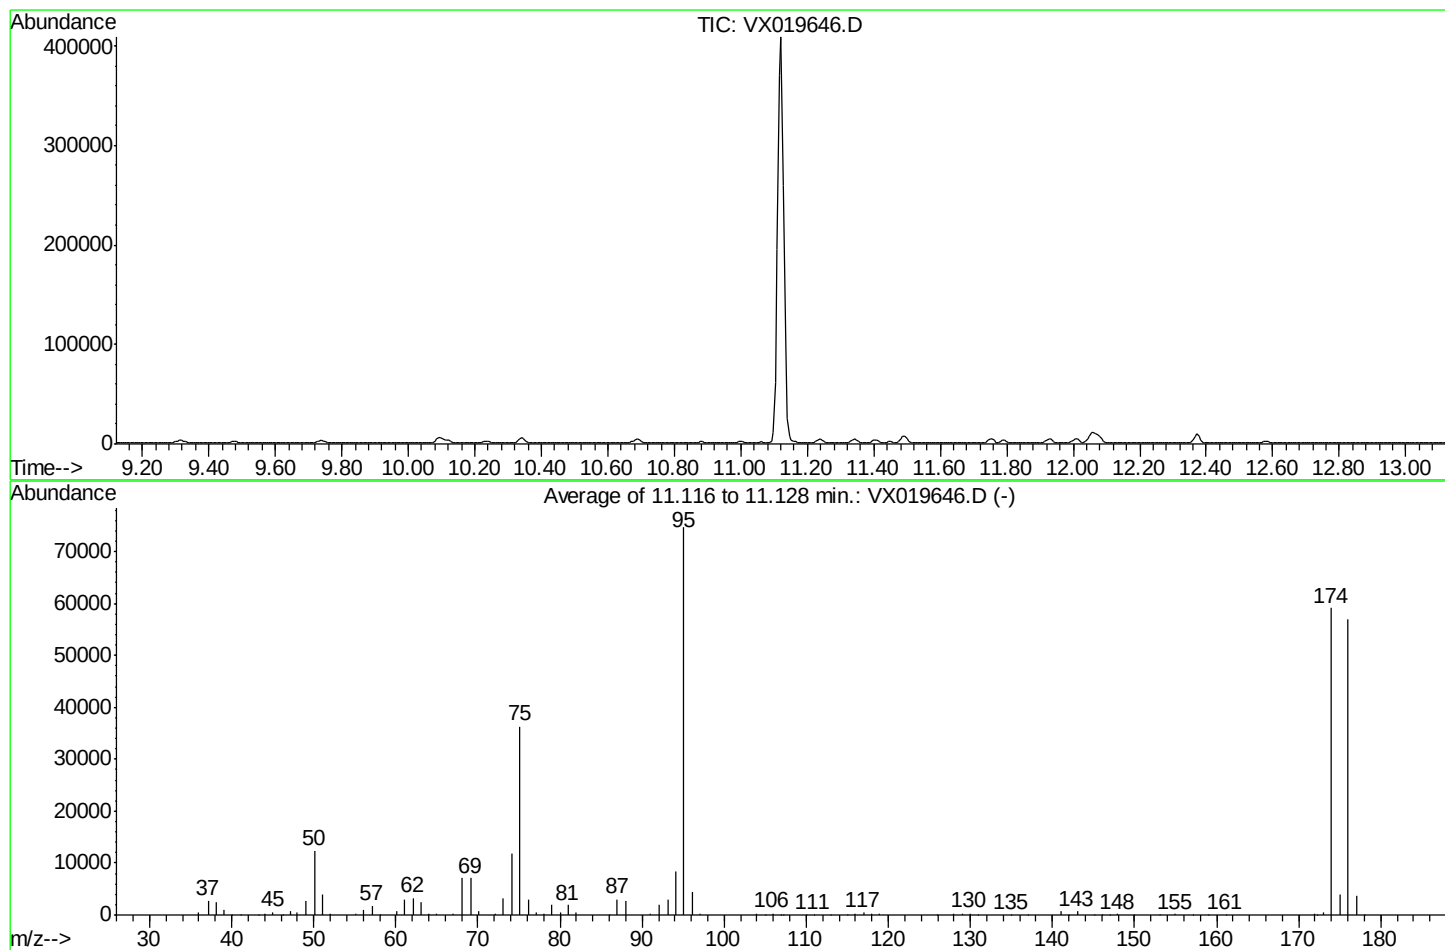

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12368	PASS
75	95	30	60	48.7	36357	PASS
95	95	100	100	100.0	74661	PASS
96	95	5	9	6.1	4550	PASS
173	174	0.00	2	0.8	465	PASS
174	95	50	100	79.1	59090	PASS
175	174	5	9	6.8	4026	PASS
176	174	95	101	96.5	57026	PASS
177	176	5	9	6.6	3752	PASS