

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
 Data File : VX033067.D
 Acq On : 25 Nov 2022 14:55
 Operator : JC/MD
 Sample : N5742-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB111822

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	24	30	45	rBV	24538	73839	12.83%	2.217%
2	2.940	296	304	315	rBV	9337	21240	3.69%	0.638%
3	4.580	562	573	581	rBV2	2350	7544	1.31%	0.227%
4	5.391	694	706	720	rBV	65420	187876	32.64%	5.642%
5	5.550	721	732	750	rVB	142526	405030	70.36%	12.163%
6	5.958	789	799	820	rBV	69026	184565	32.06%	5.542%
7	6.763	920	931	952	rBV	211224	501095	87.05%	15.047%
8	8.647	1234	1240	1263	rVB	315656	497558	86.44%	14.941%
9	10.055	1465	1471	1483	rBV	424020	575622	100.00%	17.285%
10	11.079	1634	1639	1649	rBV	269277	342409	59.49%	10.282%
11	12.024	1788	1794	1805	rBV	416973	533339	92.65%	16.016%




Sum of corrected areas: 3330117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033067.D
Acq On : 25 Nov 2022 14:55
Operator : JC/MD
Sample : N5742-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB111822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

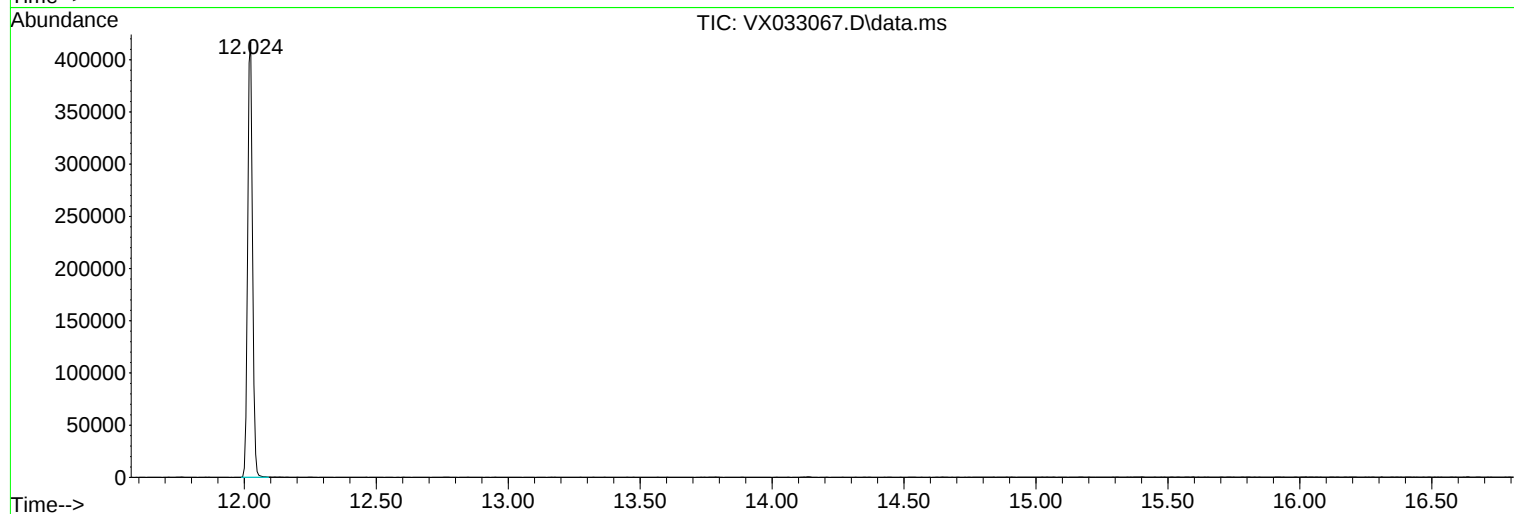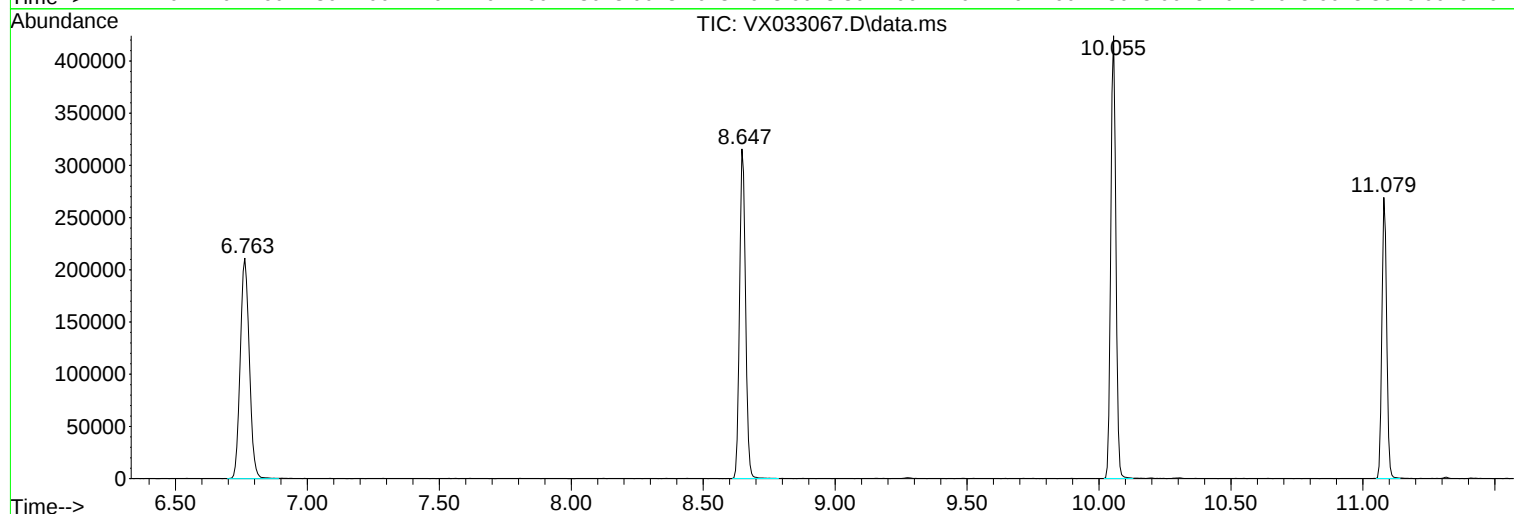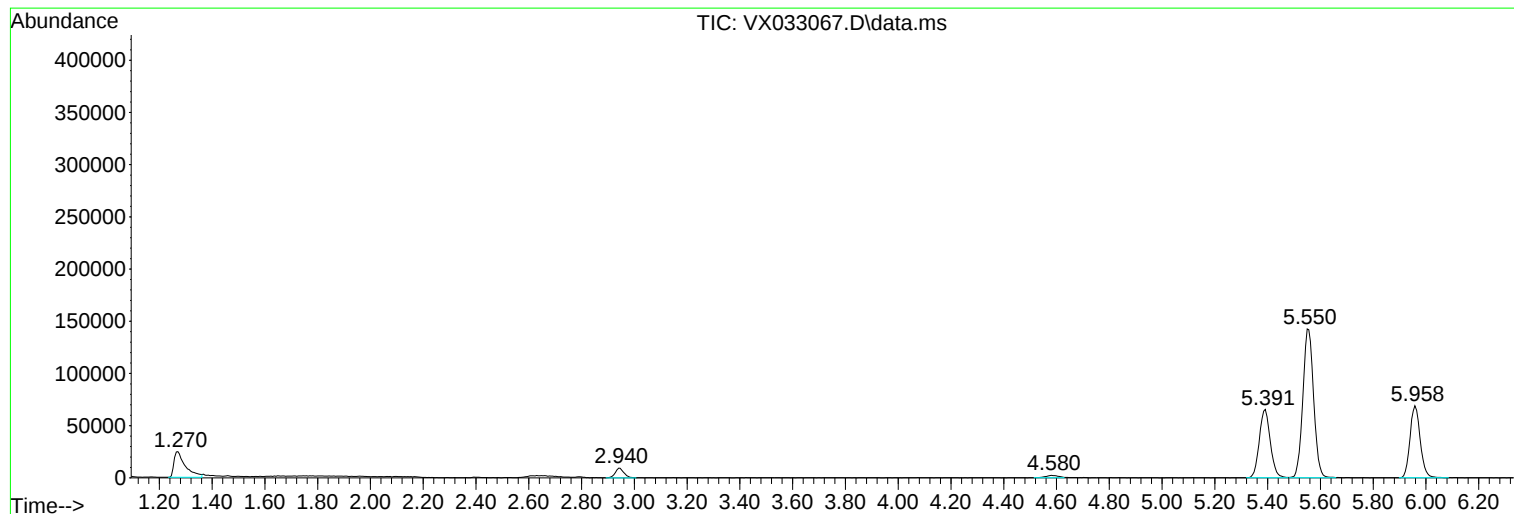

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033067.D
Acq On : 25 Nov 2022 14:55
Operator : JC/MD
Sample : N5742-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB111822







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	9.12 ug/l	73839	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	64
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

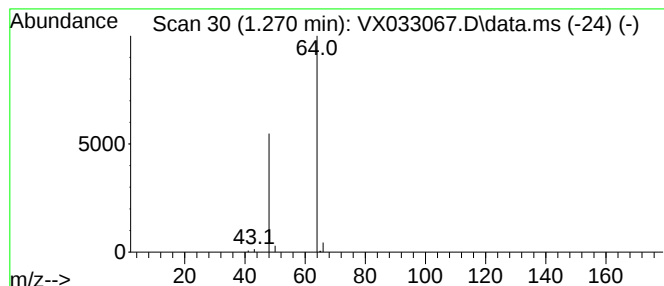

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033067.D
Acq On : 25 Nov 2022 14:55
Operator : JC/MD
Sample : N5742-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB111822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.270	9.1	ug/l	73839	1	5.556	405030	50.0