

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
 Data File : VX033070.D
 Acq On : 25 Nov 2022 16:04
 Operator : JC/MD
 Sample : N5741-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	26	32	37	rBV2	10517	25660	4.44%	0.754%
2	2.989	300	312	325	rBV3	8079	32277	5.58%	0.948%
3	3.111	325	332	345	rVB	24689	58238	10.07%	1.711%
4	3.764	431	439	451	rVB4	2860	7411	1.28%	0.218%
5	5.391	694	706	722	rBV	62476	185795	32.13%	5.460%
6	5.550	722	732	747	rVB	137983	391467	67.69%	11.503%
7	5.958	789	799	819	rBV	69191	183468	31.72%	5.391%
8	6.257	838	848	862	rBV4	10302	36079	6.24%	1.060%
9	6.763	921	931	945	rBV	208931	497289	85.99%	14.613%
10	8.433	1199	1205	1212	rVB2	3579	6465	1.12%	0.190%
11	8.647	1234	1240	1248	rBV	313669	496346	85.83%	14.585%
12	8.720	1248	1252	1260	rVB	7414	12546	2.17%	0.369%
13	8.848	1267	1273	1280	rVB	4744	7758	1.34%	0.228%
14	9.458	1367	1373	1380	rVB3	3424	5830	1.01%	0.171%
15	10.055	1465	1471	1485	rVB	436751	578315	100.00%	16.994%
16	11.079	1634	1639	1654	rBV	269903	341354	59.03%	10.031%
17	12.024	1788	1794	1803	rBV	422351	536813	92.82%	15.774%




Sum of corrected areas: 3403111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033070.D
Acq On : 25 Nov 2022 16:04
Operator : JC/MD
Sample : N5741-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

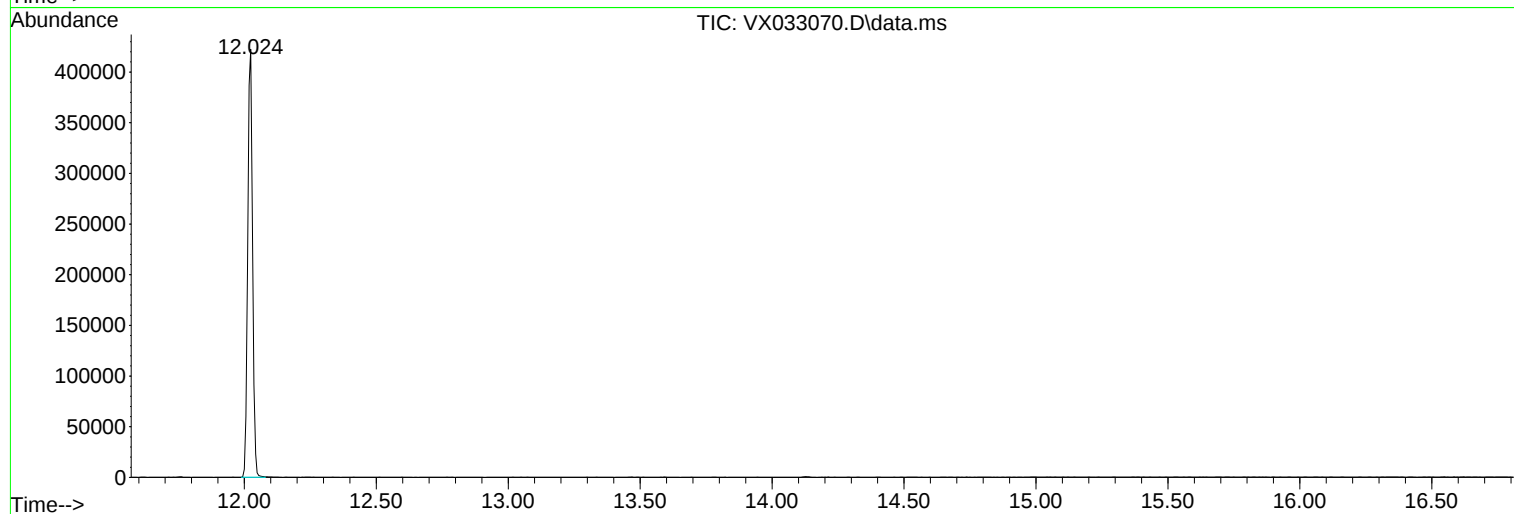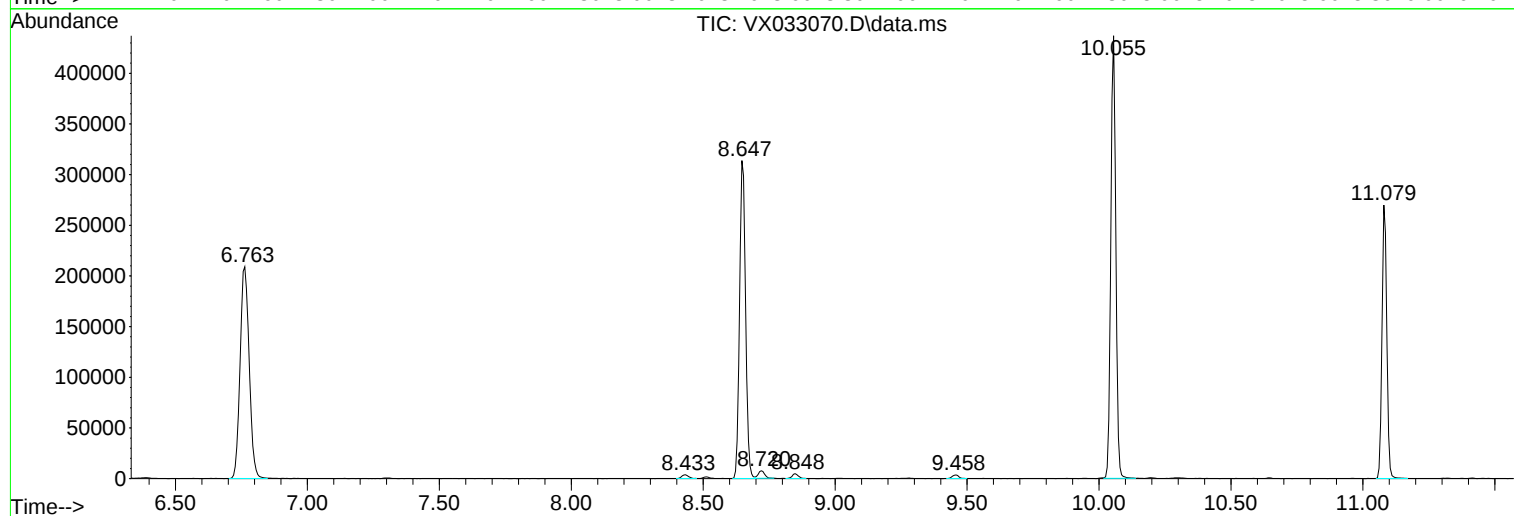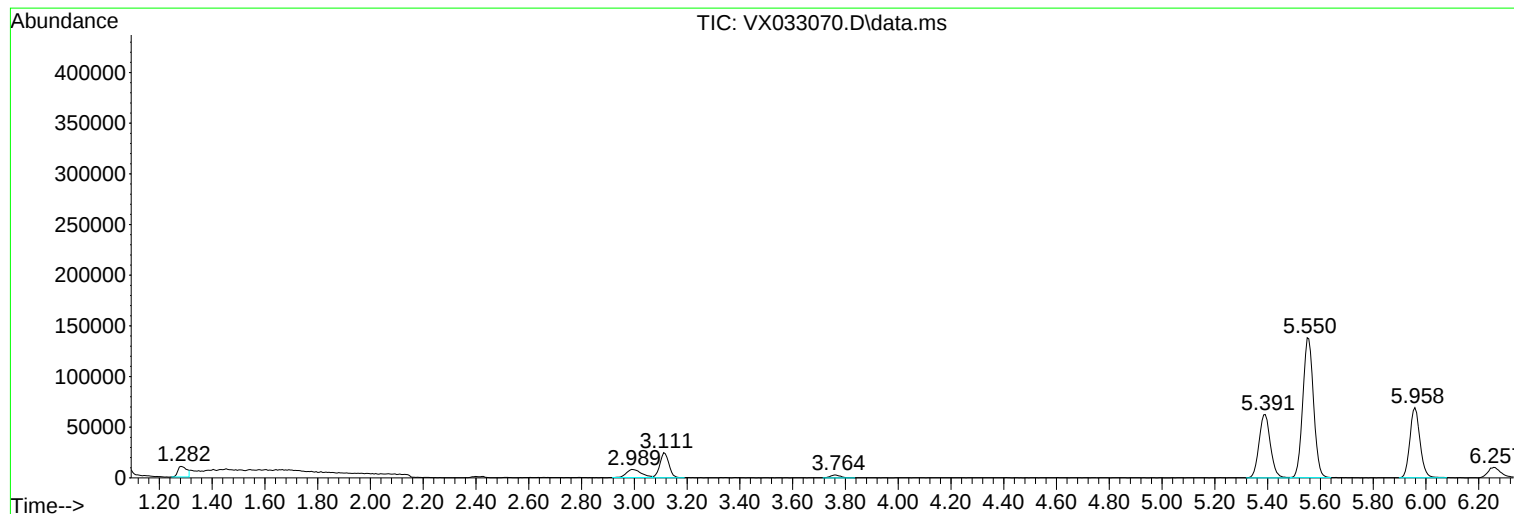

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033070.D
Acq On : 25 Nov 2022 16:04
Operator : JC/MD
Sample : N5741-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033070.D
Acq On : 25 Nov 2022 16:04
Operator : JC/MD
Sample : N5741-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc