

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
 Data File : VX033072.D
 Acq On : 25 Nov 2022 16:51
 Operator : JC/MD
 Sample : N5742-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB111822

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	49	rBV	37049	101846	18.61%	3.184%
2	2.947	295	305	315	rBV	15132	35492	6.49%	1.109%
3	4.587	560	574	587	rBV	3655	14137	2.58%	0.442%
4	5.385	692	705	720	rBV	60339	177095	32.36%	5.536%
5	5.550	722	732	750	rVB	130696	370721	67.74%	11.589%
6	5.958	787	799	811	rBV2	64852	175325	32.04%	5.481%
7	6.763	919	931	949	rBV	195985	470529	85.98%	14.709%
8	8.647	1234	1240	1252	rBV	308084	476655	87.10%	14.900%
9	10.055	1465	1471	1482	rBV	413560	547261	100.00%	17.107%
10	11.079	1634	1639	1650	rBV	257766	326978	59.75%	10.221%
11	12.024	1788	1794	1805	rBV	390121	502927	91.90%	15.722%




Sum of corrected areas: 3198966

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033072.D
Acq On : 25 Nov 2022 16:51
Operator : JC/MD
Sample : N5742-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB111822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

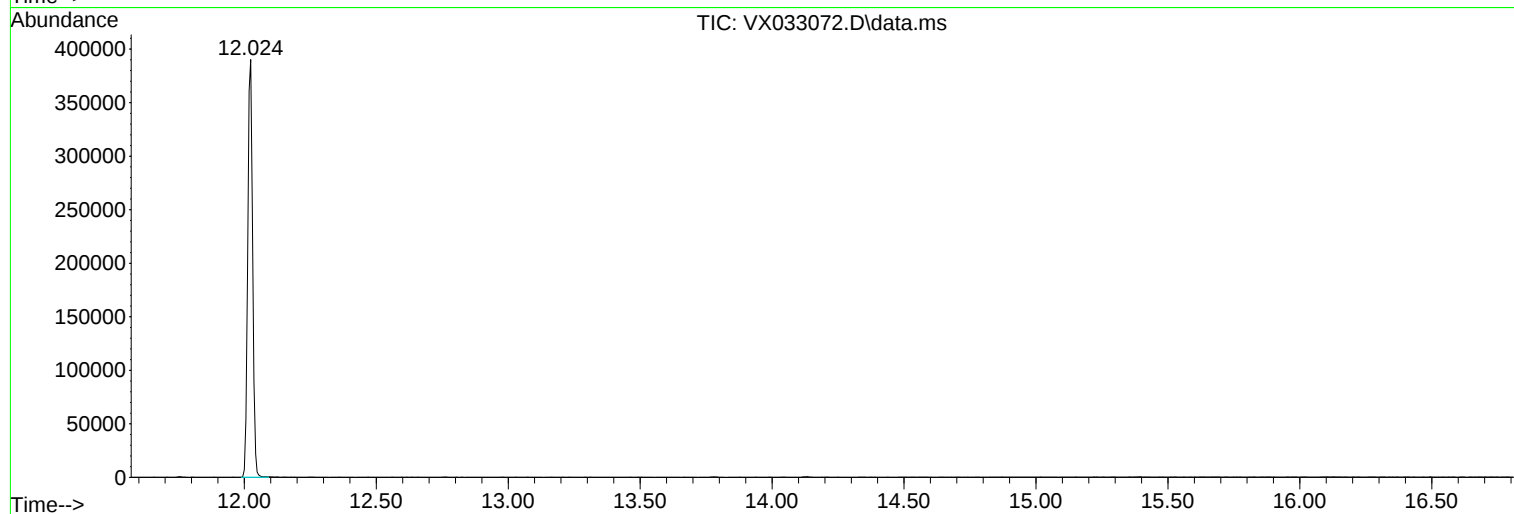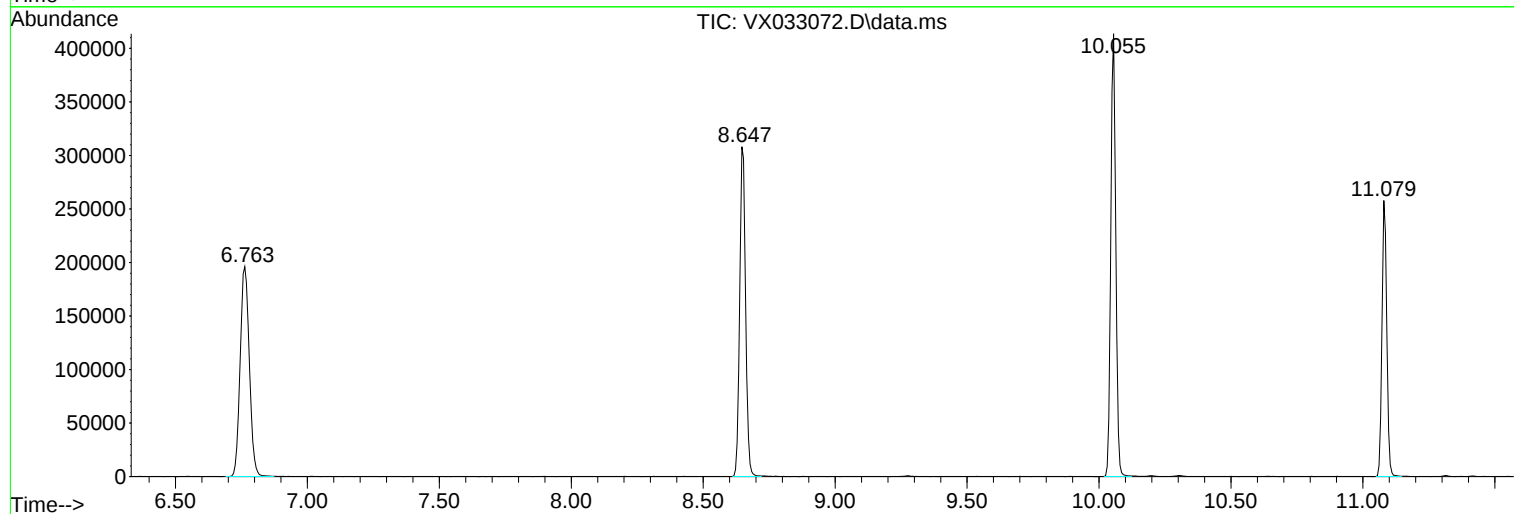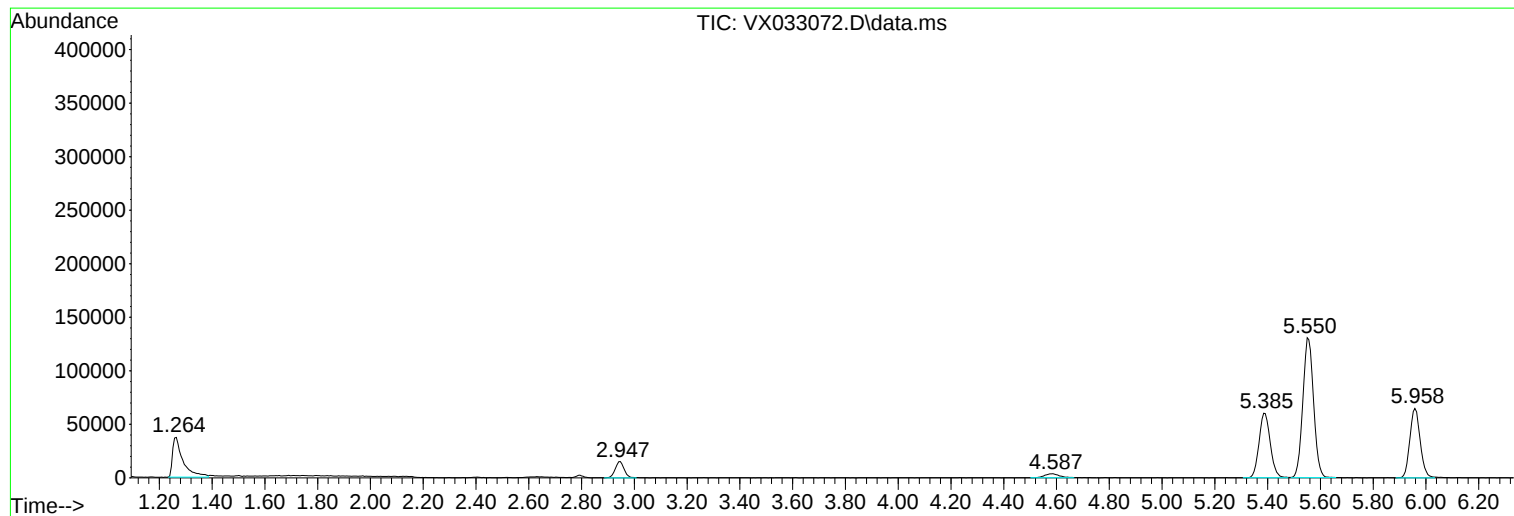

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033072.D
Acq On : 25 Nov 2022 16:51
Operator : JC/MD
Sample : N5742-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB111822









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.264	13.74 ug/l	101846	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	64
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	4

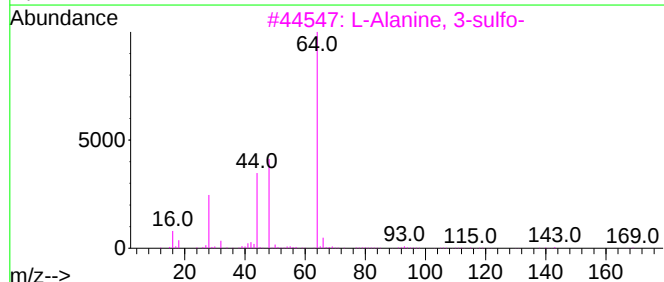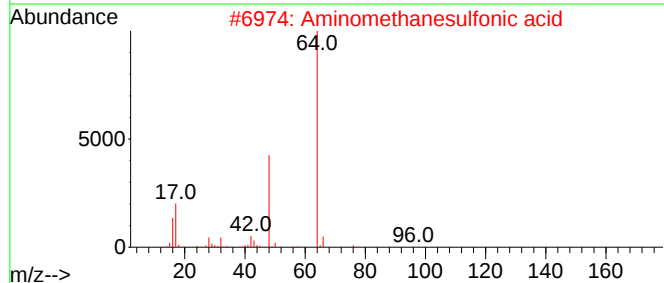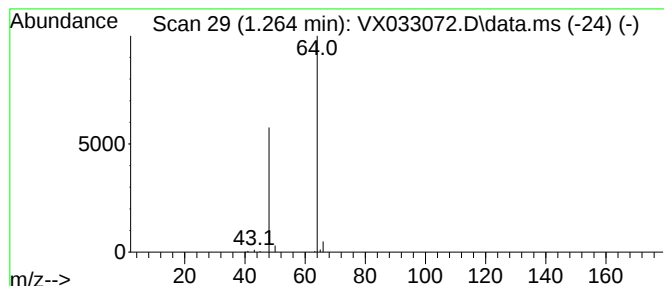

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033072.D
Acq On : 25 Nov 2022 16:51
Operator : JC/MD
Sample : N5742-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB111822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.264	13.7	ug/l	101846	1	5.556	370721	50.0