

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033076.D
Acq On : 25 Nov 2022 18:23
Operator : JC/MD
Sample : N5747-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38I

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260

Signal : TIC: VX033076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	44	rBV	14412	38154	2.18%	0.748%
2	3.111	322	332	351	rBV	769601	1751648	100.00%	34.342%
3	3.763	429	439	448	rBV2	10478	28129	1.61%	0.551%
4	5.385	694	705	721	rBV2	64376	190074	10.85%	3.726%
5	5.556	721	733	747	rVB2	141614	405347	23.14%	7.947%
6	5.958	788	799	813	rBV	69751	186138	10.63%	3.649%
7	6.763	920	931	949	rBV	216878	508022	29.00%	9.960%
8	8.647	1234	1240	1250	rBV	318314	503055	28.72%	9.863%
9	10.055	1465	1471	1480	rBV	439438	587695	33.55%	11.522%
10	11.079	1634	1639	1655	rBV	270254	351367	20.06%	6.889%
11	12.024	1788	1794	1802	rBV	440060	551013	31.46%	10.803%




Sum of corrected areas: 5100642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033076.D
Acq On : 25 Nov 2022 18:23
Operator : JC/MD
Sample : N5747-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

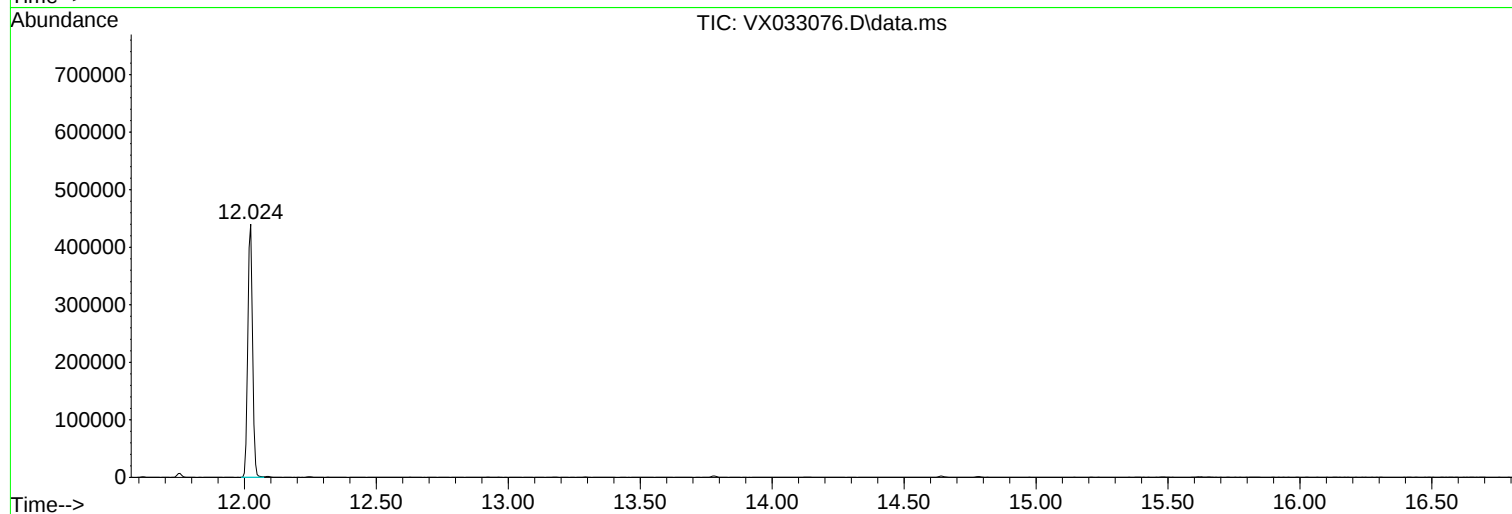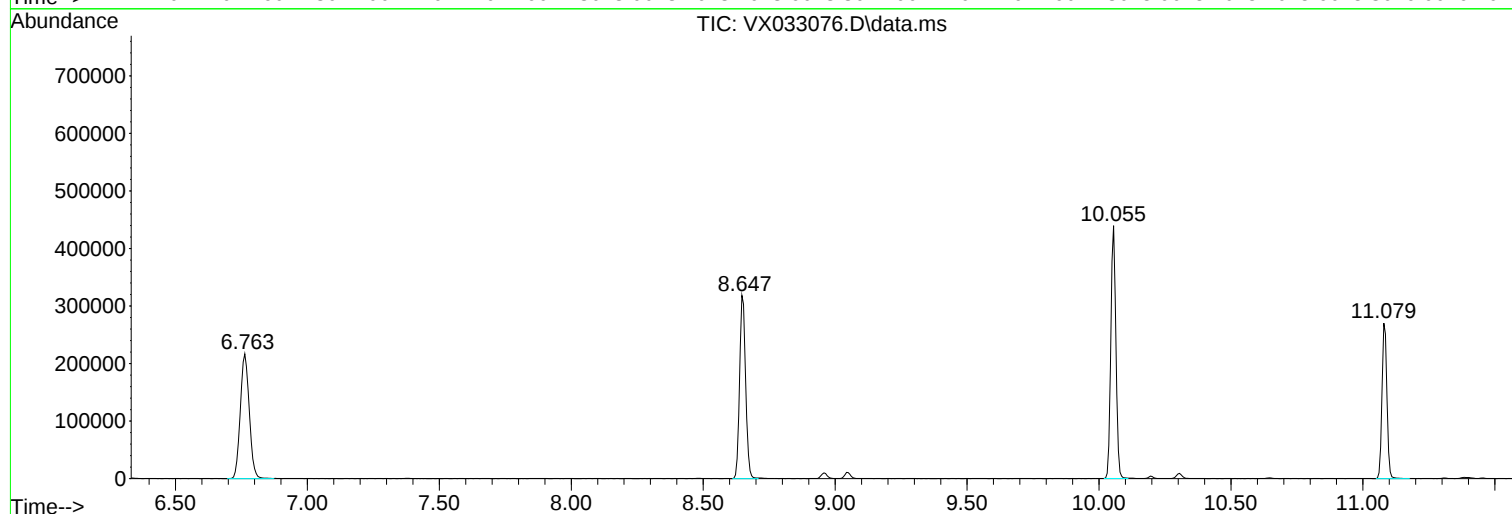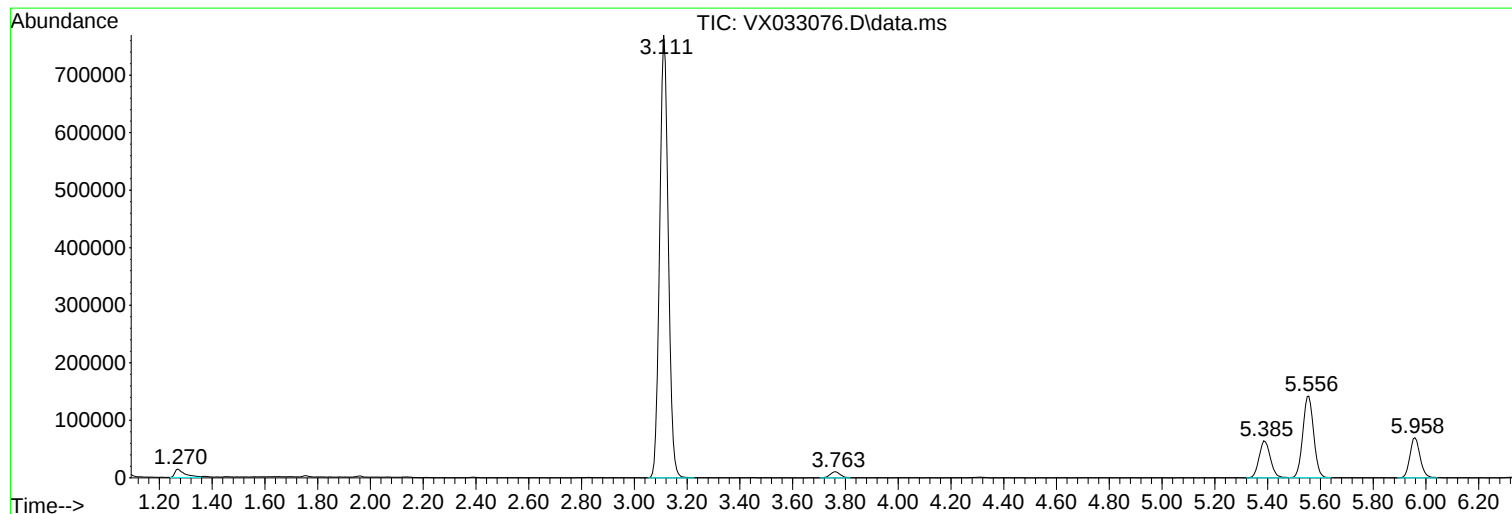

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033076.D
Acq On : 25 Nov 2022 18:23
Operator : JC/MD
Sample : N5747-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112522\
Data File : VX033076.D
Acq On : 25 Nov 2022 18:23
Operator : JC/MD
Sample : N5747-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc