

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112618\
 Data File : VX006202.D
 Acq On : 27 Nov 2018 04:04
 Operator : JC/MD
 Sample : PB115023ZHE#05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB115023ZHE#05

Quant Time: Nov 27 05:03:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 21 08:15:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	266060	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	401797	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	394053	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	182329	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	173149	56.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.32%	
35) Dibromofluoromethane	5.50	113	137718	53.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.80%	
50) Toluene-d8	8.71	98	516045	52.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.92%	
62) 4-Bromofluorobenzene	11.14	95	167221	45.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.60%	
Target Compounds						
16) Acetone	2.45	43	11899	8.698	ug/l	99
18) Methyl Acetate	2.78	43	4848	1.382	ug/l #	88
20) Methylene Chloride	2.86	84	212247	102.870	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112618\
Data File : VX006202.D
Acq On : 27 Nov 2018 04:04
Operator : JC/MD
Sample : PB115023ZHE#05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB115023ZHE#05

Quant Time: Nov 27 05:03:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 21 08:15:54 2018
Response via : Initial Calibration

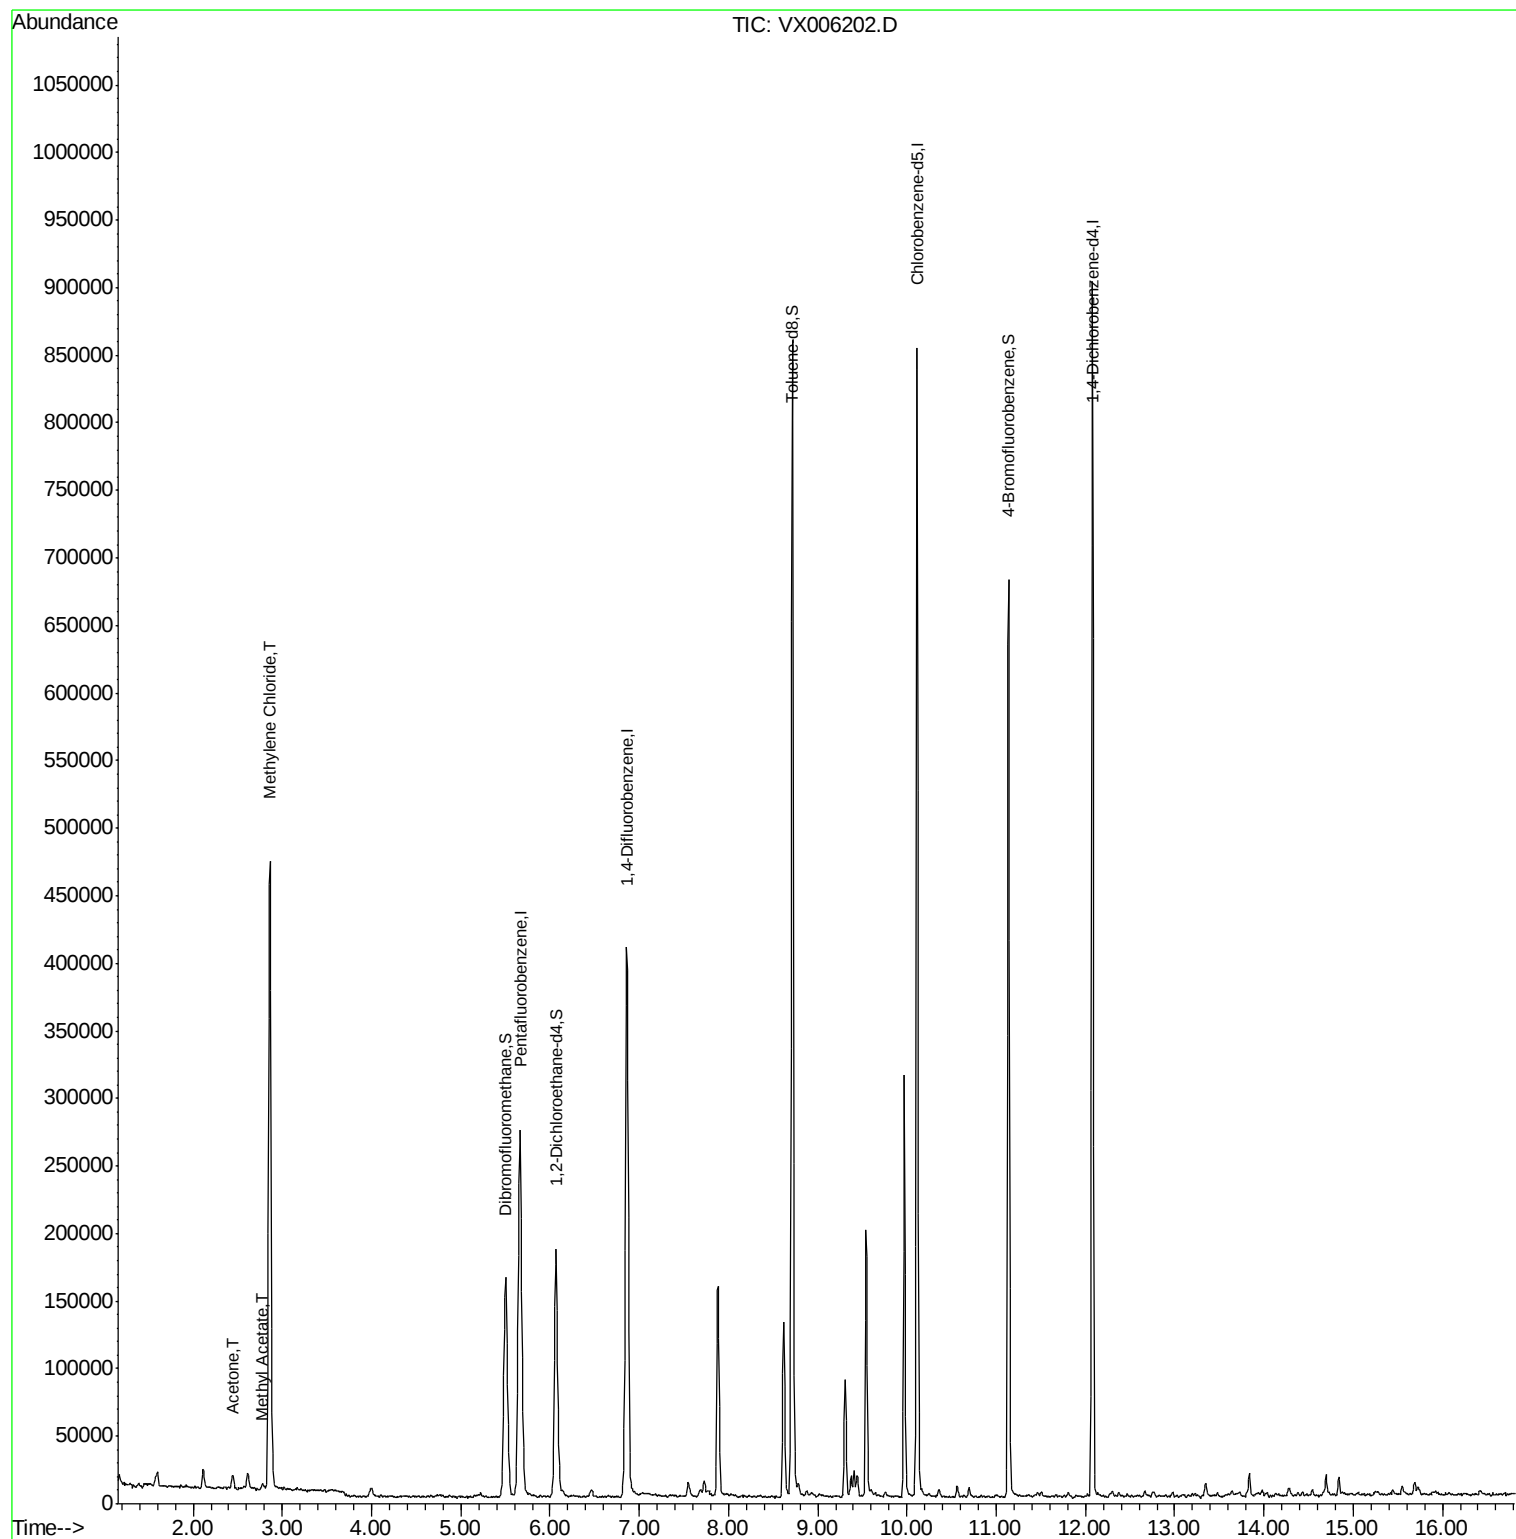

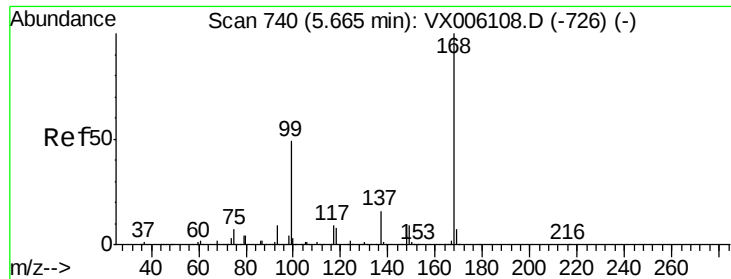

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006202.D

Acq: 27 Nov 2018 04:04

Instrument :

MSVOA_X

ClientSampleId :


PB115023ZHE#05

Tot Ion:168 Resp: 266060

Ion Ratio Lower Upper




168 100

99 53.2 39.2 58.8

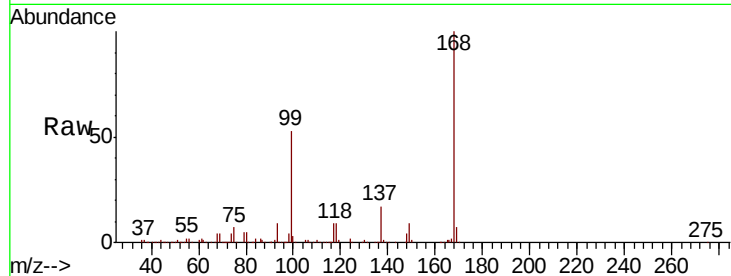

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

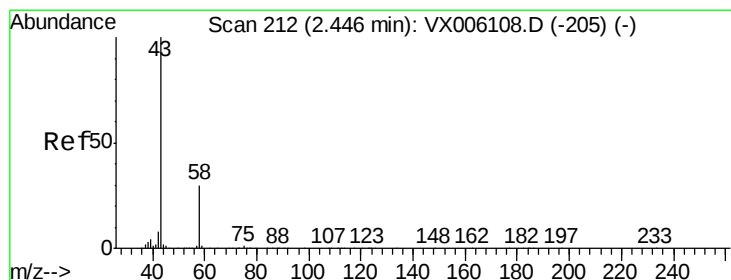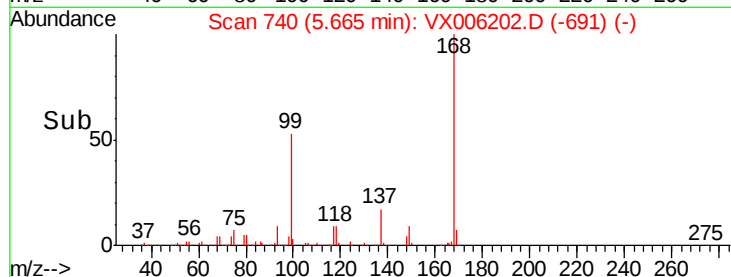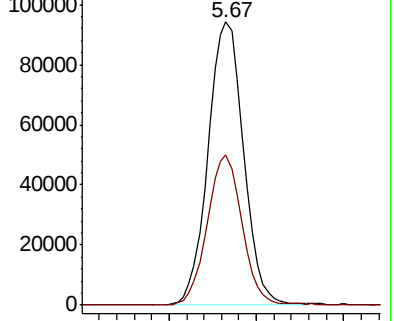

#16

Acetone

Concen: 8.698 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX006202.D


Acq: 27 Nov 2018 04:04

Tgt Ion: 43 Resp: 11899

Ion Ratio Lower Upper



43 100


58 29.5 23.8 35.8

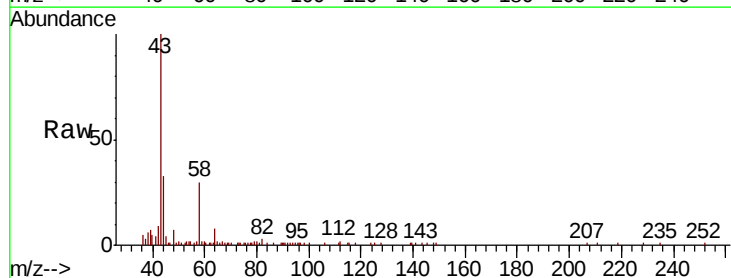

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



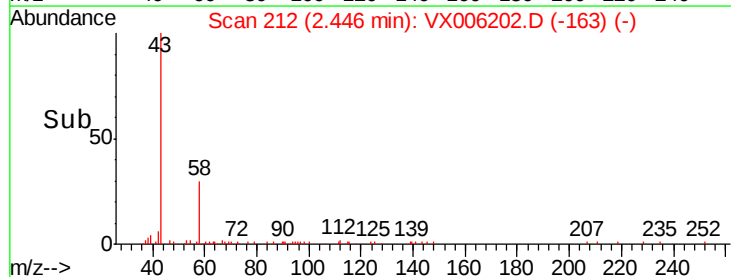
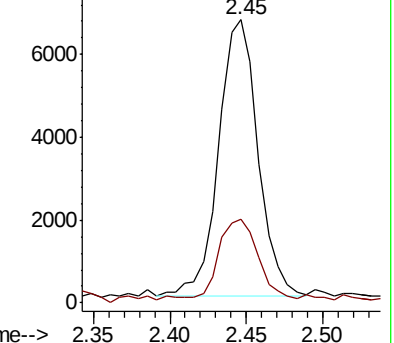


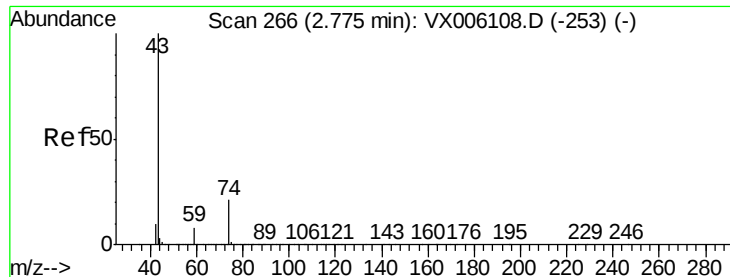

#18
Methvl Acetate
Concen: 1.382 ug/l
RT: 2.78 min Scan# 266
Delta R.T. 0.00 min
Lab File: VX006202.D
Acq: 27 Nov 2018 04:04




Instrument :
MSVOA_X
ClientSampleId :
PB115023ZHE#05


Tot Ion: 43 Resp: 4848
Ion Ratio Lower Upper
43 100
74 27.4 17.3 25.9#

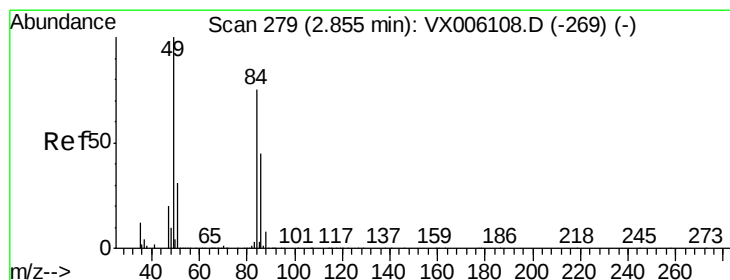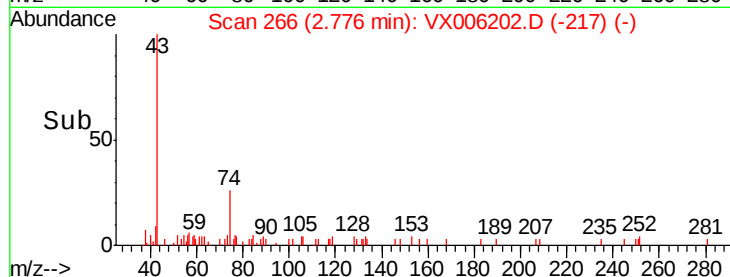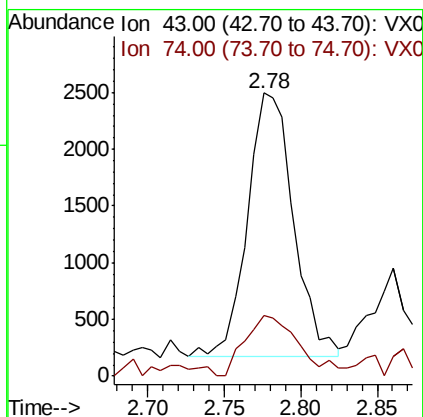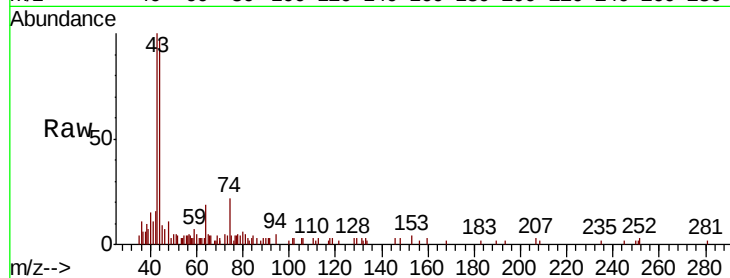

#20
Methylene Chloride
Concen: 102.870 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.01 min
Lab File: VX006202.D
Acq: 27 Nov 2018 04:04

Tgt Ion: 84 Resp: 212247
Ion Ratio Lower Upper
84 100
49 125.4 106.6 159.8
51 40.0 32.6 49.0
86 64.2 48.4 72.6


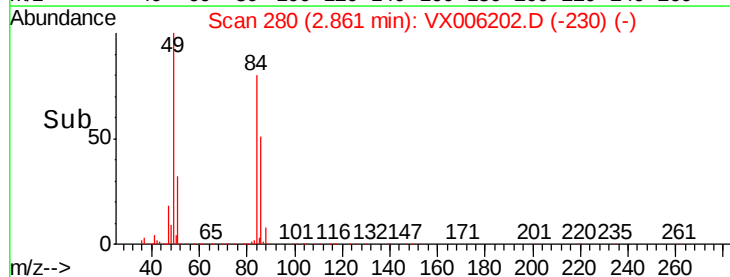
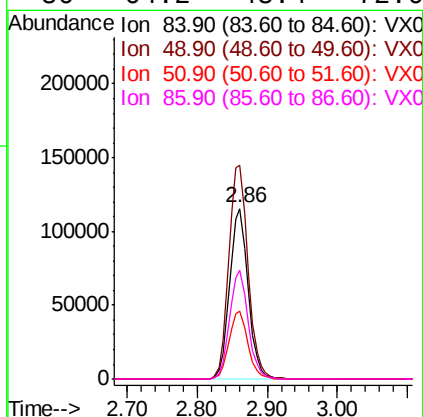
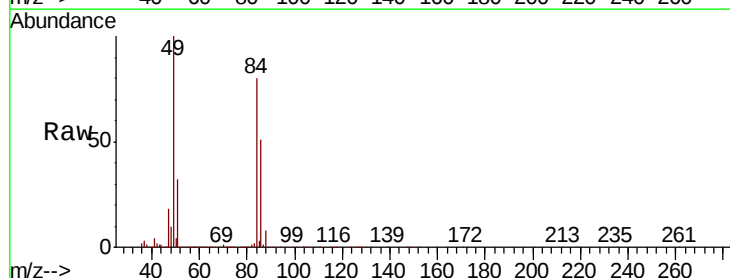


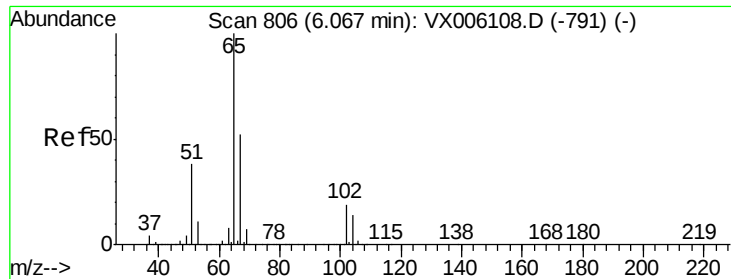

#33
 1,2-Dichloroethane-d4
 Concen: 56.163 ug/l
 RT: 6.07 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: VX006202.D
 Acq: 27 Nov 2018 04:04




Instrument :
 MSVOA_X
 ClientSampleId :
 PB115023ZHE#05


Tot Ion: 65 Resp: 173149
 Ion Ratio Lower Upper
 65 100
 67 52.6 0.0 105.8

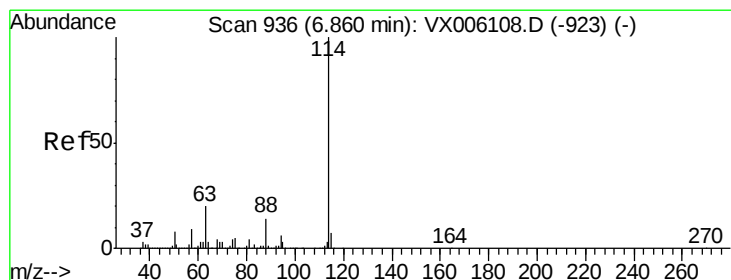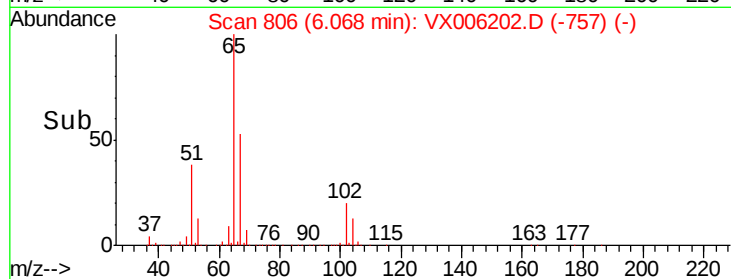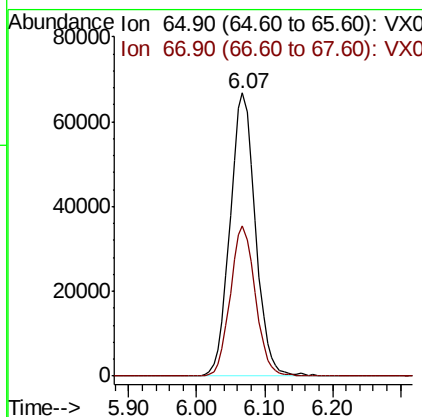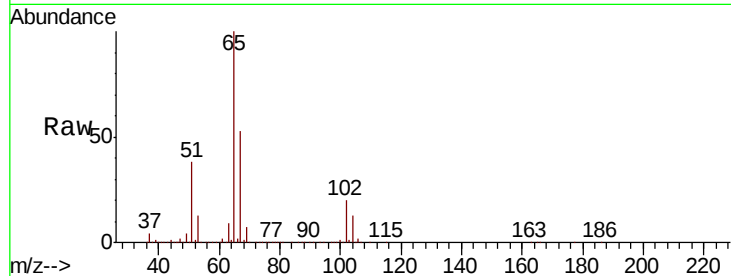

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX006202.D
 Acq: 27 Nov 2018 04:04

Tgt Ion: 114 Resp: 401797
 Ion Ratio Lower Upper
 114 100
 63 20.2 0.0 39.2
 88 15.4 0.0 28.6

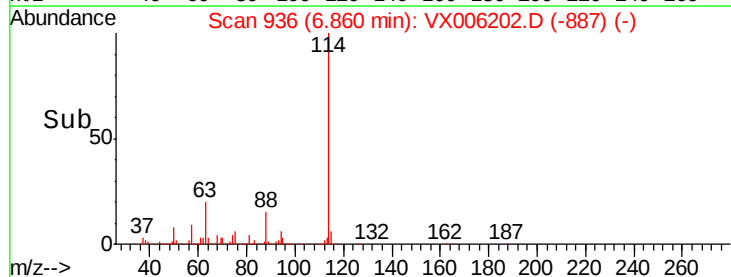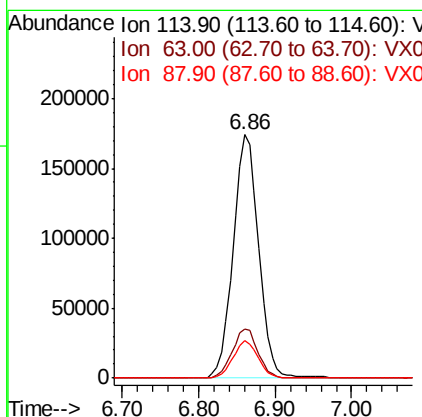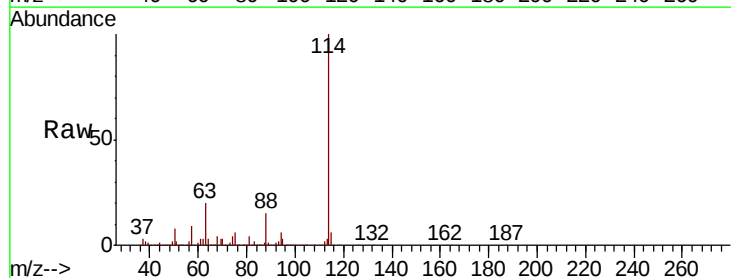

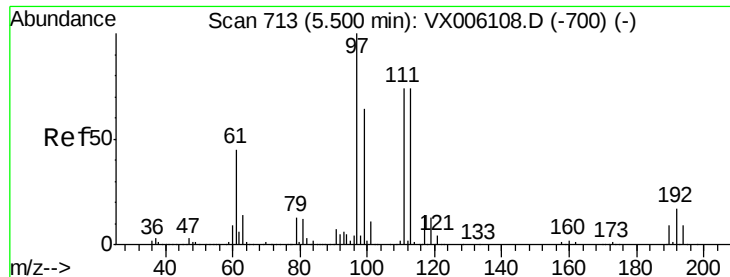

#35

Dibromofluoromethane

Concen: 53.395 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006202.D

Acq: 27 Nov 2018 04:04

Instrument :

MSVOA_X

ClientSampleId :

PB115023ZHE#05


Tot Ion:113 Resp: 137718

Ion Ratio Lower Upper

113 100

111 103.1 81.5 122.3




192 22.8 18.6 28.0

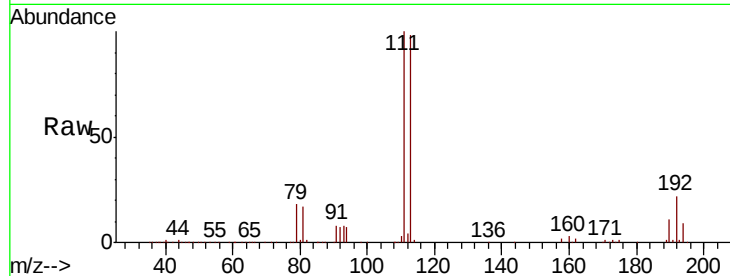

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

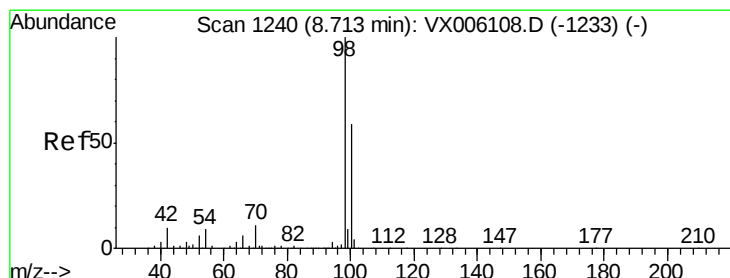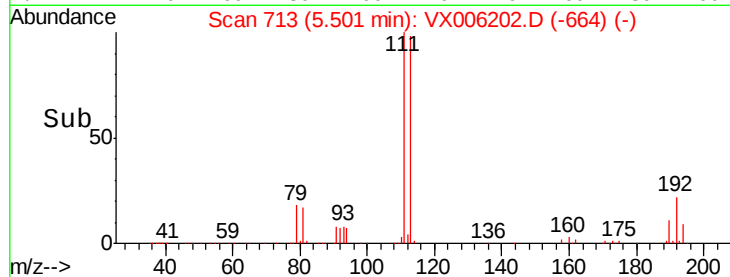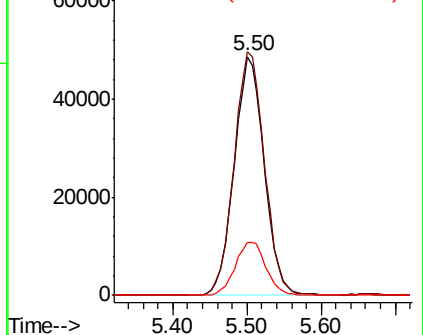

#50

Toluene-d8

Concen: 52.457 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006202.D


Acq: 27 Nov 2018 04:04

Tgt Ion: 98 Resp: 516045

Ion Ratio Lower Upper



98 100


100 62.5 51.0 76.4

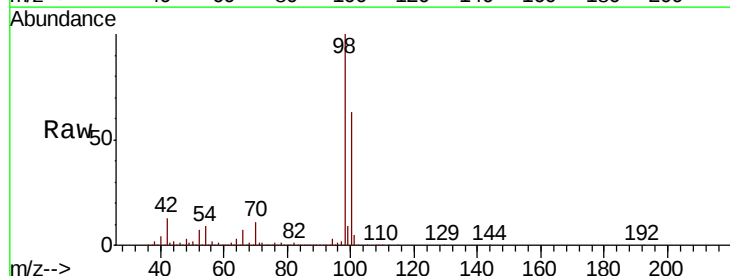

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

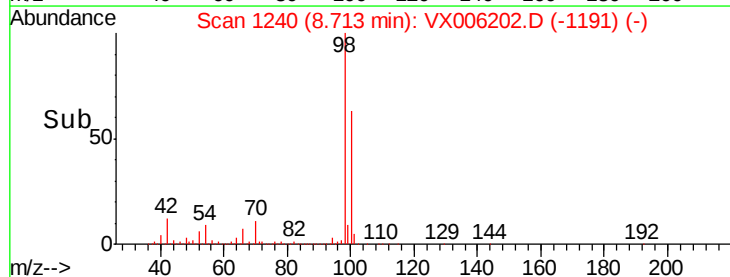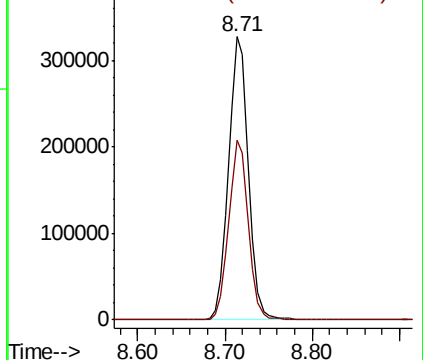

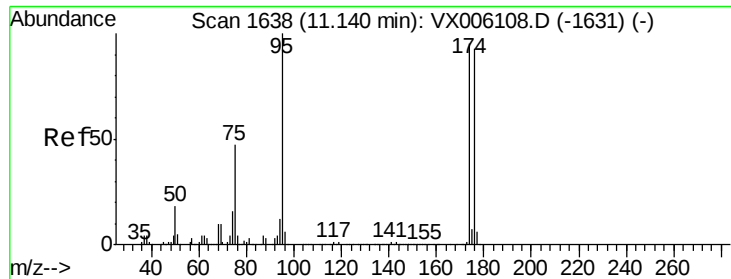

#62

4-Bromofluorobenzene

Concen: 45.304 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.00 min

Lab File: VX006202.D

Acq: 27 Nov 2018 04:04

Instrument :

MSVOA_X

ClientSampleId :

PB115023ZHE#05


Tot Ion: 95 Resp: 167221

Ion Ratio Lower Upper

95 100

174 93.7 0.0 184.4




176 90.1 0.0 179.0

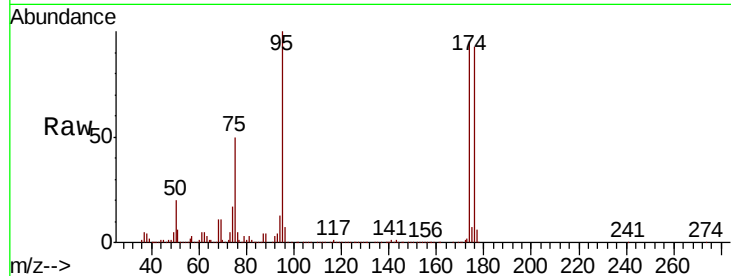

Abundance Ion 94.90 (94.60 to 95.60): VX006202.D (-1589) (-)

Ion 173.80 (173.50 to 174.50): VX006202.D (-1589) (-)

Ion 175.80 (175.50 to 176.50): VX006202.D (-1589) (-)

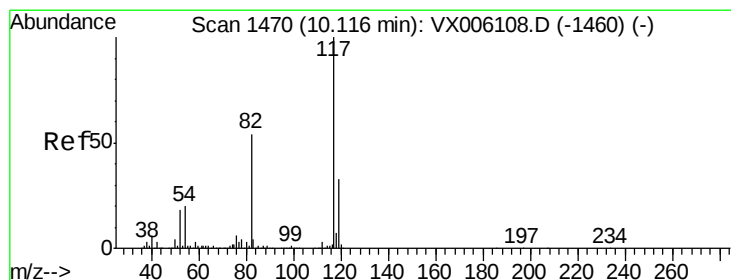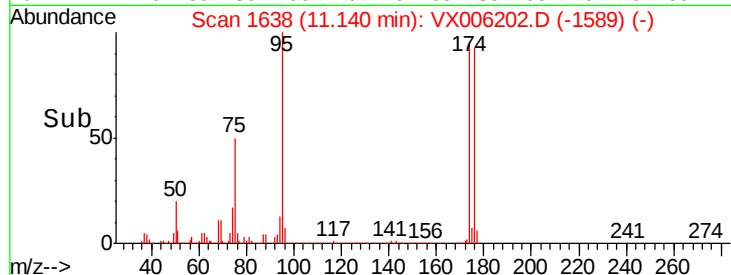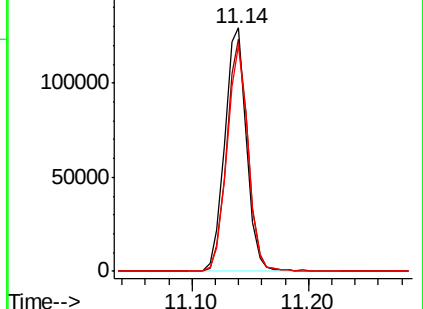

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VX006202.D

Acq: 27 Nov 2018 04:04


Tgt Ion: 117 Resp: 394053

Ion Ratio Lower Upper

117 100

82 53.9 43.0 64.4



119 31.6 26.1 39.1

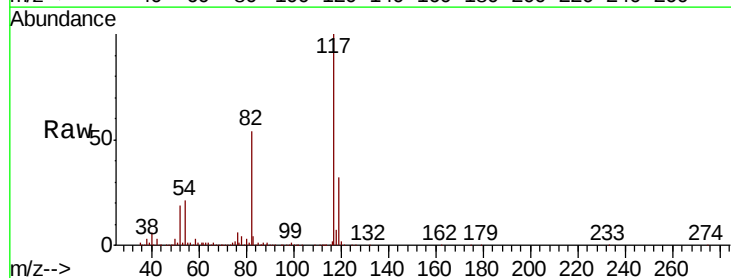


Abundance Ion 116.90 (116.60 to 117.60): VX006202.D (-1421) (-)

Ion 82.00 (81.70 to 82.70): VX006202.D (-1421) (-)

Ion 118.90 (118.60 to 119.60): VX006202.D (-1421) (-)

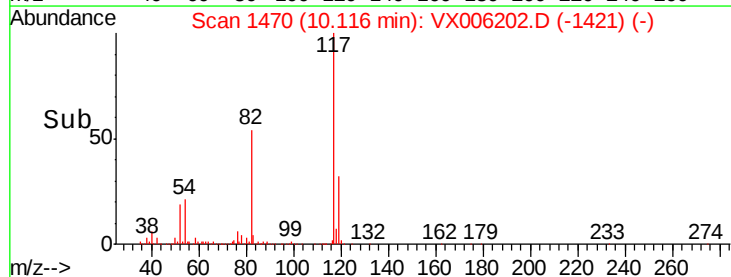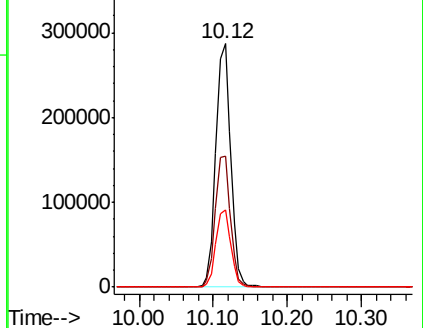

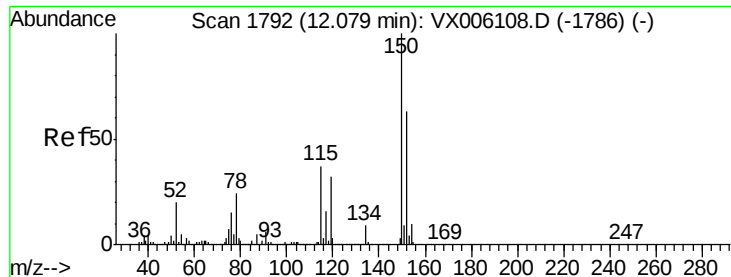

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX006202.D

Acq: 27 Nov 2018 04:04

Instrument :

MSVOA_X

ClientSampleId :

PB115023ZHE#05


Tot Ion:152 Resp: 182329

Ion Ratio Lower Upper

152 100

115 55.2 39.0 116.9

150 156.0 0.0 346.6

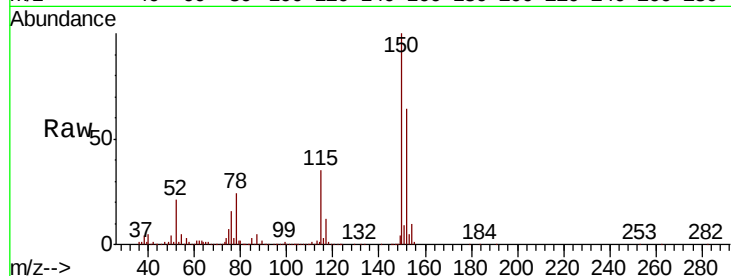

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

