


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX112618\
 Data File : VX006164.D
 Acq On : 26 Nov 2018 09:15
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
 Title : SW846 8260
 Last Update : Wed Nov 21 08:15:54 2018

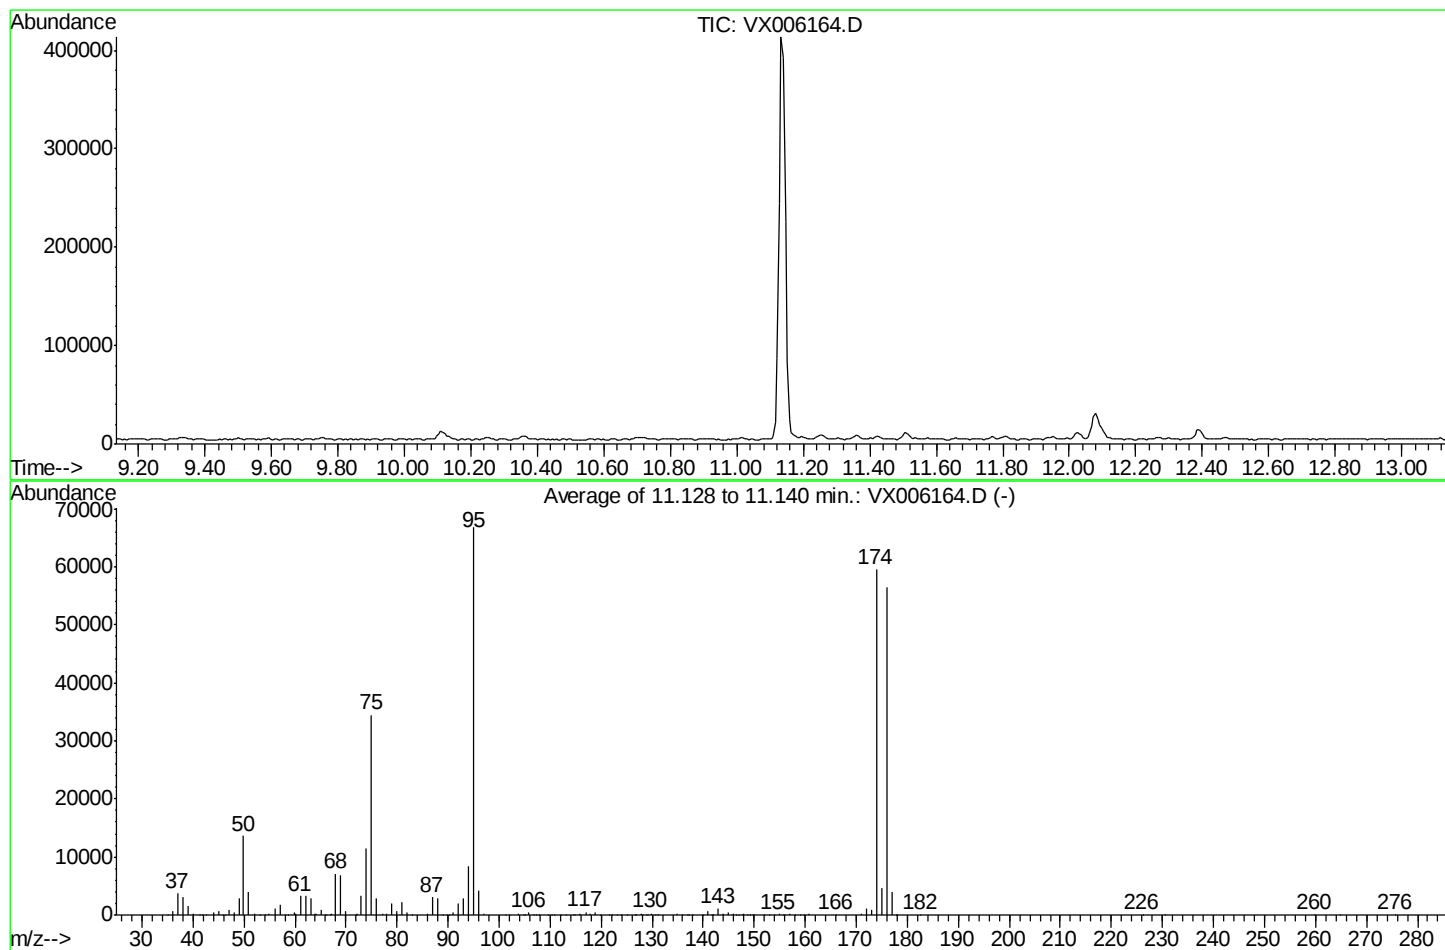

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	13571	PASS
75	95	30	60	51.6	34429	PASS
95	95	100	100	100.0	66778	PASS
96	95	5	9	6.4	4249	PASS
173	174	0.00	2	1.5	920	PASS
174	95	50	100	89.1	59528	PASS
175	174	5	9	7.7	4607	PASS
176	174	95	101	95.0	56554	PASS
177	176	5	9	6.9	3874	PASS