


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX112618\
Data File : VX006189.D
Acq On : 26 Nov 2018 21:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Title : SW846 8260
Last Update : Wed Nov 21 08:15:54 2018

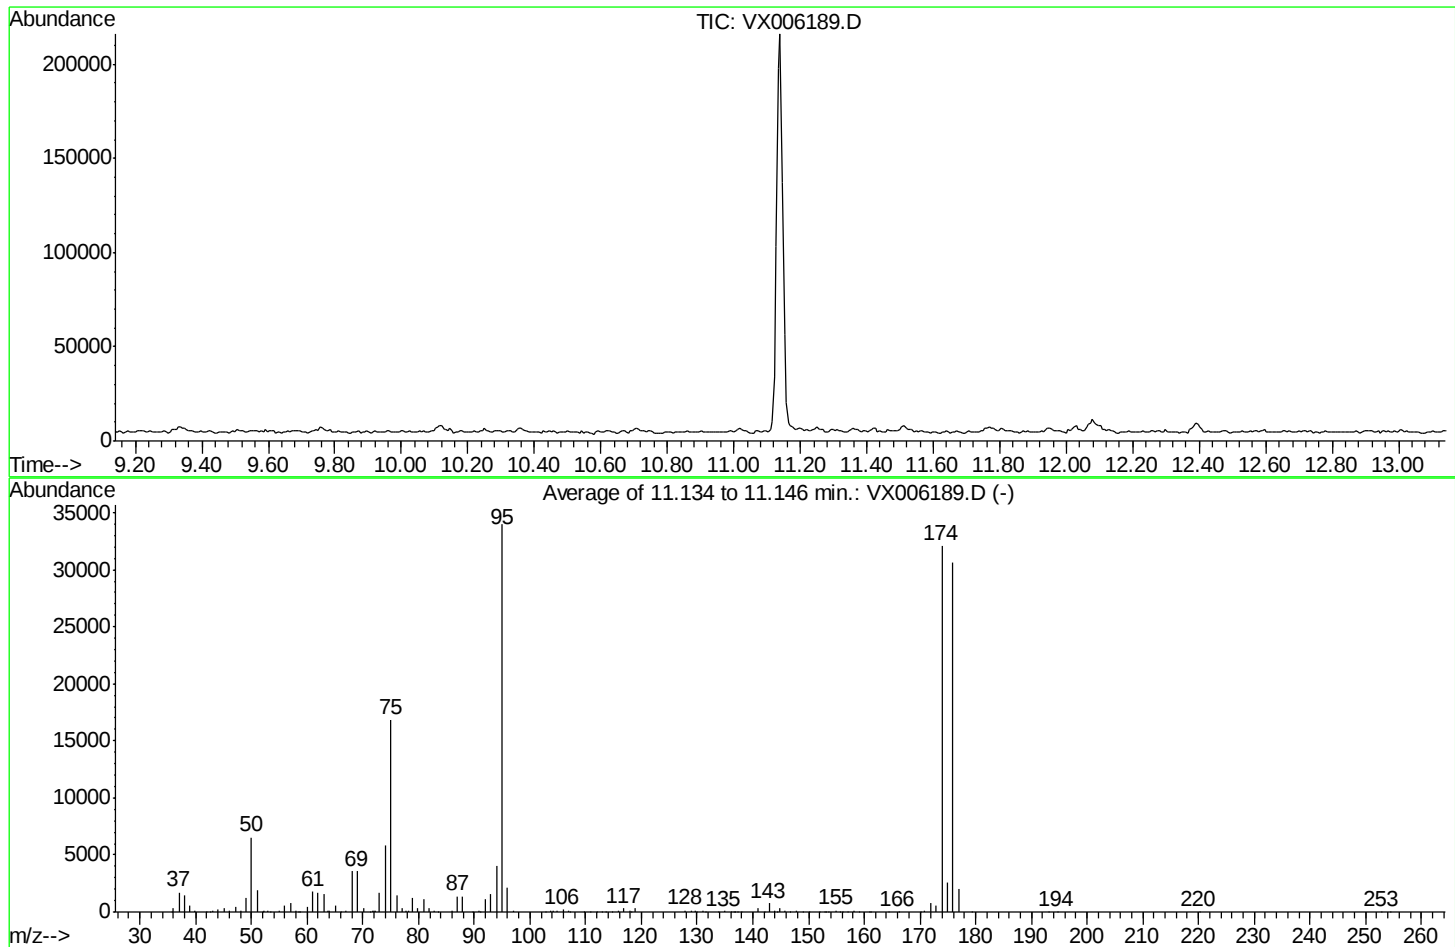

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6563	PASS
75	95	30	60	49.6	16837	PASS
95	95	100	100	100.0	33973	PASS
96	95	5	9	6.1	2089	PASS
173	174	0.00	2	1.7	547	PASS
174	95	50	100	94.5	32101	PASS
175	174	5	9	8.0	2561	PASS
176	174	95	101	95.4	30624	PASS
177	176	5	9	6.5	1995	PASS