

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112619\
 Data File : VX013604.D
 Acq On : 26 Nov 2019 17:17
 Operator : JC/SP
 Sample : VX1126WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1126WBL01

Quant Time: Nov 26 17:57:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 26 15:53:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	675215	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1083438	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	955305	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	422982	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	392480	50.08	ug/l	0.00
Spiked Amount			Recovery	=	100.16%	
35) Dibromofluoromethane	5.48	113	325253	48.56	ug/l	0.00
Spiked Amount			Recovery	=	97.12%	
50) Toluene-d8	8.71	98	1283469	49.18	ug/l	0.00
Spiked Amount			Recovery	=	98.36%	
62) 4-Bromofluorobenzene	11.13	95	429850	45.68	ug/l	0.00
Spiked Amount			Recovery	=	91.36%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112619\
Data File : VX013604.D
Acq On : 26 Nov 2019 17:17
Operator : JC/SP
Sample : VX1126WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1126WBL01

Quant Time: Nov 26 17:57:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 26 15:53:00 2019
Response via : Initial Calibration

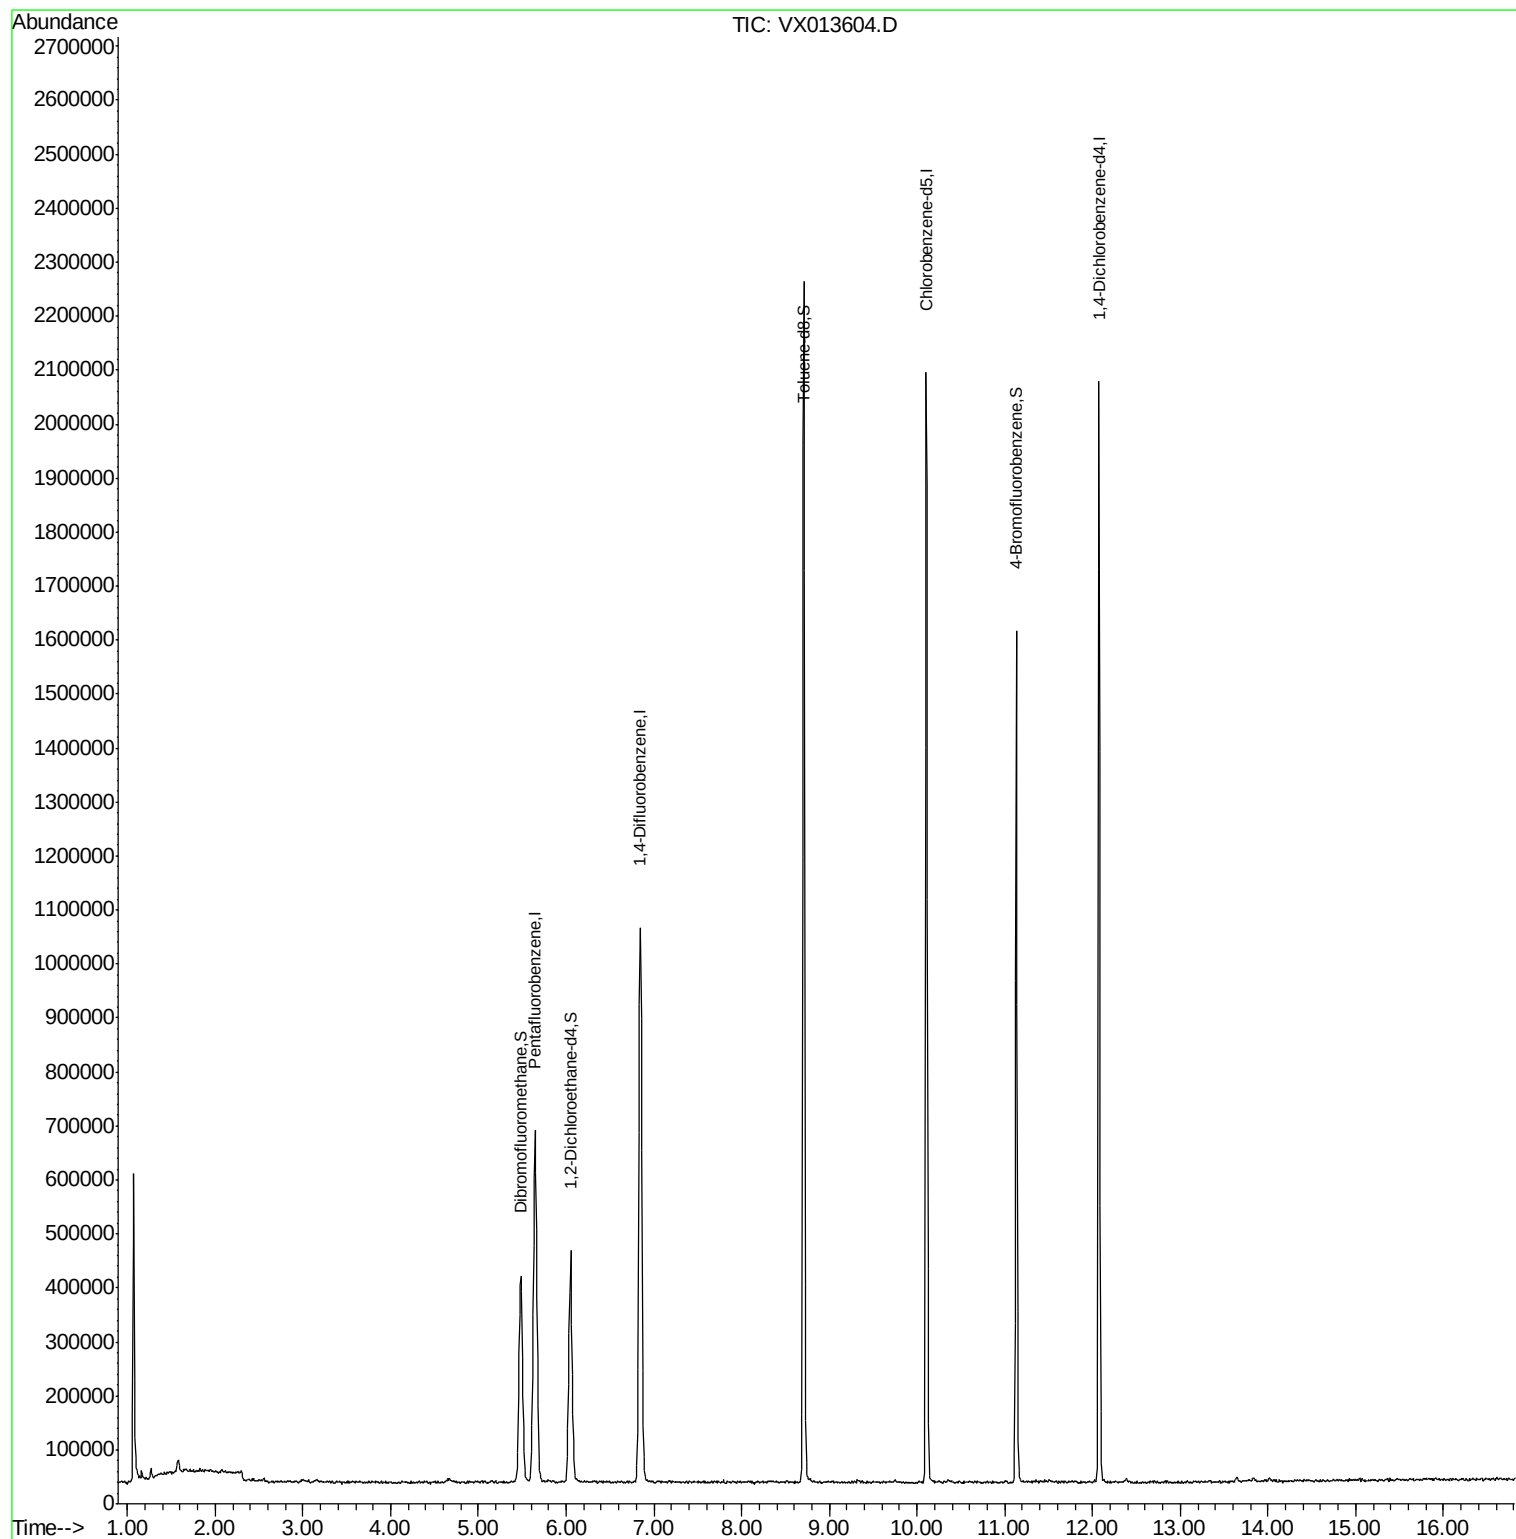

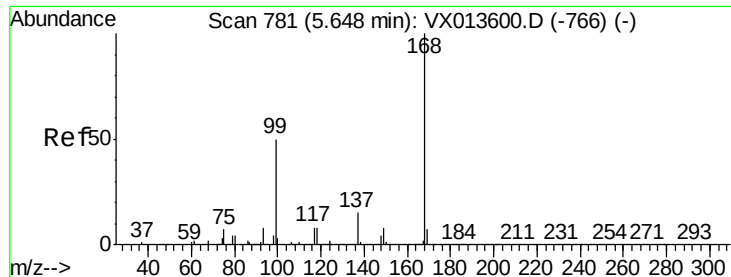

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX013604.D

Acq: 26 Nov 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :


VX1126WBL01

Tot Ion:168 Resp: 675215

Ion Ratio Lower Upper

168 100

99 48.9 39.8 59.8

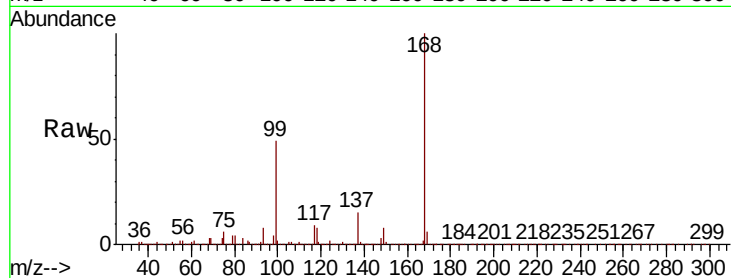

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000



150000

100000

50000

0

Time-->

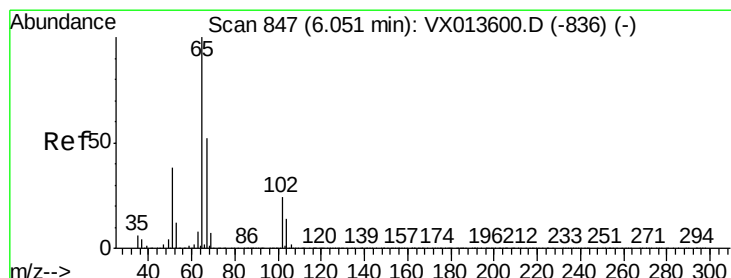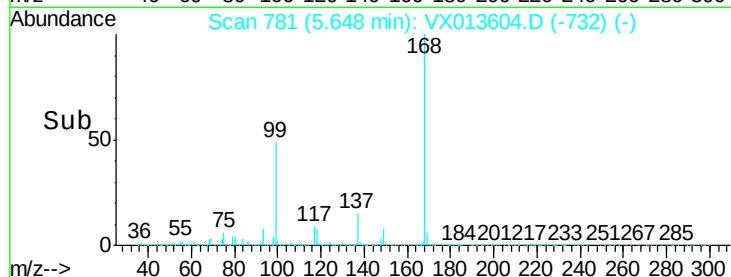

#33

1,2-Dichloroethane-d4

Concen: 50.076 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX013604.D


Acq: 26 Nov 2019 17:17

Tgt Ion: 65 Resp: 392480

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.4

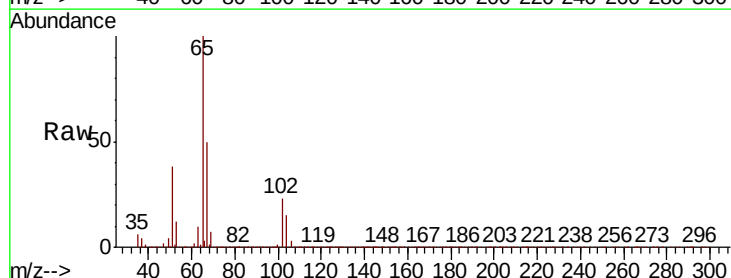

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05


150000


100000

50000

0

Time-->

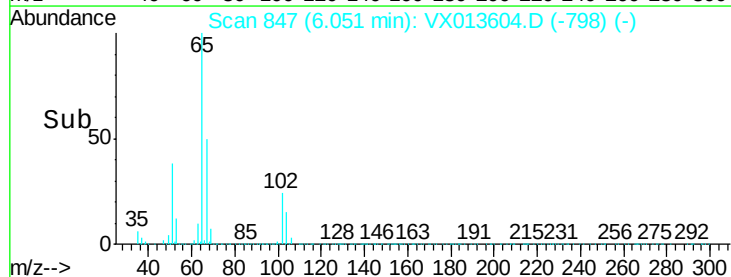

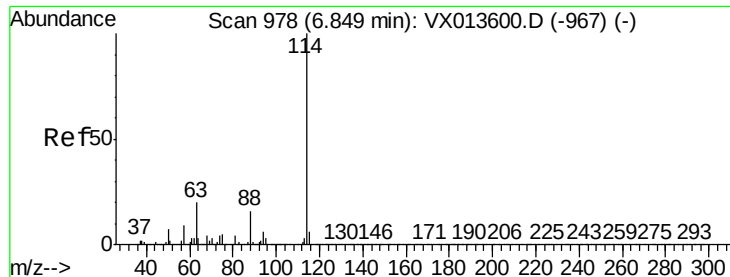

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 977

Delta R.T. -0.01 min

Lab File: VX013604.D

Acq: 26 Nov 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :

VX1126WBL01


Tot Ion:114 Resp: 1083438

Ion Ratio Lower Upper

114 100

63 20.1 0.0 39.6

88 16.0 0.0 31.4

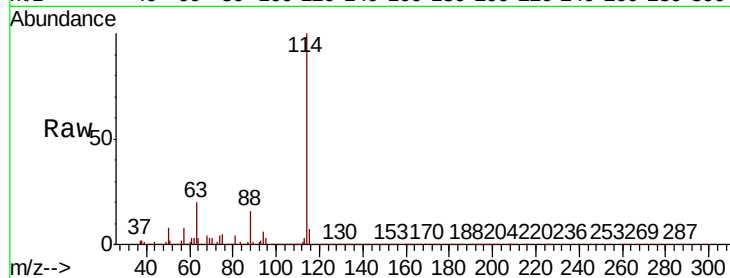



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.84

Time-->

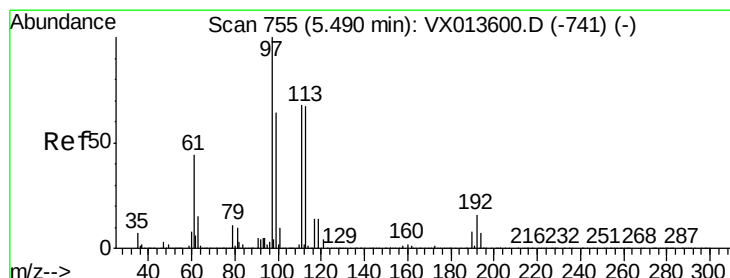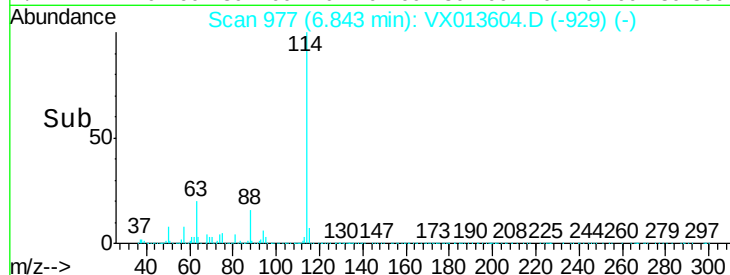

#35

Dibromofluoromethane

Concen: 48.560 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.01 min

Lab File: VX013604.D

Acq: 26 Nov 2019 17:17


Tgt Ion:113 Resp: 325253

Ion Ratio Lower Upper

113 100

111 103.4 83.6 125.4

192 23.8 19.2 28.8

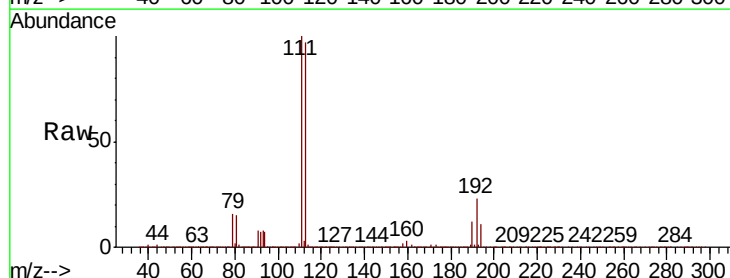


Abundance Ion 112.80 (112.50 to 113.50): V


Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

5.48

Time-->

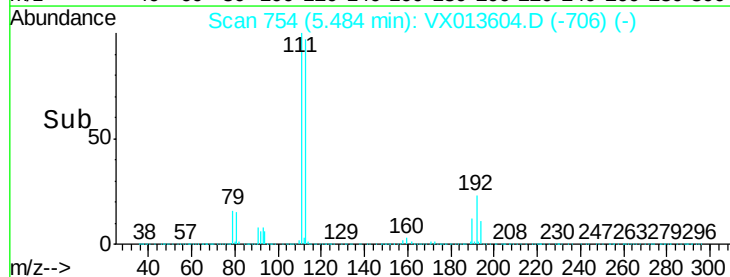

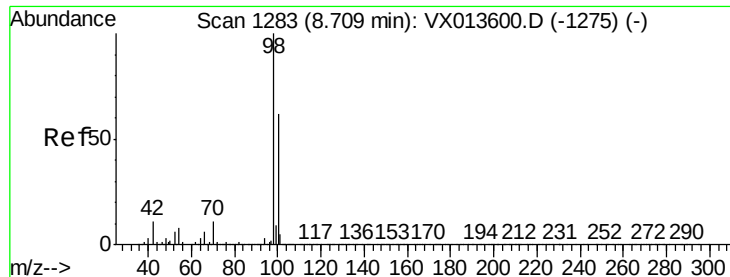

#50

Toluene-d8

Concen: 49.183 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX013604.D

Acq: 26 Nov 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :





VX1126WBL01

Tot Ion: 98 Resp: 1283469

Ion Ratio Lower Upper

98 100

100 65.6 53.1 79.7

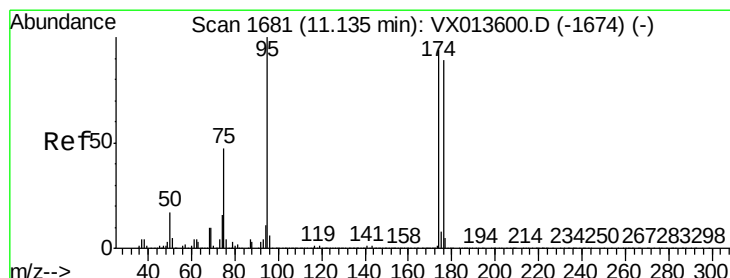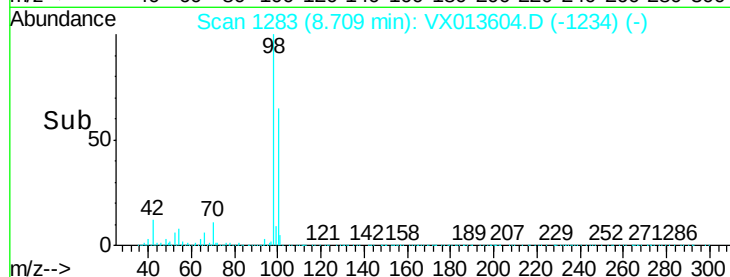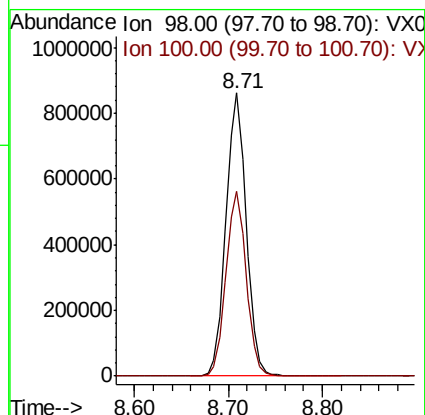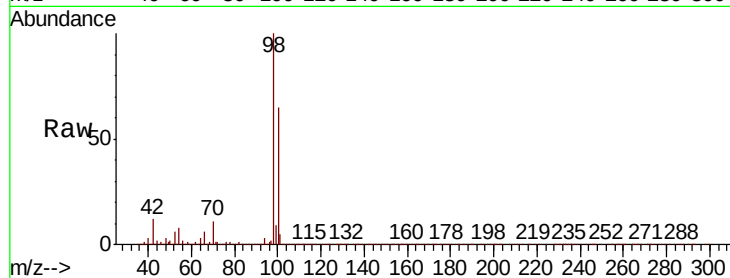

#62

4-Bromofluorobenzene

Concen: 45.679 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX013604.D

Acq: 26 Nov 2019 17:17




Tgt Ion: 95 Resp: 429850


Ion Ratio Lower Upper

95 100

174 89.4 0.0 180.0

176 86.3 0.0 173.6


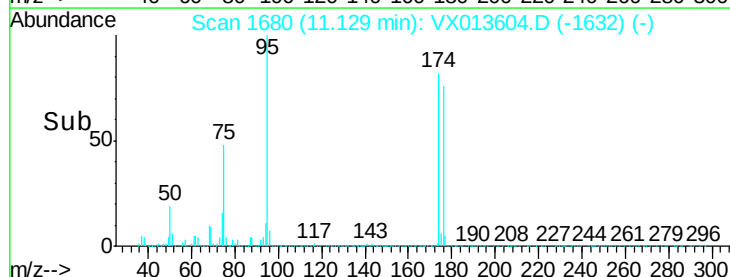
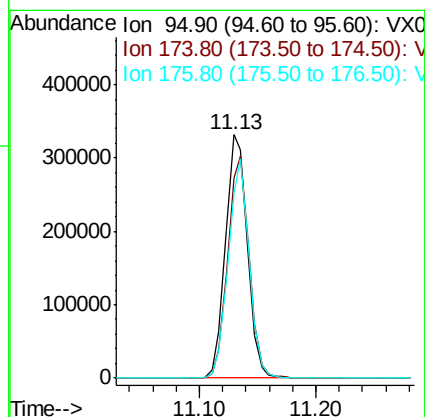
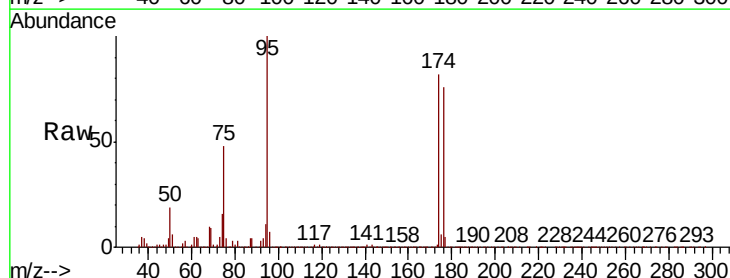


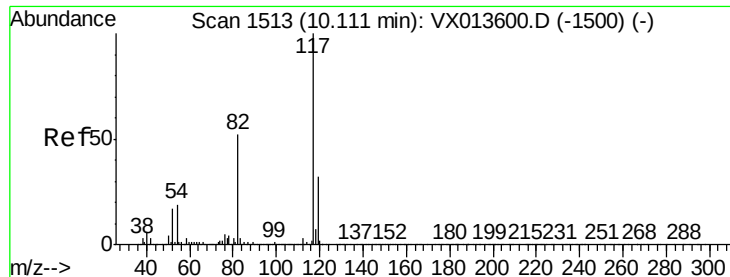

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013604.D
Acq: 26 Nov 2019 17:17

Instrument :
MSVOA_X
ClientSampleId :
VX1126WBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	53.9	41.8	62.8
119	32.3	25.8	38.8

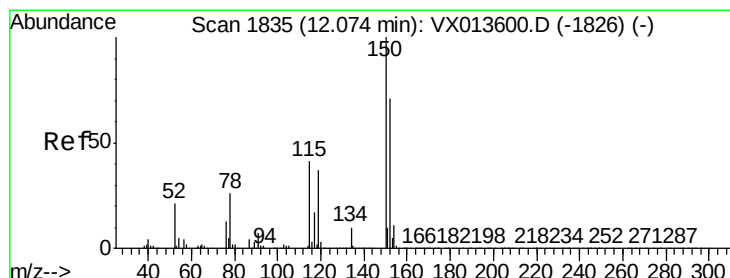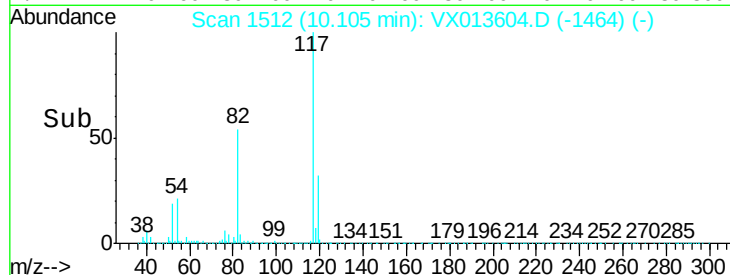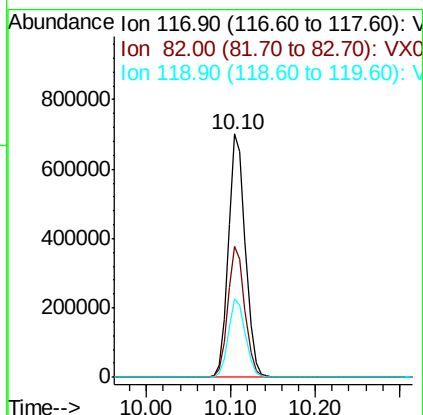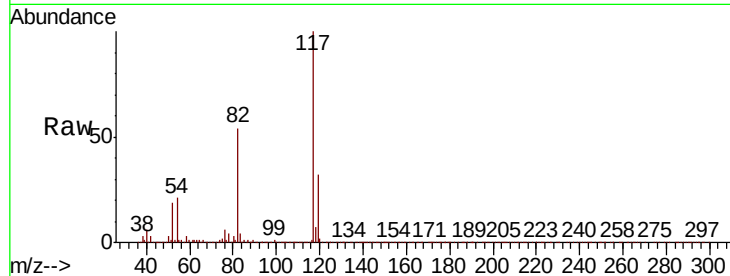

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX013604.D
Acq: 26 Nov 2019 17:17

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.7	38.4	115.1
150	156.1	0.0	346.8

