

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025344.D
 Acq On : 26 Nov 2021 10:13
 Operator : JC/MD
 Sample : VX1126WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 26 23:56:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 26 23:56:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	156559	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	141320	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	66644	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	51512	48.212	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	96.420%		
7) Chloroethane-d5	1.666	69	43906	49.790	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.580%		
11) 1,1-Dichloroethene-d2	2.306	63	65946	38.710	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.420%		
21) 2-Butanone-d5	4.452	46	84748	106.555	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	106.550%		
24) Chloroform-d	5.062	84	95249	51.008	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.020%		
26) 1,2-Dichloroethane-d4	5.958	65	61575	52.903	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.800%		
32) Benzene-d6	5.976	84	195743	52.262	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.520%		
36) 1,2-Dichloropropane-d6	7.311	67	60853	52.476	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.960%		
41) Toluene-d8	8.646	98	178628	50.528	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.060%		
43) trans-1,3-Dichloroprop...	8.951	79	29464	50.537	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	101.080%		
47) 2-Hexanone-d5	9.384	63	63509	105.211	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.210%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	85550	52.200	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.400%		
66) 1,2-Dichlorobenzene-d4	12.323	152	70111	53.638	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.280%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.306	101	826	0.910	ug/L	# 24
44) trans-1,3-Dichloropropene	8.951	75	1599	1.079	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025344.D
Acq On : 26 Nov 2021 10:13
Operator : JC/MD
Sample : VX1126WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 26 23:56:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 26 23:56:11 2021
Response via : Initial Calibration




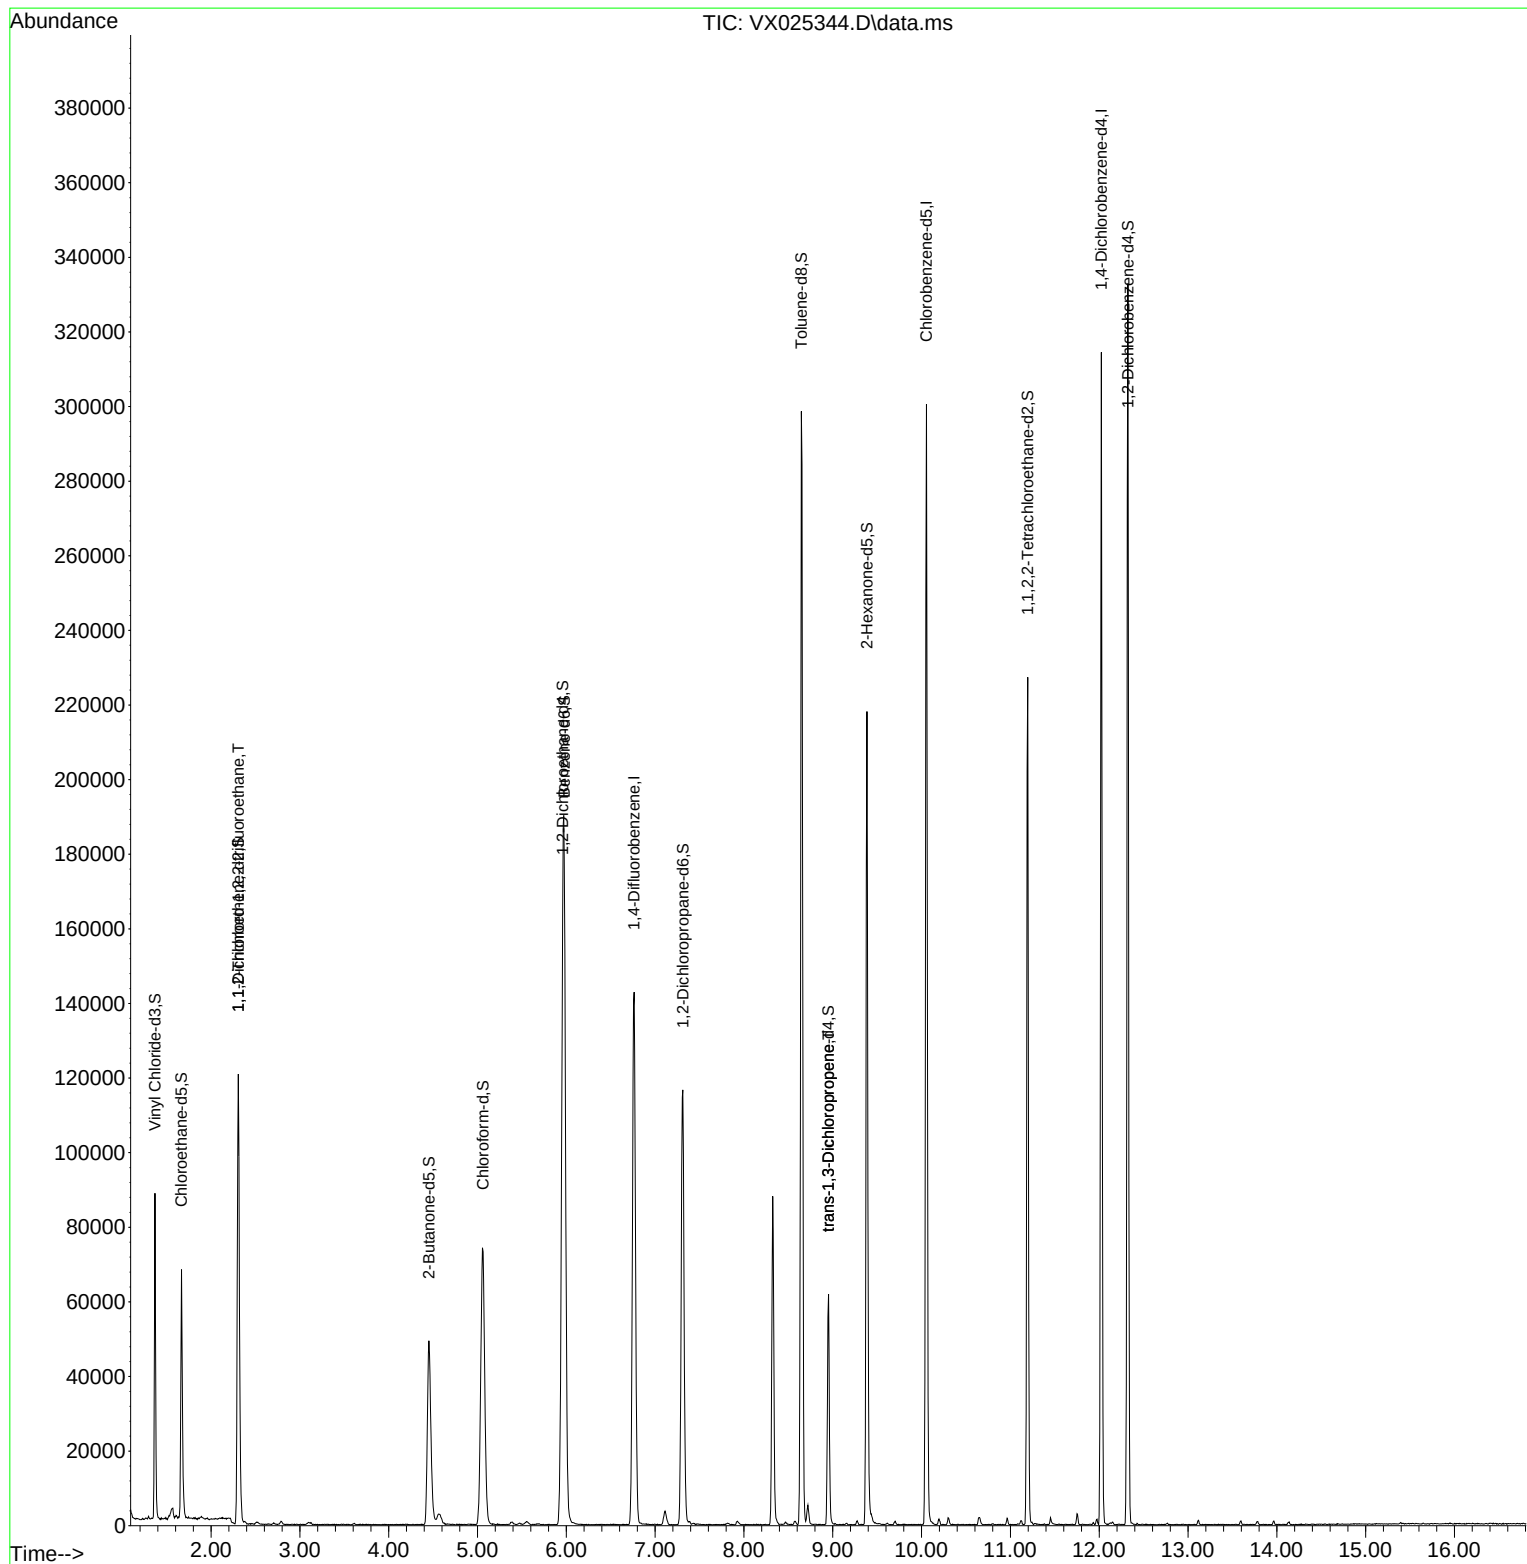


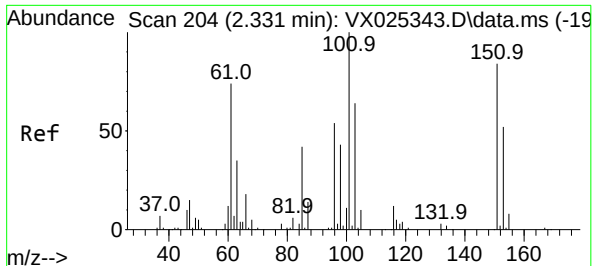

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.910 ug/L
RT: 2.306 min Scan# 204
Delta R.T. -0.025 min
Lab File: VX025344.D
Acq: 26 Nov 2021 10:13

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:101 Resp: 826
Ion Ratio Lower Upper
101 100
85 0.0 34.3 51.5#
151 9.0 65.2 97.8#

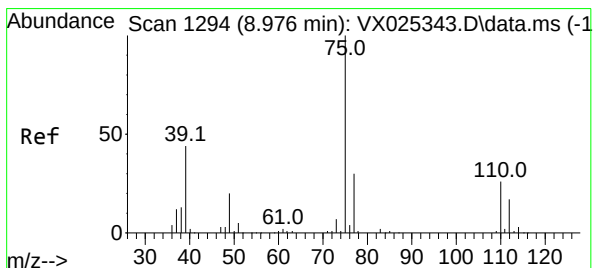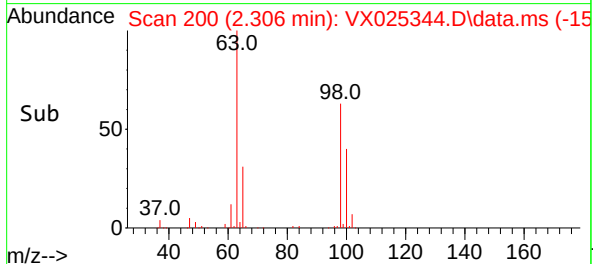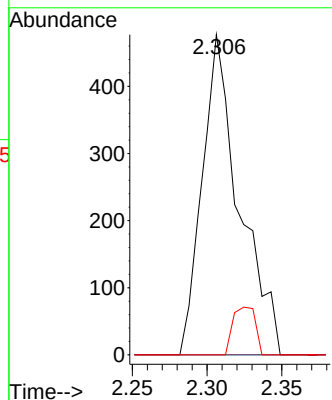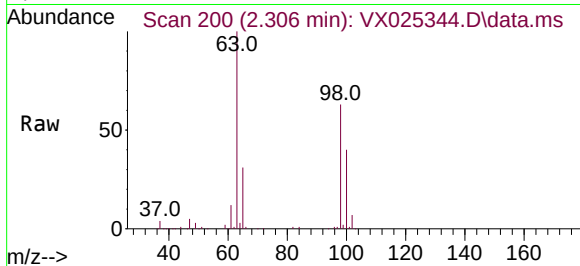

#44
trans-1,3-Dichloropropene
Concen: 1.079 ug/L
RT: 8.951 min Scan# 1290
Delta R.T. -0.025 min
Lab File: VX025344.D
Acq: 26 Nov 2021 10:13

Tgt Ion: 75 Resp: 1599
Ion Ratio Lower Upper
75 100
77 38.3 23.0 42.8

