

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025345.D
 Acq On : 26 Nov 2021 10:43
 Operator : JC/MD
 Sample : M4799-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0P61

Quant Time: Nov 26 23:56:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 26 23:56:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	161258	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	145154	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	69854	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	49634	45.101	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.200%		
7) Chloroethane-d5	1.666	69	43494	47.886	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.780%		
11) 1,1-Dichloroethene-d2	2.306	63	65645	37.411	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.820%		
21) 2-Butanone-d5	4.452	46	82935	101.237	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.240%		
24) Chloroform-d	5.062	84	95820	49.819	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.640%		
26) 1,2-Dichloroethane-d4	5.958	65	61518	51.314	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.620%		
32) Benzene-d6	5.976	84	194906	50.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.320%		
36) 1,2-Dichloropropane-d6	7.311	67	60985	51.201	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.400%		
41) Toluene-d8	8.646	98	180727	49.771	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.540%		
43) trans-1,3-Dichloroprop...	8.951	79	29486	49.239	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.480%		
47) 2-Hexanone-d5	9.384	63	62754	101.215	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.210%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	85516	50.801	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.600%		
66) 1,2-Dichlorobenzene-d4	12.323	152	71689	52.325	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.640%		
Target Compounds					Qvalue	
13) Acetone	2.379	43	3557	5.280	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025345.D
Acq On : 26 Nov 2021 10:43
Operator : JC/MD
Sample : M4799-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0P61

Quant Time: Nov 26 23:56:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 26 23:56:11 2021
Response via : Initial Calibration

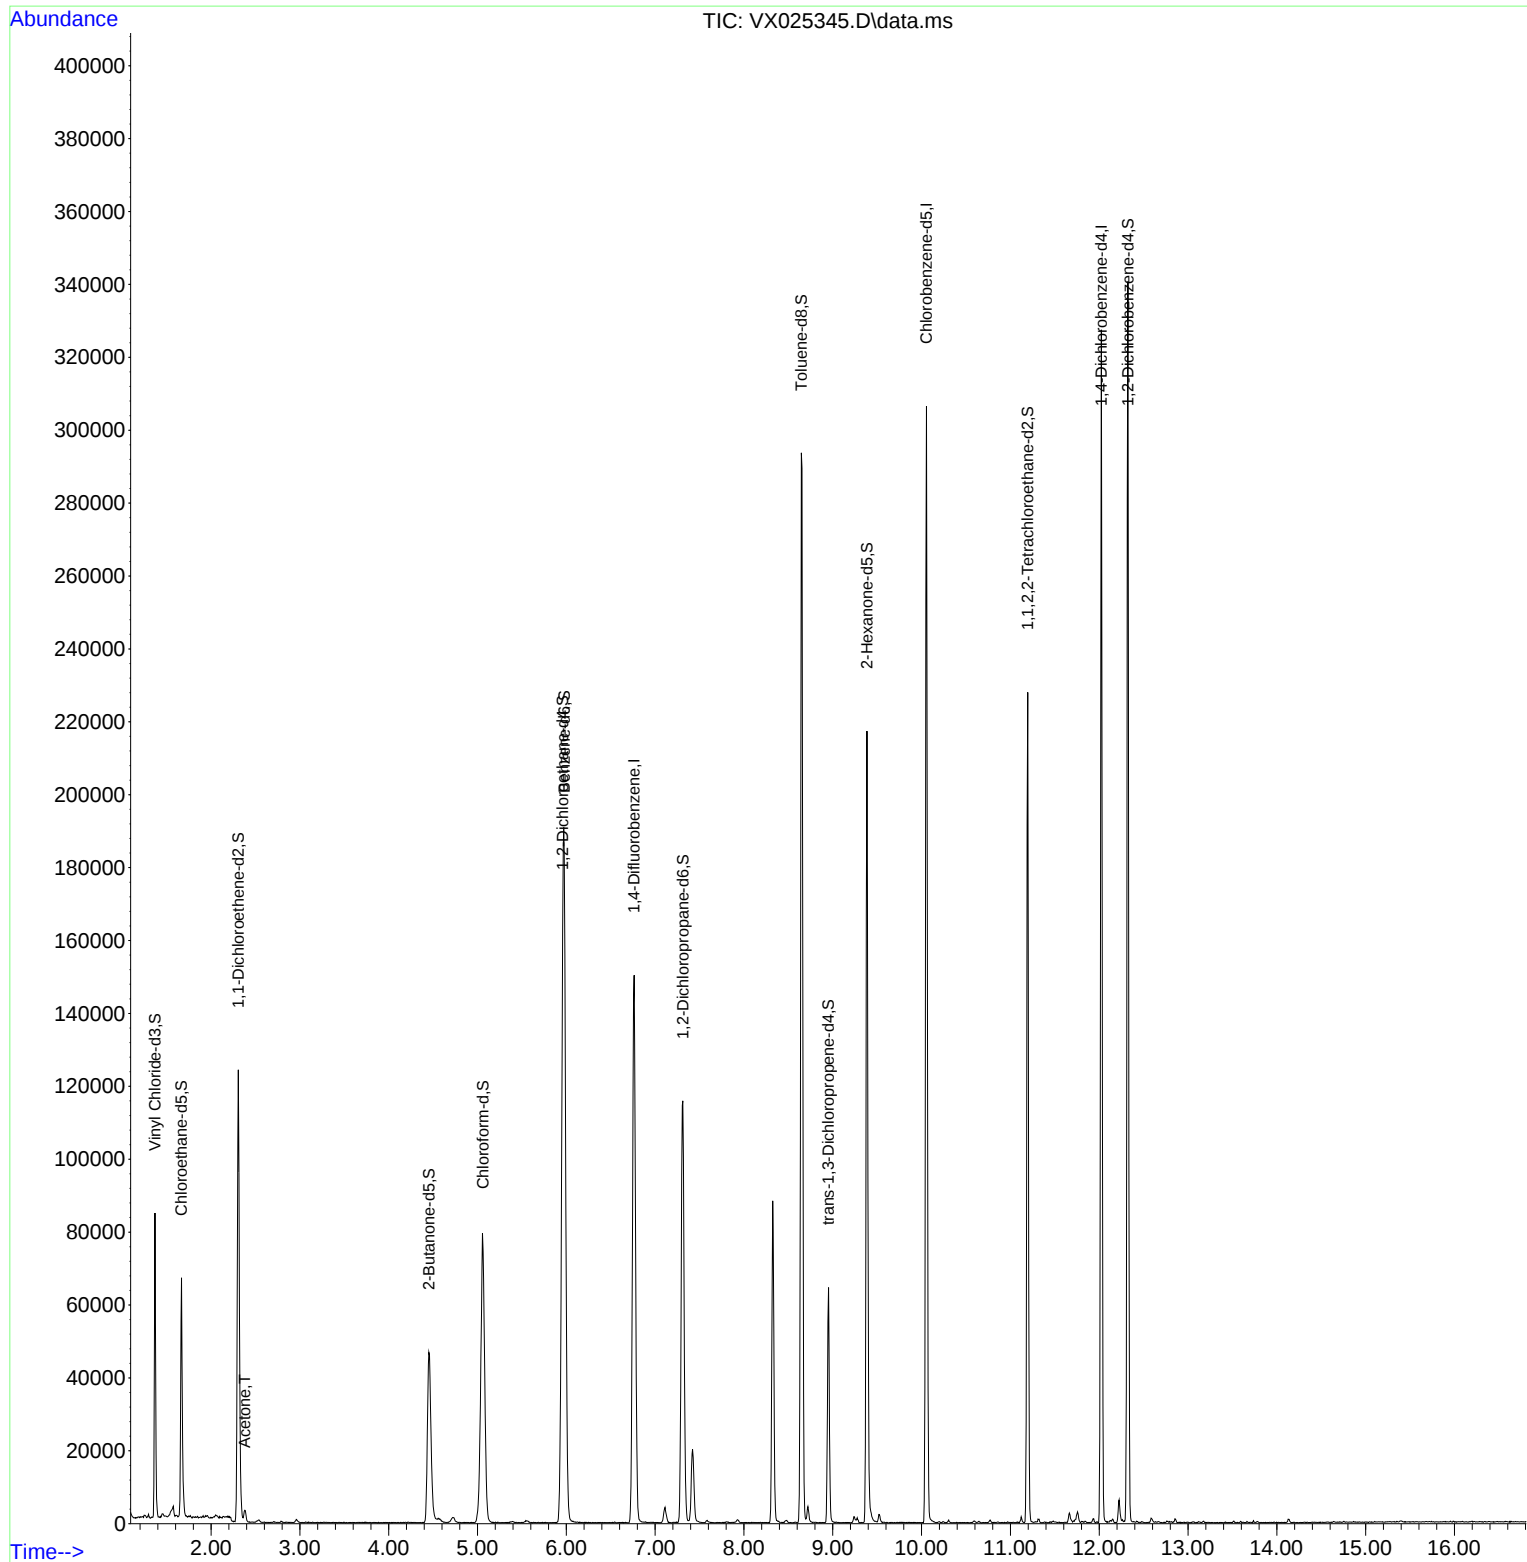

Abundance Scan 212 (2.380 min): VX025343.D\data.ms (-20

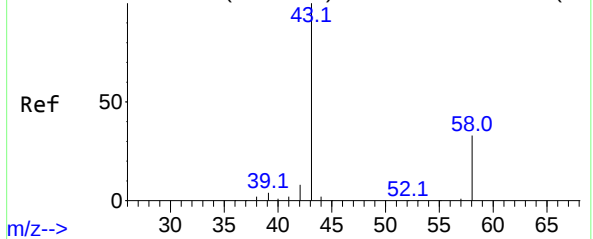

#13

Acetone

Concen: 5.280 ug/L

RT: 2.379 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX025345.D

Acq: 26 Nov 2021 10:43


Instrument :

MSVOA_X

ClientSampleId :

C0P61

Abundance Scan 212 (2.379 min): VX025345.D\data.ms

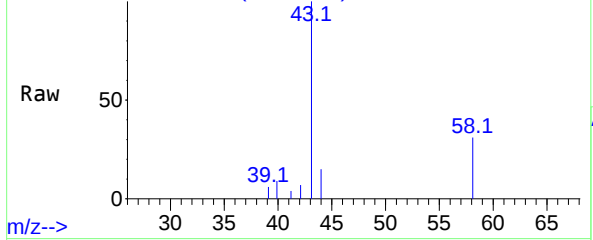

Tgt Ion: 43 Resp: 3557

Ion Ratio Lower Upper

43 100

58 33.3 0.0 65.6

Abundance Scan 212 (2.379 min): VX025345.D\data.ms (-16

